
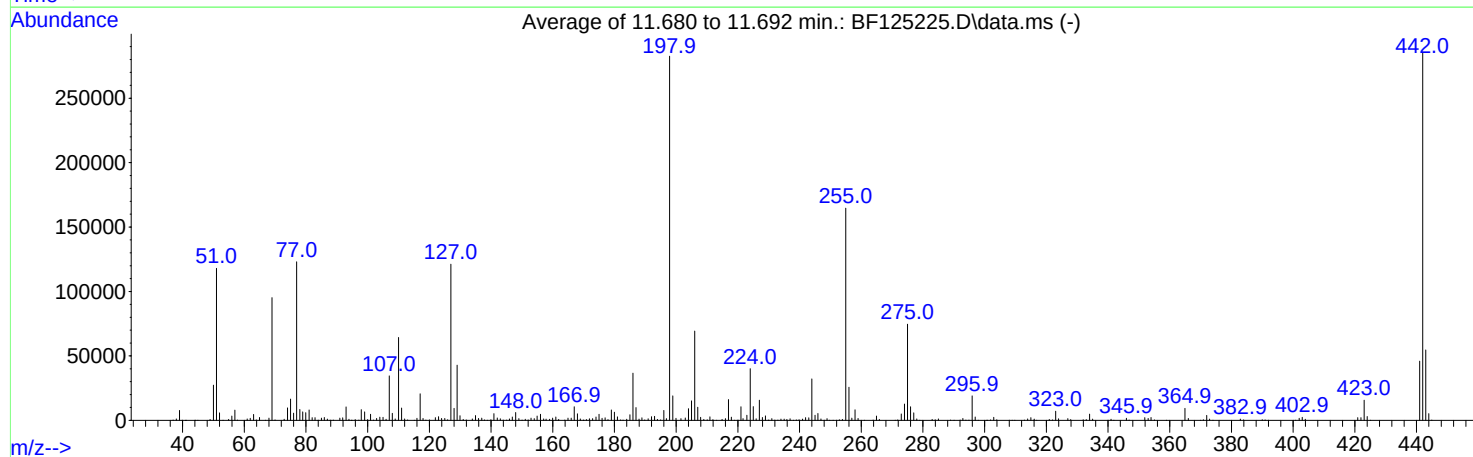


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082621\
 Data File : BF125225.D
 Acq On : 26 Aug 2021 14:13
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 24 12:39:21 2021

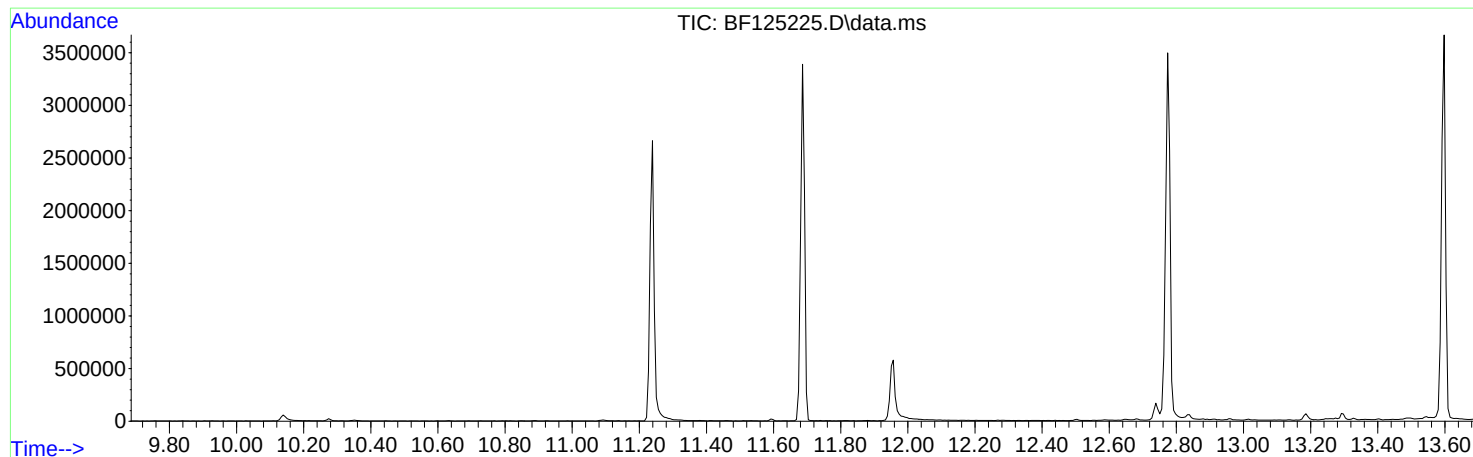




AutoFind: Scans 1631, 1632, 1633; Background Corrected with Scan 1626

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.7	117976	PASS
68	69	0.00	2	1.8	1723	PASS
69	198	0.00	100	33.7	95253	PASS
70	69	0.00	2	0.4	417	PASS
127	198	10	80	42.9	121237	PASS
197	198	0.00	2	0.5	1407	PASS
198	198	100	100	100.0	282645	PASS
199	198	5	9	6.7	19043	PASS
275	198	10	60	26.4	74635	PASS
365	198	1	100	3.3	9362	PASS
441	198	0.01	100	16.3	46009	PASS
442	442	50	100	100.0	285456	PASS
443	442	15	24	19.1	54627	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082621\
Data File : BF125225.D
Acq On : 26 Aug 2021 14:13
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 26 14:56:44 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 24 12:39:21 2021
Response via : Initial Calibration

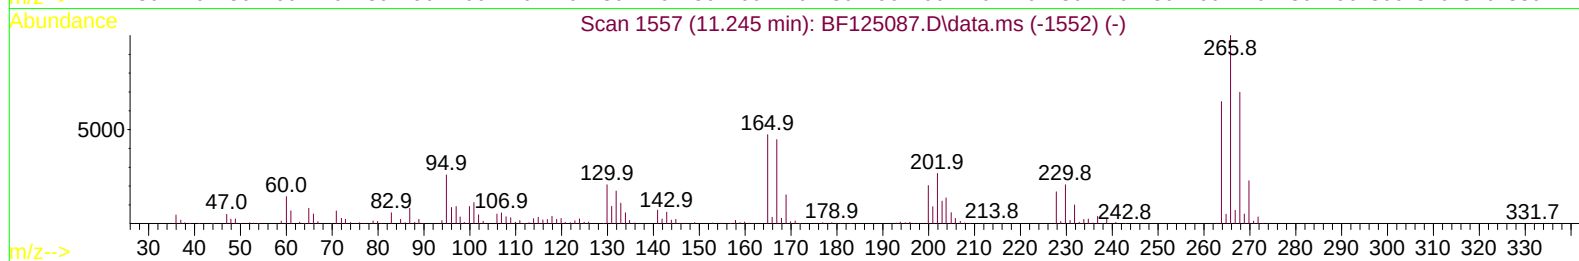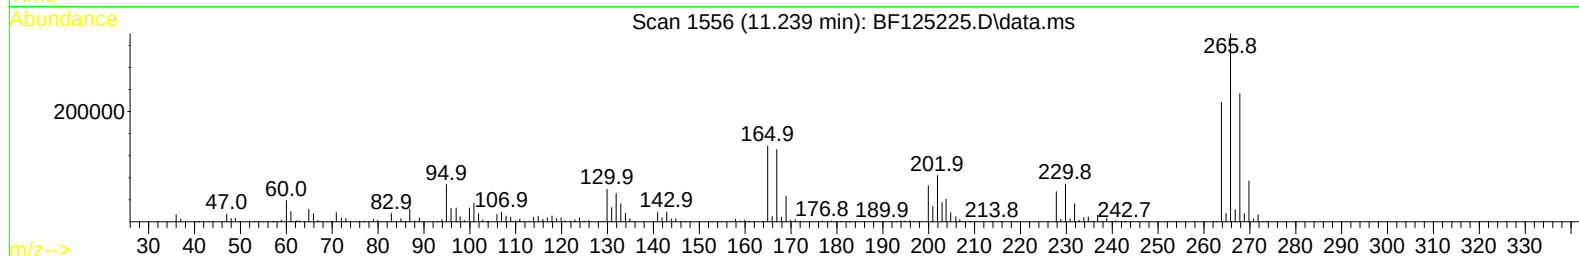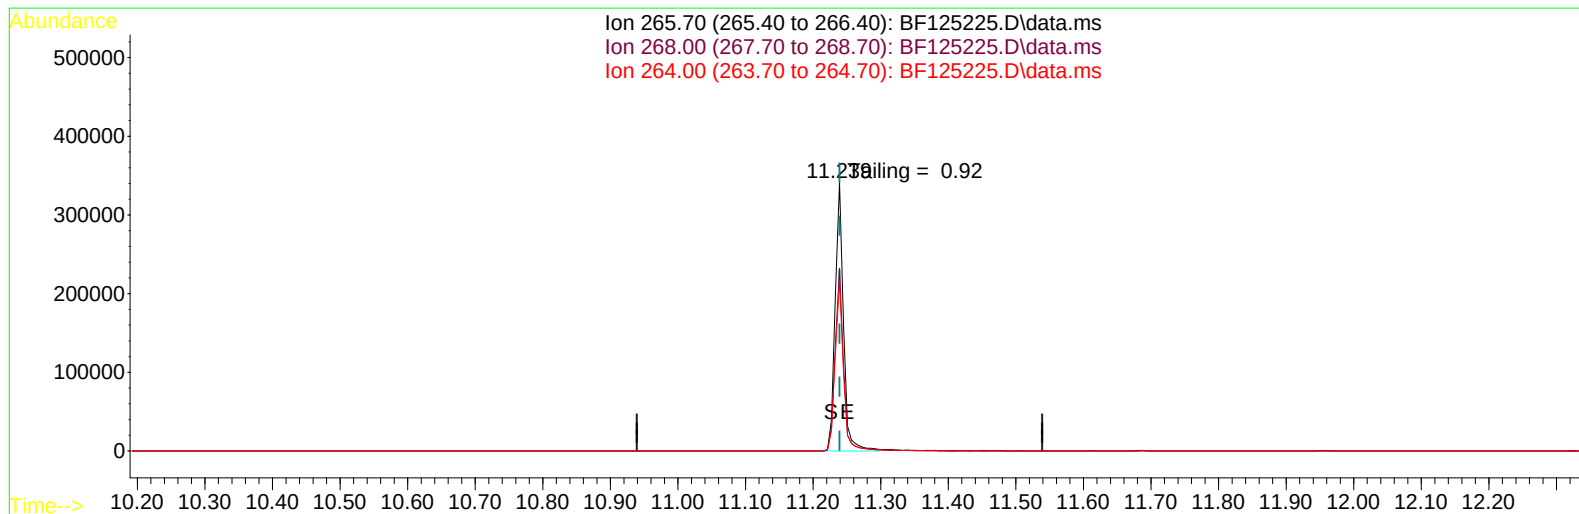

TIC: BF125225.D\data.ms

(70) Pentachlorophenol (C)

11.239min (-0.000) 300359.57 ng




response 294645

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	68.16
264.00	69.90	63.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082621\
 Data File : BF125225.D
 Acq On : 26 Aug 2021 14:13
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Aug 26 14:56:44 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 24 12:39:21 2021
 Response via : Initial Calibration

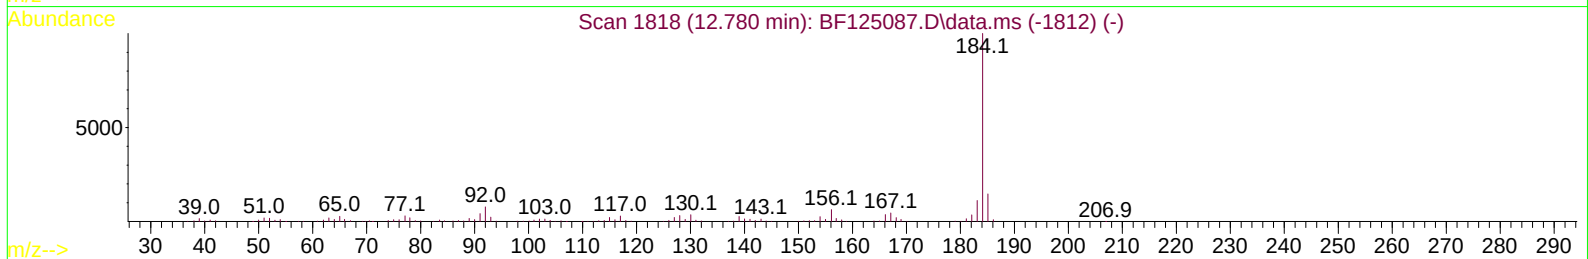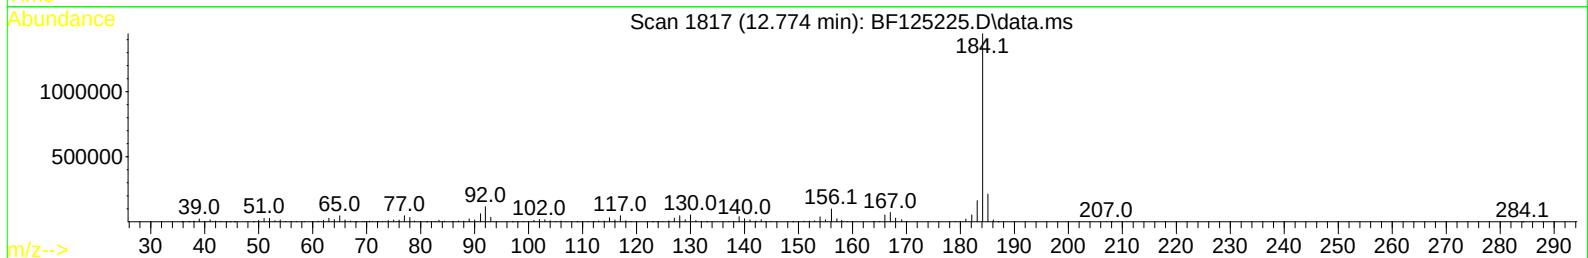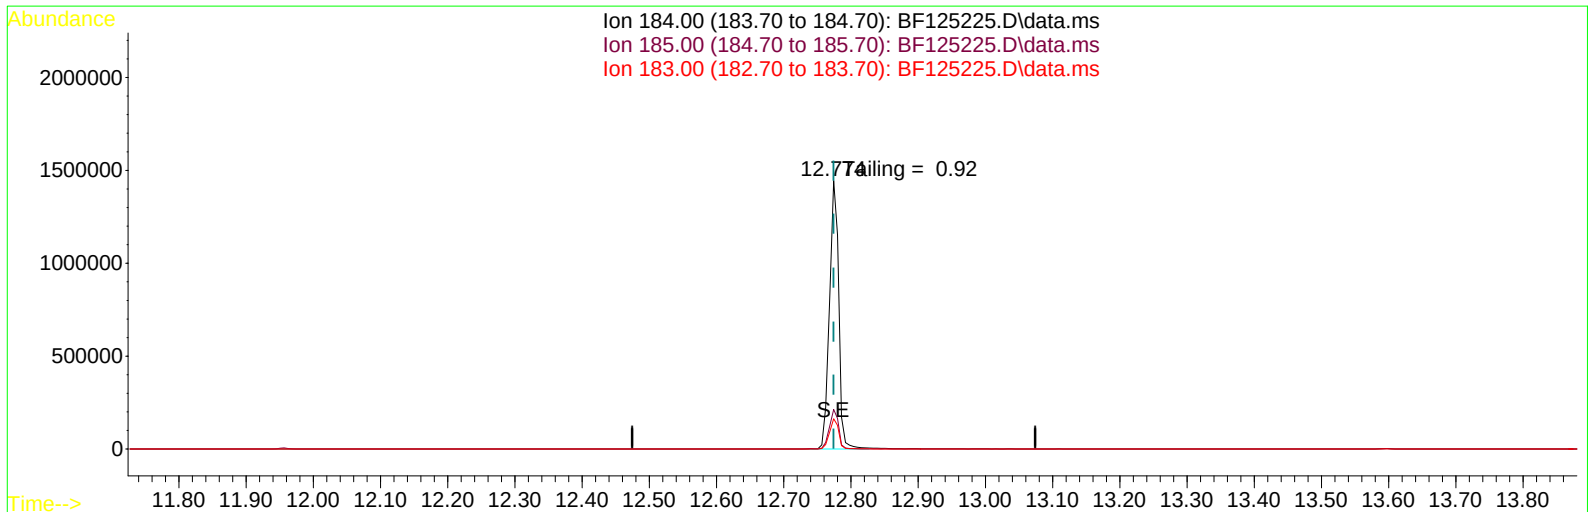

TIC: BF125225.D\data.ms

(77) Benzidine

12.774min (-0.000) 43272.50 ng

response 1393403

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.73
183.00	10.10	11.26
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/26/2021	BNA_F	<u>BF125225.D</u>
Compound Name	Response	Retention Time
DDT	618673	13.59
DDD	11442	13.29
DDE	1823	12.95
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13265	631938	2.10