

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082622\
 Data File : BF130015.D
 Acq On : 26 Aug 2022 12:47
 Operator : CG\JU
 Sample : N4291-01RE
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 Y-7RE

Quant Time: Aug 27 06:06:15 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 25 14:45:09 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.745	152	128504	20.000	ng	-0.01
21) Naphthalene-d8	8.028	136	528530	20.000	ng	-0.01
39) Acenaphthene-d10	9.780	164	278346	20.000	ng	-0.01
64) Phenanthrene-d10	11.269	188	474328	20.000	ng	-0.01
76) Chrysene-d12	13.921	240	246227	20.000	ng	0.00
86) Perylene-d12	15.362	264	202546	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.392	112	293991	37.879	ng	0.00
7) Phenol-d6	6.416	99	218273	22.458	ng	0.00
23) Nitrobenzene-d5	7.322	82	830638	84.131	ng	-0.01
42) 2,4,6-Tribromophenol	10.580	330	218999	78.393	ng	0.00
45) 2-Fluorobiphenyl	9.104	172	1524583	83.189	ng	-0.01
79) Terphenyl-d14	12.857	244	1436690	97.088	ng	0.00
Target Compounds						
35) Caprolactam	8.469	113	26638	11.155	ng	Qvalue 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082622\
Data File : BF130015.D
Acq On : 26 Aug 2022 12:47
Operator : CG\JU
Sample : N4291-01RE
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
Y-7RE

Quant Time: Aug 27 06:06:15 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 25 14:45:09 2022
Response via : Initial Calibration



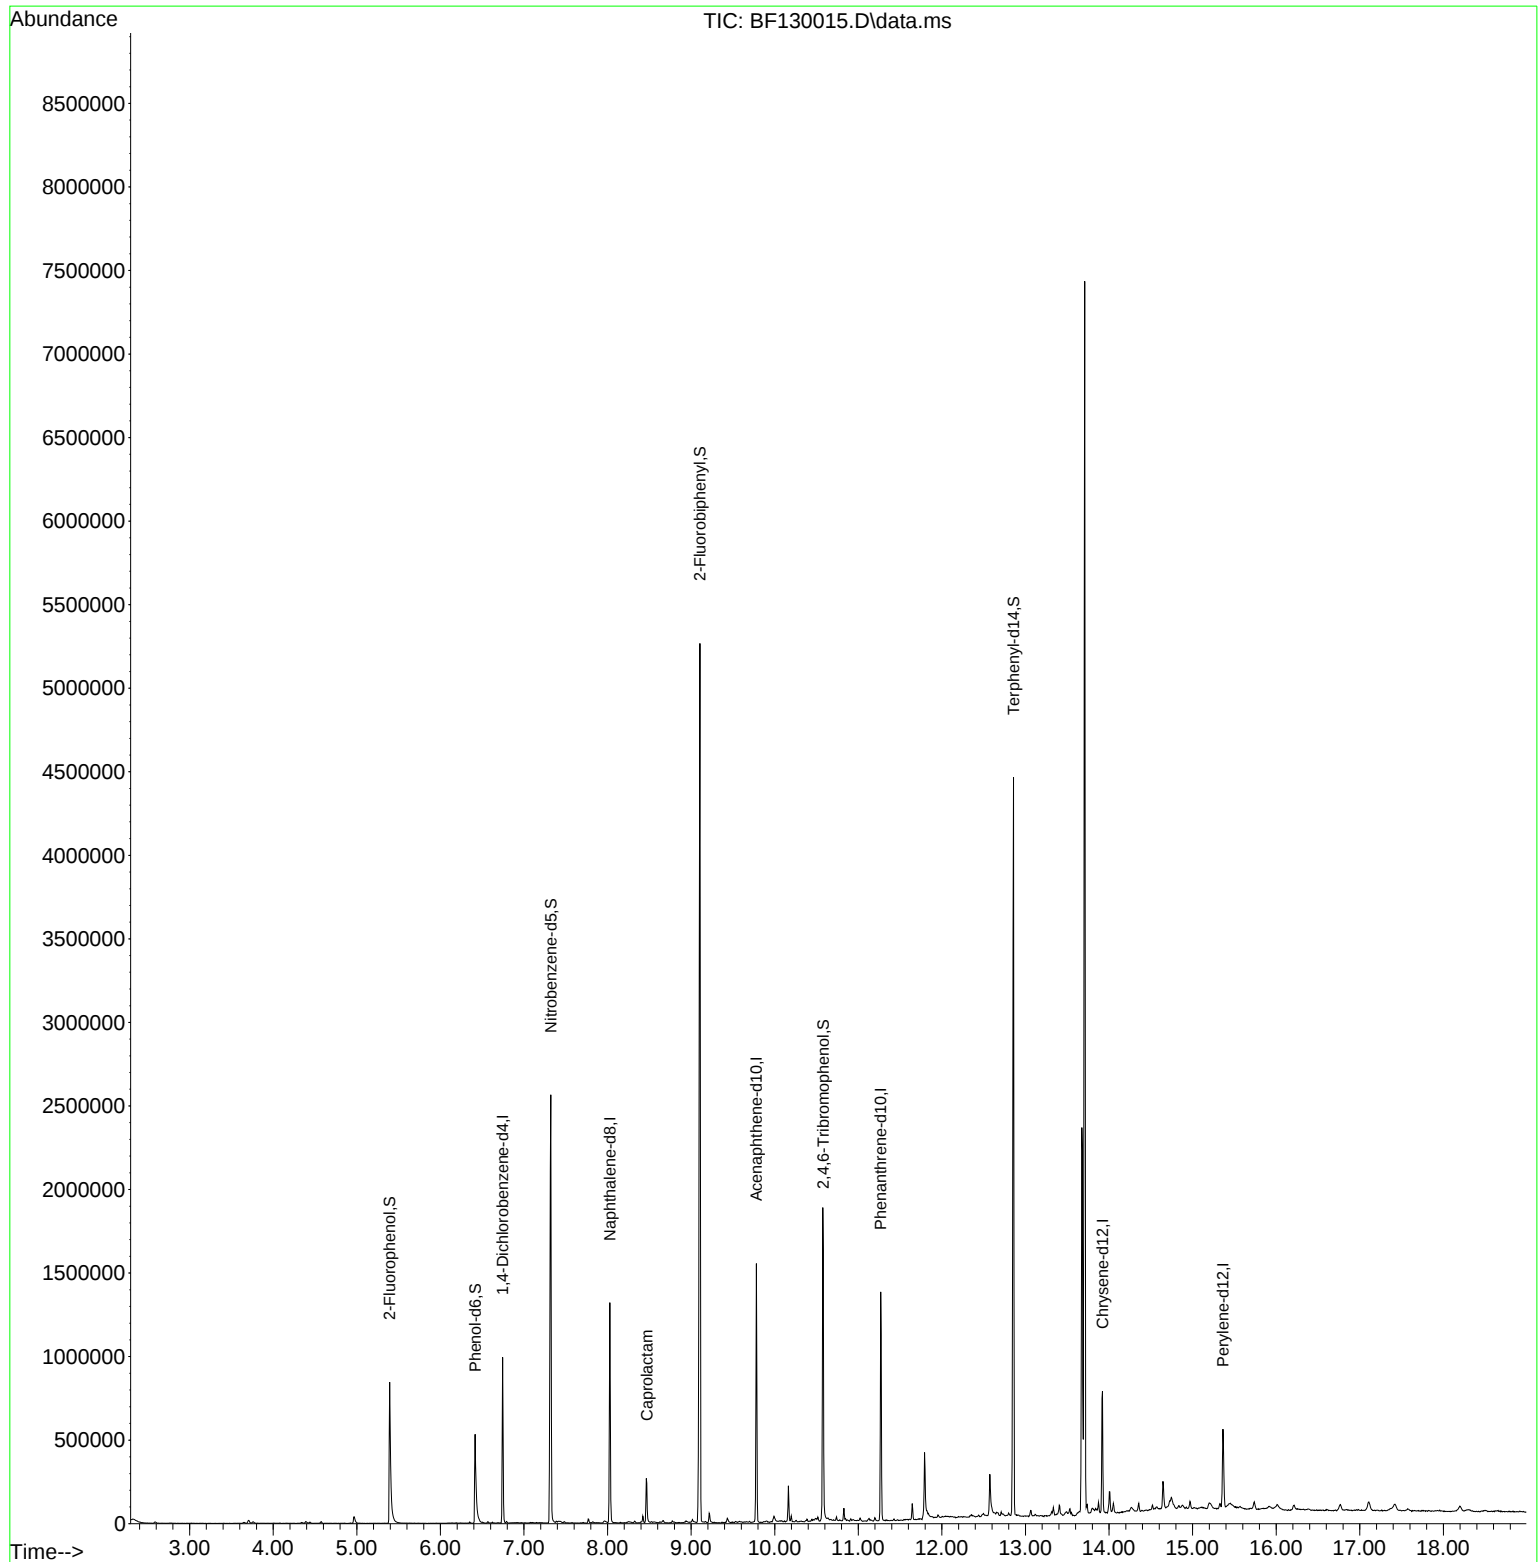




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.745 min Scan# 71
Delta R.T. -0.012 min
Lab File: BF130015.D
Acq: 26 Aug 2022 12:47




Instrument :
BNA_F
ClientSampleId :
Y-7RE


Tgt Ion:152 Resp: 128504
Ion Ratio Lower Upper
152 100
150 153.9 126.9 190.3
115 65.7 53.4 80.0

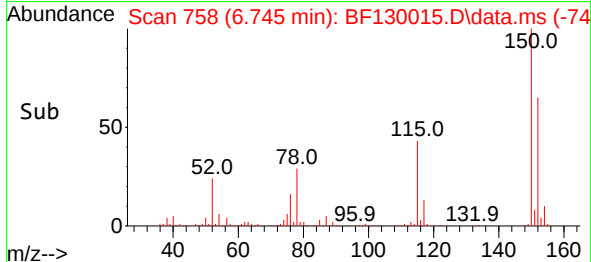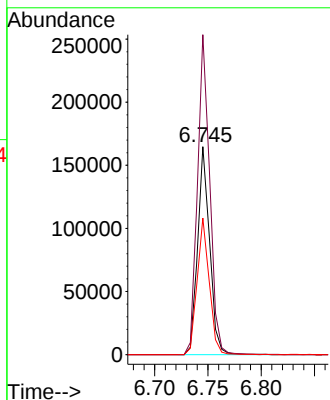

#5
2-Fluorophenol
Concen: 37.879 ng
RT: 5.392 min Scan# 528
Delta R.T. -0.000 min
Lab File: BF130015.D
Acq: 26 Aug 2022 12:47

Tgt Ion:112 Resp: 293991
Ion Ratio Lower Upper
112 100
64 59.8 47.6 71.4
63 32.1 24.6 37.0


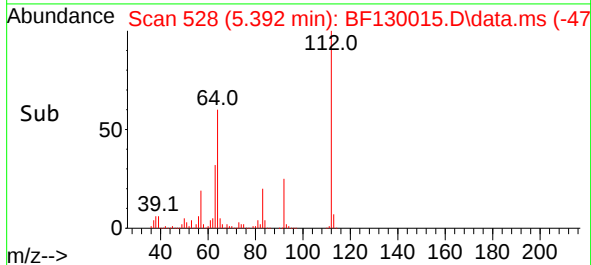
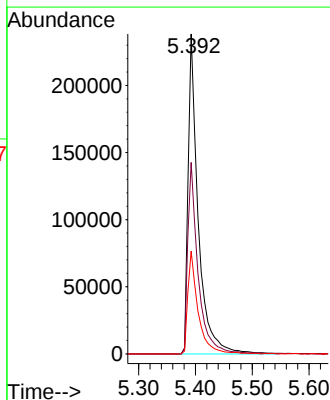
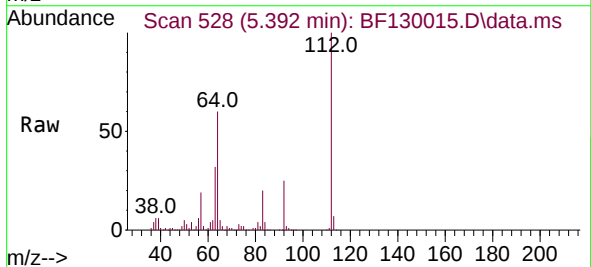


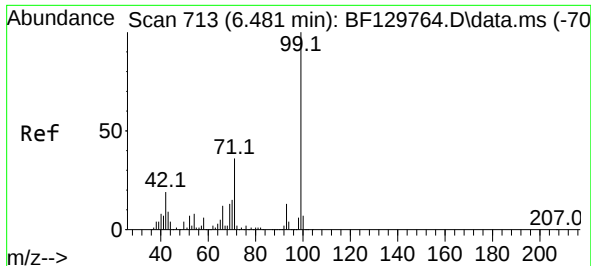

#7
Phenol-d6
Concen: 22.458 ng
RT: 6.416 min Scan# 70
Delta R.T. -0.006 min
Lab File: BF130015.D
Acq: 26 Aug 2022 12:47




Instrument :
BNA_F
ClientSampleId :
Y-7RE

Tgt Ion: 99 Resp: 218273
Ion Ratio Lower Upper
99 100
42 19.7 15.0 22.4
71 37.1 28.8 43.2

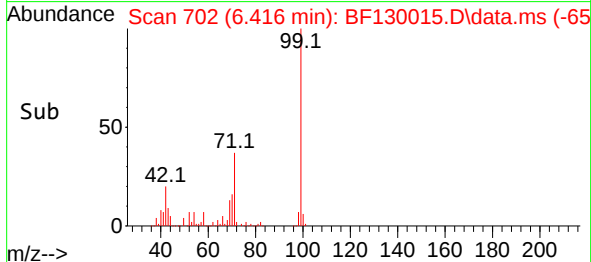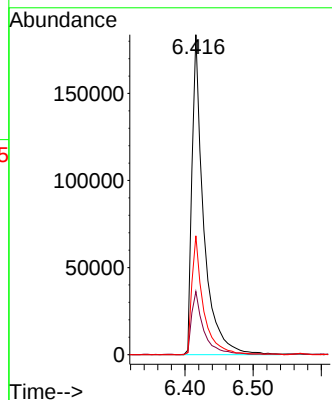

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.028 min Scan# 976
Delta R.T. -0.012 min
Lab File: BF130015.D
Acq: 26 Aug 2022 12:47

Tgt Ion: 136 Resp: 528530
Ion Ratio Lower Upper
136 100
137 11.2 8.4 12.6
54 7.9 6.2 9.2
68 5.2 4.2 6.4


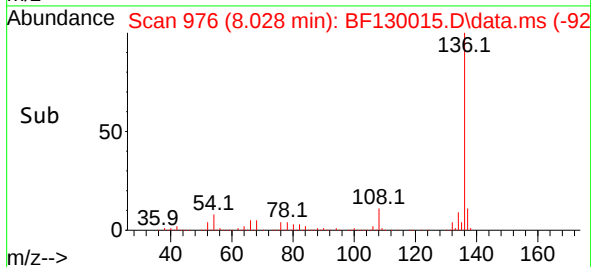
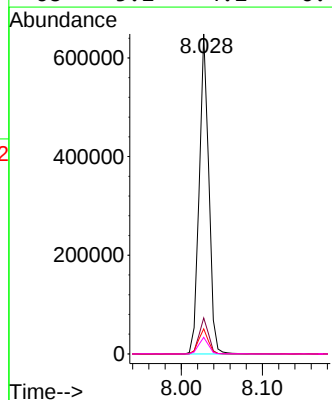
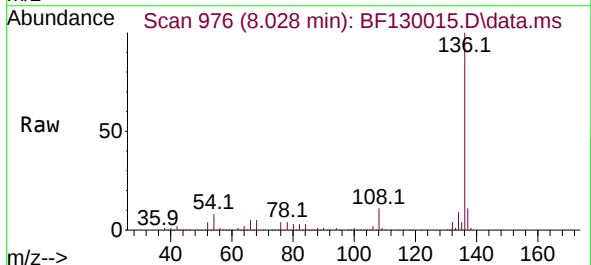




#23
Nitrobenzene-d5
Concen: 84.131 ng
RT: 7.322 min Scan# 81
Delta R.T. -0.012 min
Lab File: BF130015.D
Acq: 26 Aug 2022 12:47




Instrument :
BNA_F
ClientSampleId :
Y-7RE


Tgt Ion: 82 Resp: 830638
Ion Ratio Lower Upper
82 100
128 43.0 36.1 54.1
54 51.1 40.0 60.0

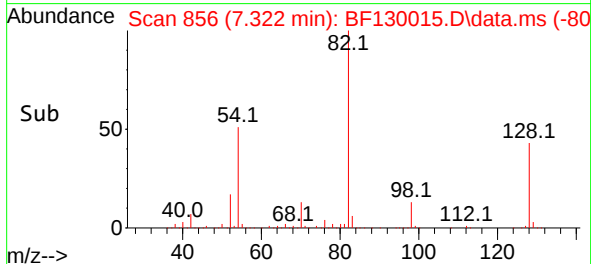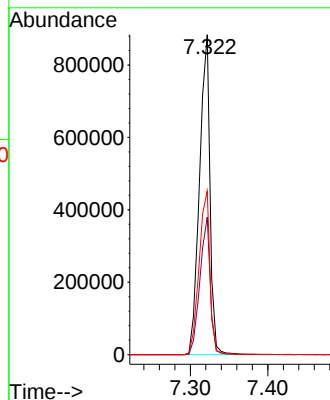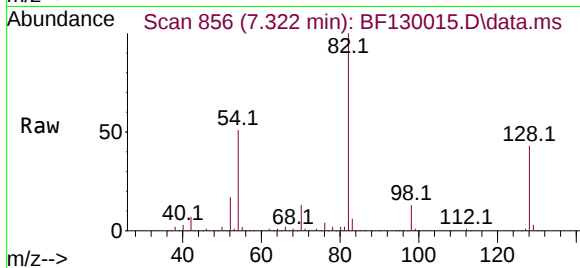

#35
Caprolactam
Concen: 11.155 ng
RT: 8.469 min Scan# 1051
Delta R.T. -0.041 min
Lab File: BF130015.D
Acq: 26 Aug 2022 12:47

Tgt Ion: 113 Resp: 26638
Ion Ratio Lower Upper
113 100
55 166.0 148.8 188.8
56 126.1 109.1 149.1


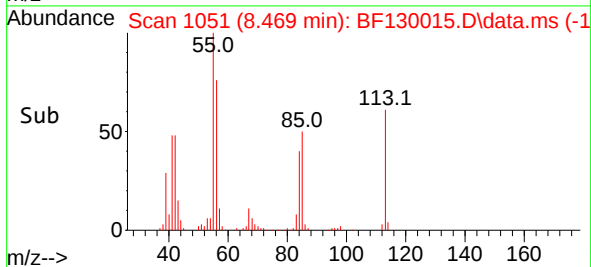
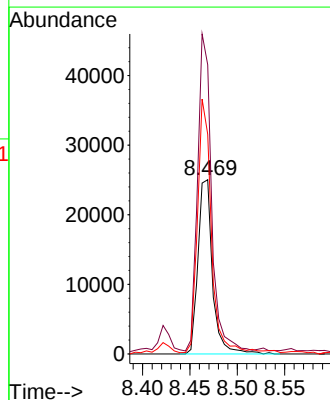
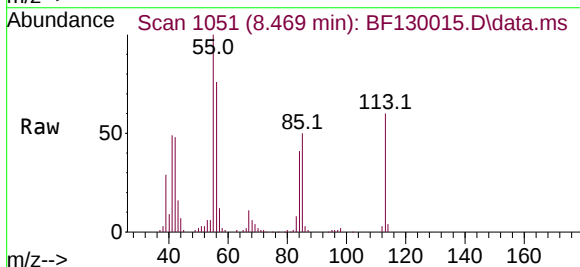




#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.780 min Scan# 11
Delta R.T. -0.012 min
Lab File: BF130015.D
Acq: 26 Aug 2022 12:47




Instrument :
BNA_F
ClientSampleId :
Y-7RE


Tgt Ion:164 Resp: 278346
Ion Ratio Lower Upper
164 100
162 103.7 82.0 123.0
160 45.4 35.4 53.0

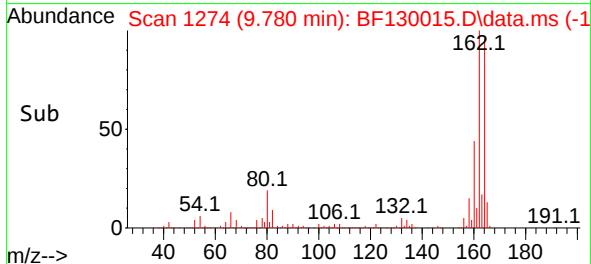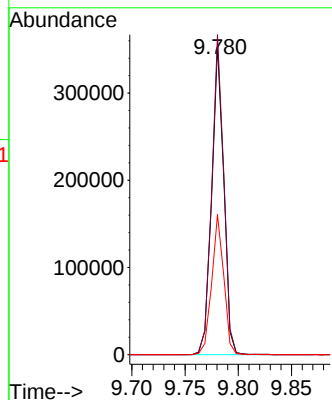

#42
2,4,6-Tribromophenol
Concen: 78.393 ng
RT: 10.580 min Scan# 1410
Delta R.T. -0.006 min
Lab File: BF130015.D
Acq: 26 Aug 2022 12:47

Tgt Ion:330 Resp: 218999
Ion Ratio Lower Upper
330 100
332 103.3 82.6 124.0
141 36.8 27.6 41.4


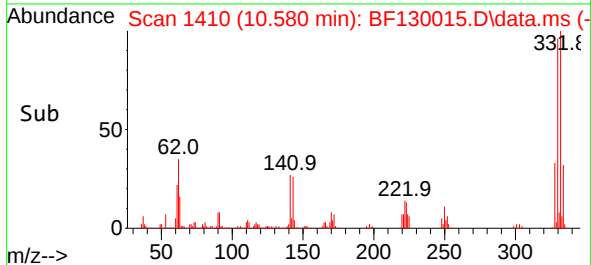
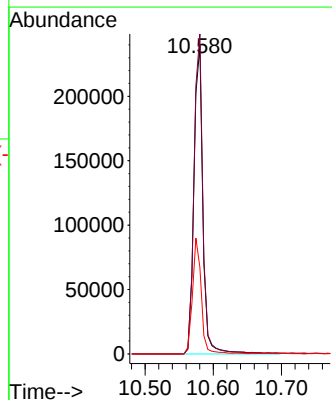
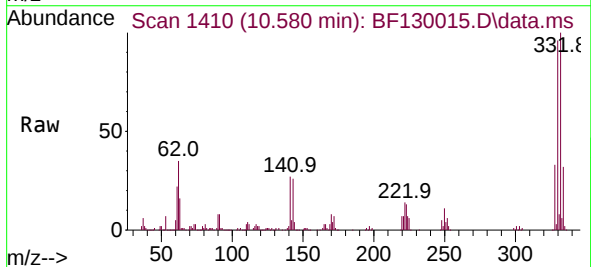


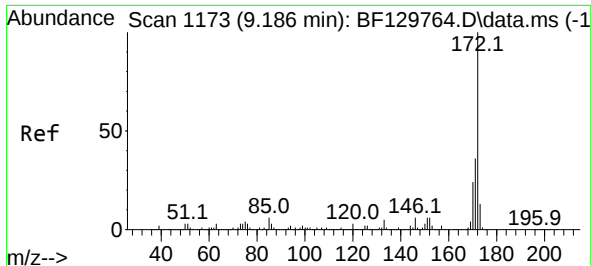

#45
2-Fluorobiphenyl
Concen: 83.189 ng
RT: 9.104 min Scan# 1173
Delta R.T. -0.012 min
Lab File: BF130015.D
Acq: 26 Aug 2022 12:47




Instrument :
BNA_F
ClientSampleId :
Y-7RE


Tgt Ion:172 Resp: 1524583
Ion Ratio Lower Upper
172 100
171 35.5 28.4 42.6
170 23.8 19.1 28.7

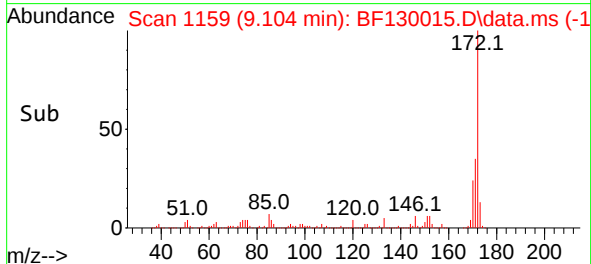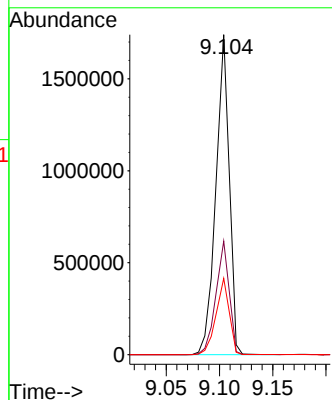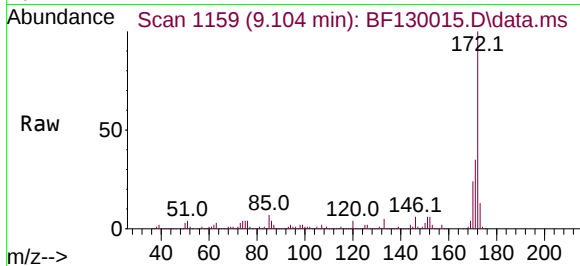

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.269 min Scan# 1527
Delta R.T. -0.012 min
Lab File: BF130015.D
Acq: 26 Aug 2022 12:47

Tgt Ion:188 Resp: 474328
Ion Ratio Lower Upper
188 100
94 9.6 7.4 11.2
80 10.9 7.9 11.9

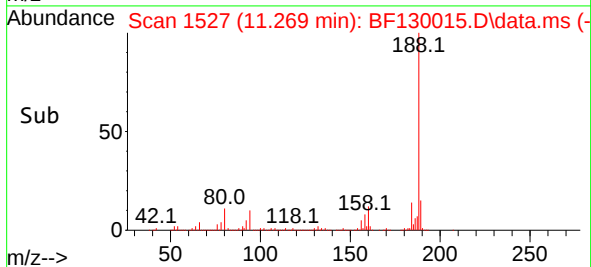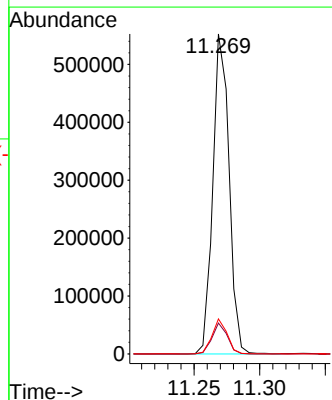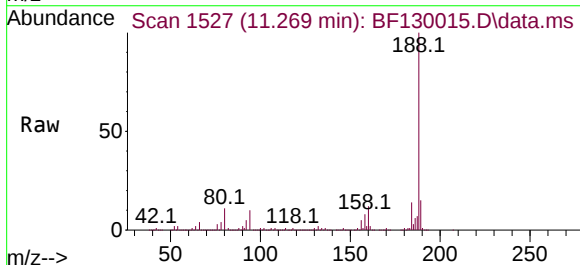



#76

Chrysene-d12

Concen: 20.000 ng

RT: 13.921 min Scan# 1992

Delta R.T. -0.006 min

Lab File: BF130015.D

Acq: 26 Aug 2022 12:47

Instrument :

BNA_F

ClientSampleId :

Y-7RE





Tgt Ion:240 Resp: 246227

Ion Ratio Lower Upper

240 100

120 9.8 9.2 13.8

236 25.3 20.7 31.1

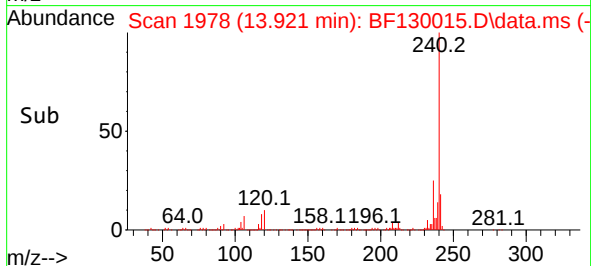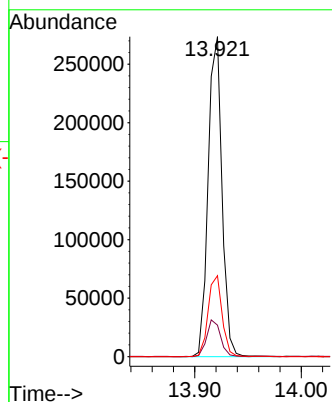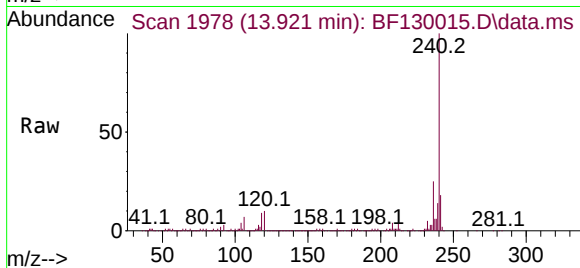

#79

Terphenyl-d14

Concen: 97.088 ng

RT: 12.857 min Scan# 1797

Delta R.T. -0.006 min

Lab File: BF130015.D

Acq: 26 Aug 2022 12:47




Tgt Ion:244 Resp: 1436690


Ion Ratio Lower Upper

244 100

212 7.3 5.9 8.9

122 11.7 9.9 14.9

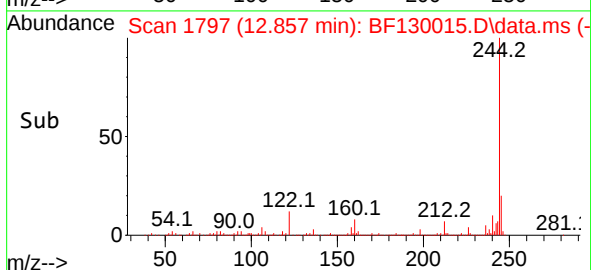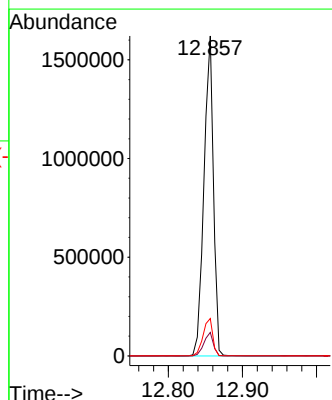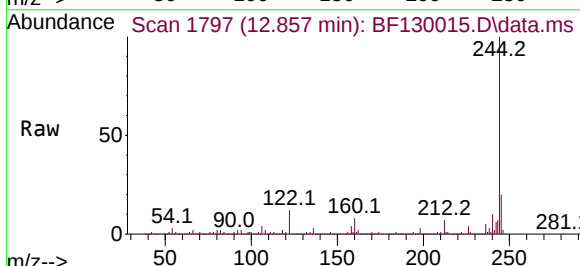

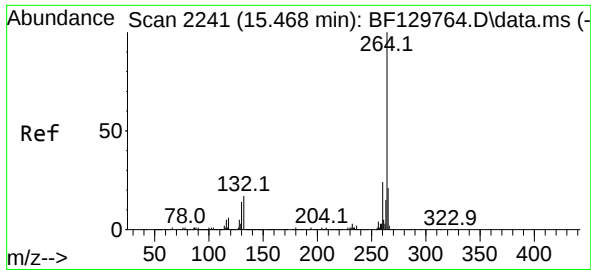

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.362 min Scan# 21

Delta R.T. -0.006 min

Lab File: BF130015.D


Acq: 26 Aug 2022 12:47

Instrument :

BNA_F

ClientSampleId :

Y-7RE

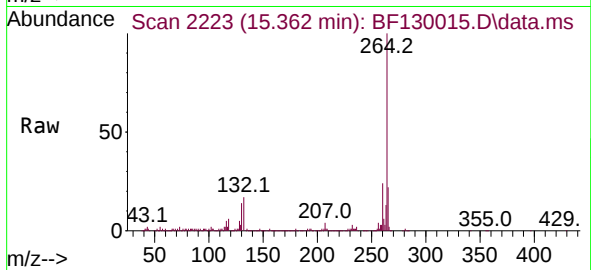

Tgt Ion:264 Resp: 202546

Ion Ratio Lower Upper

264 100

260 23.7 19.1 28.7

265 21.6 16.7 25.1

