

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082622\
 Data File : BF130016.D
 Acq On : 26 Aug 2022 13:21
 Operator : CG\JU
 Sample : N4262-07
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-107(42.5FT)

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF130016.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.334	3	8	19	rVB	50224	81393	1.69%	0.331%
2	4.434	360	365	379	rVB	385886	447079	9.31%	1.817%
3	4.969	453	456	470	rBV	47075	68393	1.42%	0.278%
4	5.387	524	527	547	rBV	1684110	1898596	39.53%	7.715%
5	6.410	698	701	725	rBV	1072813	1211036	25.22%	4.921%
6	6.746	755	758	767	rBV	953887	779369	16.23%	3.167%
7	7.322	851	856	859	rBV	2501983	2537581	52.84%	10.311%
8	8.028	972	976	983	rBV	1267609	1082856	22.55%	4.400%
9	9.104	1154	1159	1162	rBV	5449525	4802525	100.00%	19.515%
10	9.781	1270	1274	1278	rBV	1584914	1261026	26.26%	5.124%
11	10.581	1405	1410	1413	rBV	3249563	2868535	59.73%	11.656%
12	11.269	1524	1527	1531	rBV	1461879	1235613	25.73%	5.021%
13	12.857	1792	1797	1800	rBV	5475042	4801204	99.97%	19.510%
14	13.916	1974	1977	1982	rBV	902049	827514	17.23%	3.363%
15	14.004	1987	1992	1996	rBV	114864	123138	2.56%	0.500%
16	15.363	2219	2223	2233	rVB	472211	583568	12.15%	2.371%




Sum of corrected areas: 24609426

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082622\
Data File : BF130016.D
Acq On : 26 Aug 2022 13:21
Operator : CG\JU
Sample : N4262-07
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-107(42.5FT)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

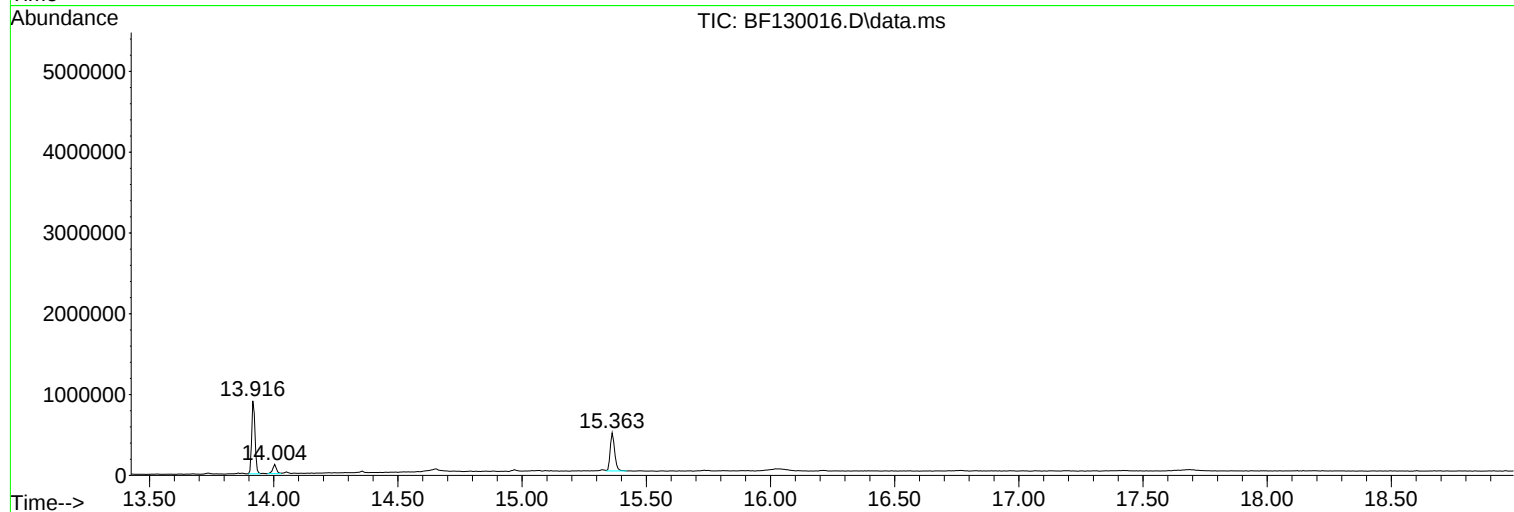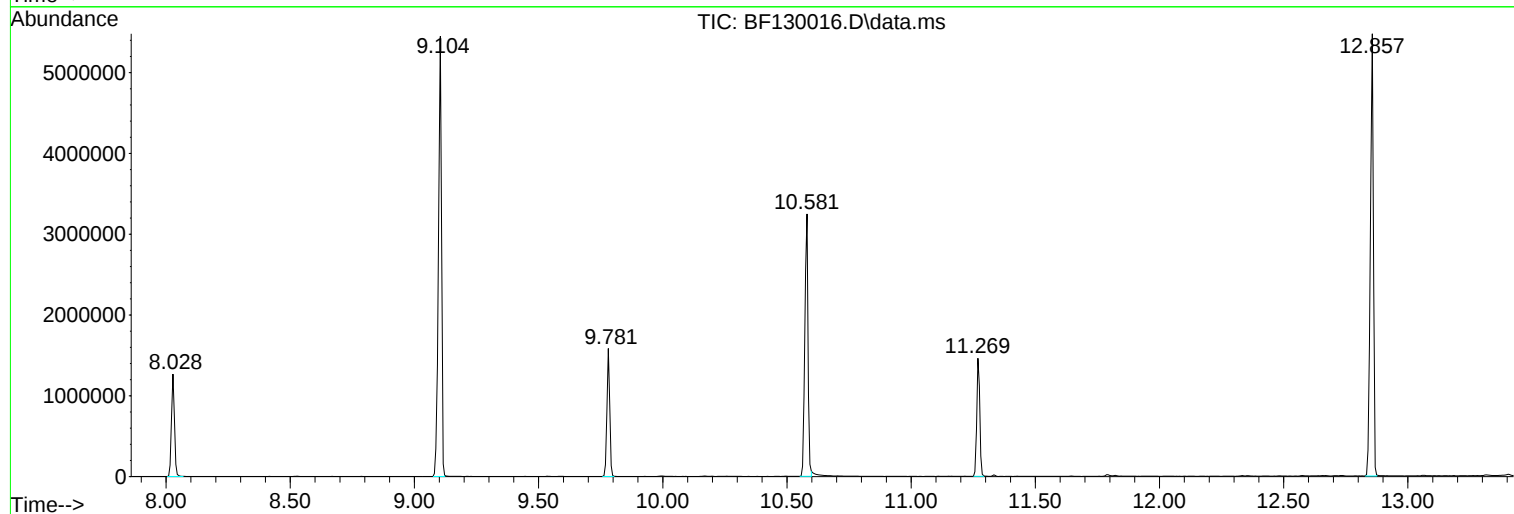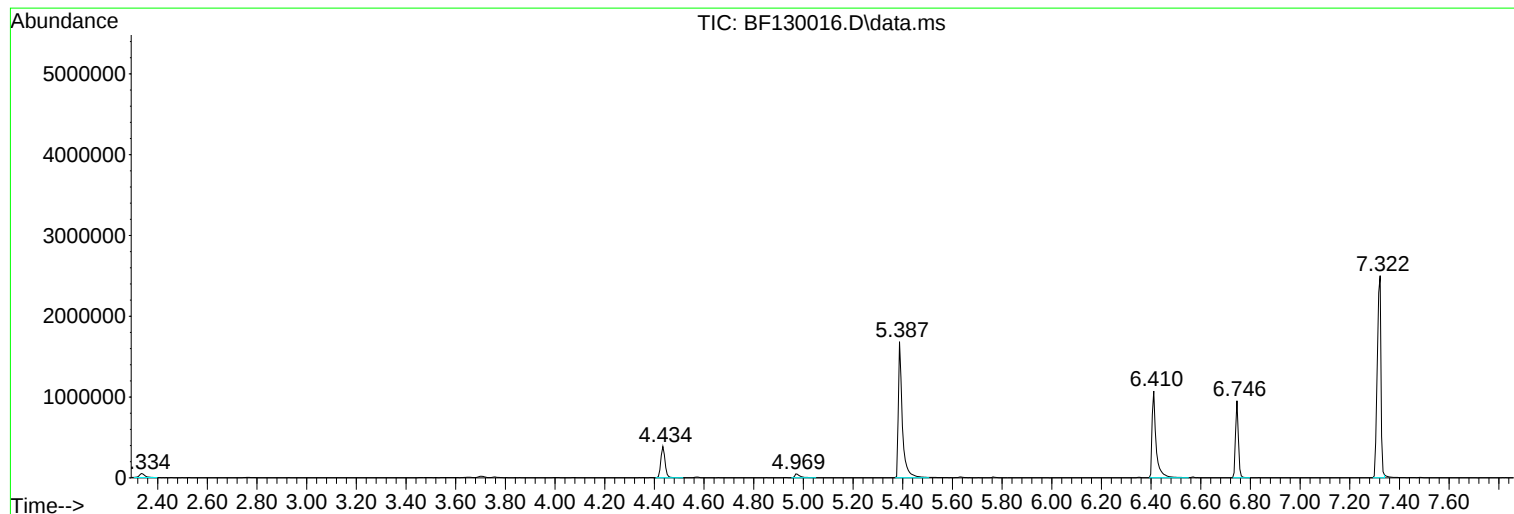

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082622\
Data File : BF130016.D
Acq On : 26 Aug 2022 13:21
Operator : CG\JU
Sample : N4262-07
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-107(42.5FT)










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 Triphenylphosphine oxide Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.004	2.98 ng	123138	Chrysene-d12	13.916

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	97
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19N03S	1000483-83-4	91
3			Cobalt,(.eta.<5>-2,4-cyclopentad...	277	C16H15BCo	036682-12-9	35
4			2-Phenyl-6-(trifluoromethyl)-1H-...	277	C15H10F3NO	1000387-59-3	32
5			1H-Indole-3-acetic acid, 5-[(tri...	277	C14H19N03Si	072101-35-0	17

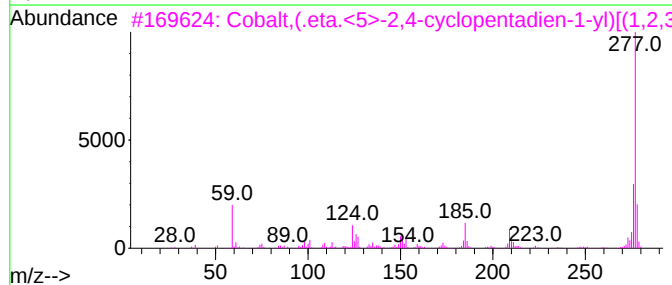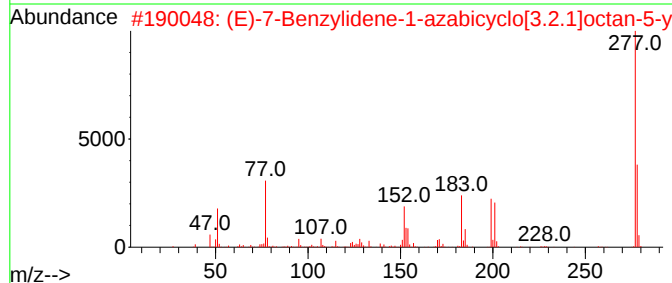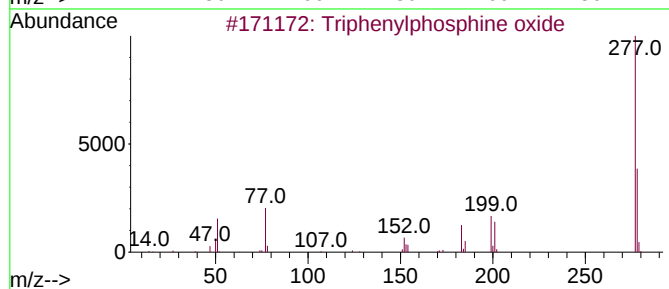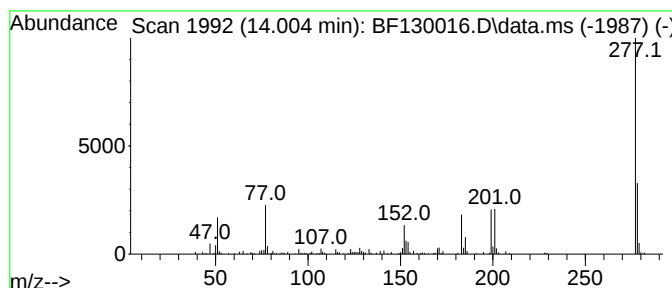

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082622\
Data File : BF130016.D
Acq On : 26 Aug 2022 13:21
Operator : CG\JU
Sample : N4262-07
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-107(42.5FT)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	14.004	3.0	ng	123138	5	13.916	827514	20.0