

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082622\
 Data File : BF130024.D
 Acq On : 26 Aug 2022 17:58
 Operator : CG\JU
 Sample : N4277-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 B-2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF130024.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.969	453	456	469	rBV	175217	240656	7.81%	1.208%
2	5.387	524	527	546	rBV	2491191	2750605	89.24%	13.811%
3	6.410	698	701	717	rBV	2894537	2711720	87.98%	13.616%
4	6.745	755	758	769	rBV	872526	703674	22.83%	3.533%
5	7.322	852	856	866	rBV	1864883	1771534	57.48%	8.895%
6	8.028	973	976	987	rVB	1133730	909455	29.51%	4.567%
7	9.104	1155	1159	1162	rBV	3894549	3082183	100.00%	15.476%
8	9.781	1271	1274	1278	rBV	1115576	863601	28.02%	4.336%
9	10.575	1406	1409	1419	rBV	1542145	1410070	45.75%	7.080%
10	10.669	1423	1425	1430	rVB	33496	41637	1.35%	0.209%
11	11.269	1524	1527	1530	rBV	768463	659558	21.40%	3.312%
12	11.298	1530	1532	1536	rVB	59787	54194	1.76%	0.272%
13	12.486	1731	1734	1738	rBV	135270	116645	3.78%	0.586%
14	12.716	1768	1773	1779	rVB	121085	137552	4.46%	0.691%
15	12.851	1792	1796	1800	rBV	2365512	1938066	62.88%	9.731%
16	13.327	1872	1877	1885	rBV	589310	548790	17.81%	2.756%
17	13.798	1952	1957	1967	rBV10	28162	106191	3.45%	0.533%
18	13.916	1973	1977	1981	rBV	688713	676715	21.96%	3.398%
19	13.945	1981	1982	1986	rVB	67096	43515	1.41%	0.218%
20	14.004	1989	1992	1998	rBV	103719	104732	3.40%	0.526%
21	14.651	2100	2102	2106	rVB3	37835	40601	1.32%	0.204%
22	14.951	2150	2153	2155	rBV	86266	106712	3.46%	0.536%
23	15.245	2200	2203	2210	rBV	52904	76107	2.47%	0.382%
24	15.310	2211	2214	2216	rVV	72727	92530	3.00%	0.465%
25	15.363	2220	2223	2234	rVB	532871	656266	21.29%	3.295%
26	15.739	2284	2287	2293	rVB	56417	72207	2.34%	0.363%




Sum of corrected areas: 19915516

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082622\
Data File : BF130024.D
Acq On : 26 Aug 2022 17:58
Operator : CG\JU
Sample : N4277-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
B-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

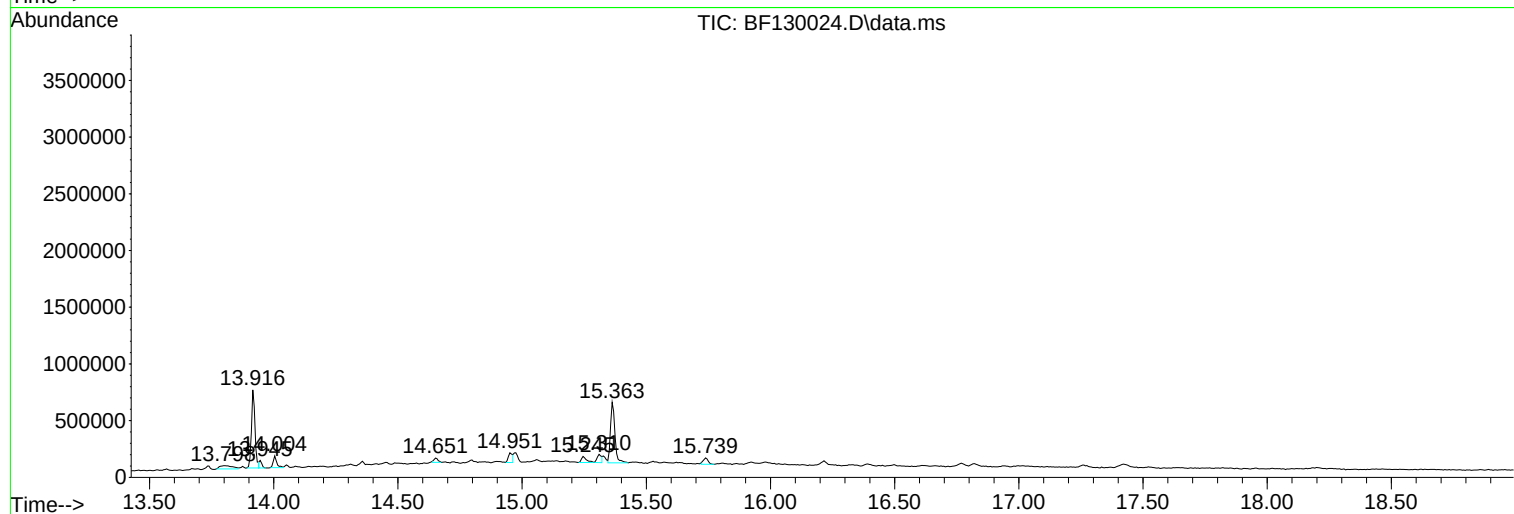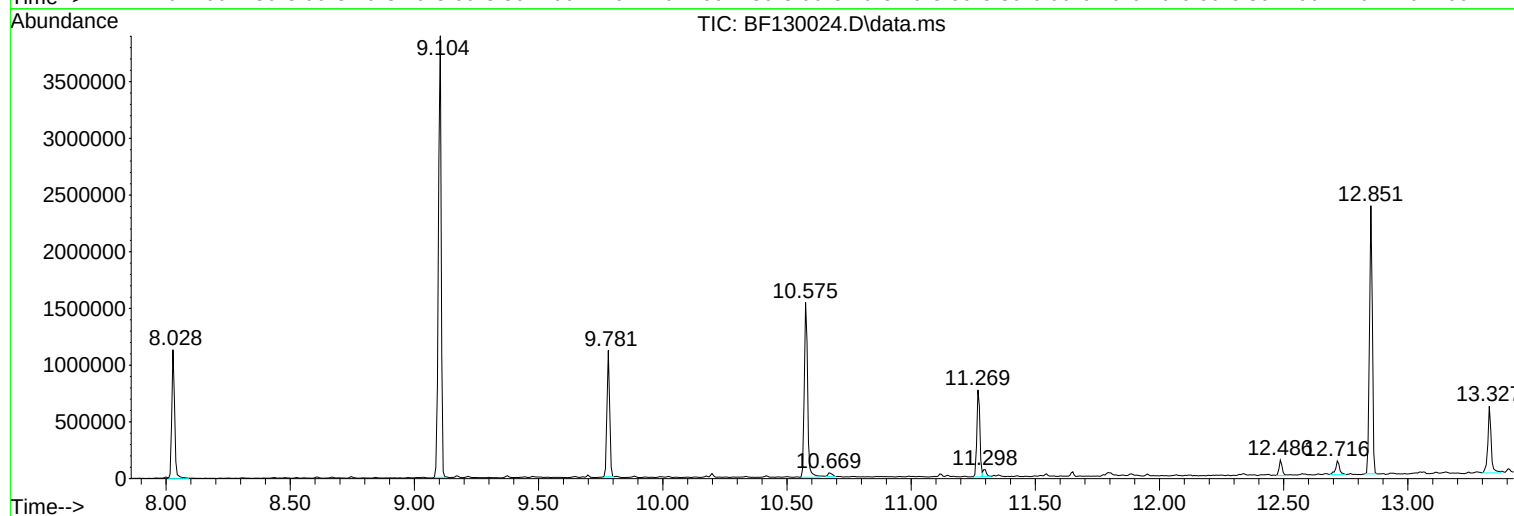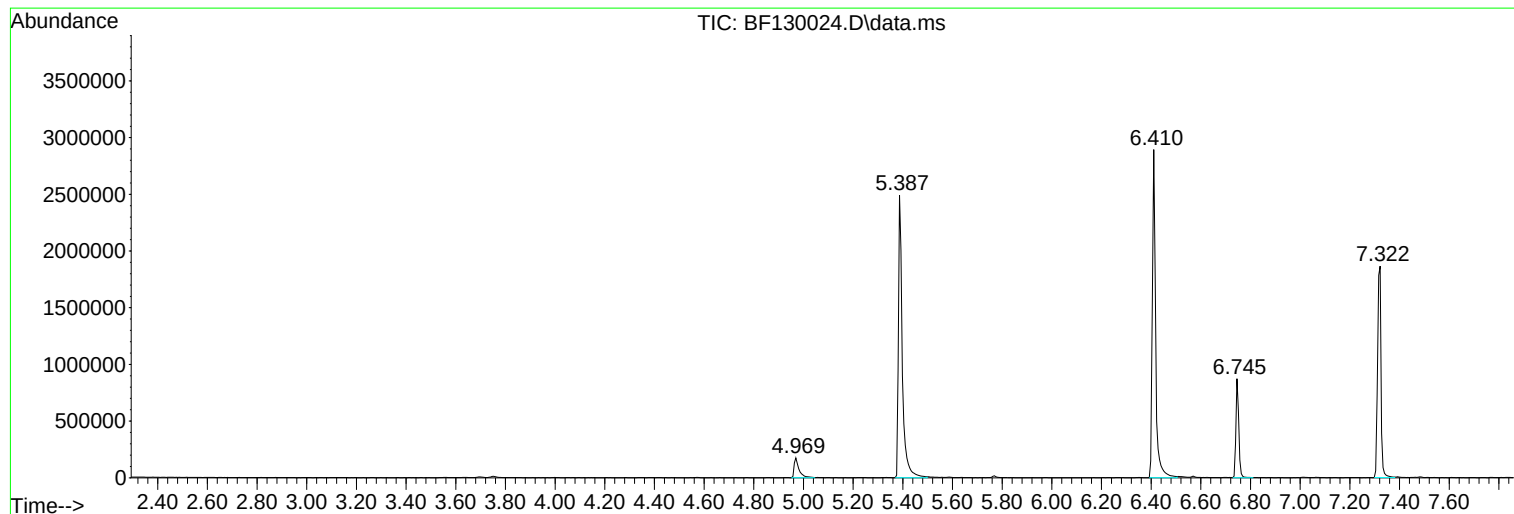

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082622\
Data File : BF130024.D
Acq On : 26 Aug 2022 17:58
Operator : CG\JU
Sample : N4277-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
B-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082622\
Data File : BF130024.D
Acq On : 26 Aug 2022 17:58
Operator : CG\JU
Sample : N4277-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
B-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------