


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082622\
 Data File : BF130012.D
 Acq On : 26 Aug 2022 09:55
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 25 14:45:09 2022

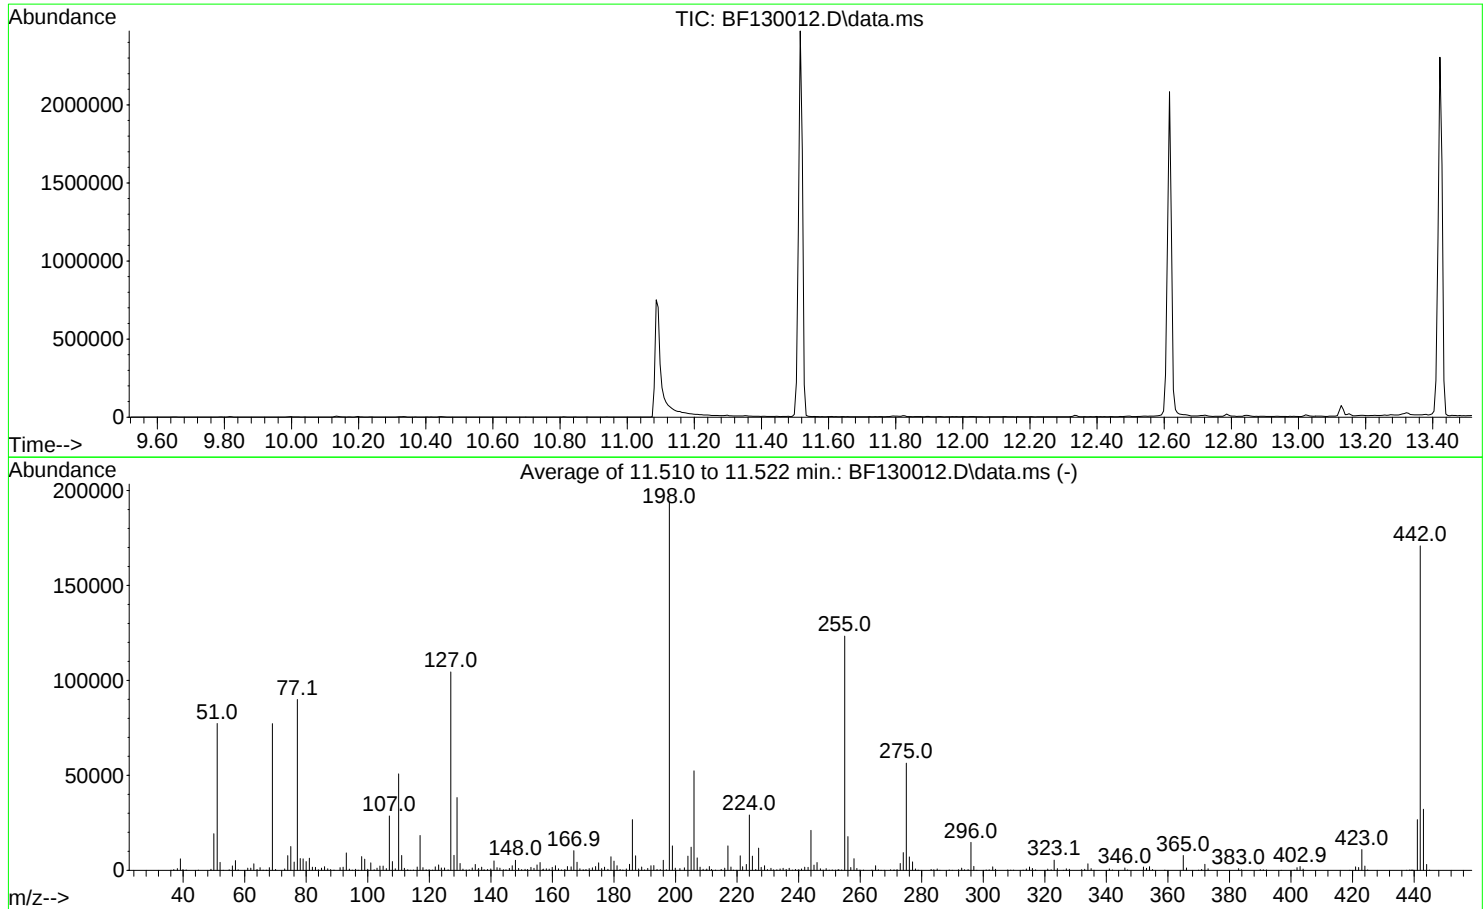




AutoFind: Scans 1568, 1569, 1570; Background Corrected with Scan 1562

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.9	77349	PASS
68	69	0.00	2	1.8	1423	PASS
69	198	0.00	100	39.9	77219	PASS
70	69	0.00	2	0.6	446	PASS
127	198	10	80	53.9	104483	PASS
197	198	0.00	2	0.1	286	PASS
198	198	100	100	100.0	193728	PASS
199	198	5	9	6.6	12855	PASS
275	198	10	60	29.1	56435	PASS
365	198	1	100	4.0	7787	PASS
441	198	0.01	100	13.8	26640	PASS
442	442	50	100	100.0	170856	PASS
443	442	15	24	18.8	32142	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082622\
 Data File : BF130012.D
 Acq On : 26 Aug 2022 09:55
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Aug 27 06:22:25 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 25 14:45:09 2022
 Response via : Initial Calibration

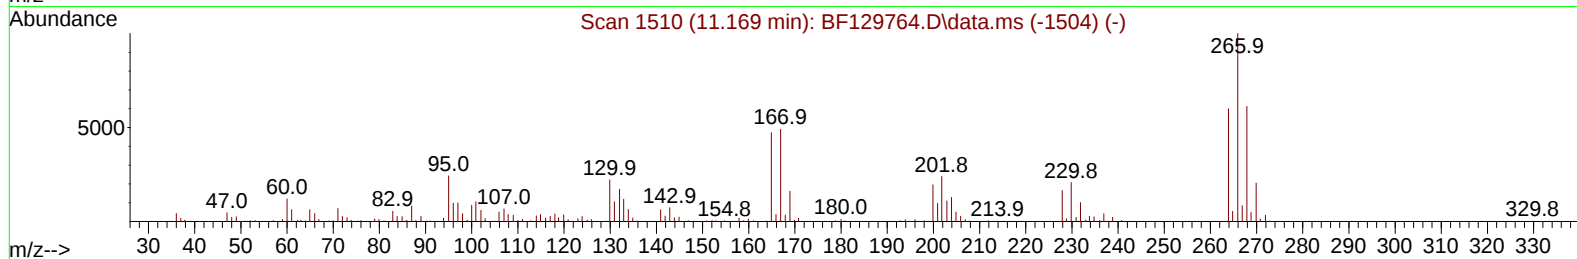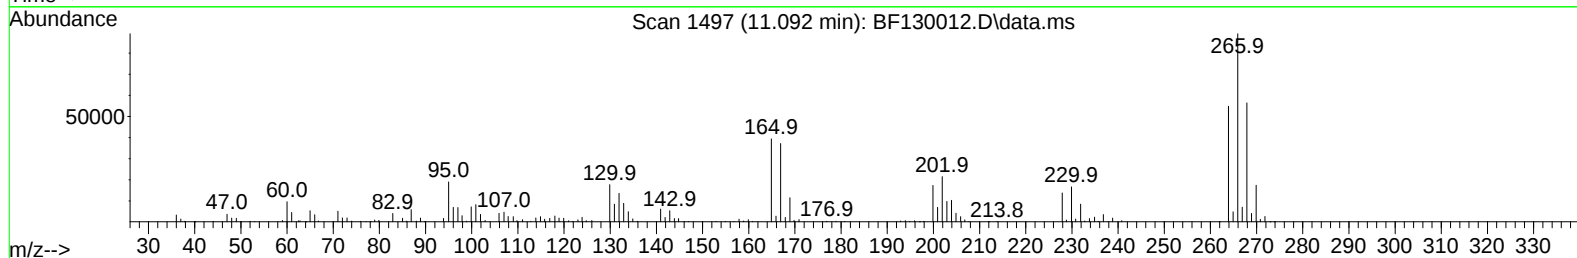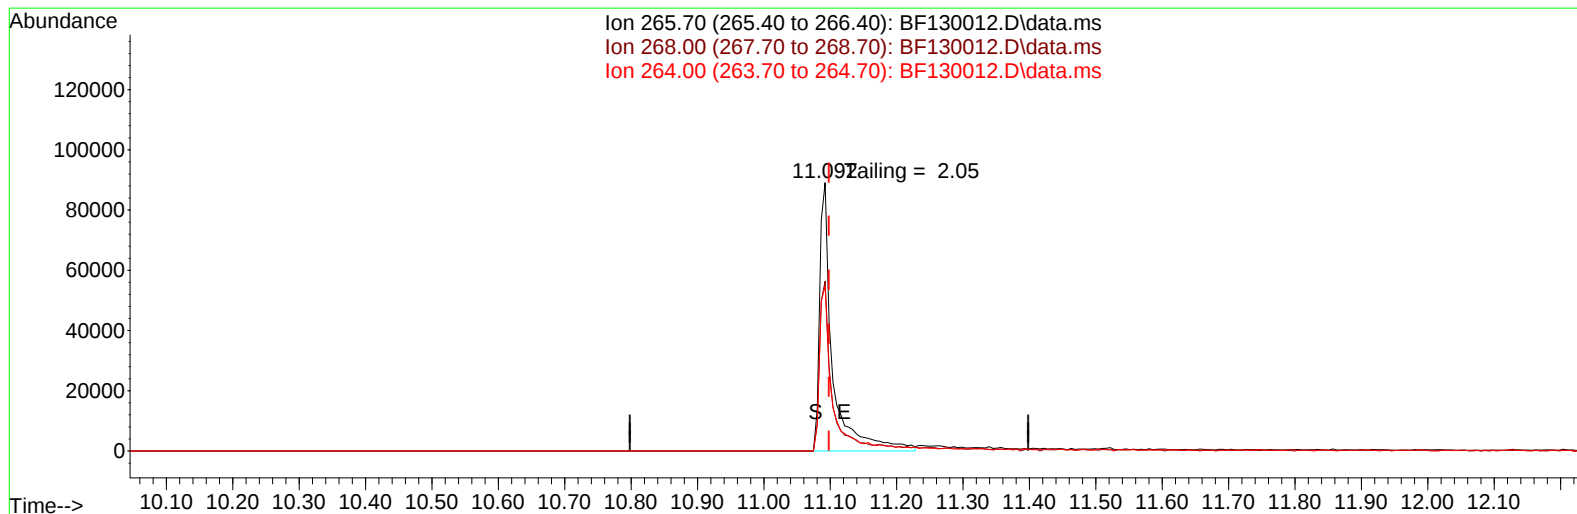

TIC: BF130012.D\data.ms

(70) Pentachlorophenol (C)

11.092min (-0.006) 313082.21 ng




response 122220

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	63.27
264.00	59.90	61.48
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082622\
Data File : BF130012.D
Acq On : 26 Aug 2022 09:55
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 27 06:22:25 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 25 14:45:09 2022
Response via : Initial Calibration

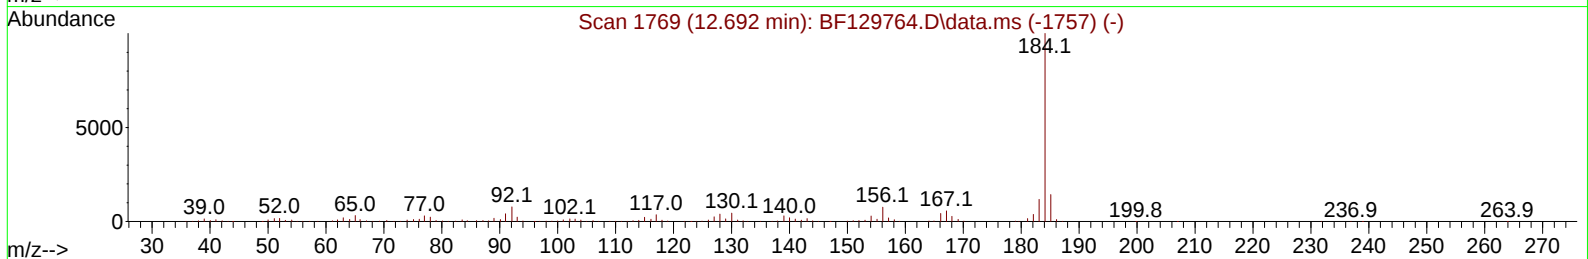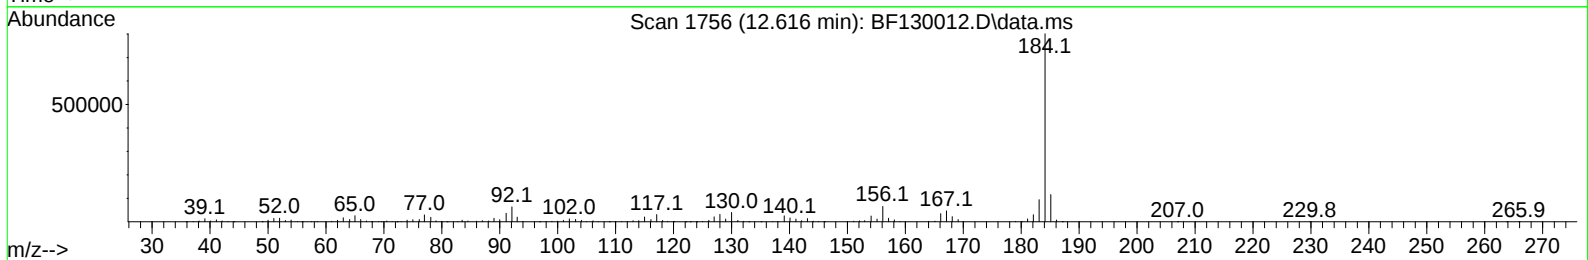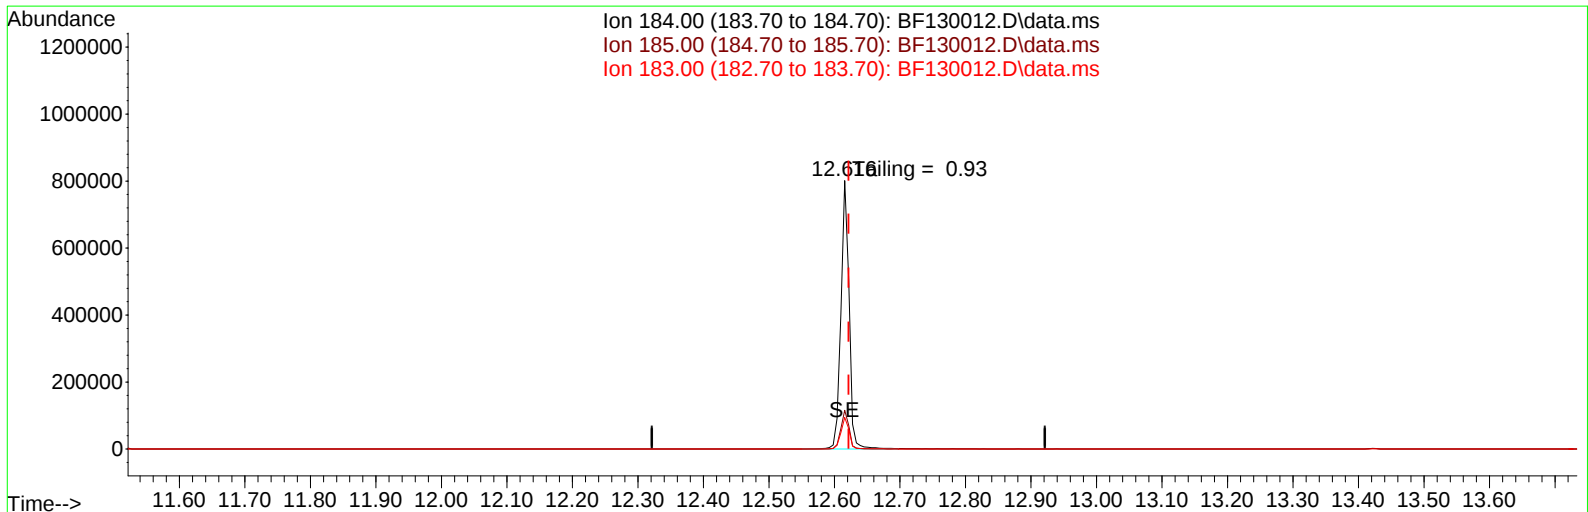

TIC: BF130012.D\data.ms

(77) Benzidine

12.616min (-0.006) 32984.01 ng

response 693391

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.45
183.00	11.80	11.77
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/26/2022	BNA_F	<u>BF130012.D</u>
Compound Name	Response	Retention Time
DDT	369345	13.421
DDD	14240	13.127
DDE	1923	12.786
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16163	385508	4.19

Instrument :
BNA_F
ClientSampleId :
DFTPP