


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF082715\
 Data File : BF081234.D
 Acq On : 27 Aug 2015 2:25
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\625-TERPINEOL-BF082715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 27 06:31:06 2015

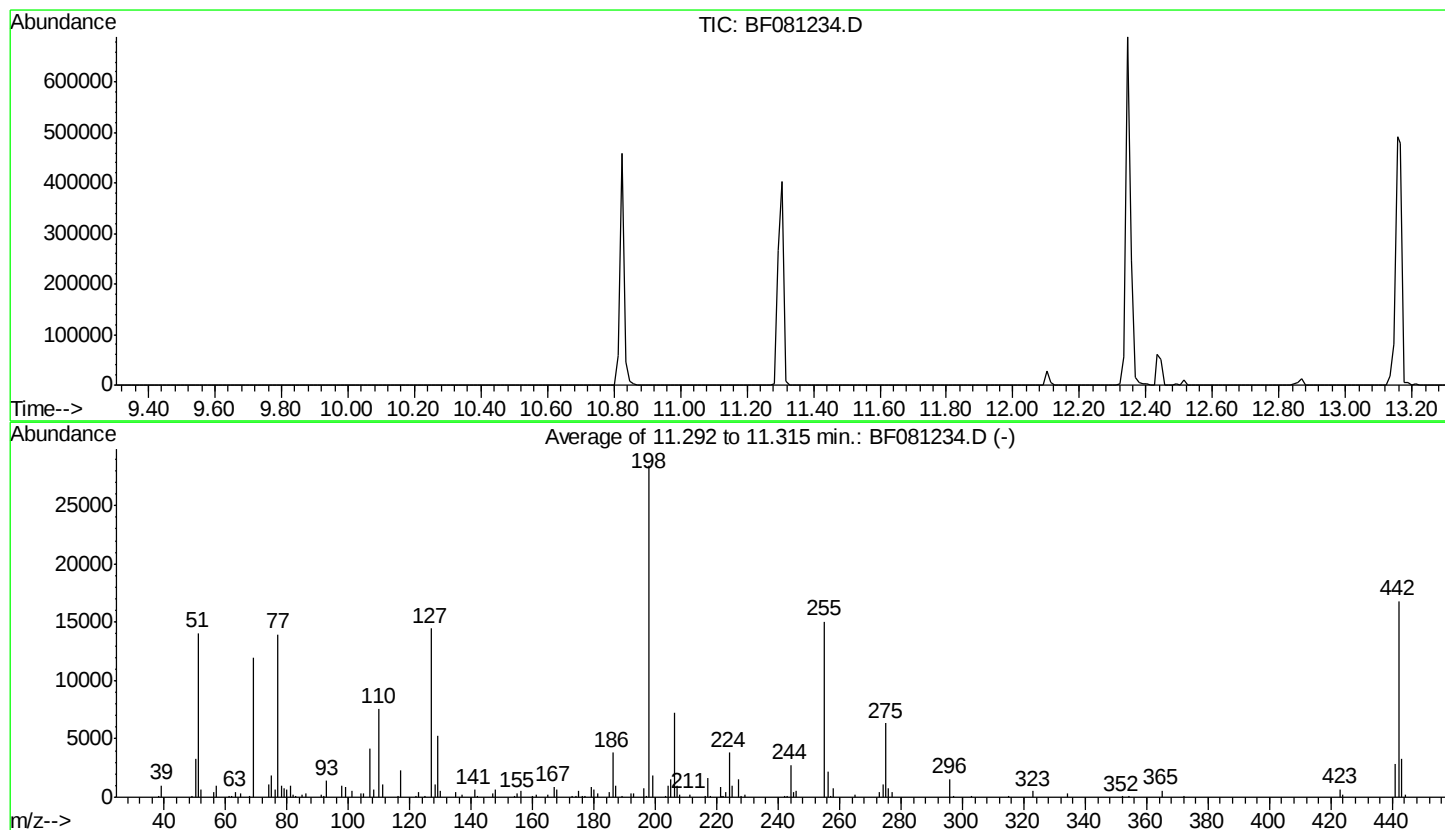

AutoFind: Scans 836, 837, 838; Background Corrected with Scan 832

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	49.4	14048	PASS
68	69	0.00	2	0.9	113	PASS
69	198	0.00	100	42.2	11990	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	50.8	14453	PASS
197	198	0.00	1	0.4	106	PASS
198	198	100	100	100.0	28429	PASS
199	198	5	9	6.4	1829	PASS
275	198	10	30	22.4	6356	PASS
365	198	1	100	2.1	587	PASS
441	443	0.01	100	85.4	2826	PASS
442	198	40	100	59.2	16834	PASS
443	442	17	23	19.7	3311	PASS