

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082721\
 Data File : BF125247.D
 Acq On : 27 Aug 2021 10:15
 Operator : JU/CG
 Sample : PB138720BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB138720BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF125247.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.263	18	30	36	rVB	104877	153249	2.58%	0.411%
2	5.540	582	587	590	rBV	5381304	5658118	95.28%	15.158%
3	6.539	751	757	760	rBV	4837586	5392896	90.81%	14.448%
4	6.916	817	821	824	rBV	1244045	1093902	18.42%	2.931%
5	7.475	911	916	919	rBV	3526541	3590424	60.46%	9.619%
6	8.192	1034	1038	1050	rBV	1427377	1399185	23.56%	3.748%
7	9.269	1216	1221	1224	rBV	6184558	5938468	100.00%	15.909%
8	9.951	1332	1337	1347	rBV	1676645	1463407	24.64%	3.920%
9	10.739	1466	1471	1474	rBV	4006215	3556291	59.89%	9.527%
10	11.433	1586	1589	1597	rBV	1458096	1367602	23.03%	3.664%
11	13.021	1855	1859	1863	rBV	5809517	5470691	92.12%	14.656%
12	14.074	2034	2038	2058	rVB	1189298	1133287	19.08%	3.036%
13	15.574	2287	2293	2302	rBV	822724	1109858	18.69%	2.973%




Sum of corrected areas: 37327378

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082721\
Data File : BF125247.D
Acq On : 27 Aug 2021 10:15
Operator : JU/CG
Sample : PB138720BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB138720BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

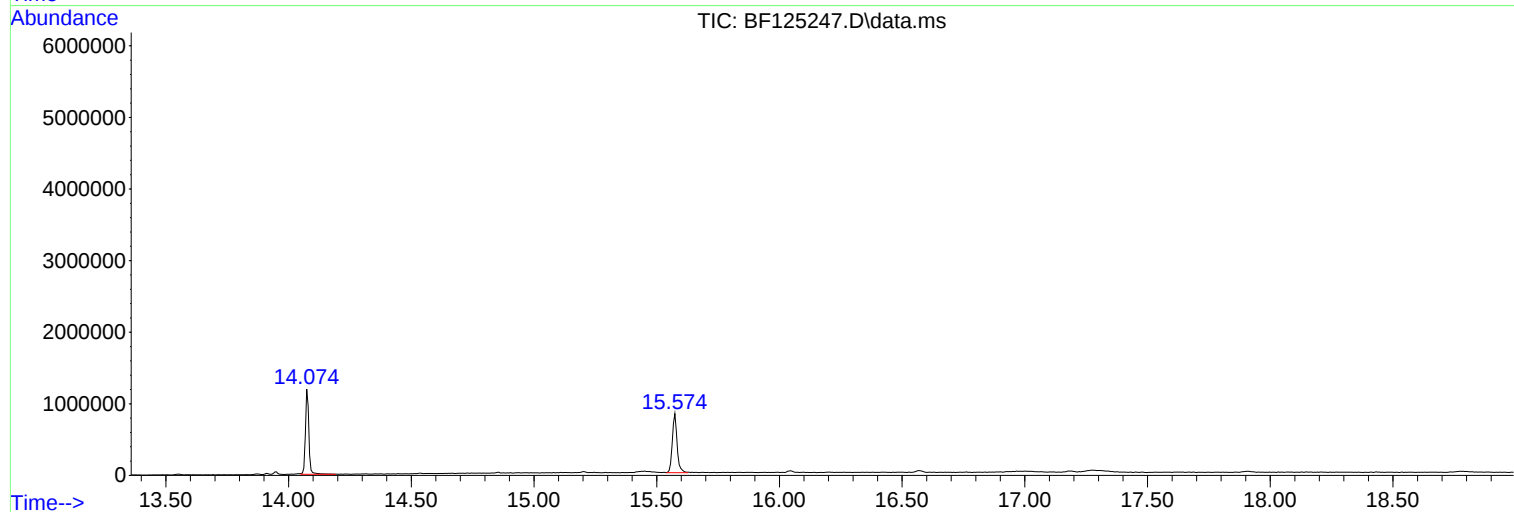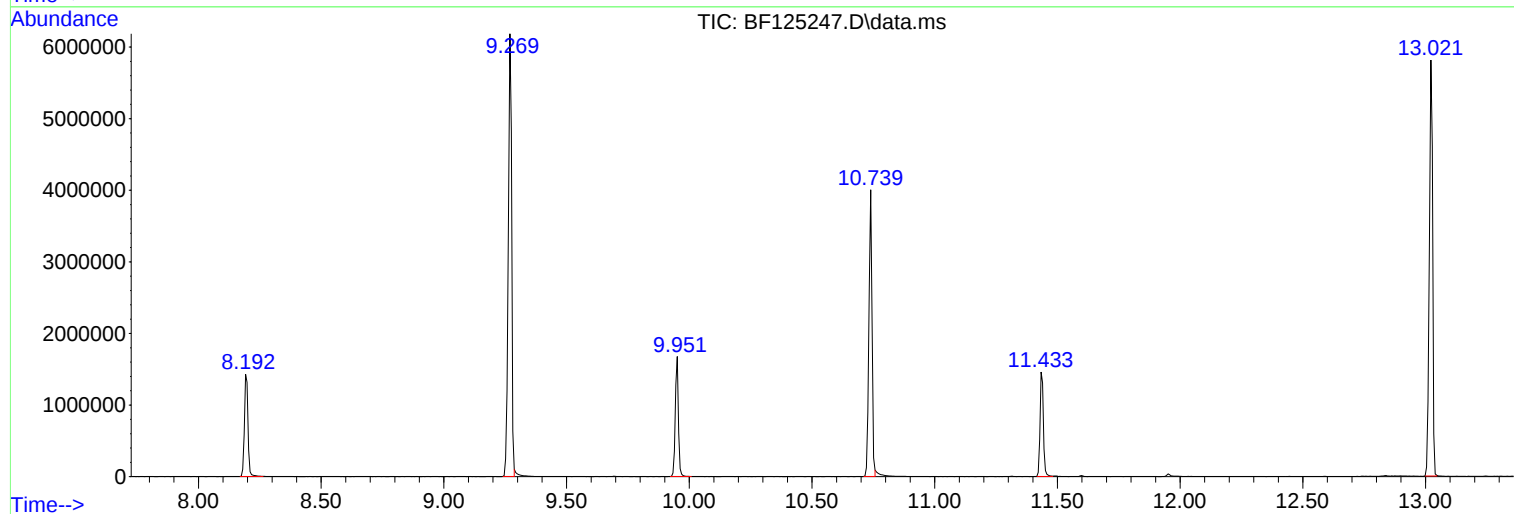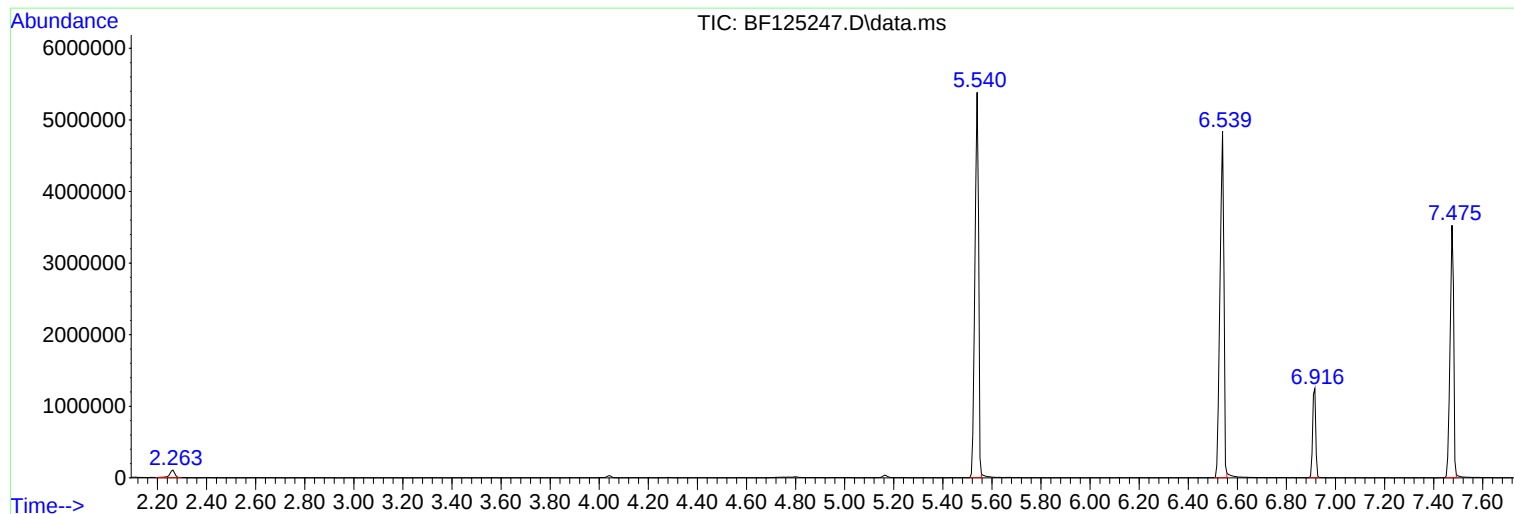

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082721\
Data File : BF125247.D
Acq On : 27 Aug 2021 10:15
Operator : JU/CG
Sample : PB138720BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB138720BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.263	2.80 ng	153249	1,4-Dichlorobenzene-d4	6.916

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39
3			2,5-Dimethyl-4-hydroxy-3-hexanone	144	C8H16O2	000815-77-0	28
4			Silane, tetramethyl-	88	C4H12Si	000075-76-3	17
5			Boronic acid, ethyl-, dimethyl e...	102	C4H11BO2	007318-82-3	17

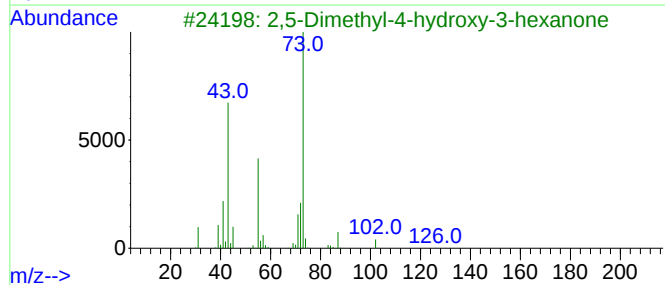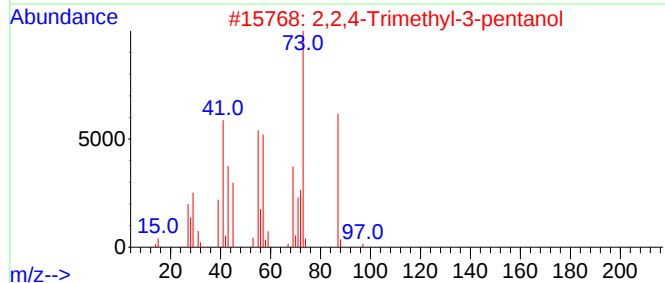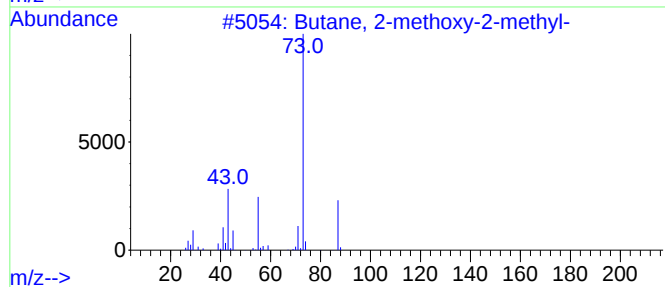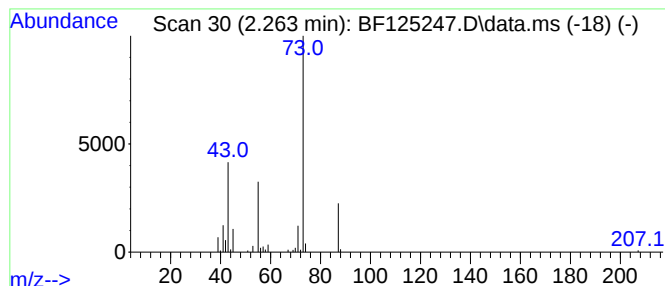

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082721\
Data File : BF125247.D
Acq On : 27 Aug 2021 10:15
Operator : JU/CG
Sample : PB138720BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB138720BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.263	2.8	ng	153249	1	6.916	1093900	20.0