
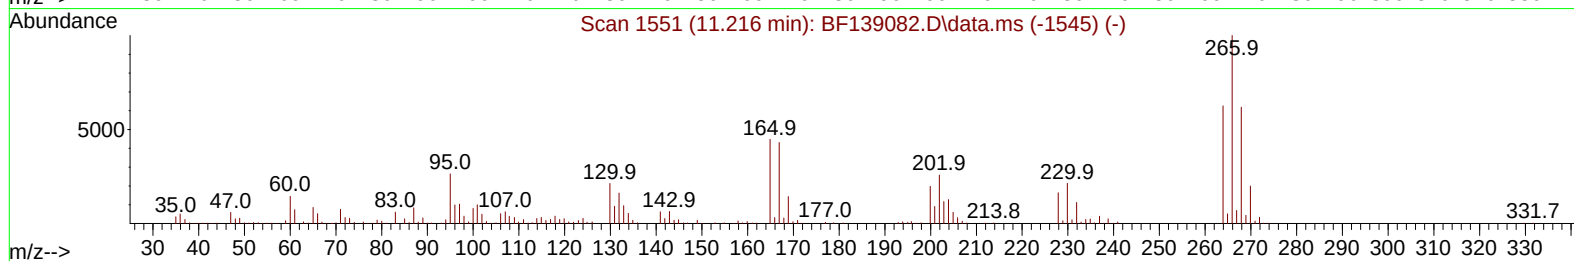
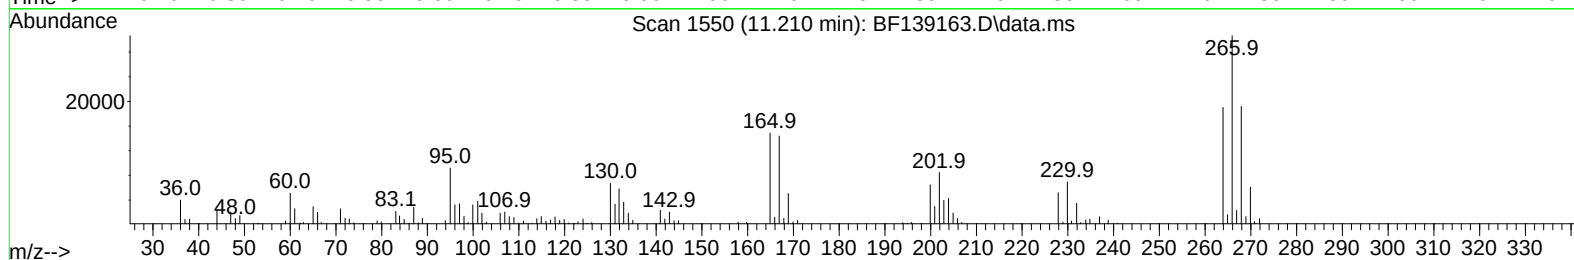


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082724\
Data File : BF139163.D
Acq On : 26 Aug 2024 15:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 26 15:39:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 21 01:25:05 2024
Response via : Initial Calibration

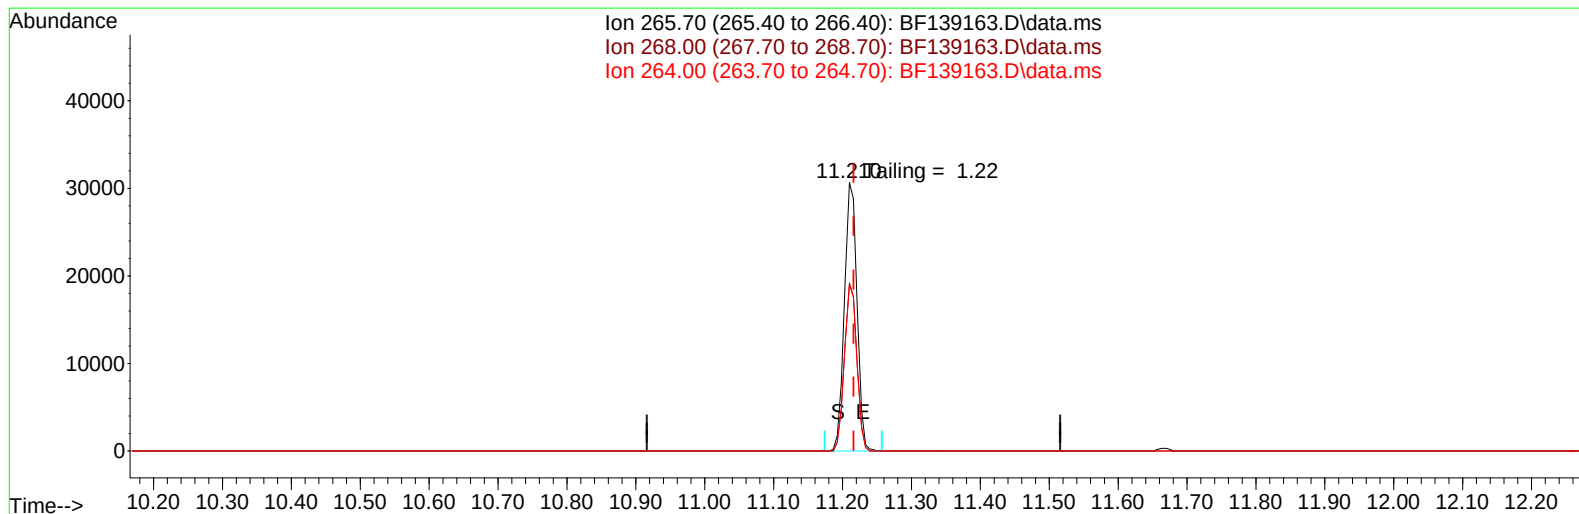

TIC: BF139163.D\data.ms

(70) Pentachlorophenol (C)




11.210min (-0.006) 9822.24 ng

response 38944

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	62.60
264.00	62.50	62.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082724\
Data File : BF139163.D
Acq On : 26 Aug 2024 15:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 26 15:39:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 21 01:25:05 2024
Response via : Initial Calibration

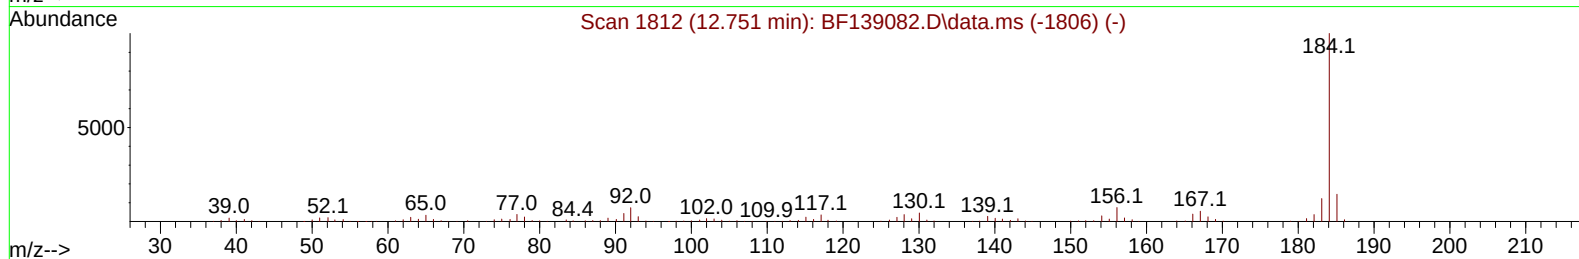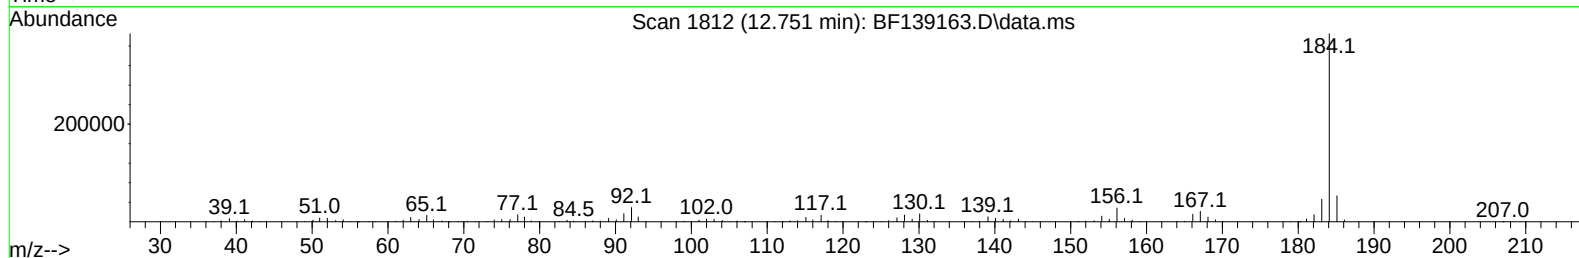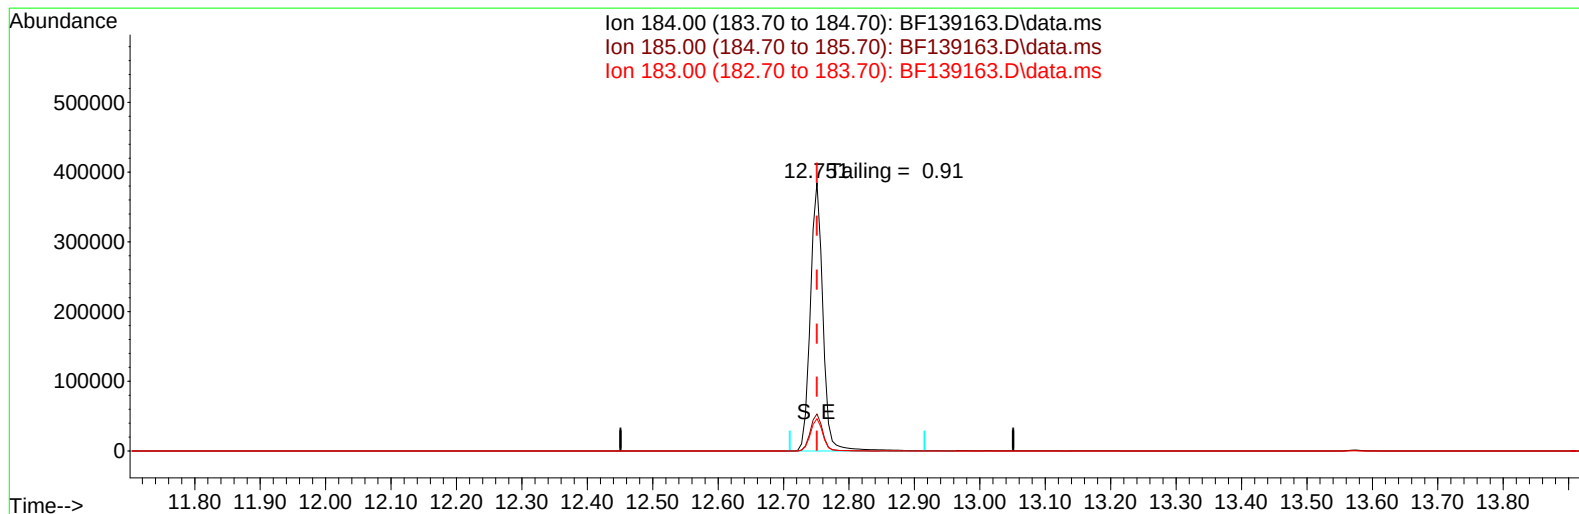

TIC: BF139163.D\data.ms

(77) Benzidine

12.751min (-0.000) 0.00 ng

response 515422

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.83
183.00	12.20	12.05
0.00	0.00	0.00