
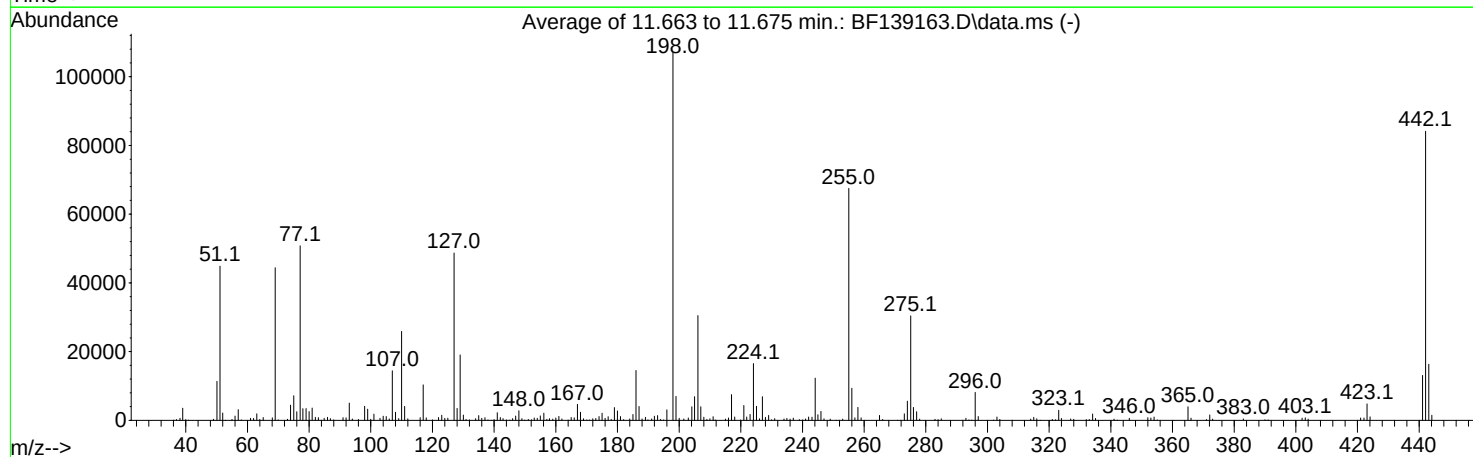


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082724\
Data File : BF139163.D
Acq On : 26 Aug 2024 15:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082724.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Aug 27 02:51:47 2024

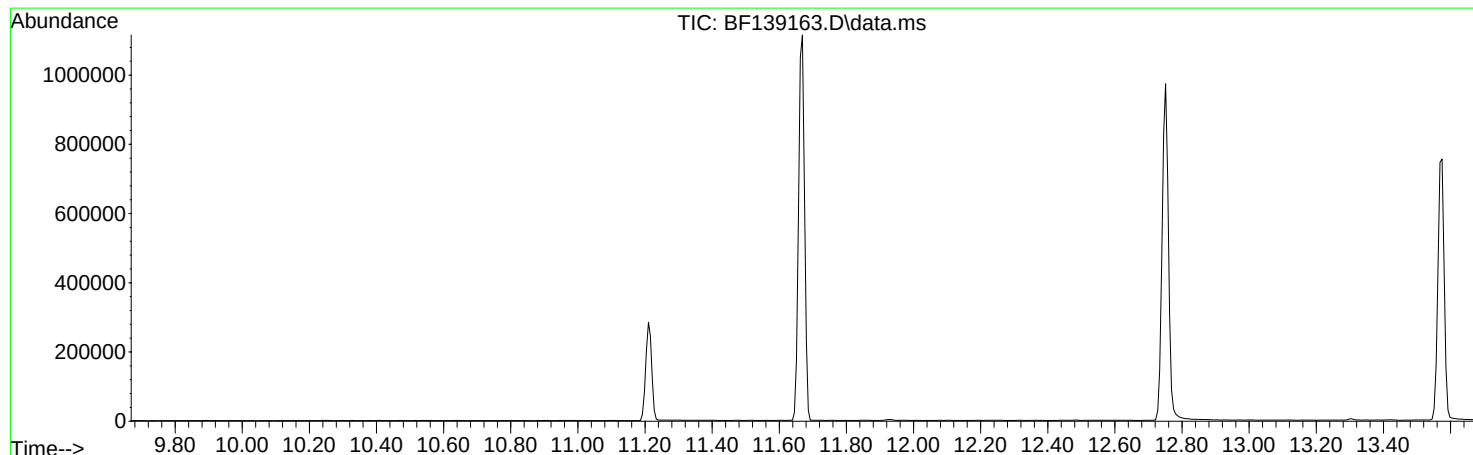

AutoFind: Scans 1627, 1628, 1629; Background Corrected with Scan 1621

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.9	44901	PASS
68	69	0.00	2	1.6	731	PASS
69	198	0.00	100	41.5	44403	PASS
70	69	0.00	2	0.3	142	PASS
127	198	10	80	45.5	48699	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	107037	PASS
199	198	5	9	6.5	6964	PASS
275	198	10	60	28.4	30392	PASS
365	198	1	100	3.7	3962	PASS
441	198	0.01	100	12.2	13076	PASS
442	442	50	100	100.0	84149	PASS
443	442	15	24	19.4	16356	PASS

DDT Breakdown


Date	Instrument Name	DFTPP Data File
8/27/2024	BNA_F	<u>BF139163.D</u>
Compound Name	Response	Retention Time
DDT	103329	13.574
DDD	766	13.304
DDE	0	12.945
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
766	104095	0.74

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082724\
Data File : BF139163.D
Acq On : 26 Aug 2024 15:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 26 15:39:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 21 01:25:05 2024
Response via : Initial Calibration

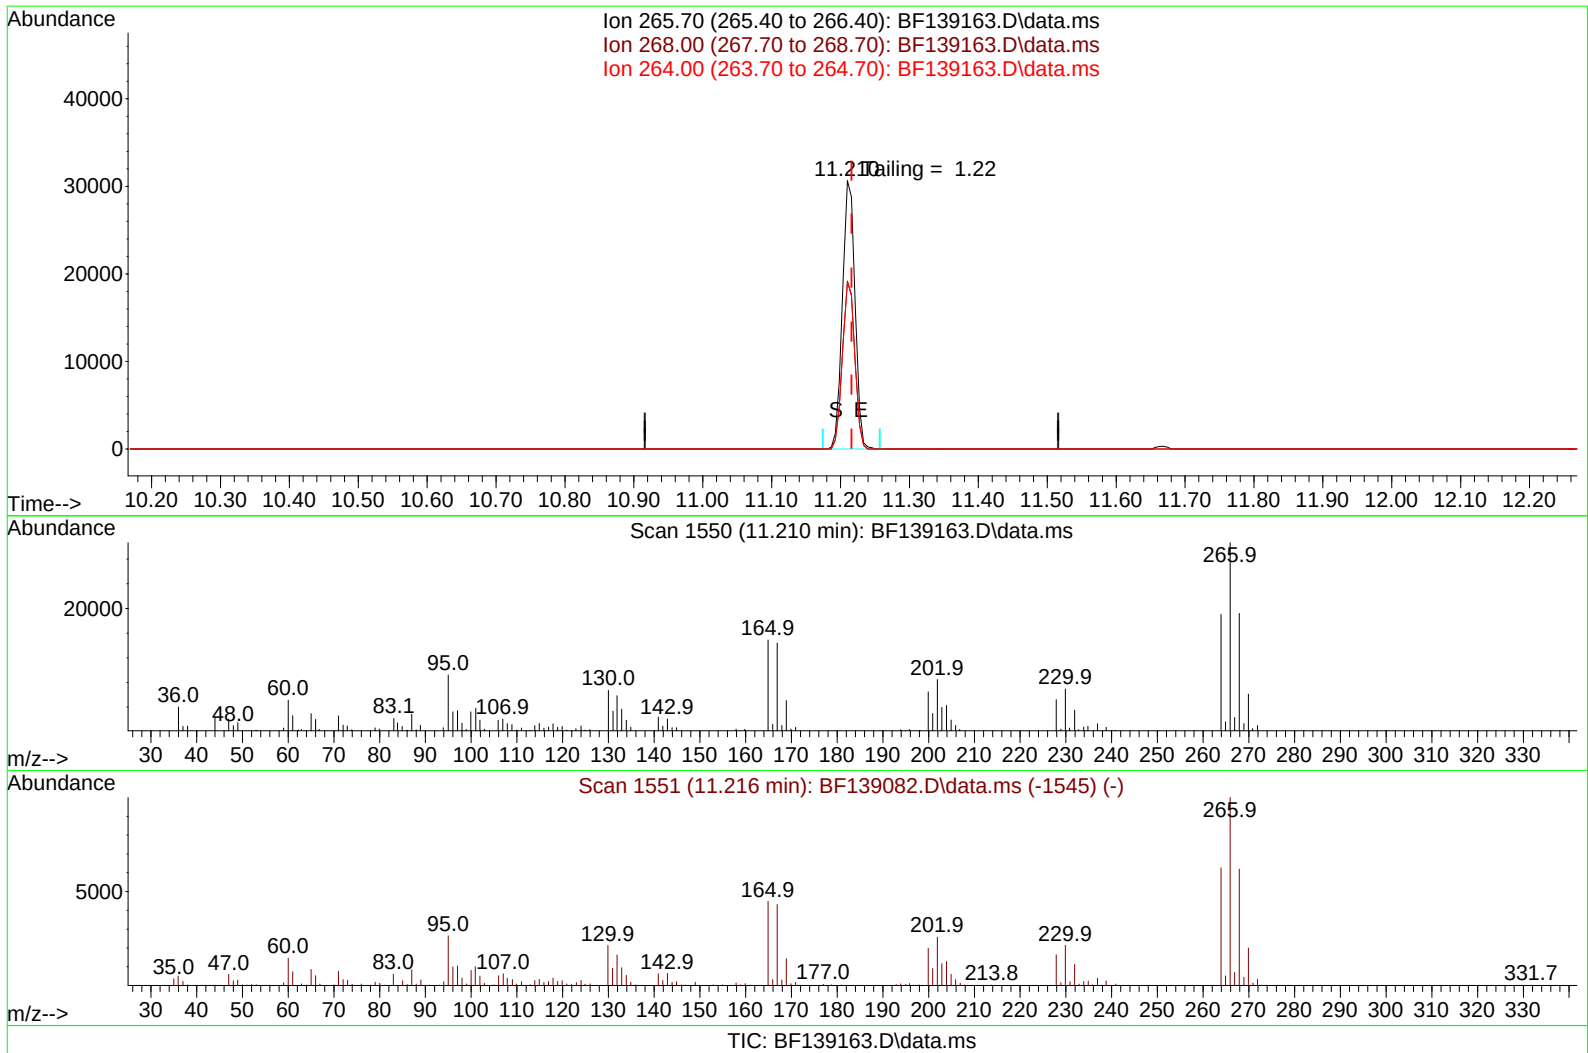

(70) Pentachlorophenol (C)

11.210min (-0.006) 9822.24 ng




response 38944

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	62.60
264.00	62.50	62.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082724\
Data File : BF139163.D
Acq On : 26 Aug 2024 15:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 26 15:39:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 21 01:25:05 2024
Response via : Initial Calibration

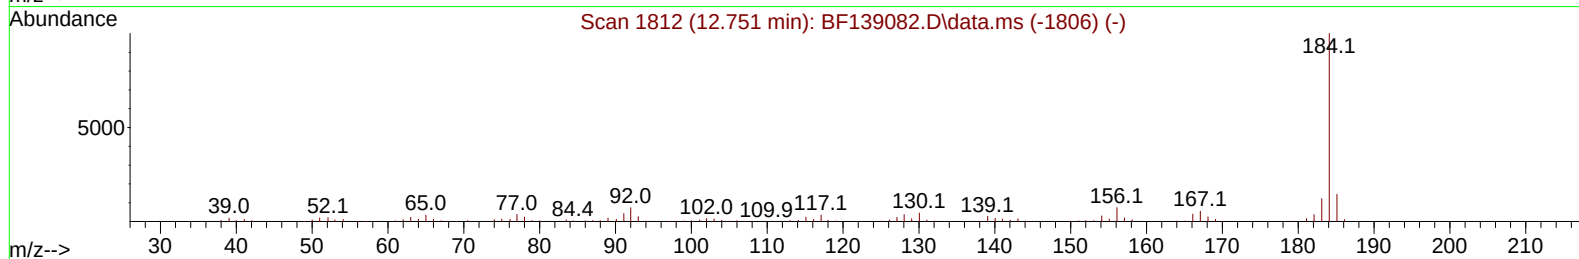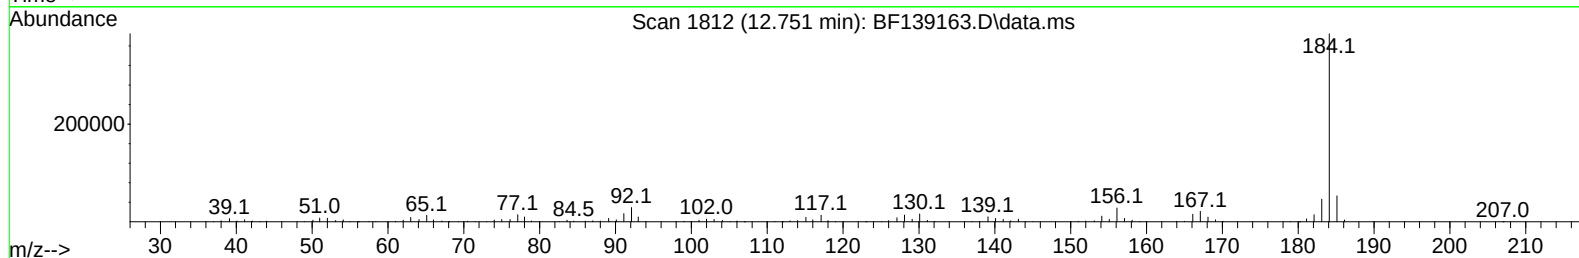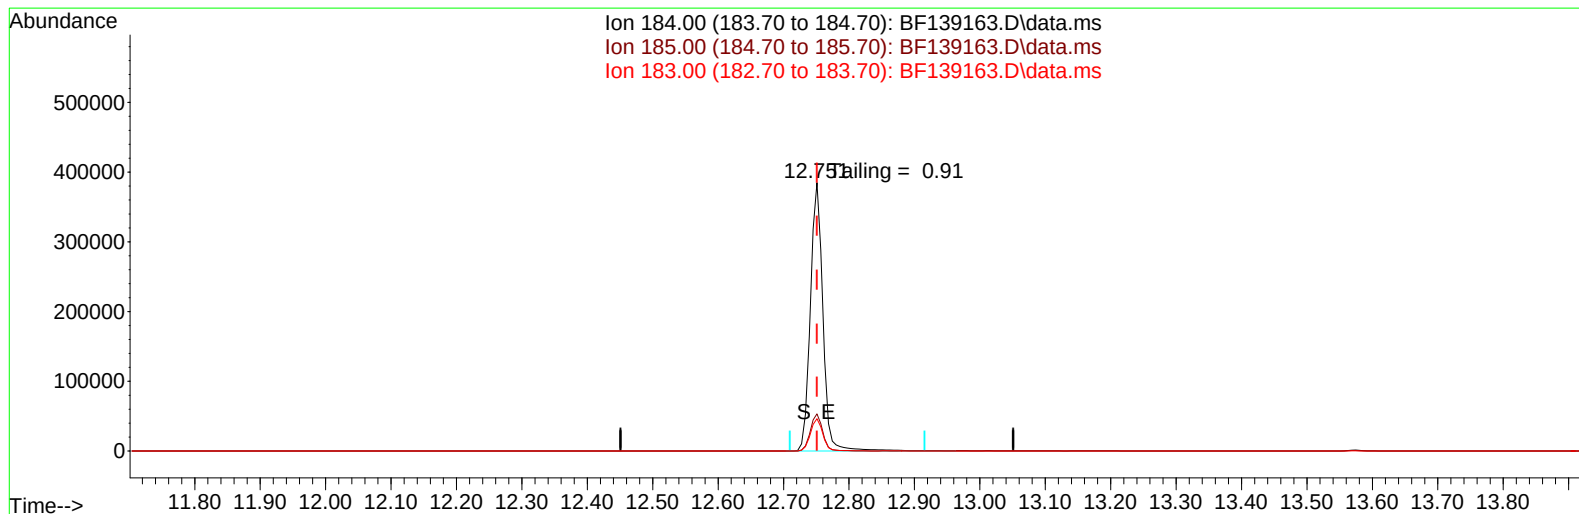

TIC: BF139163.D\data.ms

(77) Benzidine

12.751min (-0.000) 0.00 ng

response 515422

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.83
183.00	12.20	12.05
0.00	0.00	0.00