
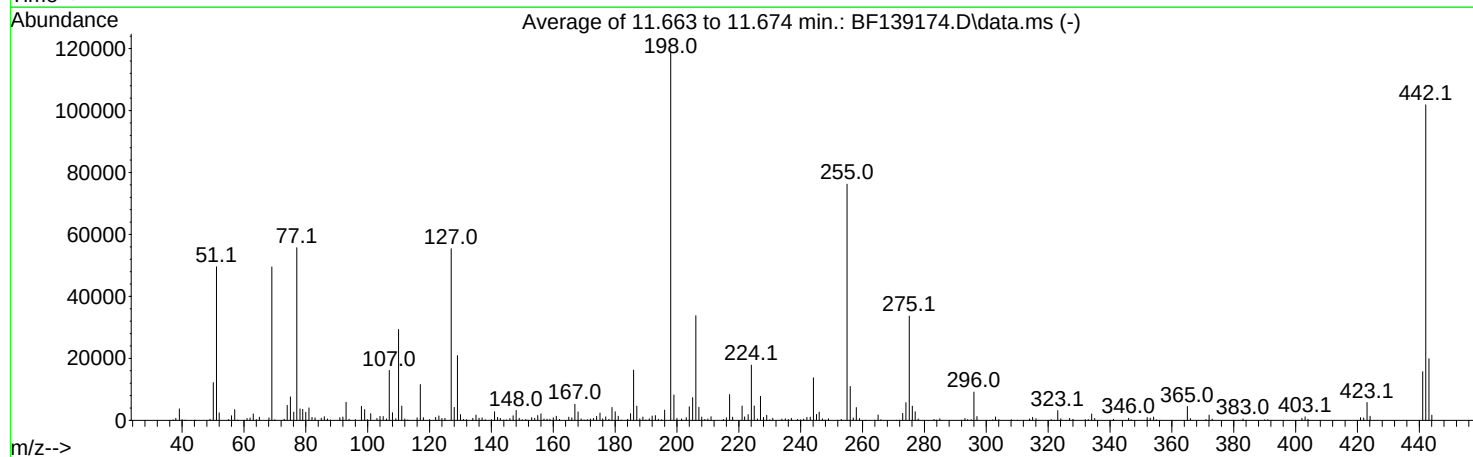


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082724\
Data File : BF139174.D
Acq On : 27 Aug 2024 08:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082724.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Aug 27 02:51:47 2024

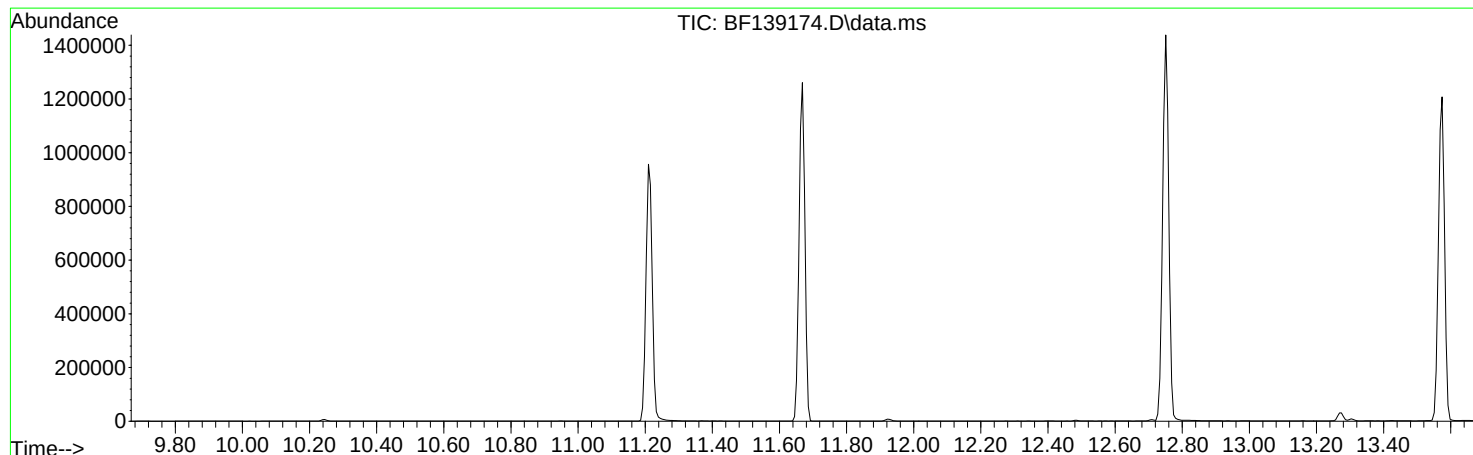

AutoFind: Scans 1627, 1628, 1629; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.8	49597	PASS
68	69	0.00	2	1.7	841	PASS
69	198	0.00	100	41.7	49517	PASS
70	69	0.00	2	0.5	230	PASS
127	198	10	80	46.7	55424	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	118728	PASS
199	198	5	9	6.9	8218	PASS
275	198	10	60	28.3	33648	PASS
365	198	1	100	3.8	4472	PASS
441	198	0.01	100	13.2	15721	PASS
442	442	50	100	100.0	101853	PASS
443	442	15	24	19.5	19886	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/27/2024	BNA_F	<u>BF139174.D</u>
Compound Name	Response	Retention Time
DDT	272695	13.574
DDD	10700	13.274
DDE	124	12.933
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10824	283519	3.82

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082724\
Data File : BF139174.D
Acq On : 27 Aug 2024 08:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 27 11:57:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 27 02:51:47 2024
Response via : Initial Calibration

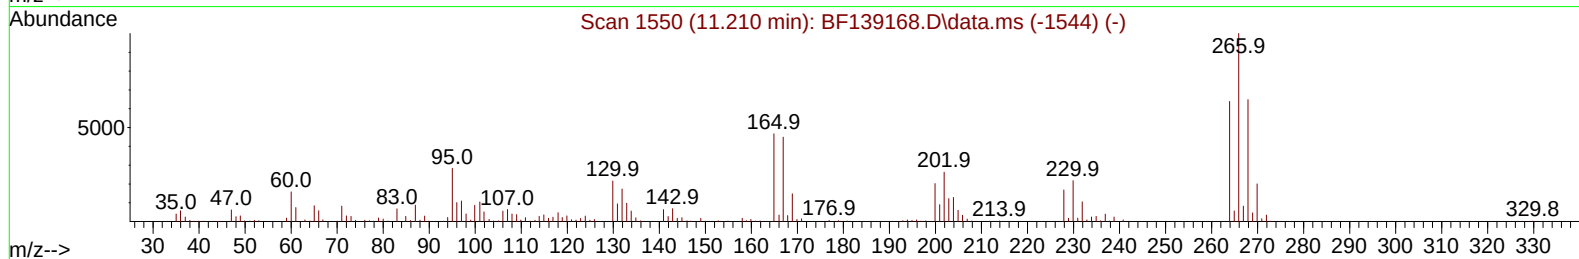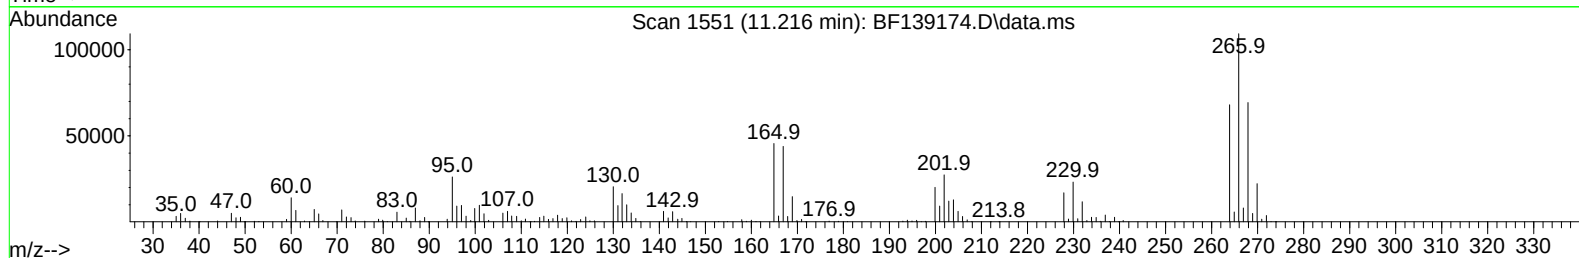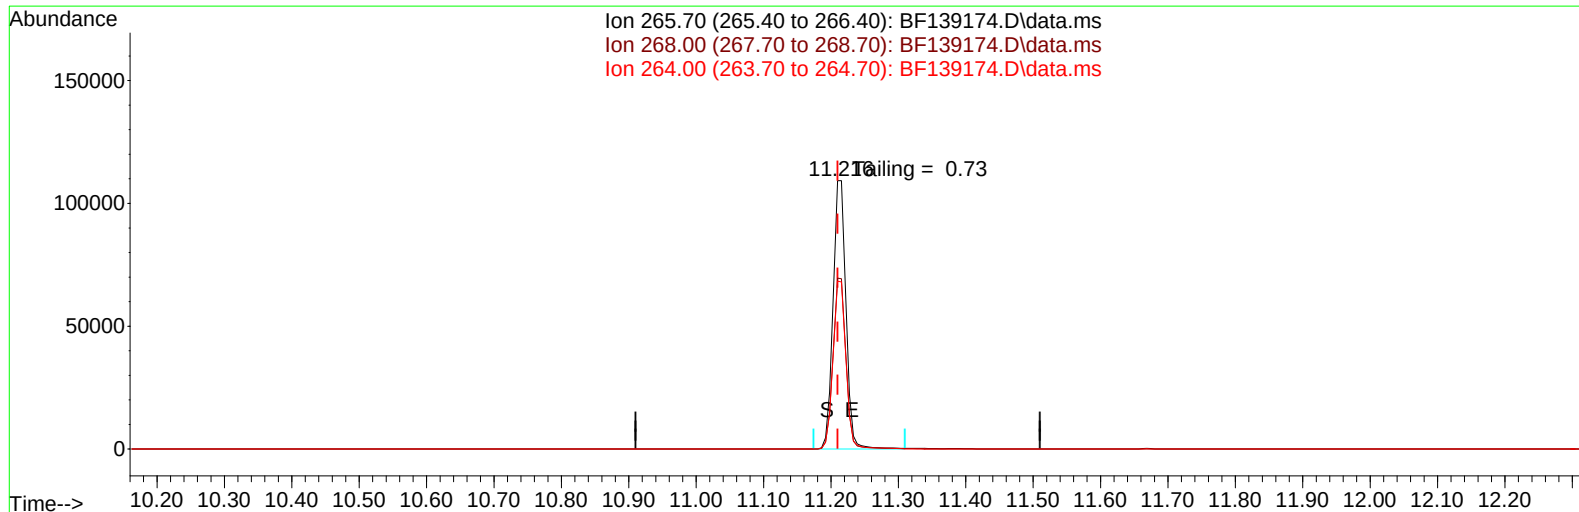

TIC: BF139174.D\data.ms

(70) Pentachlorophenol (C)

11.216min (+ 0.006) 32862.30 ng




response 146202

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.80	63.46
264.00	63.80	62.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082724\
Data File : BF139174.D
Acq On : 27 Aug 2024 08:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 27 11:57:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 27 02:51:47 2024
Response via : Initial Calibration

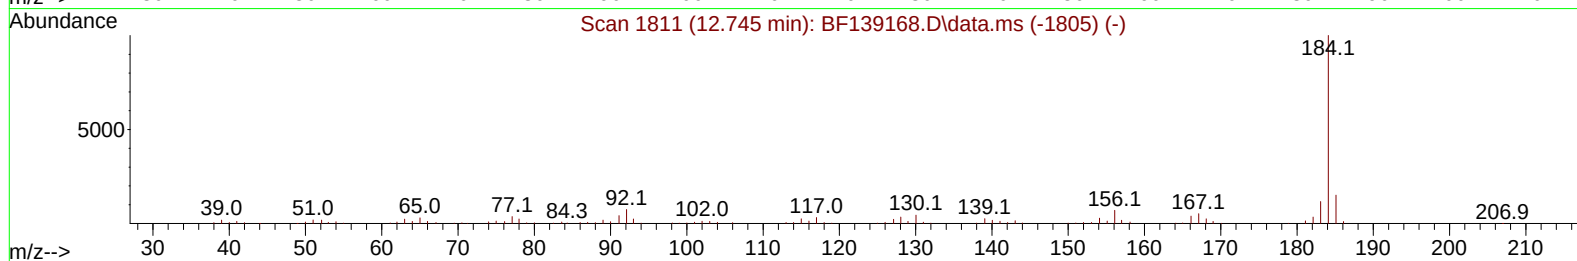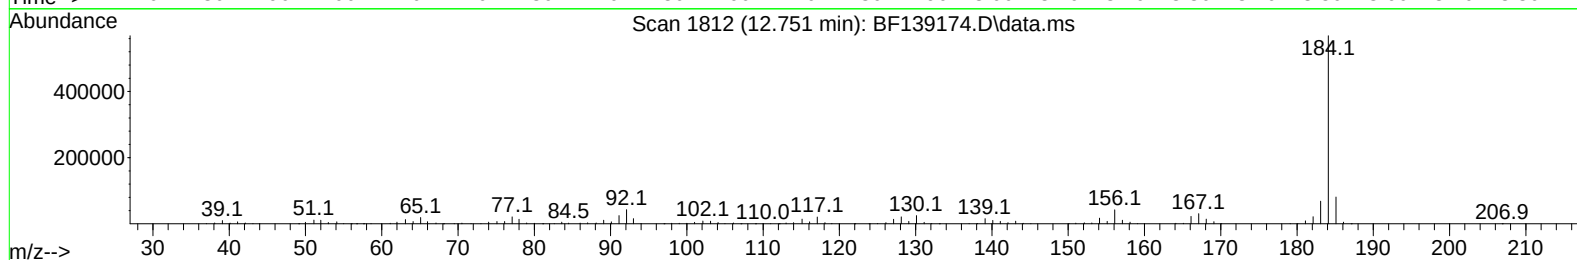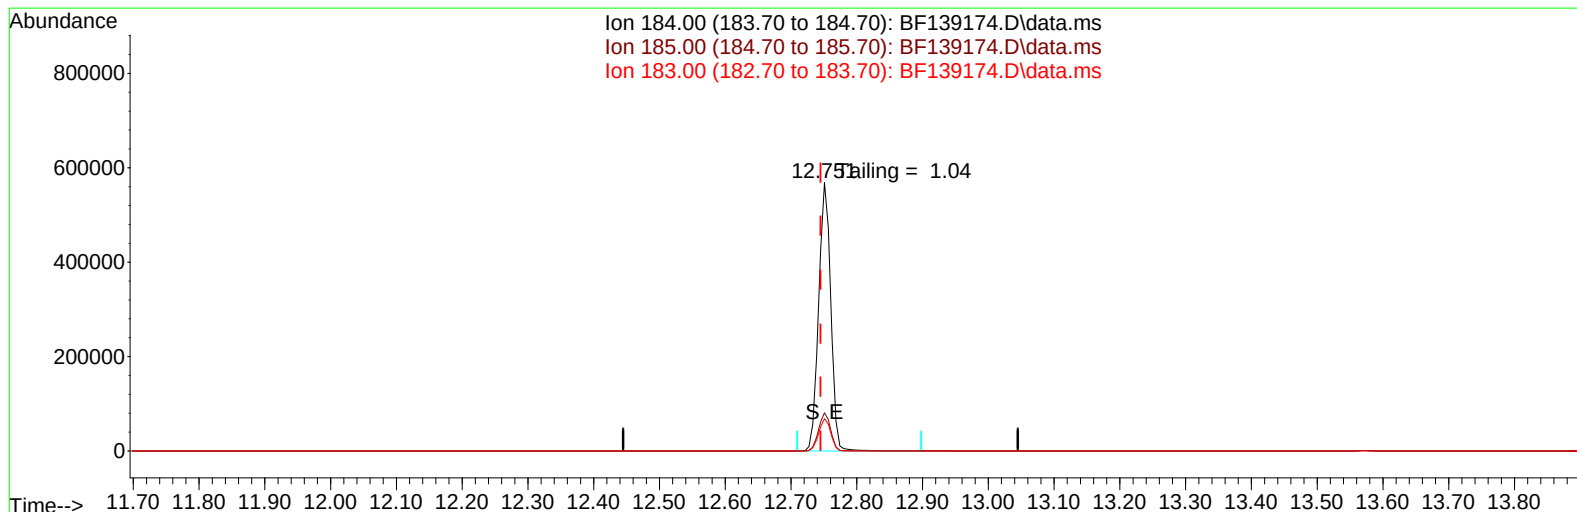

TIC: BF139174.D\data.ms

(77) Benzidine

12.751min (+ 0.006) 0.00 ng

response 730770

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.27
183.00	11.70	12.05
0.00	0.00	0.00