


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF082815\
 Data File : BF081246.D
 Acq On : 27 Aug 2015 13:56
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 24 13:58:19 2015

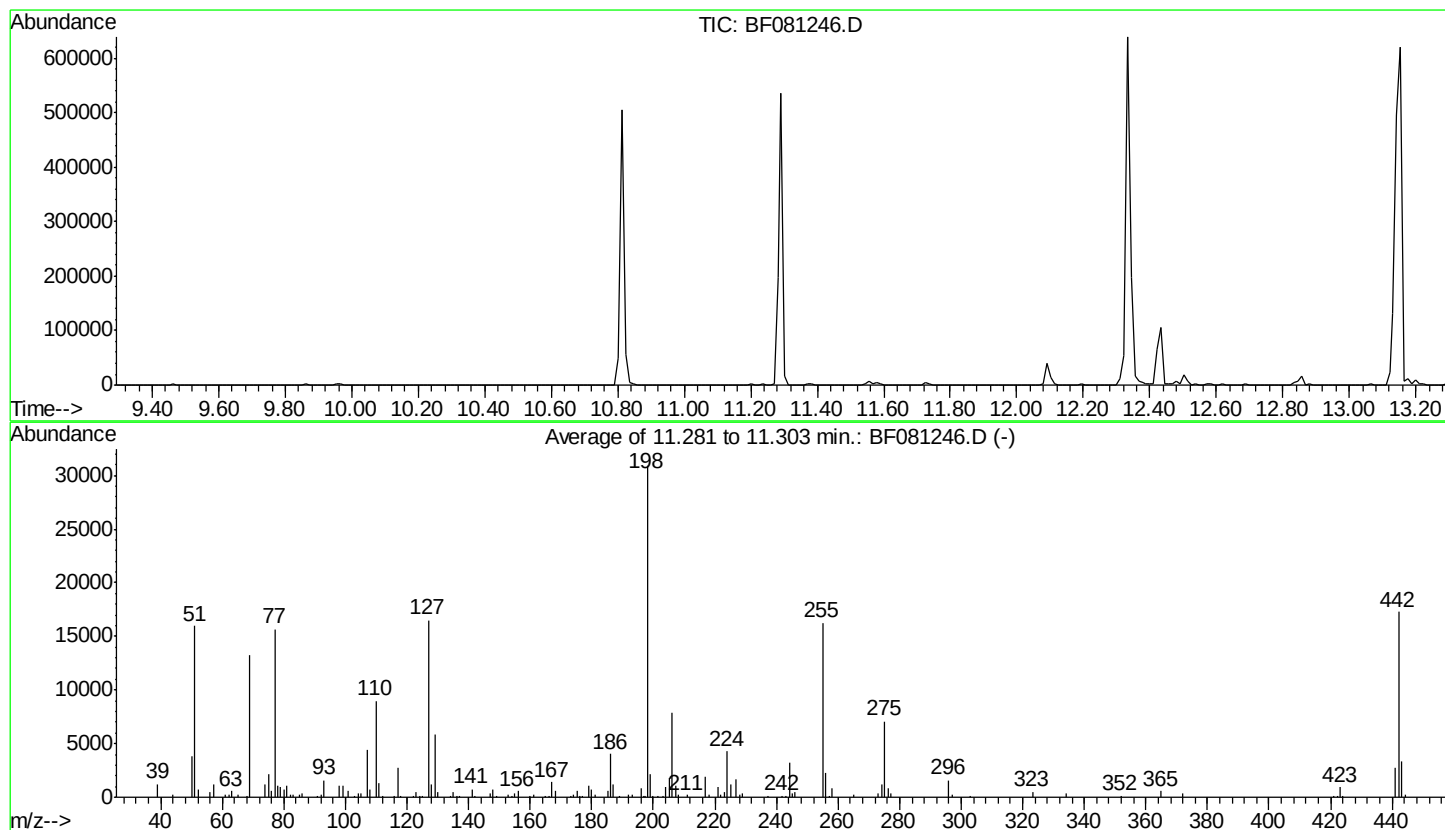

AutoFind: Scans 835, 836, 837; Background Corrected with Scan 832

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.7	15978	PASS
68	69	0.00	2	0.8	106	PASS
69	198	0.00	100	42.9	13269	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.4	16509	PASS
197	198	0.00	2	0.5	164	PASS
198	198	100	100	100.0	30921	PASS
199	198	5	9	6.8	2114	PASS
275	198	10	60	22.9	7076	PASS
365	198	1	100	1.9	581	PASS
441	442	0.01	24	16.0	2765	PASS
442	198	50	100	55.8	17257	PASS
443	442	15	24	19.7	3394	PASS