


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF082815\
 Data File : BF081254.D
 Acq On : 28 Aug 2015 00:39
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 24 13:58:19 2015

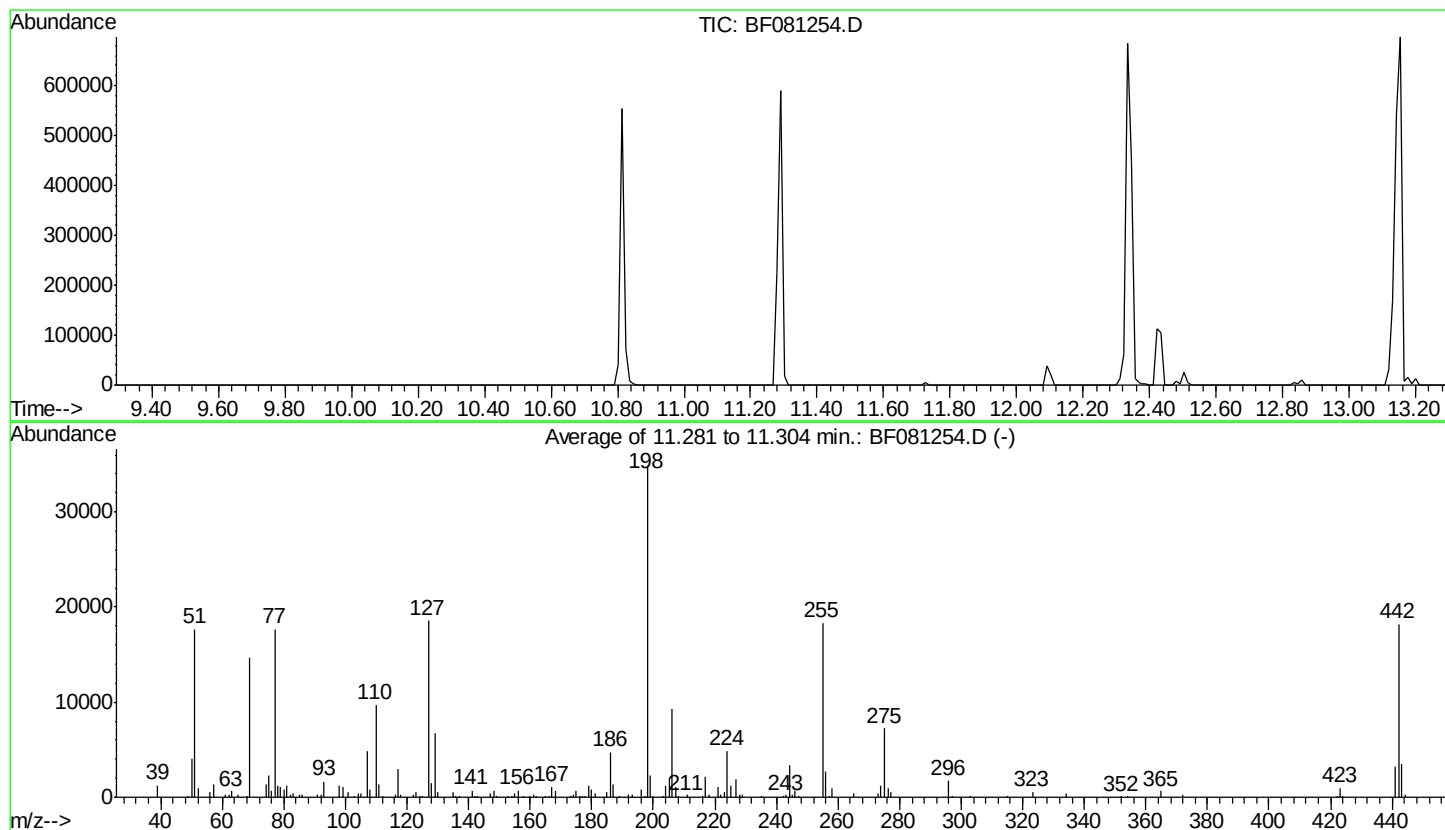

AutoFind: Scans 835, 836, 837; Background Corrected with Scan 832

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.8	17706	PASS
68	69	0.00	2	0.8	113	PASS
69	198	0.00	100	41.9	14629	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.1	18528	PASS
197	198	0.00	2	0.6	195	PASS
198	198	100	100	100.0	34876	PASS
199	198	5	9	6.6	2311	PASS
275	198	10	60	20.8	7237	PASS
365	198	1	100	1.8	625	PASS
441	442	0.01	24	17.5	3191	PASS
442	198	50	100	52.3	18235	PASS
443	442	15	24	18.9	3448	PASS