
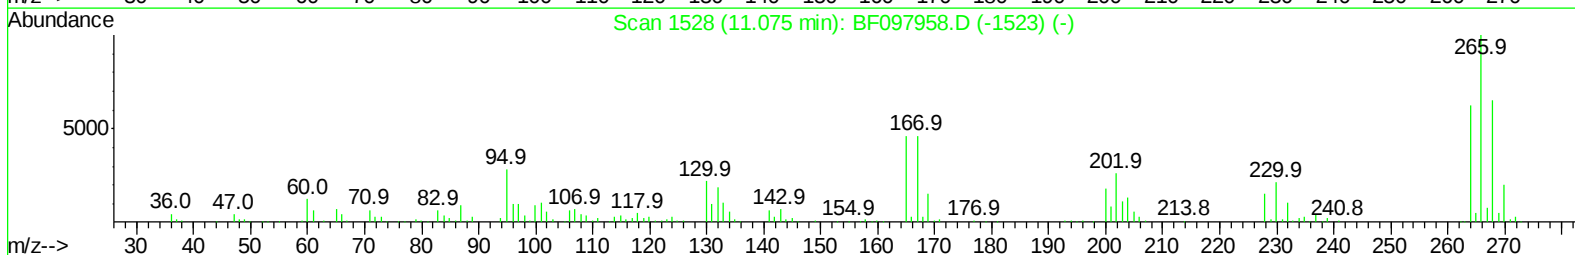
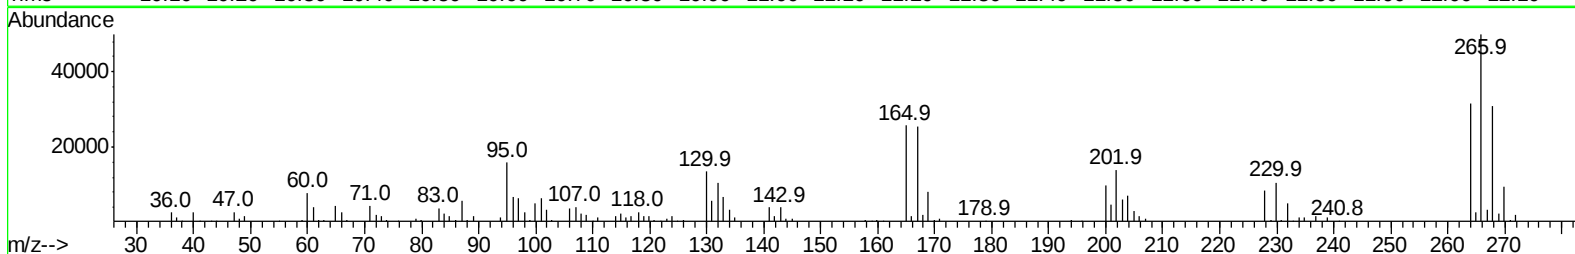


Data Path : Z:\HPCHEM1\BNA F\DATA\BF082817\  
Data File : BF098057.D  
Acq On : 28 Aug 2017 9:49  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 29 15:12:17 2017  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Aug 21 15:59:04 2017  
Response via : Initial Calibration

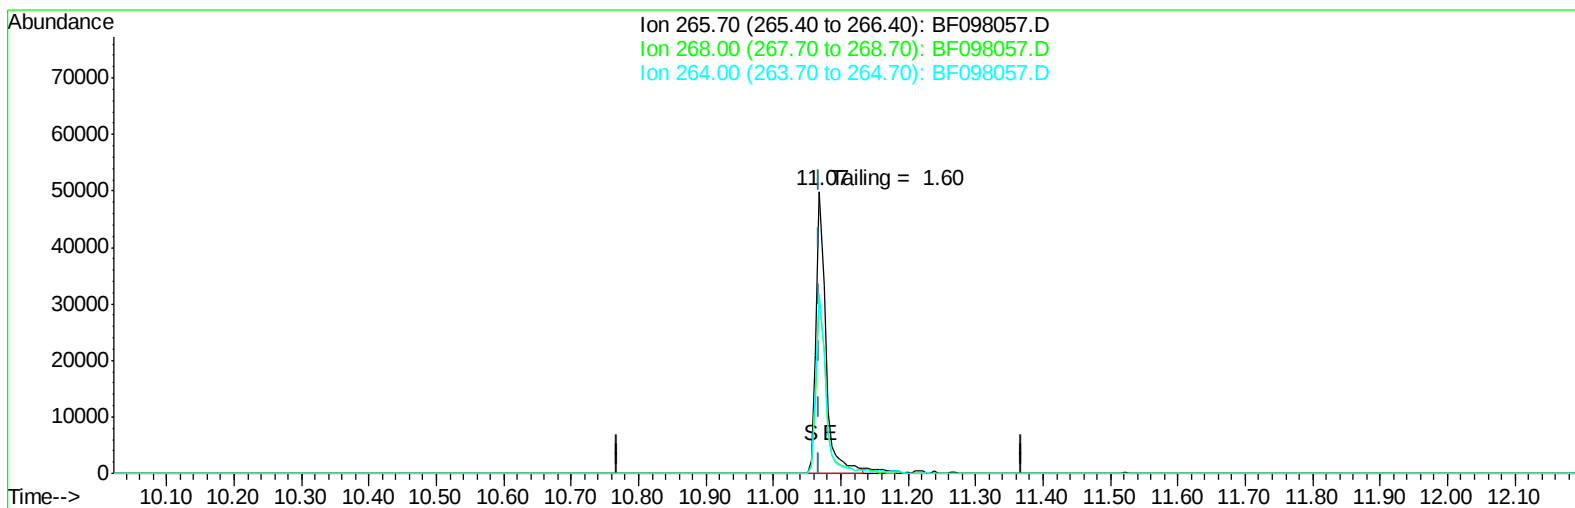

TIC: BF098057.D

(69) Pentachlorophenol (C)




11.069min (-0.000) 17488.10ng

response 49969

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.90 | 62.16 |
| 264.00 | 64.60 | 63.58 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA F\DATA\BF082817\  
Data File : BF098057.D  
Acq On : 28 Aug 2017 9:49  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 29 15:12:17 2017  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Aug 21 15:59:04 2017  
Response via : Initial Calibration

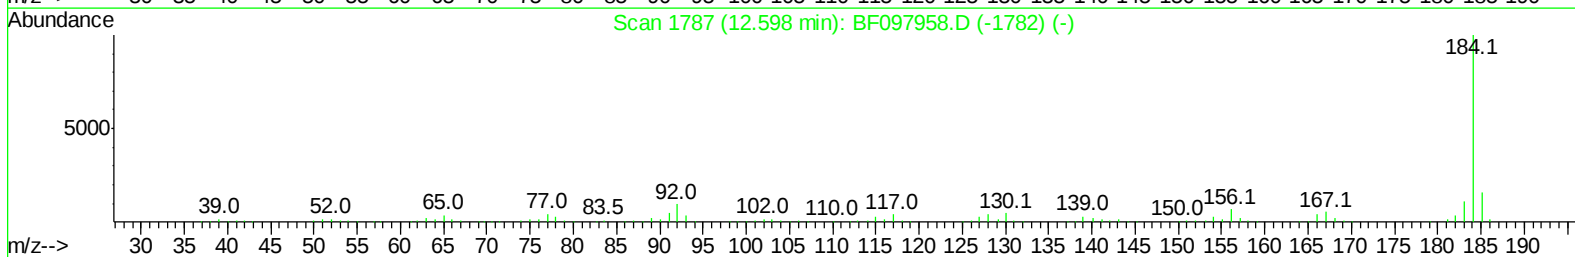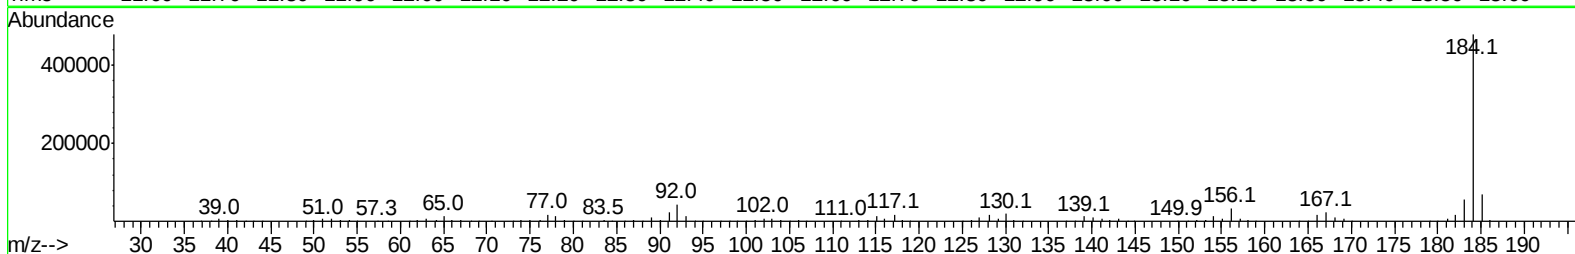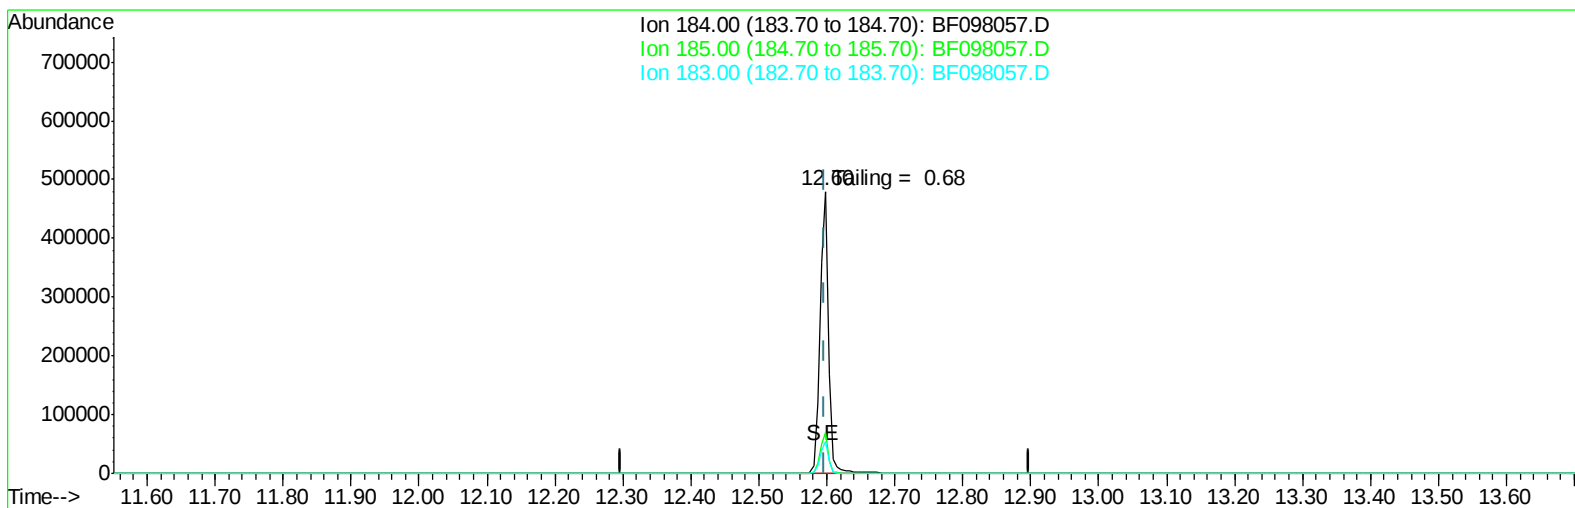

TIC: BF098057.D

(76) Benzidine

12.598min (-0.000) 11042.31ng

response 426860

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 184.00 | 100   | 100    |
| 185.00 | 19.40 | 14.53# |
| 183.00 | 12.20 | 11.51  |
| 0.00   | 0.00  | 0.00   |