
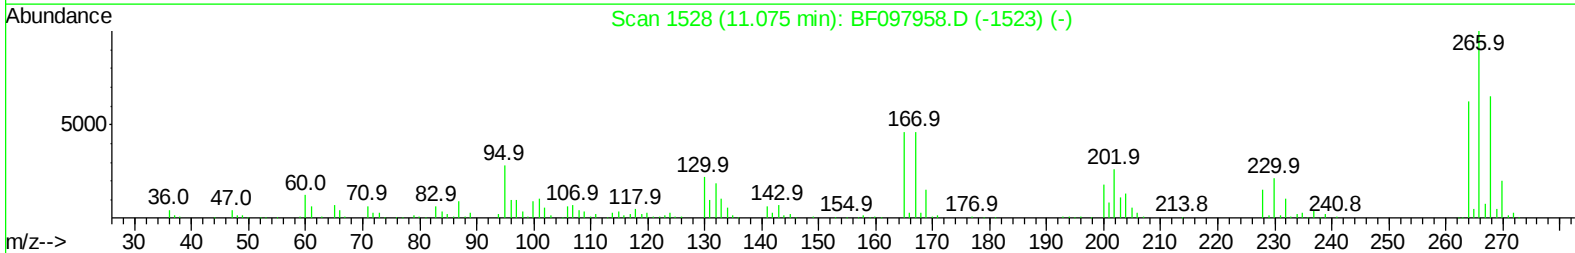
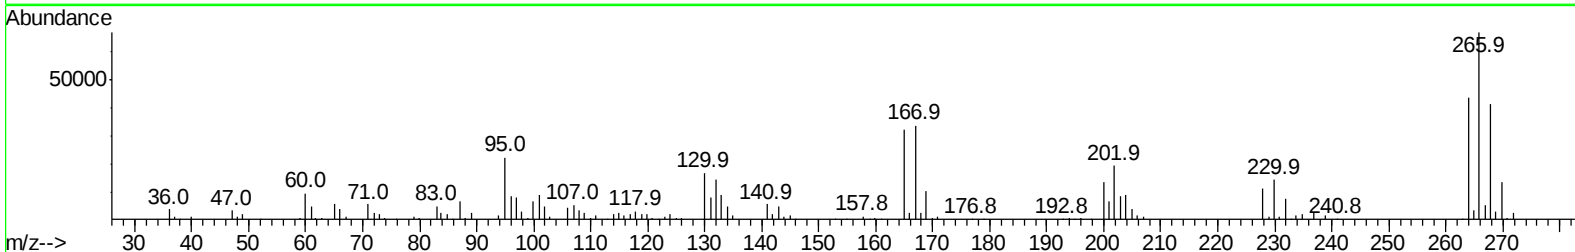


```
Data Path : Z:\HPCHEM1\BNA F\DATA\BF082817\  
Data File : BF098094.D  
Acq On    : 29 Aug 2017    4:43  
Operator  : SJ/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Aug 29 15:17:16 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 21 15:59:04 2017
Response via : Initial Calibration



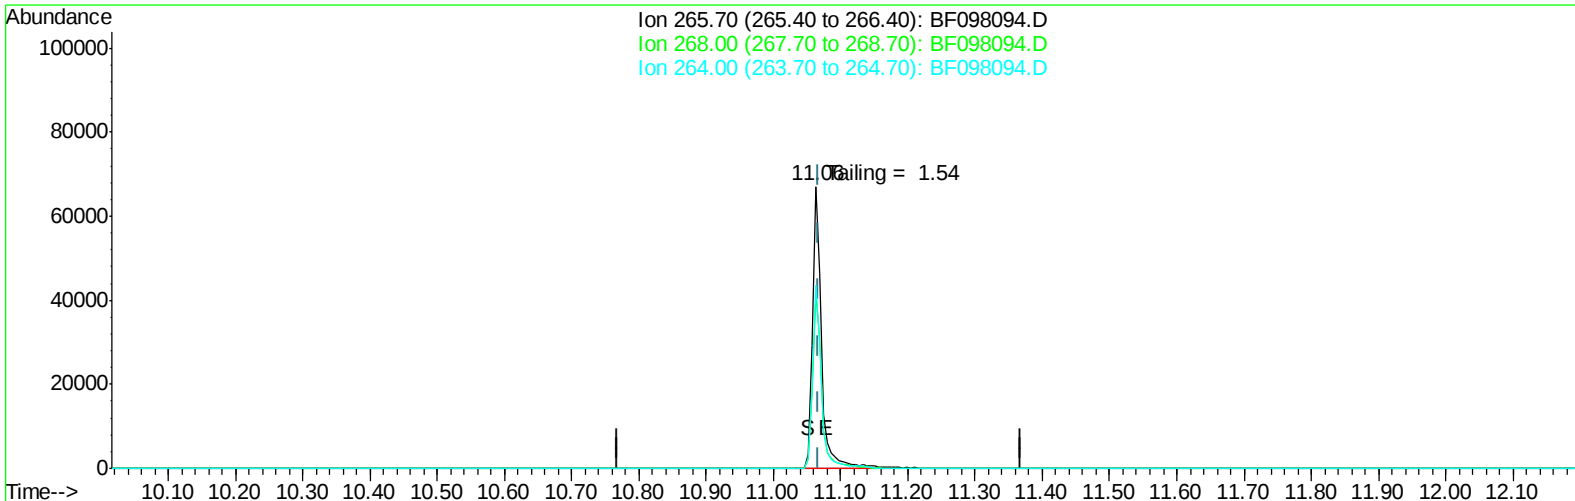


TIC: BF098094.D

(69) Pentachlorophenol (C)		
11.063min (-0.006) 37221.57ng		
response 64777		
Ion	Exp%	Act%
265.70	100	100
268.00	63.90	61.67
264.00	64.60	65.08
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF082817\
Data File : BF098094.D
Acq On : 29 Aug 2017 4:43
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 29 15:17:16 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 21 15:59:04 2017
Response via : Initial Calibration

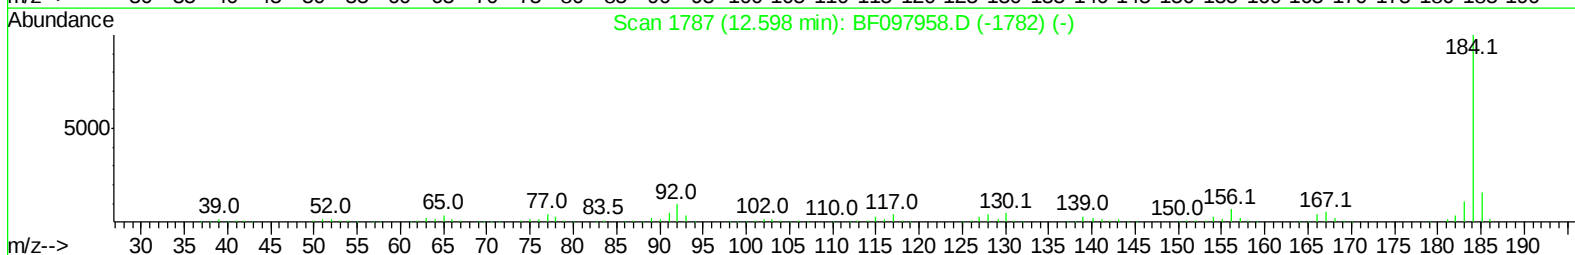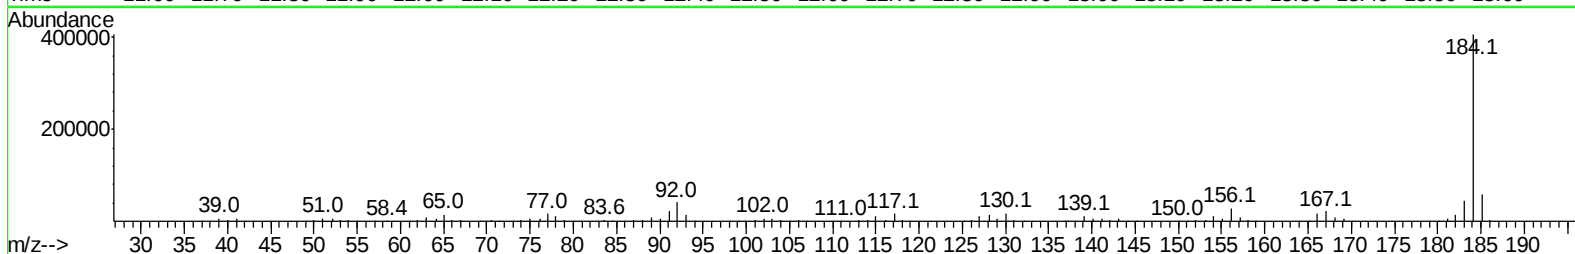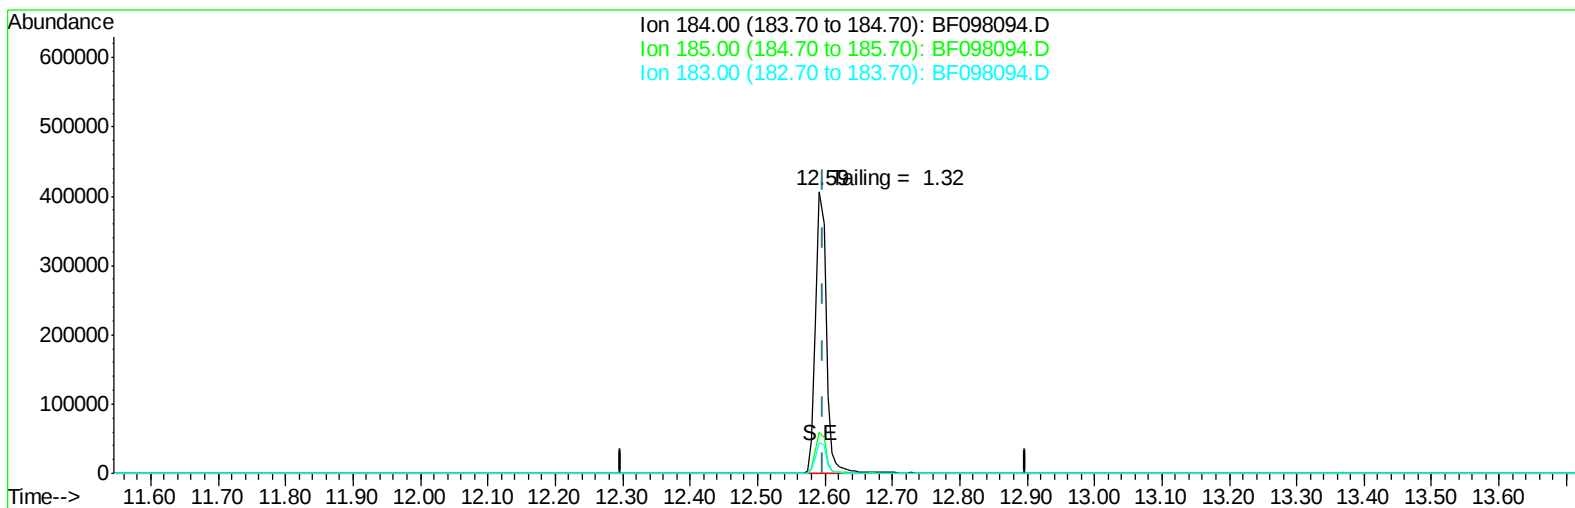

TIC: BF098094.D

(76) Benzidine

12.592min (-0.006) 0.00ng

response 437617

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.46#
183.00	12.20	11.01
0.00	0.00	0.00