

Data Path : Z:\HPCHEM1\BNA F\DATA\BF082817\
 Data File : BF098089.D
 Acq On : 29 Aug 2017 1:57
 Operator : SJ/JU
 Sample : I4959-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 RT2321-RT2315-20-02-RB36575

Quant Time: Aug 29 09:15:10 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 21 15:59:04 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.74	152	102874	20.00	ng	-0.01
21) Naphthalene-d8	8.02	136	400868	20.00	ng	-0.01
38) Acenaphthene-d10	9.77	164	172278	20.00	ng	-0.01
63) Phenanthrene-d10	11.26	188	335186	20.00	ng	0.00
75) Chrysene-d12	13.89	240	265191	20.00	ng	-0.01
86) Perylene-d12	15.31	264	191011	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.36	112	816004	120.65	ng	0.00
7) Phenol-d6	6.38	99	1013456	110.29	ng	0.00
23) Nitrobenzene-d5	7.30	82	704805	95.51	ng	-0.02
41) 2,4,6-Tribromophenol	10.56	330	213808	143.04	ng	-0.01
44) 2-Fluorobiphenyl	9.10	172	1032069	88.02	ng	-0.01
78) Terphenyl-d14	12.85	244	923628	72.63	ng	0.00


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF082817\
Data File : BF098089.D
Acq On : 29 Aug 2017 1:57
Operator : SJ/JU
Sample : I4959-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RT2321-RT2315-20-02-RB36575

Quant Time: Aug 29 09:15:10 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 21 15:59:04 2017
Response via : Initial Calibration

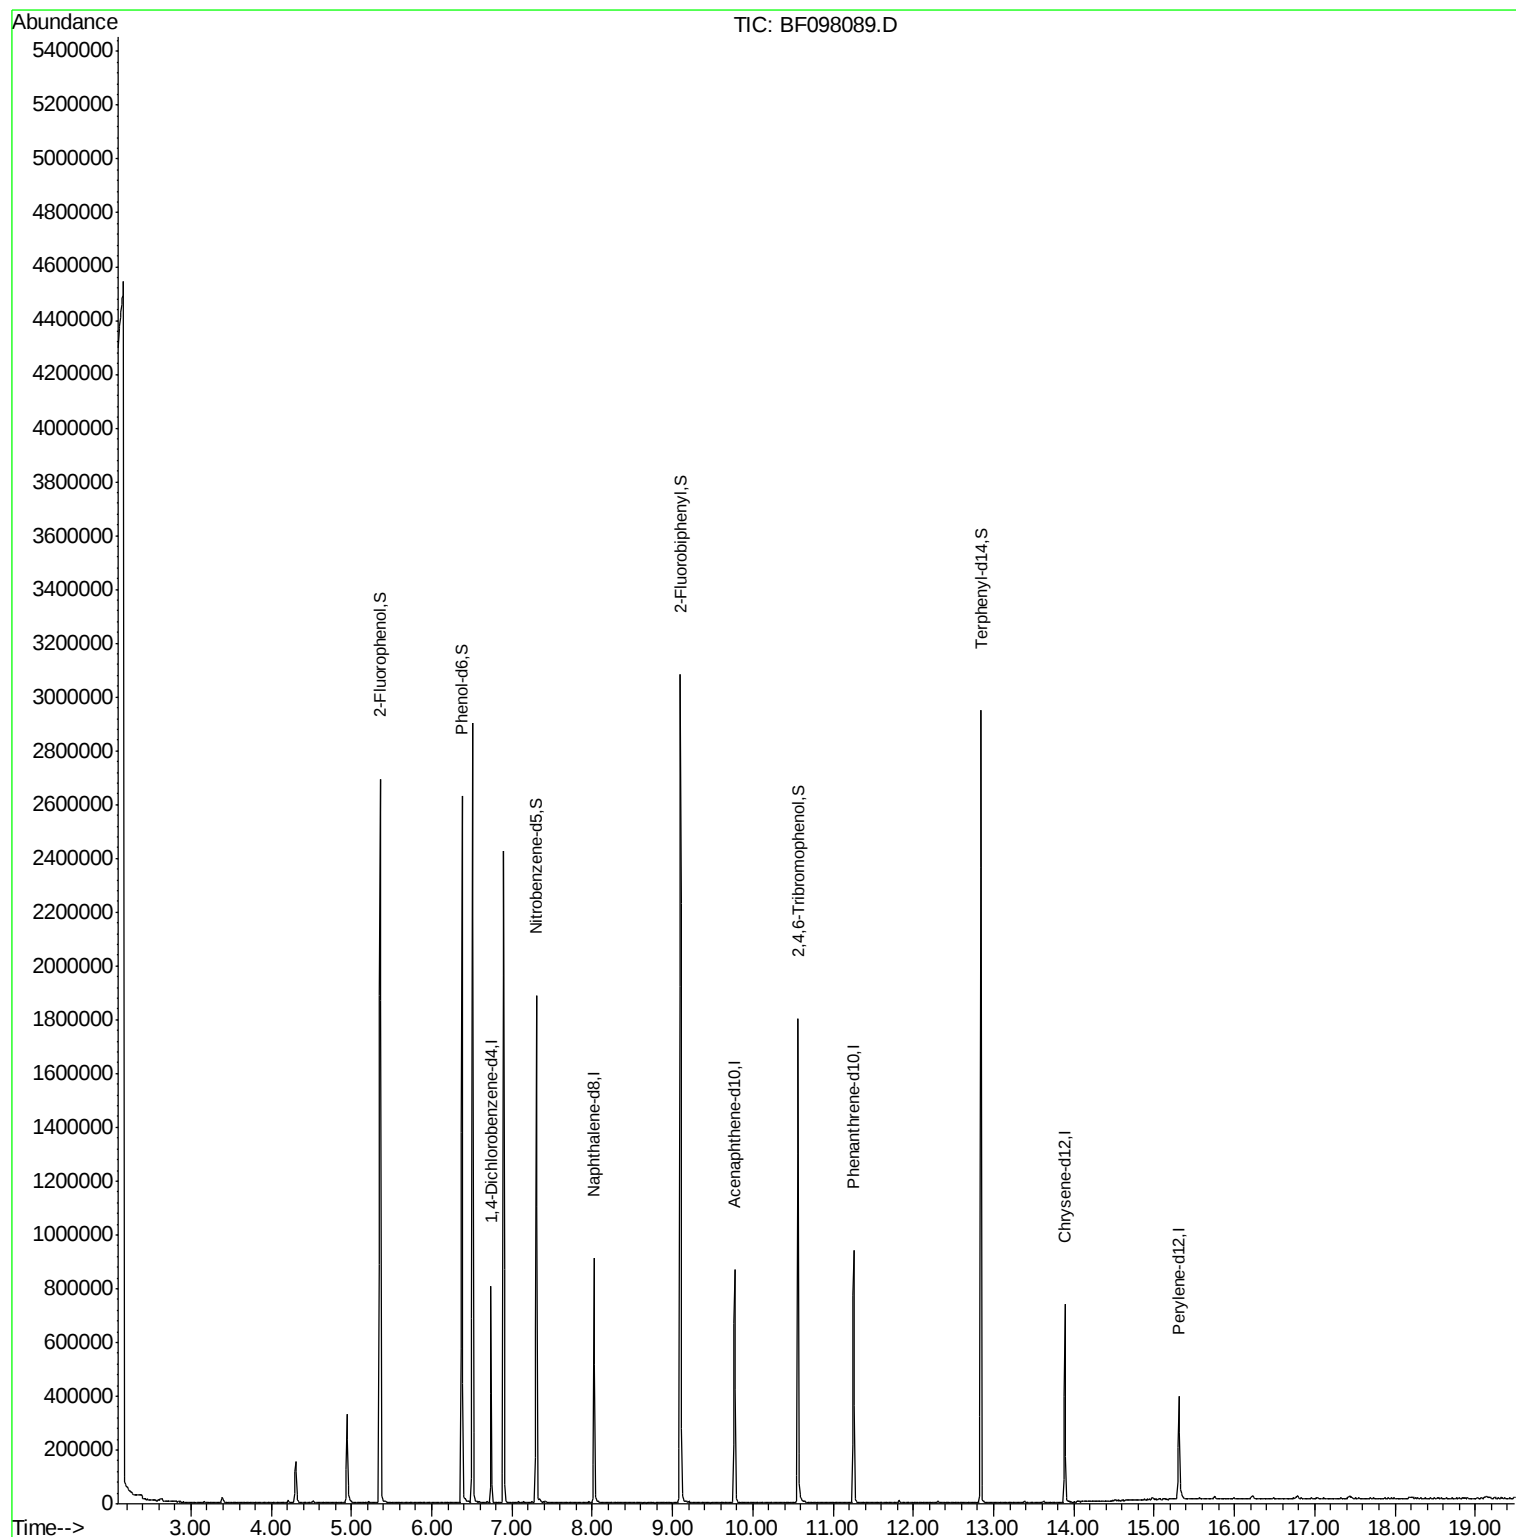




#1



1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.74 min Scan# 791
 Delta R.T. -0.01 min
 Lab File: BF098089.D
 Acq: 29 Aug 2017 1:57

Instrument :
 BNA_F
 ClientSampleId :
 RT2321-RT2315-20-02-RB36575

Tot Ion:152 Resp: 102874
 Ion Ratio Lower Upper
 152 100
 150 156.6 126.2 189.2
 115 65.5 52.2 78.2

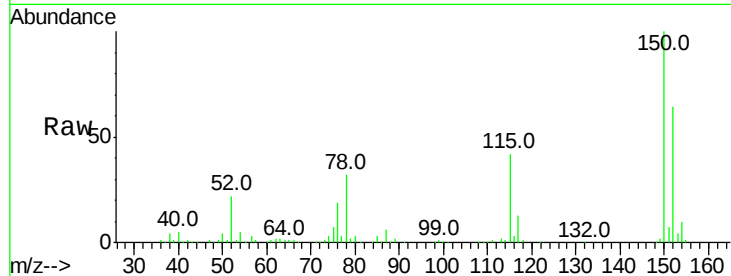


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

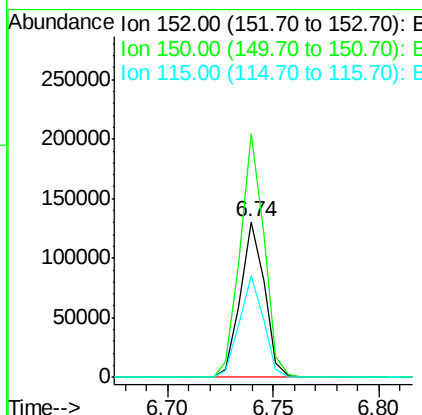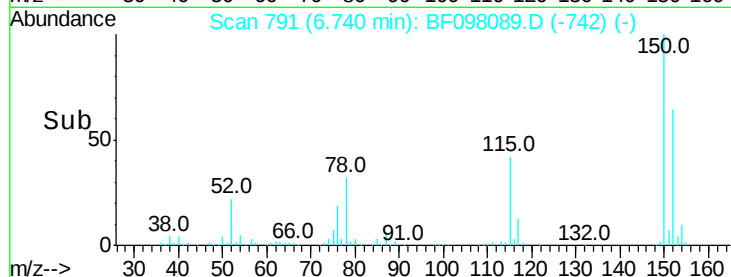



#5


2-Fluorophenol
 Concen: 120.653 ng
 RT: 5.36 min Scan# 556
 Delta R.T. 0.01 min
 Lab File: BF098089.D
 Acq: 29 Aug 2017 1:57

Tgt Ion:112 Resp: 816004
 Ion Ratio Lower Upper
 112 100
 64 60.5 46.0 69.0
 63 30.2 23.4 35.0

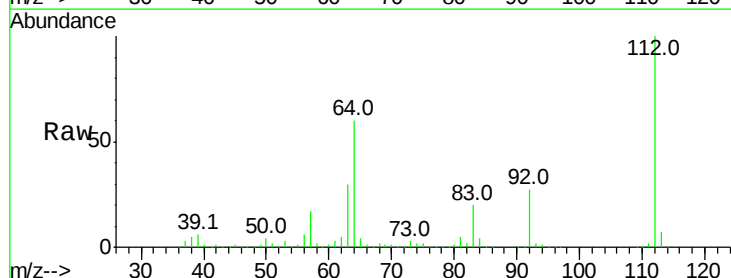

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF0
 Ion 63.00 (62.70 to 63.70): BF0

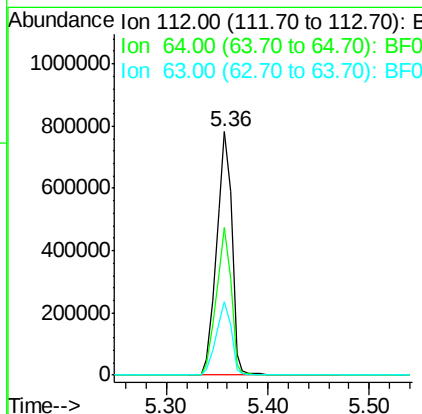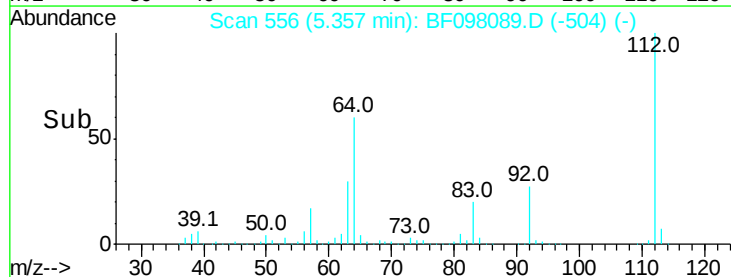

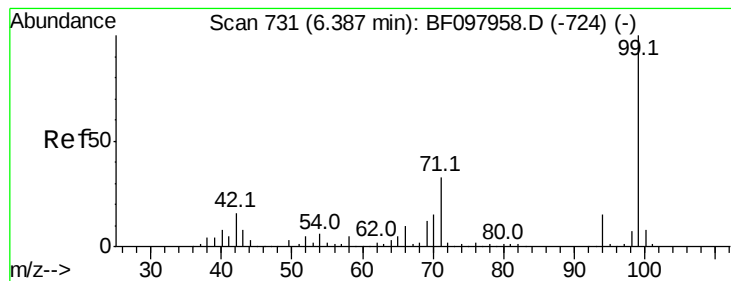

#7

Phenol-d6

Concen: 110.286 ng

RT: 6.38 min Scan# 730

Delta R.T. -0.01 min

Lab File: BF098089.D

Acq: 29 Aug 2017 1:57

Instrument :

BNA_F

ClientSampleId :

RT2321-RT2315-20-02-RB36575


Tot Ion: 99 Resp: 1013456

Ion Ratio Lower Upper

99 100

42 15.0 13.5 20.3




71 31.4 24.5 36.7

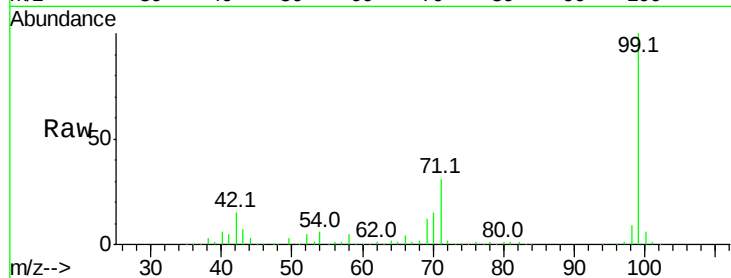

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

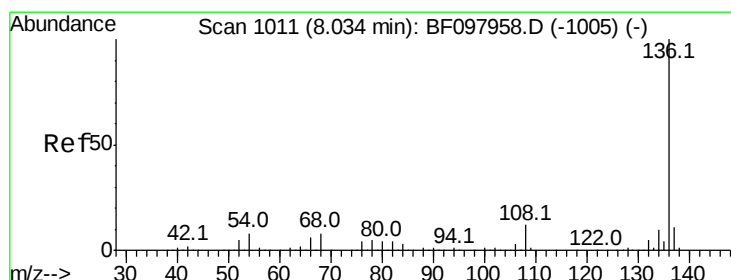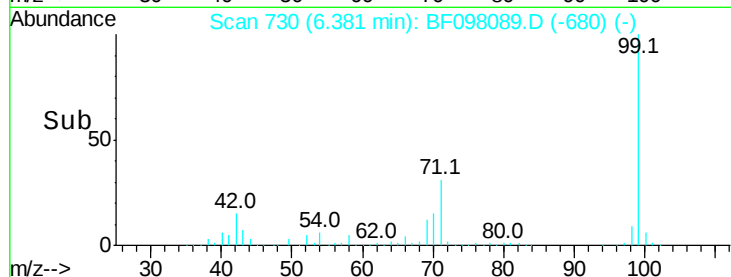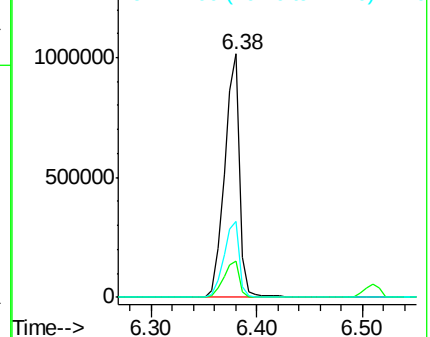

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.02 min Scan# 1009

Delta R.T. -0.01 min

Lab File: BF098089.D

Acq: 29 Aug 2017 1:57

Tgt Ion: 136 Resp: 400868


Ion Ratio Lower Upper

136 100

137 11.1 8.5 12.7

54 7.5 4.9 7.3#

68 6.9 4.1 6.1#


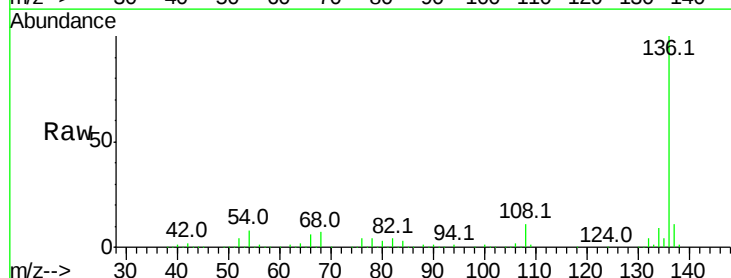



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



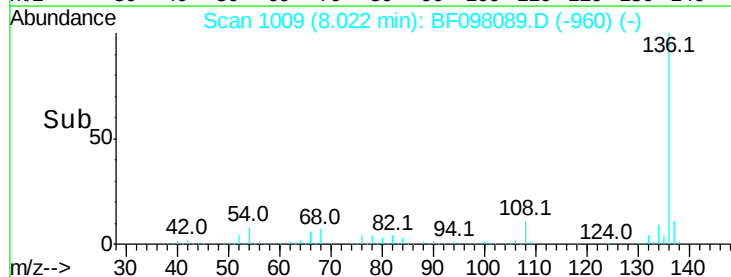
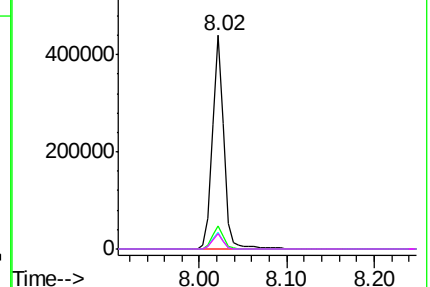


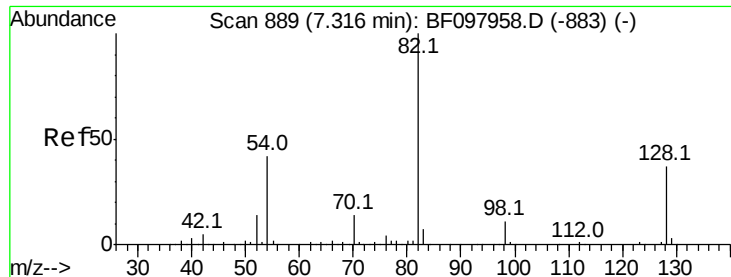

#23
 Nitrobenzene-d5
 Concen: 95.513 ng
 RT: 7.30 min Scan# 887
 Delta R.T. -0.02 min
 Lab File: BF098089.D
 Acq: 29 Aug 2017 1:57




Instrument :
 BNA_F
 ClientSampleId :
 RT2321-RT2315-20-02-RB36575


Tot Ion	Ratio	Lower	Upper
82	100		
128	38.1	34.0	51.0
54	41.0	42.2	63.2#

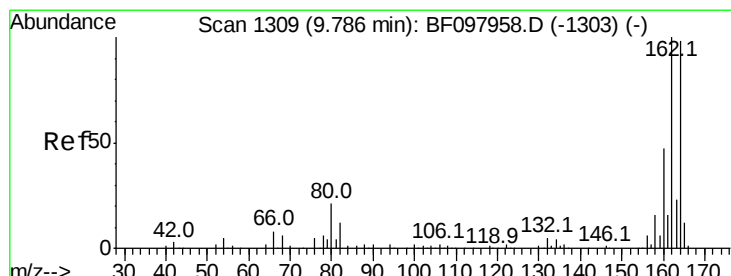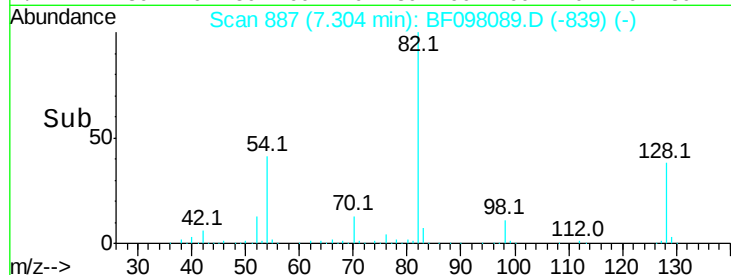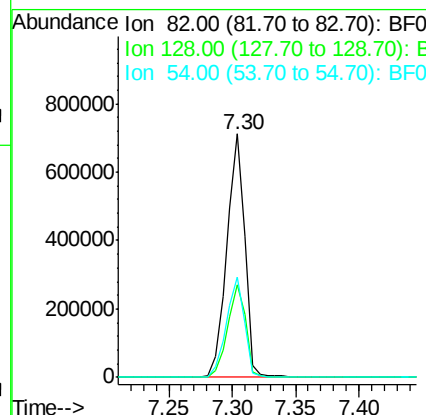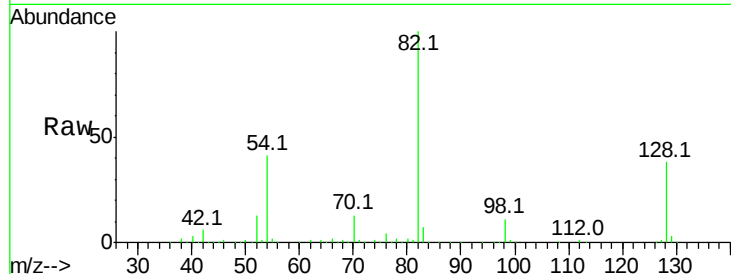

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.77 min Scan# 1307
 Delta R.T. -0.01 min
 Lab File: BF098089.D
 Acq: 29 Aug 2017 1:57

Tgt Ion	Ratio	Lower	Upper
164	100		
162	100.7	82.6	123.8
160	47.1	36.2	54.2

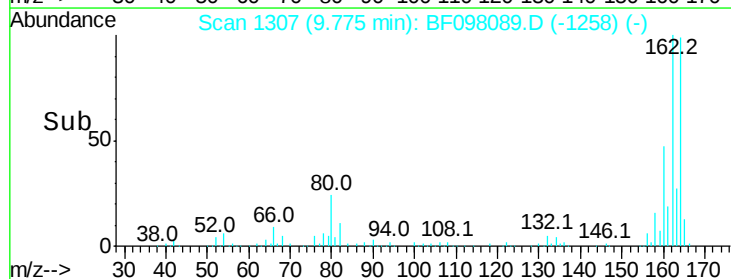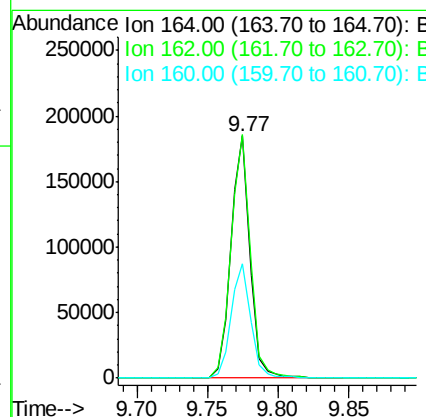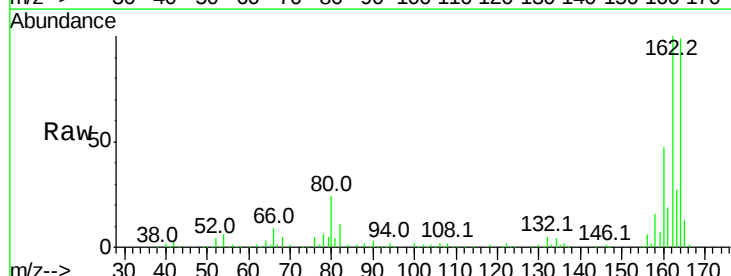


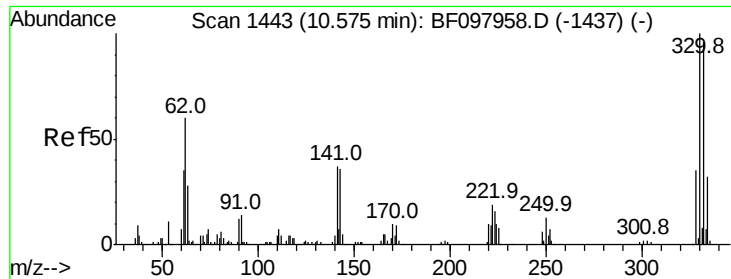




#41
 2,4,6-Tribromophenol
 Concen: 143.035 ng
 RT: 10.56 min Scan# 1441
 Delta R.T. -0.01 min
 Lab File: BF098089.D
 Acq: 29 Aug 2017 1:57

Instrument :
 BNA_F
 ClientSampleId :
 RT2321-RT2315-20-02-RB36575

Tot Ion:330 Resp: 213808
 Ion Ratio Lower Upper
 330 100
 332 96.8 76.6 115.0
 141 37.9 31.4 47.2

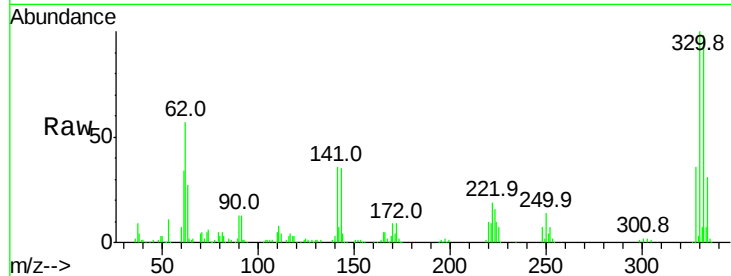


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

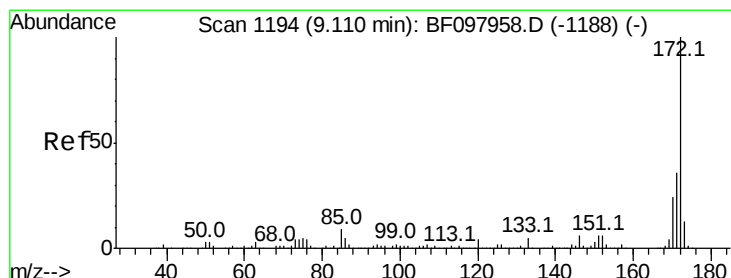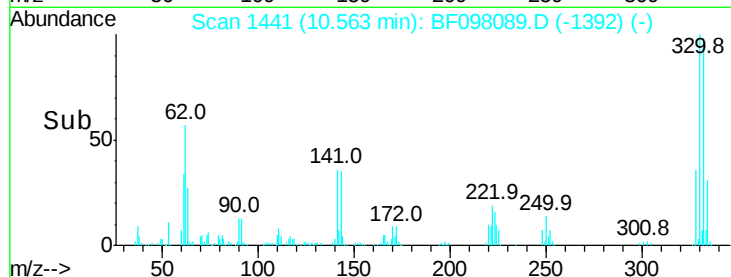
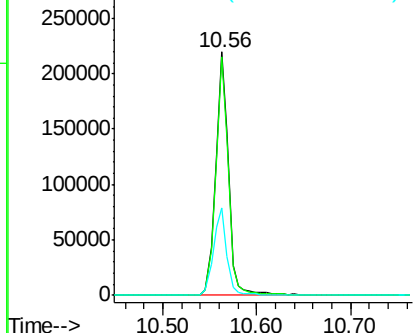



#44
 2-Fluorobiphenyl
 Concen: 88.016 ng
 RT: 9.10 min Scan# 1192
 Delta R.T. -0.01 min
 Lab File: BF098089.D
 Acq: 29 Aug 2017 1:57

Tgt Ion:172 Resp: 1032069
 Ion Ratio Lower Upper
 172 100
 171 35.9 29.6 44.4
 170 24.3 19.8 29.8

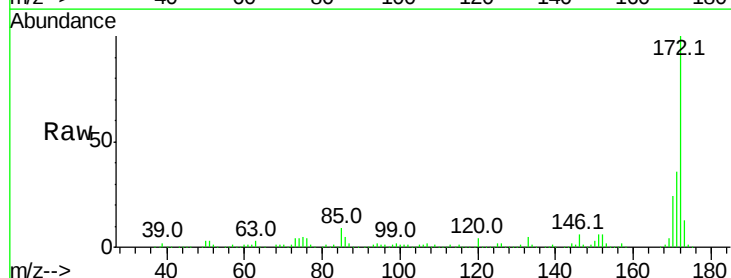

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



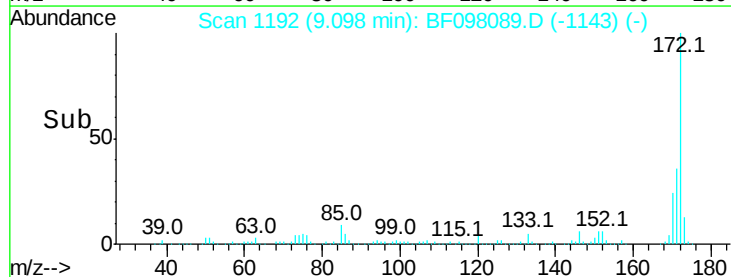
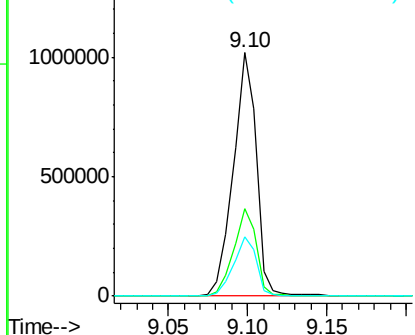


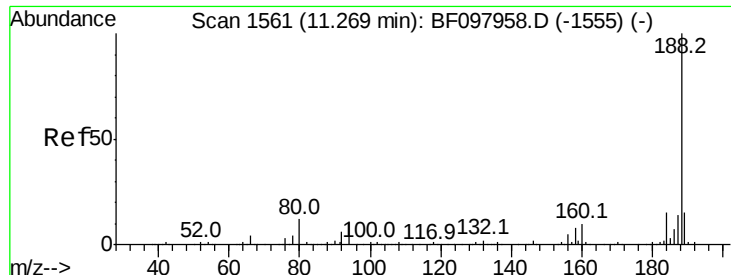

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.26 min Scan# 1559
Delta R.T. -0.01 min
Lab File: BF098089.D
Acq: 29 Aug 2017 1:57




Instrument :
BNA_F
ClientSampleId :
RT2321-RT2315-20-02-RB36575


Tot Ion	Ratio	Lower	Upper
188	100		
94	10.1	9.4	14.2
80	10.9	10.2	15.2

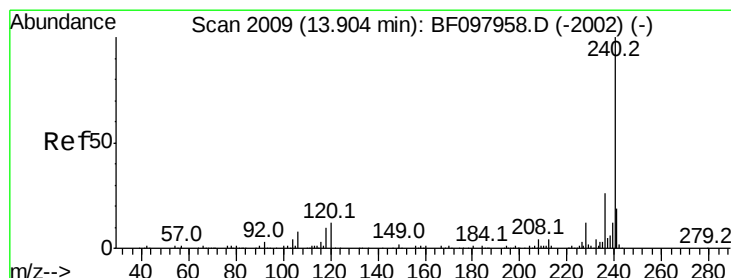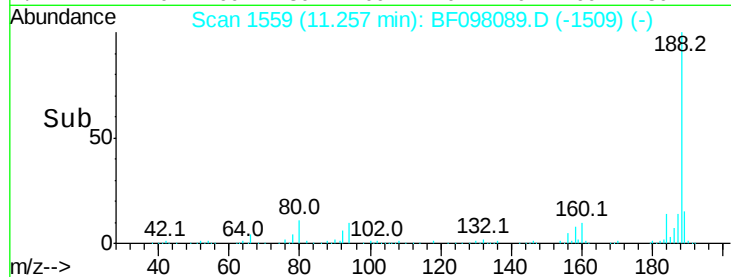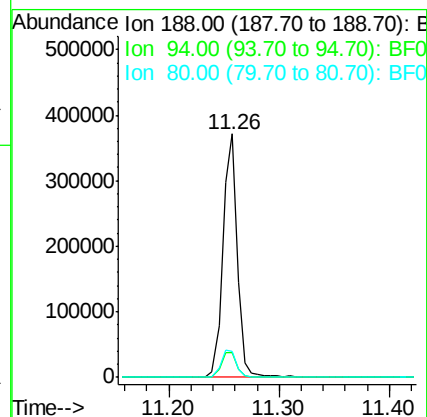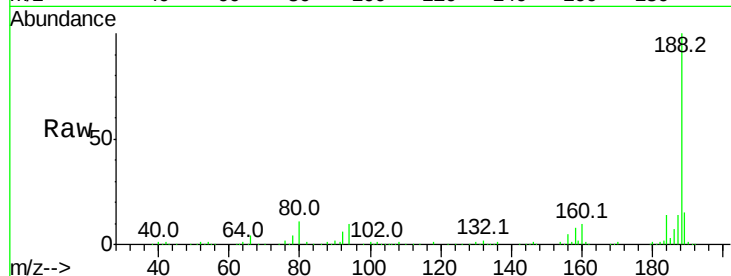

#75
Chrysene-d12
Concen: 20.000 ng
RT: 13.89 min Scan# 2006
Delta R.T. -0.01 min
Lab File: BF098089.D
Acq: 29 Aug 2017 1:57

Tgt Ion	Ratio	Lower	Upper
240	100		
120	13.4	5.8	8.8#
236	25.8	20.5	30.7

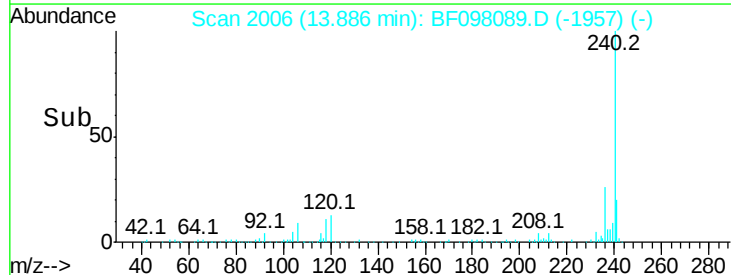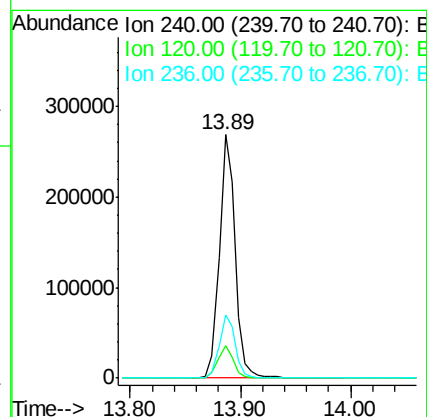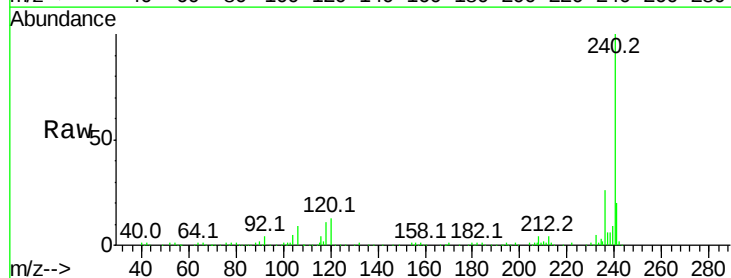

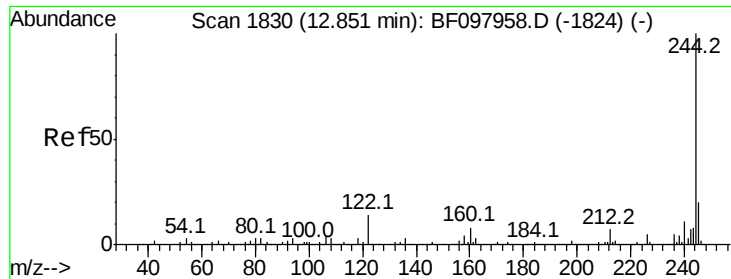

#78

Terphenyl-d14

Concen: 72.630 ng

RT: 12.85 min Scan# 1829

Delta R.T. -0.01 min

Lab File: BF098089.D

Acq: 29 Aug 2017 1:57

Instrument :

BNA_F

ClientSampleId :

RT2321-RT2315-20-02-RB36575


Tot Ion:244 Resp: 923628

Ion Ratio Lower Upper

244 100

212 7.3 6.0 9.0




122 13.0 10.3 15.5

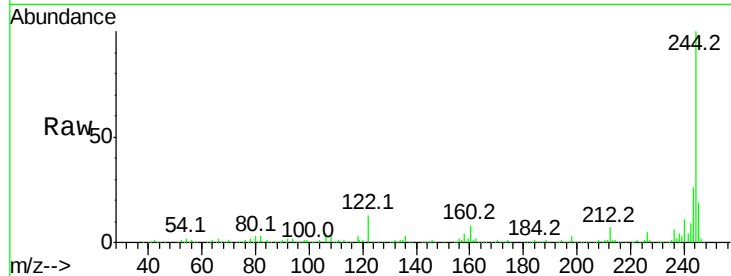

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

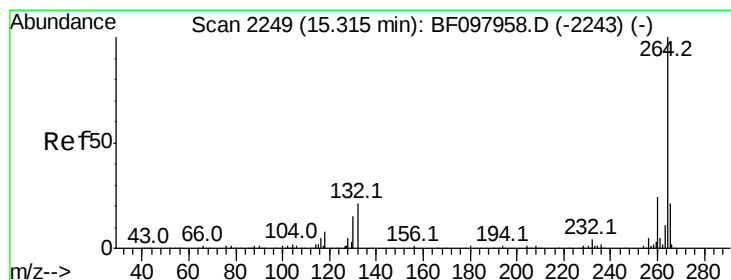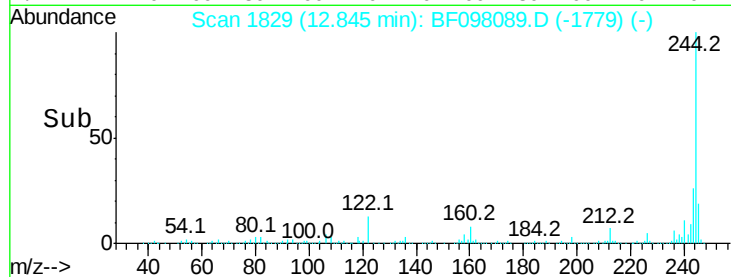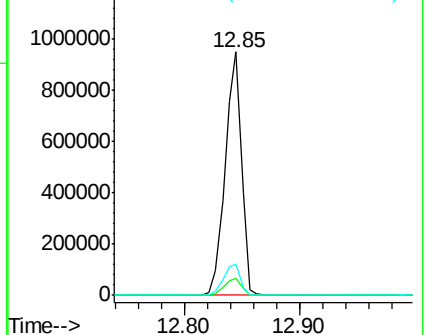

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.31 min Scan# 2248

Delta R.T. 0.00 min

Lab File: BF098089.D

Acq: 29 Aug 2017 1:57


Tgt Ion:264 Resp: 191011

Ion Ratio Lower Upper

264 100

260 25.1 19.5 29.3

265 20.8 17.2 25.8

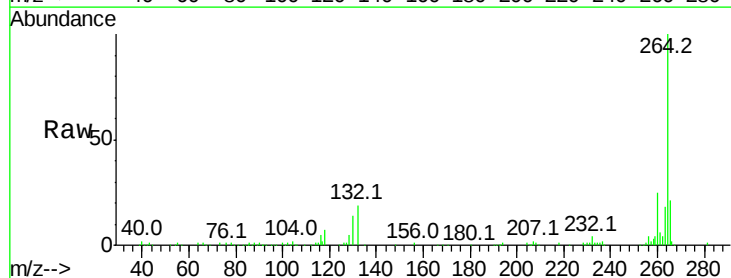

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

