

Data Path : Z:\HPCHEM1\BNA F\DATA\BF082817\
 Data File : BF098069.D
 Acq On : 28 Aug 2017 15:25
 Operator : SJ/JU
 Sample : I4969-04 5X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 BU-01-082417-B

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.916	478	481	490	rVB	50900	54651	6.82%	0.561%
2	5.340	549	553	563	rBV	806041	725207	90.44%	7.441%
3	6.369	724	728	741	rBV	872028	788122	98.29%	8.087%
4	6.504	748	751	755	rBV	875332	749317	93.45%	7.689%
5	6.739	788	791	795	rBV	767380	643220	80.22%	6.600%
6	6.898	814	818	821	rBV	634716	558046	69.59%	5.726%
7	7.304	883	887	893	rBV	468769	430349	53.67%	4.416%
8	8.028	1006	1010	1013	rBV	936992	801868	100.00%	8.228%
9	9.098	1189	1192	1202	rBV	917661	738188	92.06%	7.575%
10	9.492	1256	1259	1269	rBV	69442	71878	8.96%	0.738%
11	9.780	1304	1308	1317	rVB	824435	788737	98.36%	8.093%
12	10.186	1373	1377	1379	rBV3	7929	9923	1.24%	0.102%
13	10.210	1379	1381	1385	rVB2	13456	11438	1.43%	0.117%
14	10.322	1398	1400	1404	rBV	13432	12245	1.53%	0.126%
15	10.563	1437	1441	1451	rBV	403781	350527	43.71%	3.597%
16	10.686	1458	1462	1467	rBV3	15758	18117	2.26%	0.186%
17	11.157	1540	1542	1548	rVB3	11106	11791	1.47%	0.121%
18	11.257	1556	1559	1562	rBV	734386	694604	86.62%	7.127%
19	11.280	1562	1563	1567	rVV	143841	98323	12.26%	1.009%
20	11.333	1570	1572	1576	rVB	27629	22139	2.76%	0.227%
21	11.657	1624	1627	1629	rBV4	8617	9123	1.14%	0.094%
22	11.763	1640	1645	1647	rBV	21159	19875	2.48%	0.204%
23	11.786	1647	1649	1653	rVB	23833	22991	2.87%	0.236%
24	11.874	1660	1664	1666	rBV	25952	29777	3.71%	0.306%
25	11.892	1666	1667	1671	rVB2	14400	11798	1.47%	0.121%
26	12.057	1693	1695	1698	rBV2	11424	11782	1.47%	0.121%
27	12.310	1735	1738	1740	rBV	12868	13385	1.67%	0.137%
28	12.345	1740	1744	1750	rVV7	16227	30428	3.79%	0.312%
29	12.392	1750	1752	1756	rBV4	9785	12155	1.52%	0.125%
30	12.468	1762	1765	1769	rBV	155975	122486	15.28%	1.257%
31	12.698	1798	1804	1807	rBV2	120086	121556	15.16%	1.247%
32	12.745	1810	1812	1816	rVB4	9070	11923	1.49%	0.122%
33	12.839	1825	1828	1832	rBV	519402	473611	59.06%	4.860%
34	13.027	1853	1860	1863	rBV2	29001	50832	6.34%	0.522%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF082817\
Data File : BF098069.D
Acq On : 28 Aug 2017 15:25
Operator : SJ/JU
Sample : I4969-04 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BU-01-082417-B

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	13.086	1867	1870	1874	rVV4	17305	24621	3.07%	0.253%
36	13.127	1875	1877	1881	rVV3	11732	14519	1.81%	0.149%
37	13.745	1979	1982	1986	rBV3	32547	40557	5.06%	0.416%
38	13.892	2002	2007	2010	rBV	713192	689927	86.04%	7.079%
39	15.315	2245	2249	2253	rBV2	393262	455429	56.80%	4.673%


Sum of corrected areas: 9745465

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF082817\
Data File : BF098069.D
Acq On : 28 Aug 2017 15:25
Operator : SJ/JU
Sample : I4969-04 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BU-01-082417-B

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

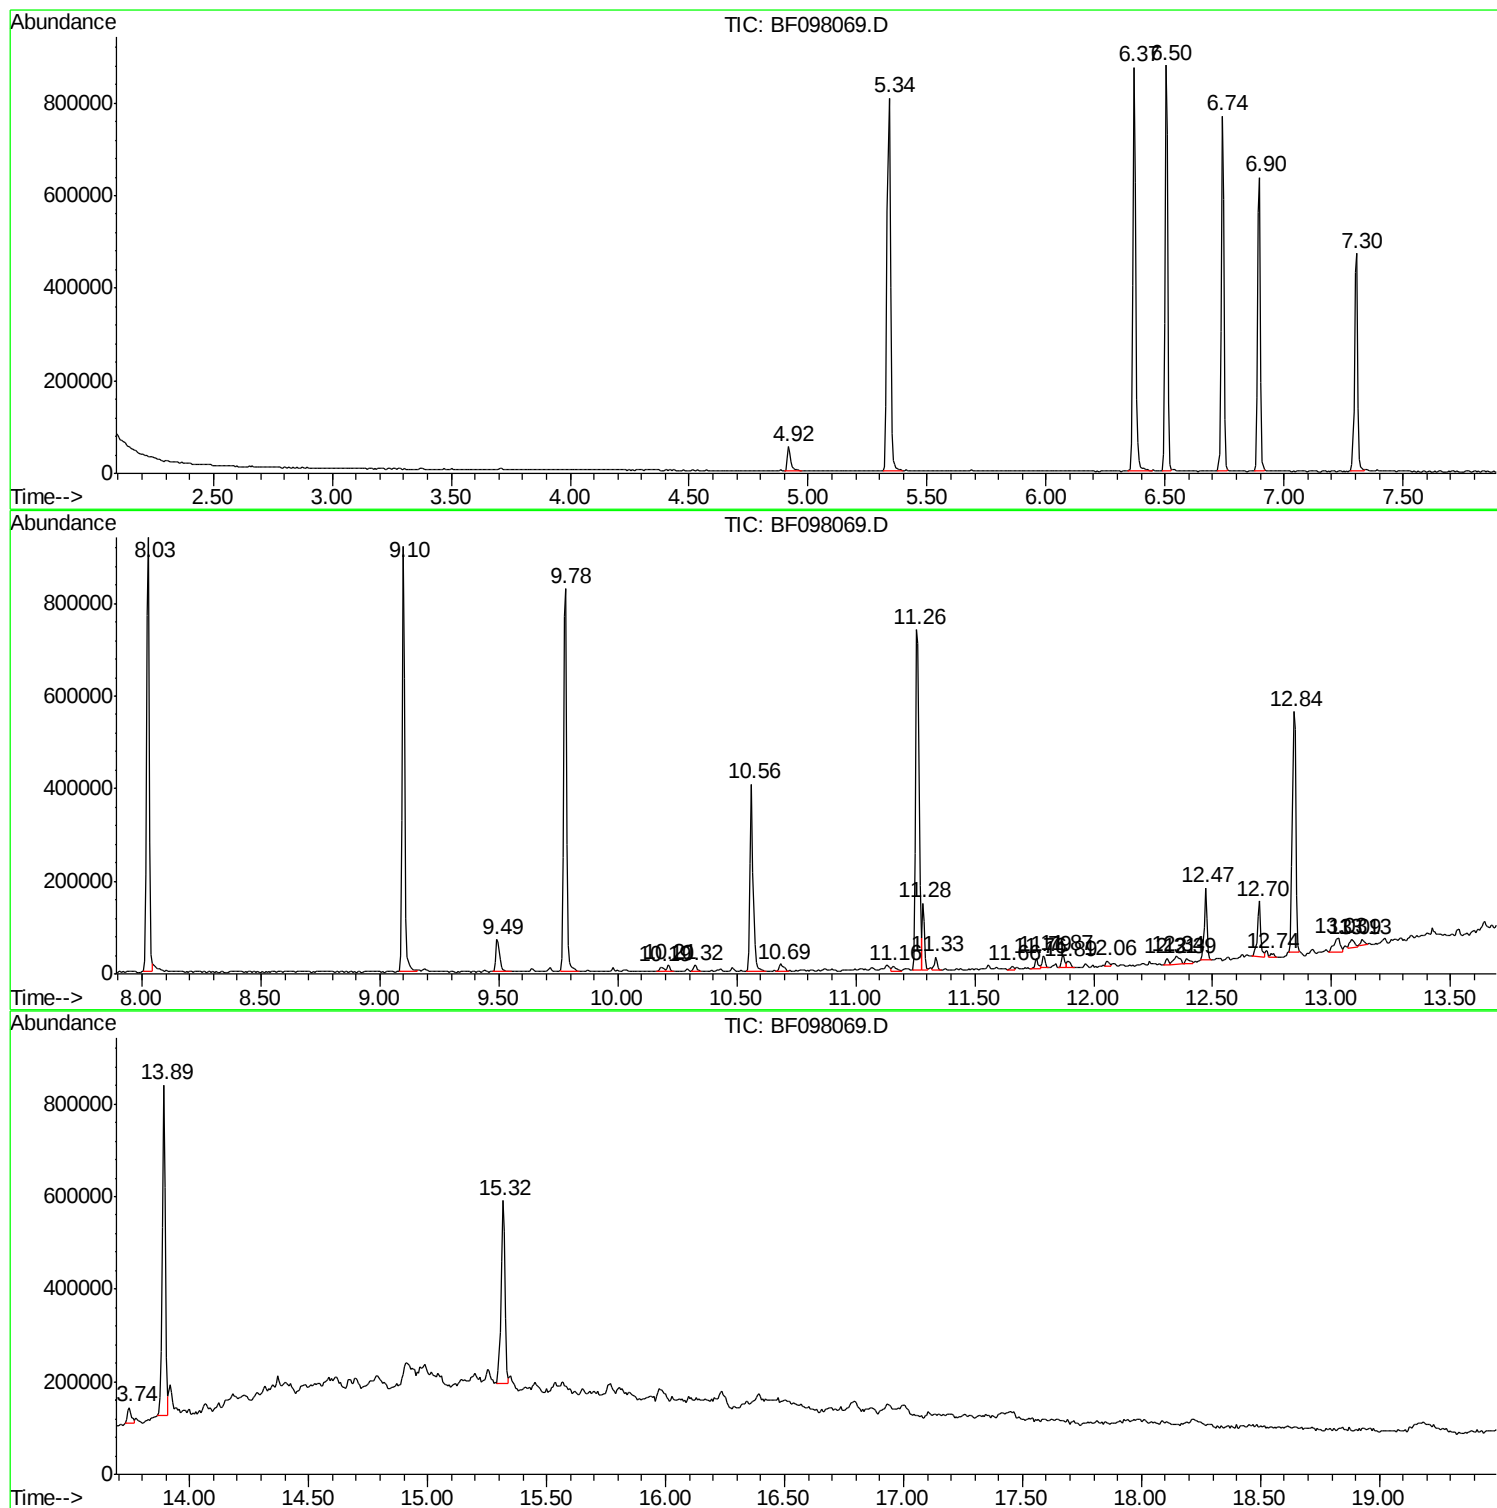

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF082817\
Data File : BF098069.D
Acq On : 28 Aug 2017 15:25
Operator : SJ/JU
Sample : I4969-04 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BU-01-082417-B










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.50 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.50	23.30 ng	749317	1,4-Dichlorobenzene-d4	6.74

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Cyclohexen-1-one	96	C6H8O	000930-68-7	10
2		5-Aminoindole	132	C8H8N2	005192-03-0	10
3		Cyclopropanamine, 1-phenyl-	133	C9H11N	1000351-26-2	10
4		1,3,5-Trifluorobenzene	132	C6H3F3	000372-38-3	9
5		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9

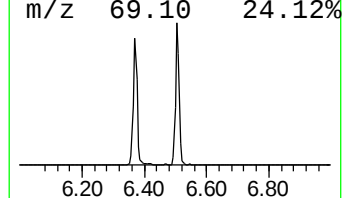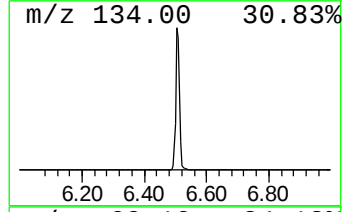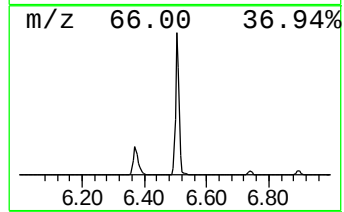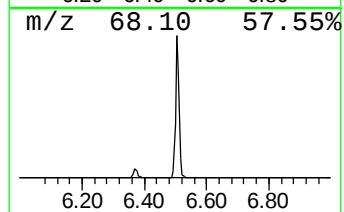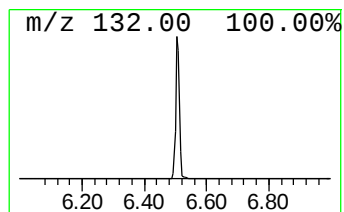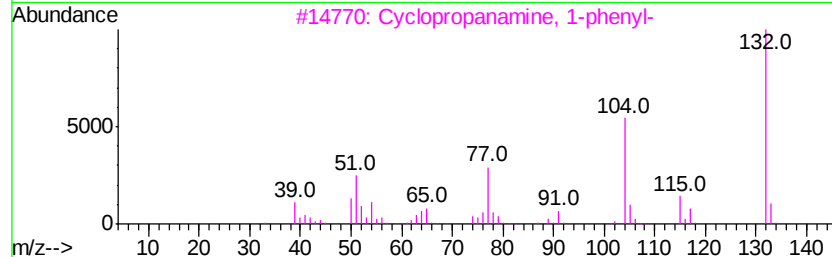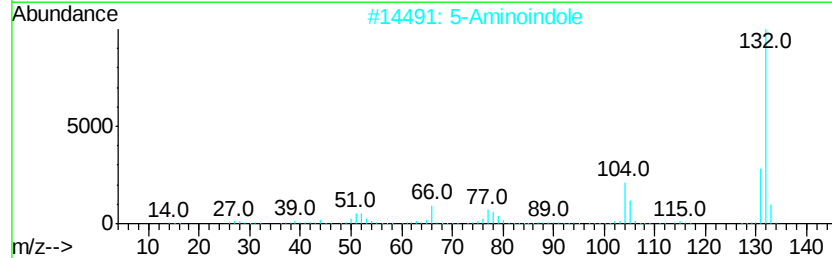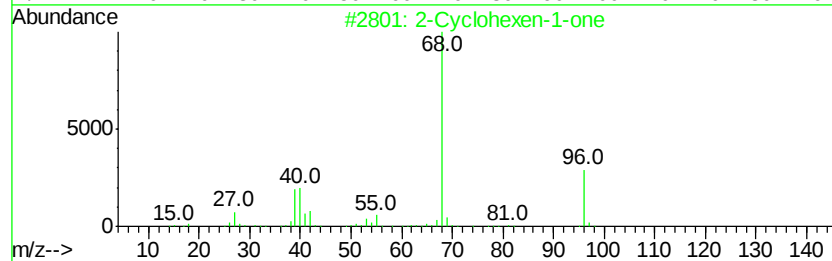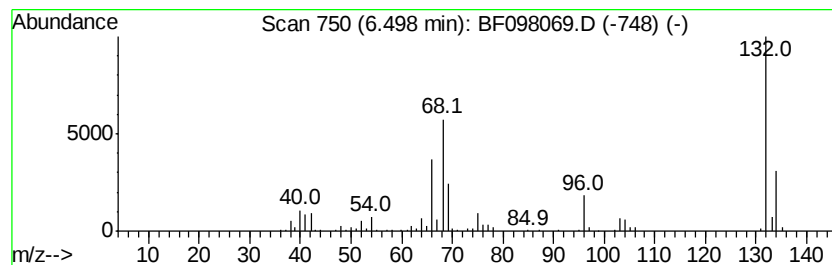

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF082817\
Data File : BF098069.D
Acq On : 28 Aug 2017 15:25
Operator : SJ/JU
Sample : I4969-04 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BU-01-082417-B

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.50	6.50	23.3	ng	749317	1	6.74	643220	20.0