


Data Path : Z:\HPCHEM1\BNA F\Data\BF082817\
 Data File : BF098057.D
 Acq On : 28 Aug 2017 9:49
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 21 15:59:04 2017

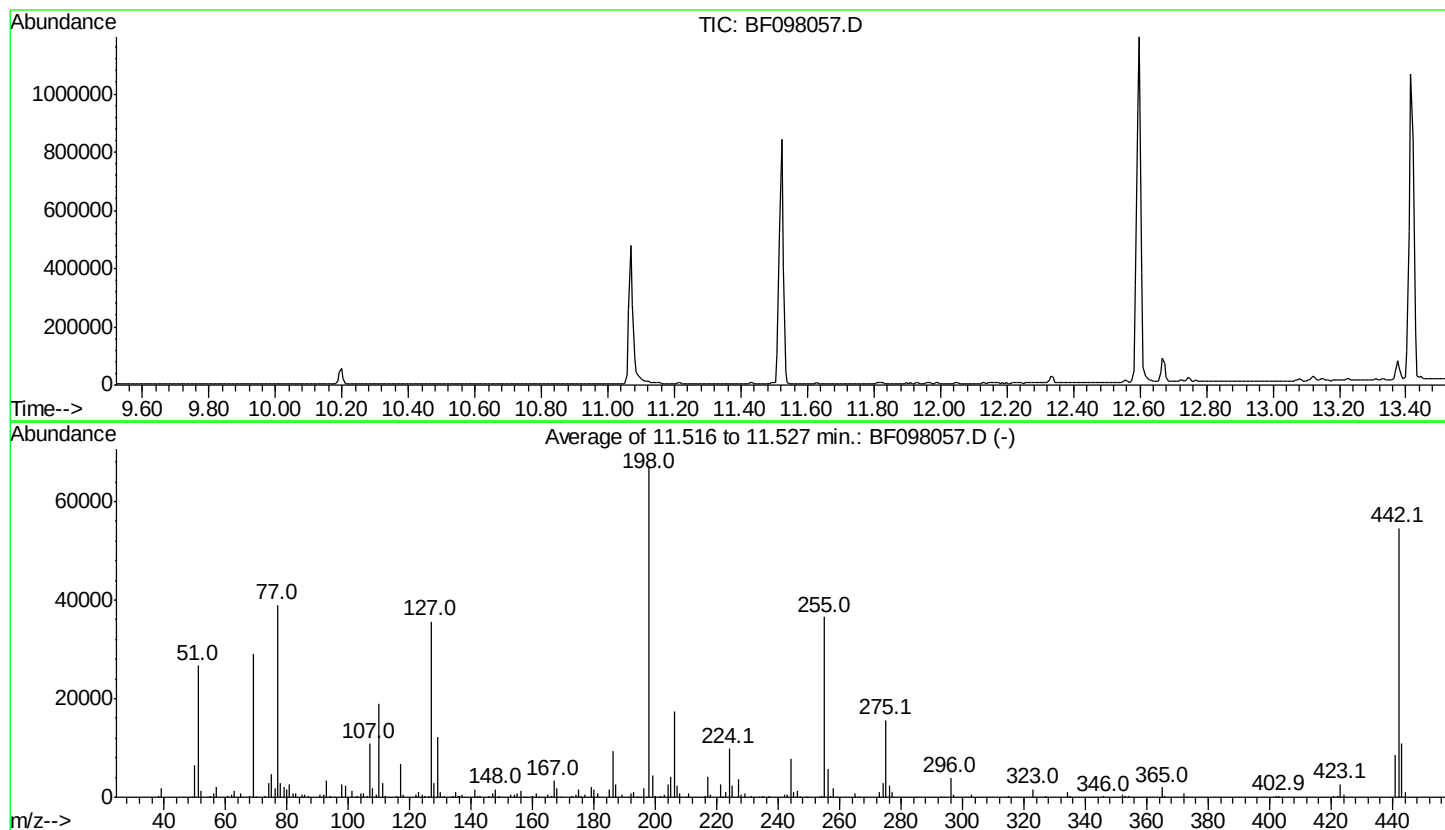

AutoFind: Scans 1603, 1604, 1605; Background Corrected with Scan 1598

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.7	26692	PASS
68	69	0.00	2	1.3	383	PASS
69	198	0.00	100	43.1	28979	PASS
70	69	0.00	2	0.4	102	PASS
127	198	10	80	52.9	35610	PASS
197	198	0.00	2	0.2	113	PASS
198	198	100	100	100.0	67253	PASS
199	198	5	9	6.7	4507	PASS
275	198	10	60	23.3	15683	PASS
365	198	1	100	3.1	2063	PASS
441	442	0.01	24	15.5	8461	PASS
442	198	50	100	81.1	54538	PASS
443	442	15	24	19.9	10874	PASS