


Data Path : Z:\HPCHEM1\BNA F\Data\BF082817\
 Data File : BF098070.D
 Acq On : 28 Aug 2017 16:12
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 21 15:59:04 2017

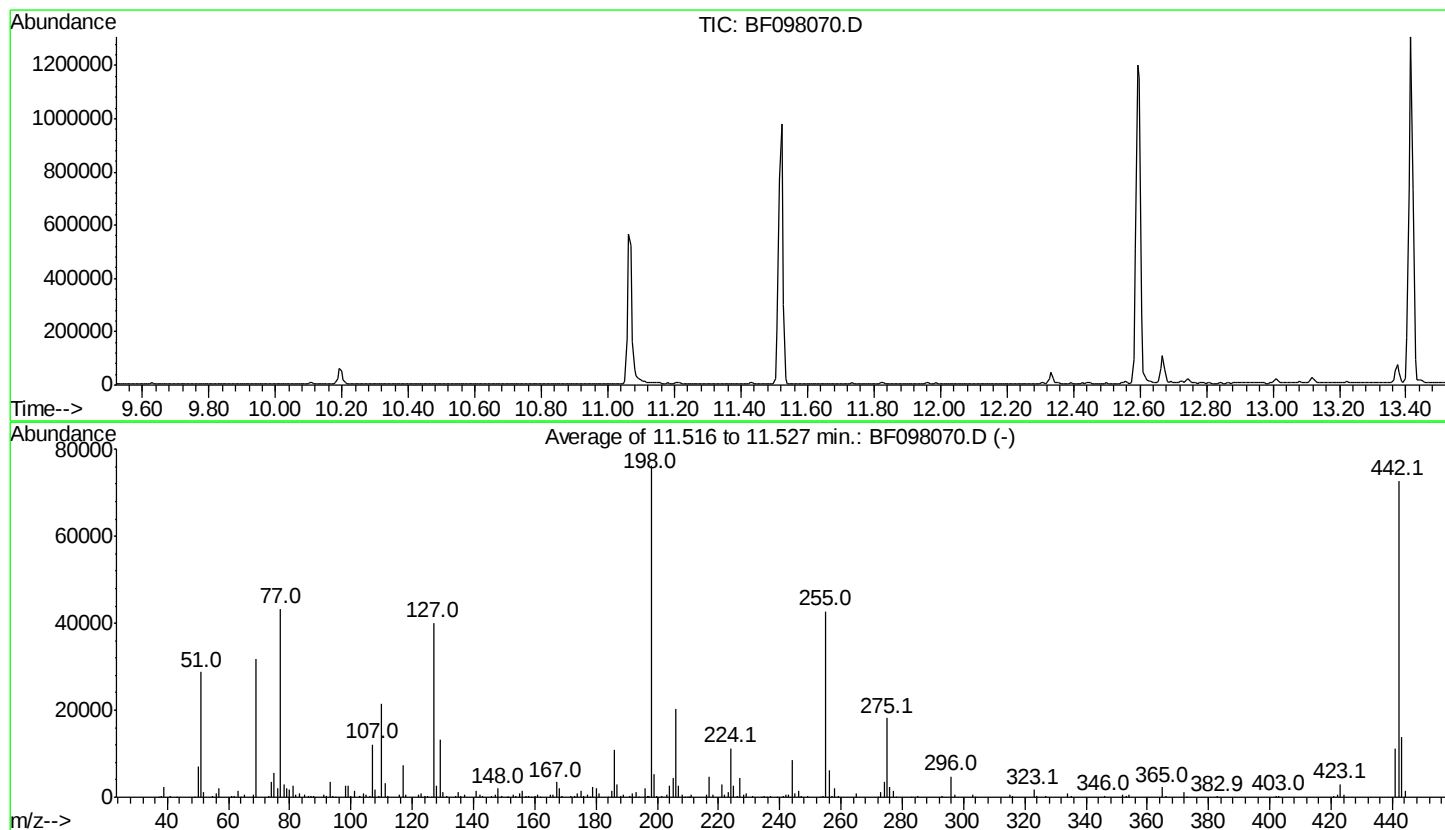

AutoFind: Scans 1603, 1604, 1605; Background Corrected with Scan 1598

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.7	28751	PASS
68	69	0.00	2	1.7	554	PASS
69	198	0.00	100	41.8	31879	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.5	40066	PASS
197	198	0.00	2	0.5	377	PASS
198	198	100	100	100.0	76248	PASS
199	198	5	9	6.9	5233	PASS
275	198	10	60	23.9	18231	PASS
365	198	1	100	3.0	2304	PASS
441	442	0.01	24	15.4	11201	PASS
442	198	50	100	95.5	72826	PASS
443	442	15	24	18.9	13768	PASS