


Data Path : Z:\HPCHEM1\BNA F\Data\BF082817\
 Data File : BF098094.D
 Acq On : 29 Aug 2017 4:43
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 21 15:59:04 2017

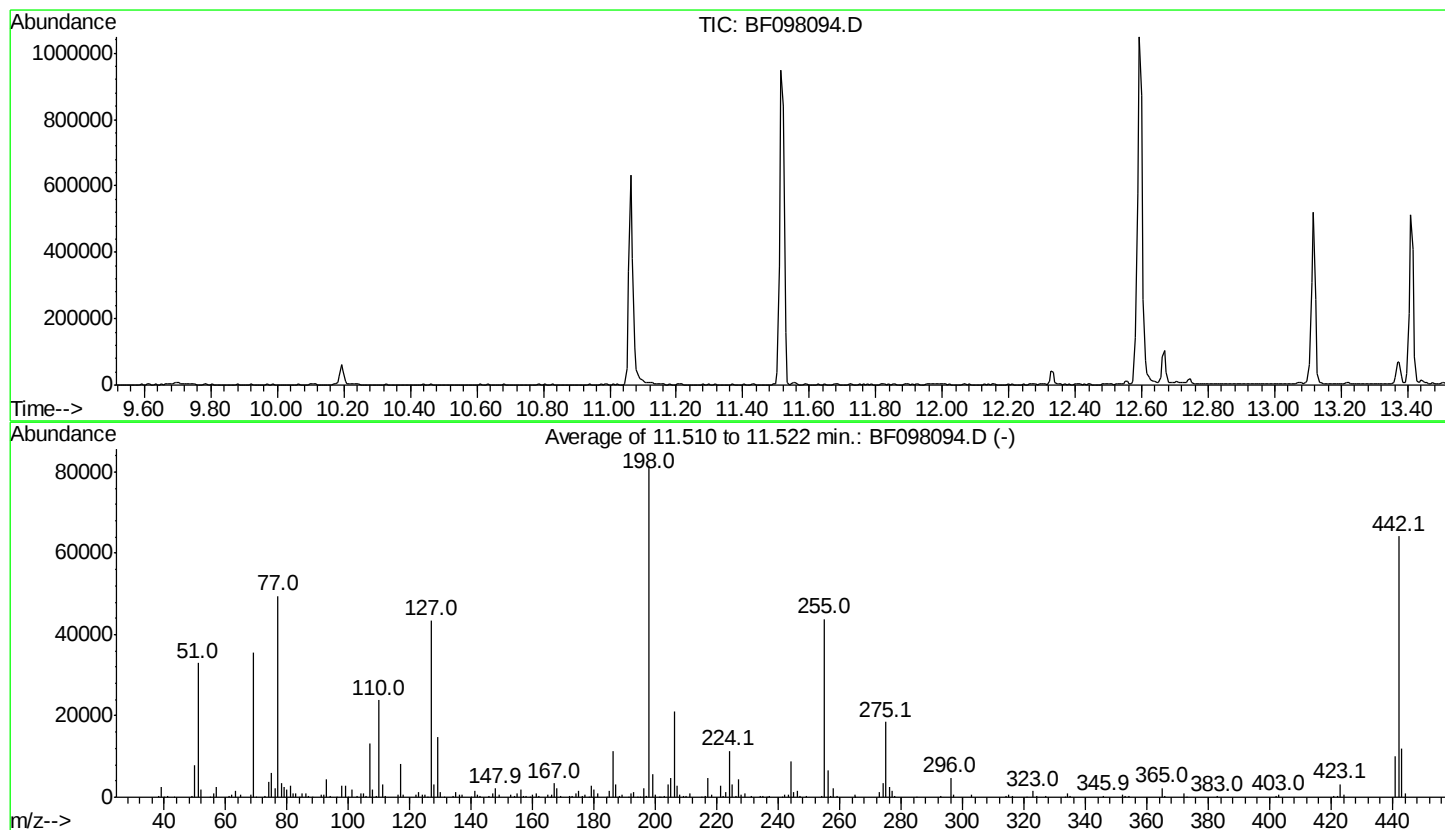

AutoFind: Scans 1602, 1603, 1604; Background Corrected with Scan 1598

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.5	32989	PASS
68	69	0.00	2	1.7	600	PASS
69	198	0.00	100	43.8	35693	PASS
70	69	0.00	2	0.3	111	PASS
127	198	10	80	53.2	43408	PASS
197	198	0.00	2	0.5	408	PASS
198	198	100	100	100.0	81533	PASS
199	198	5	9	7.1	5757	PASS
275	198	10	60	22.6	18452	PASS
365	198	1	100	2.7	2204	PASS
441	442	0.01	24	15.5	9945	PASS
442	198	50	100	78.6	64084	PASS
443	442	15	24	18.9	12090	PASS