
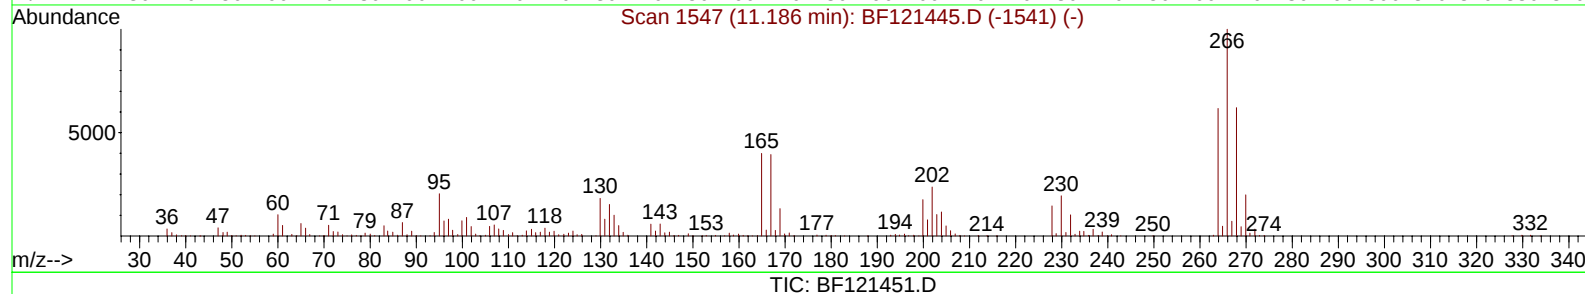
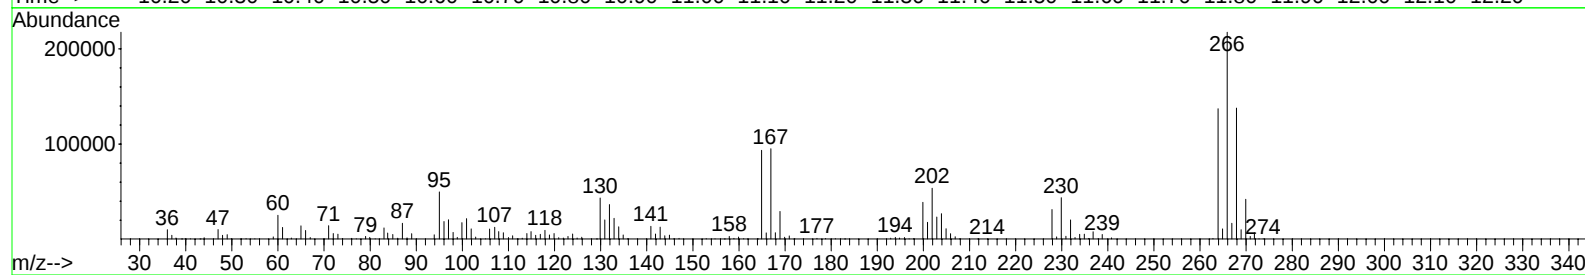


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082820\
Data File : BF121451.D
Acq On : 28 Aug 2020 10:06
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 28 18:37:25 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF082720.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 28 09:25:49 2020
Response via : Initial Calibration

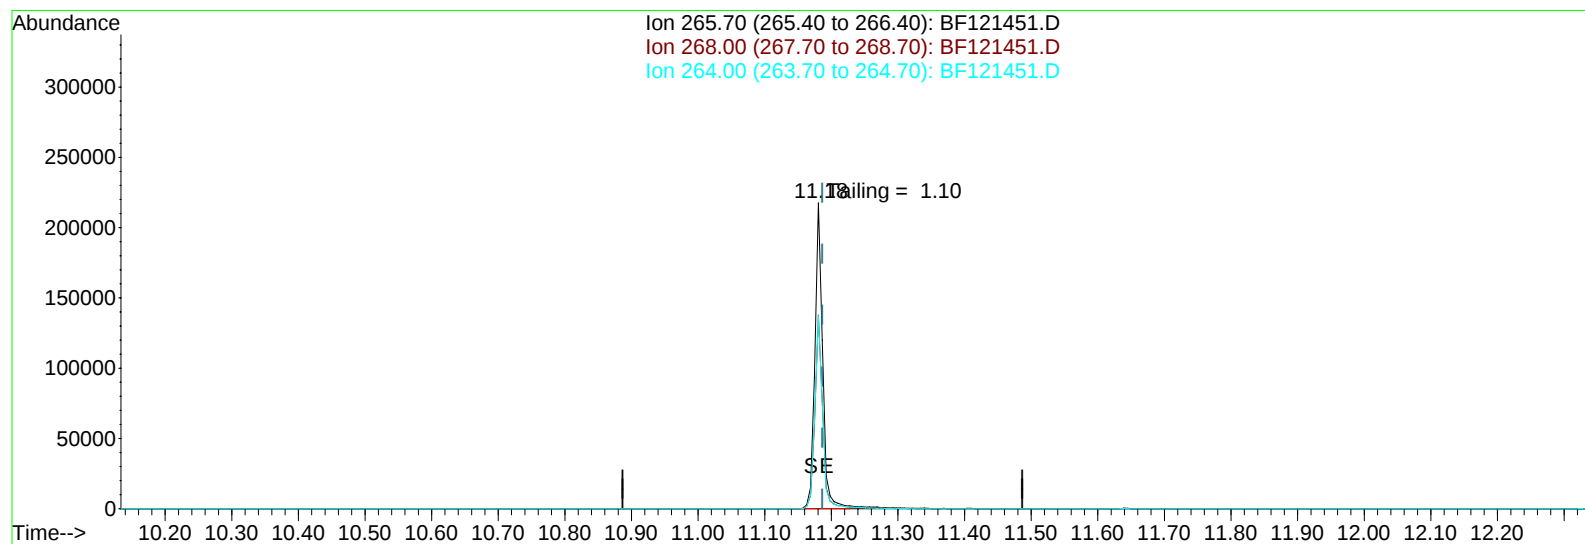

(70) Pentachlorophenol (C)




11.180min (-0.006) 122167.19ng

response 180931

Ion	Exp%	Act%
265.70	100	100
268.00	62.10	63.34
264.00	61.70	63.05
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082820\
Data File : BF121451.D
Acq On : 28 Aug 2020 10:06
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 28 18:37:25 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF082720.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 28 09:25:49 2020
Response via : Initial Calibration

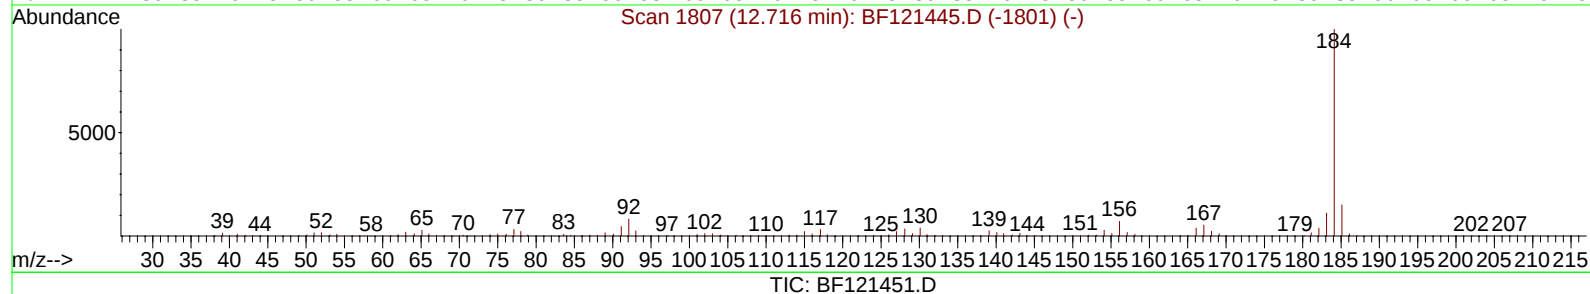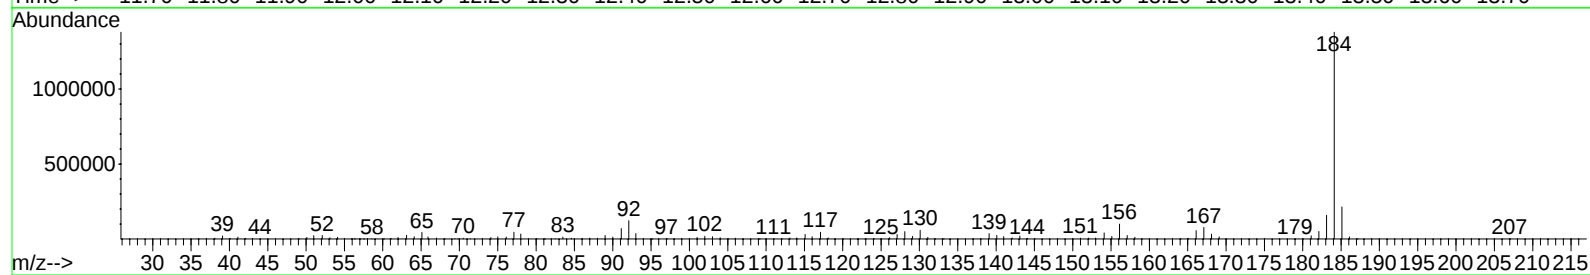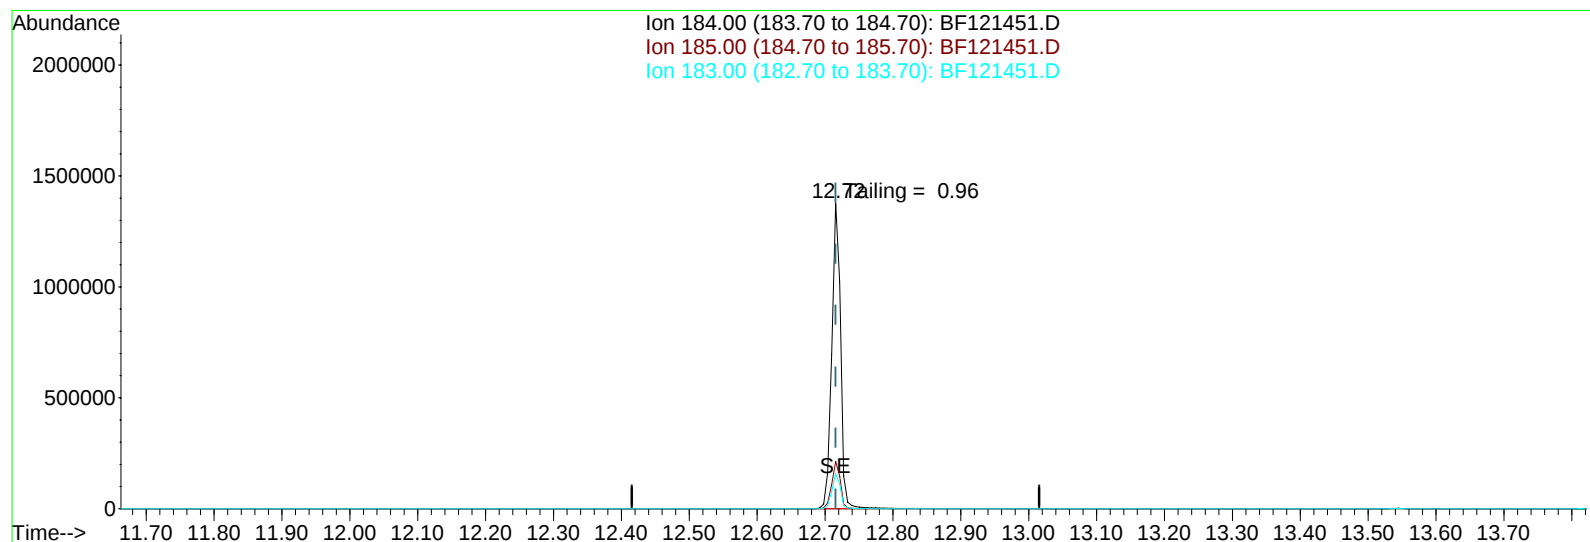

(77) Benzidine

12.716min (+0.000) 60740.44ng

response 1245226

Ion	Exp%	Act%
184.00	100	100
185.00	15.10	15.49
183.00	11.10	11.46
0.00	0.00	0.00