
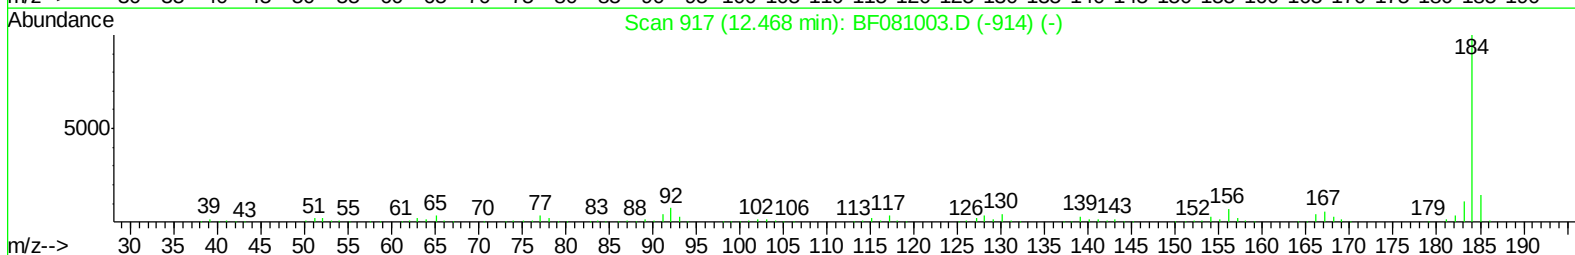
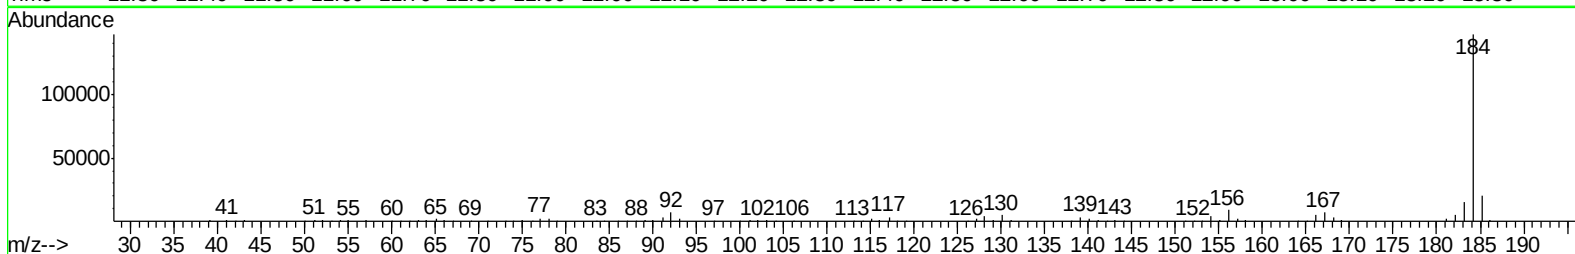


Data Path : Z:\HPCHEM1\BNA F\Data\BF082915\
Data File : BF081268.D
Acq On : 29 Aug 2015 11:45
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 31 05:42:25 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 31 01:11:18 2015
Response via : Initial Calibration

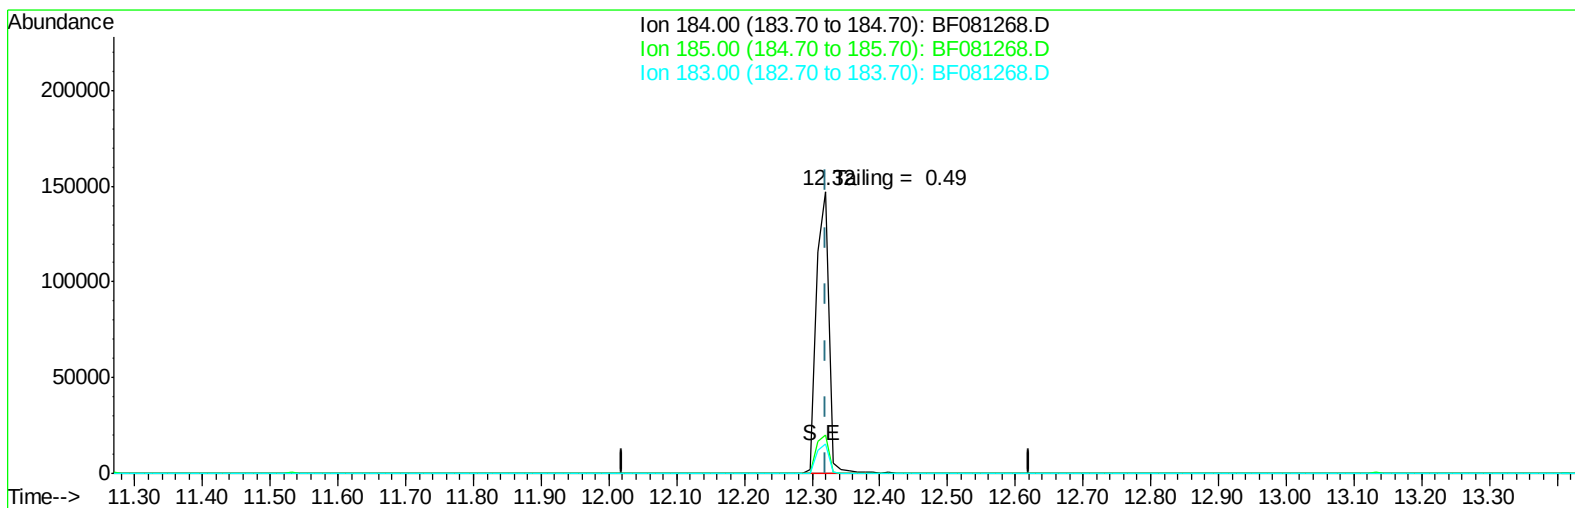

TIC: BF081268.D

(76) Benzidine




12.321min (-0.000) 0.00ng

response 188455

Ion	Exp%	Act%
184.00	100	100
185.00	15.00	13.81
183.00	11.10	10.47
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF082915\
Data File : BF081268.D
Acq On : 29 Aug 2015 11:45
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 31 05:42:25 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 31 01:11:18 2015
Response via : Initial Calibration

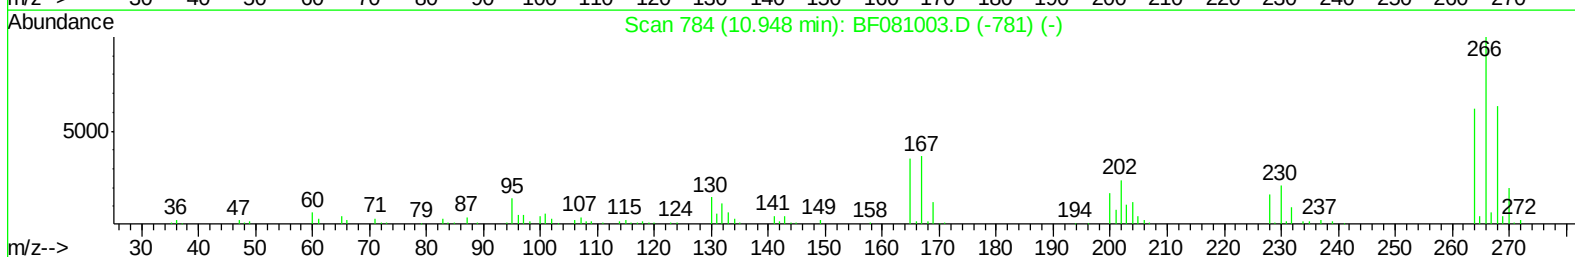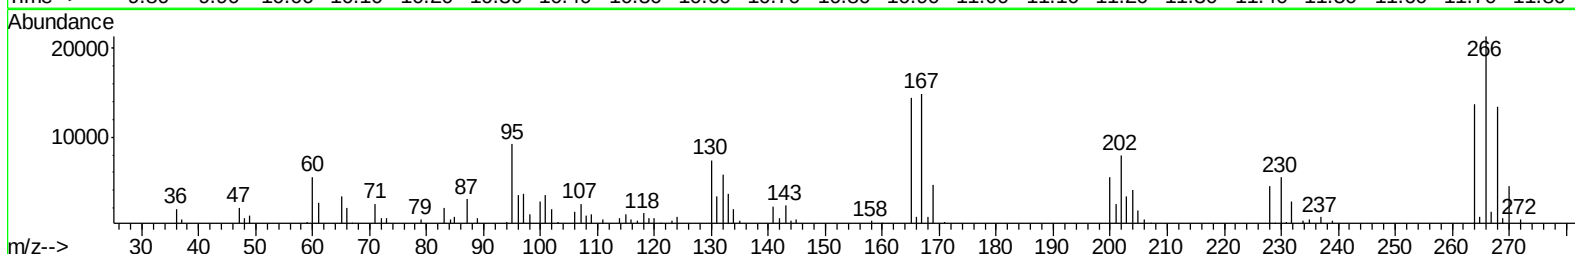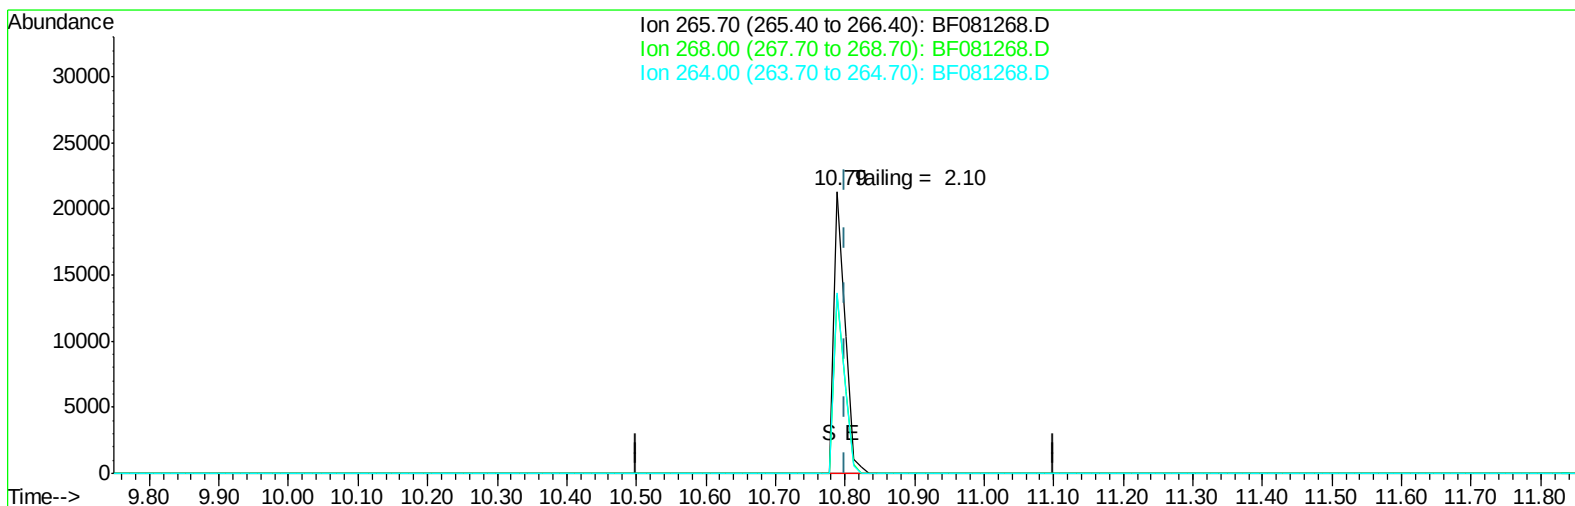

TIC: BF081268.D

(69) Pentachlorophenol (C)

10.789min (-0.011) 0.00ng

response 22781

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	63.00
264.00	63.20	64.07
0.00	0.00	0.00