


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF082915\
 Data File : BF081285.D
 Acq On : 29 Aug 2015 22:28
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 31 13:41:31 2015

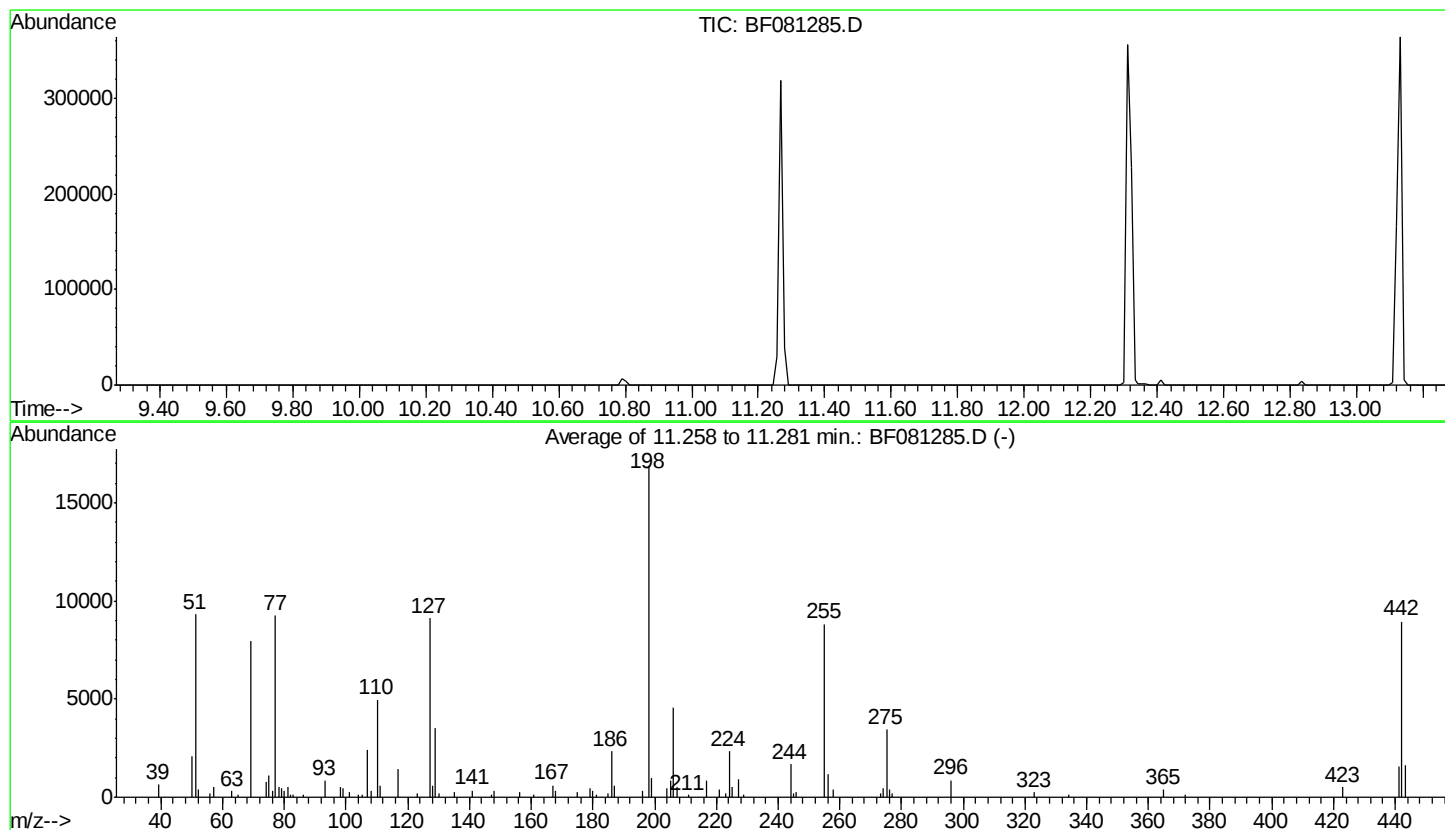

AutoFind: Scans 833, 834, 835; Background Corrected with Scan 830

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.2	9325	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	47.1	7954	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.9	9112	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	16900	PASS
199	198	5	9	5.6	950	PASS
275	198	10	60	20.4	3455	PASS
365	198	1	100	2.2	378	PASS
441	442	0.01	24	17.3	1545	PASS
442	198	50	100	53.0	8955	PASS
443	442	15	24	18.0	1613	PASS