
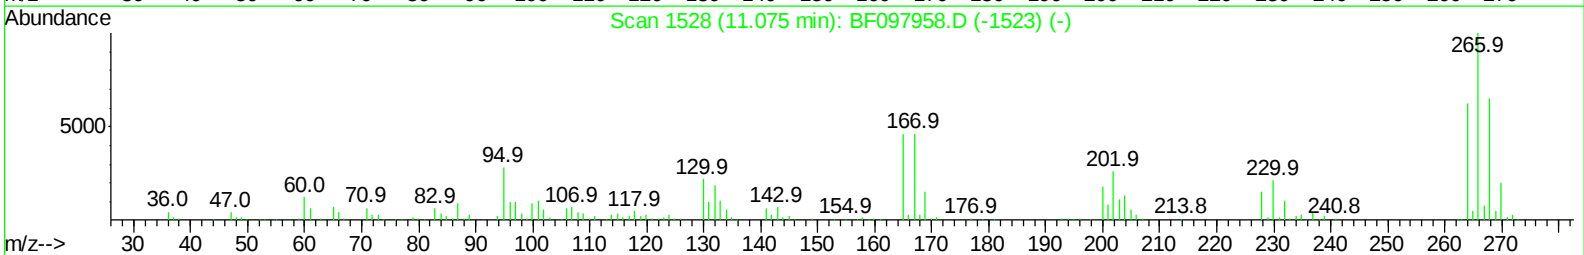
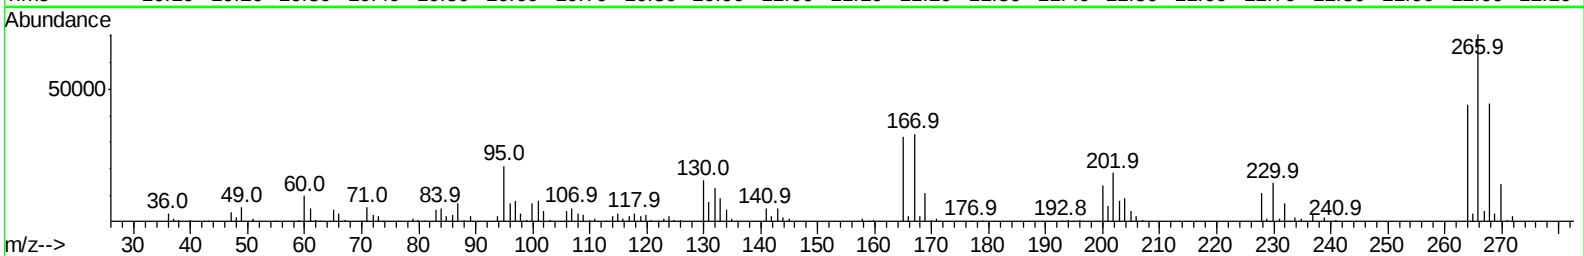


```
Data Path : Z:\HPCHEM1\BNA F\DATA\BF082917\  
Data File : BF098107.D  
Acq On    : 29 Aug 2017  13:27  
Operator  : SJ/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1      Sample Multiplier: 1
```

Quant Time: Aug 30 08:50:33 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 21 15:59:04 2017
Response via : Initial Calibration



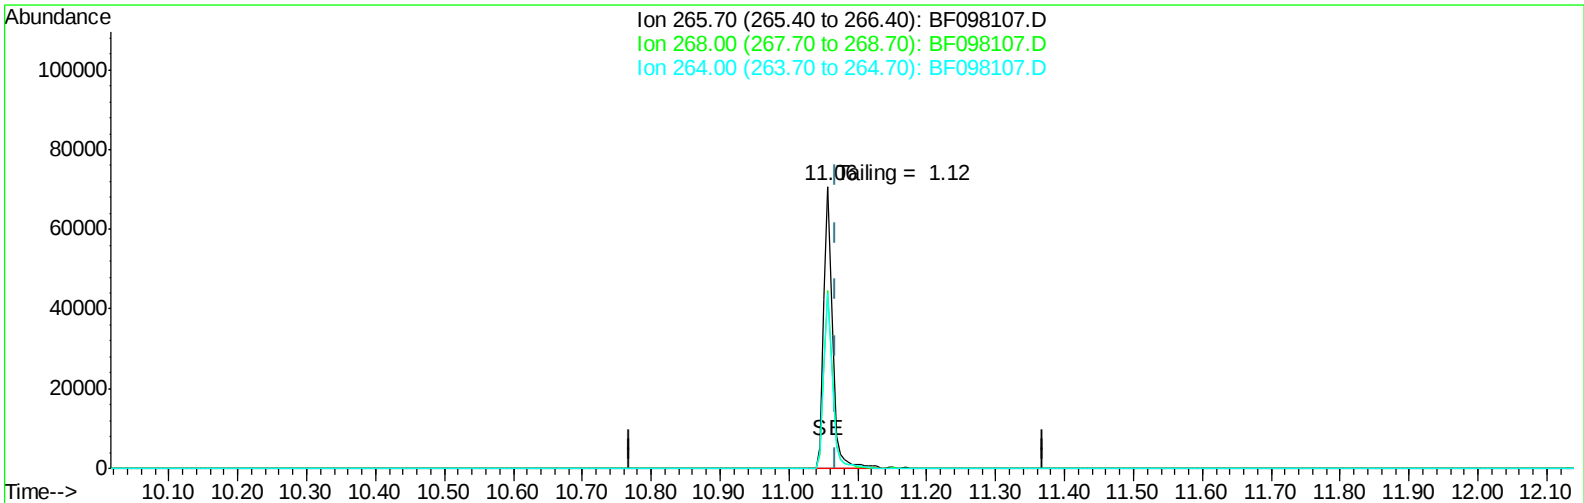


TIC: BF098107.D

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.26
264.00	64.60	62.50
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF082917\
Data File : BF098107.D
Acq On : 29 Aug 2017 13:27
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 30 08:50:33 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 21 15:59:04 2017
Response via : Initial Calibration

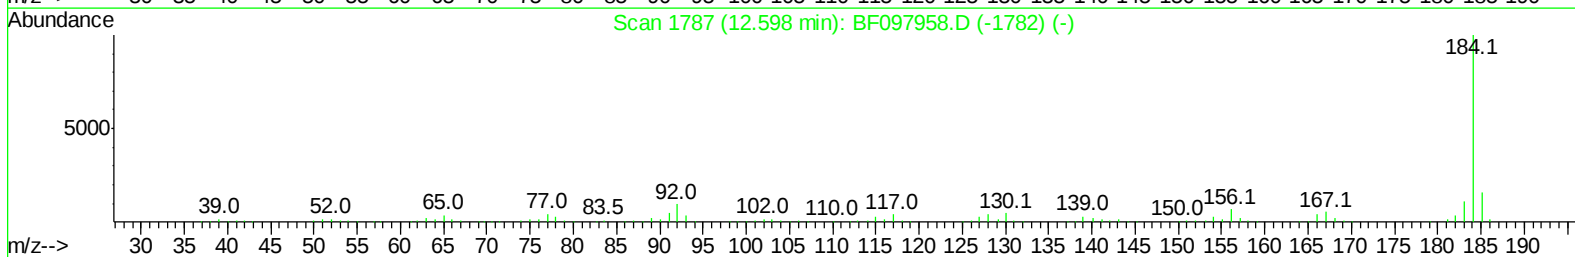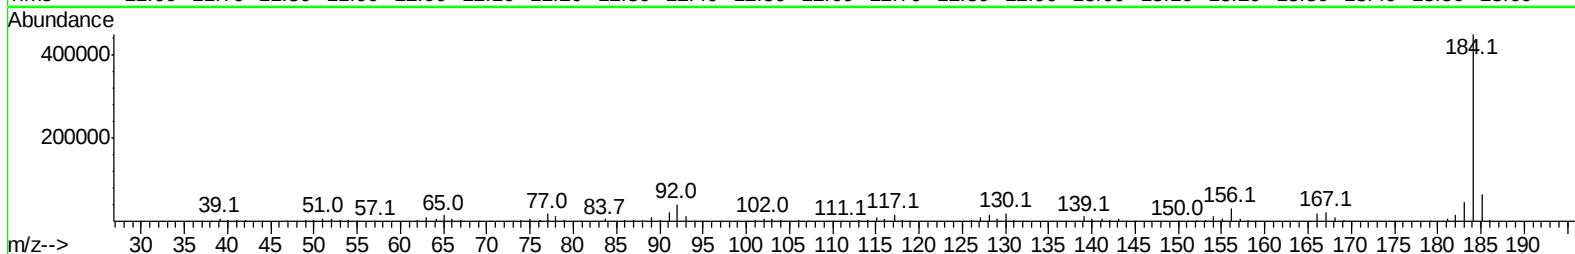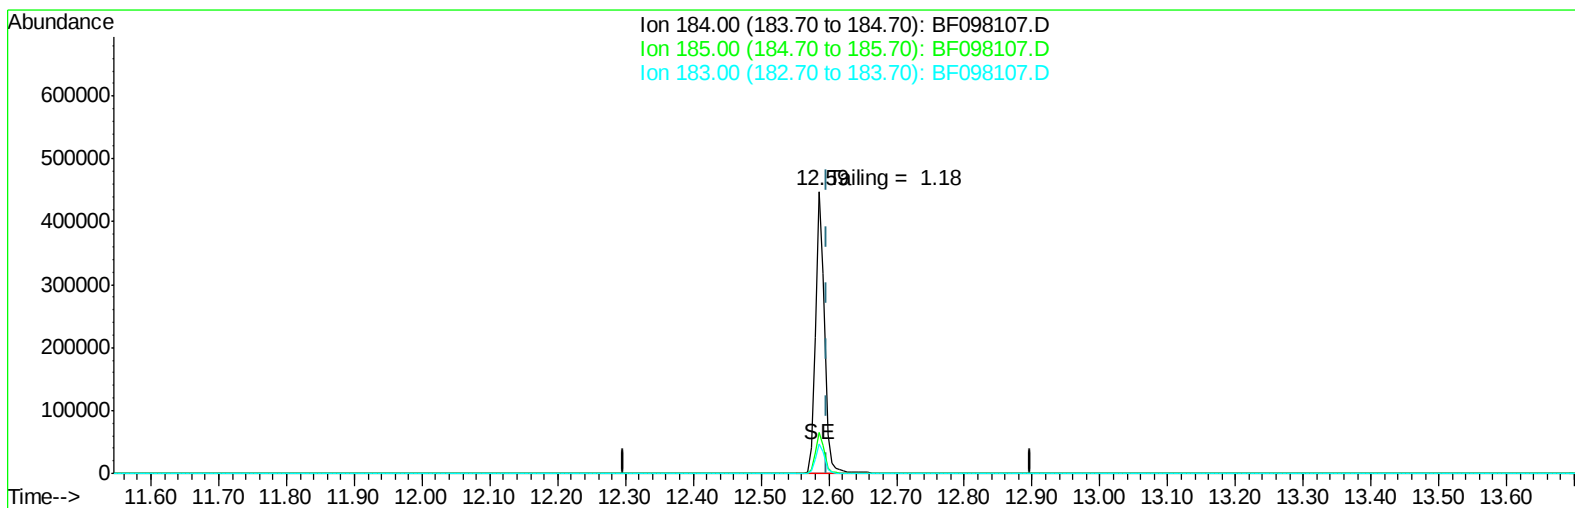

TIC: BF098107.D

(76) Benzidine

12.586min (-0.012) 21551.85ng

response 400663

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.64#
183.00	12.20	10.55
0.00	0.00	0.00