
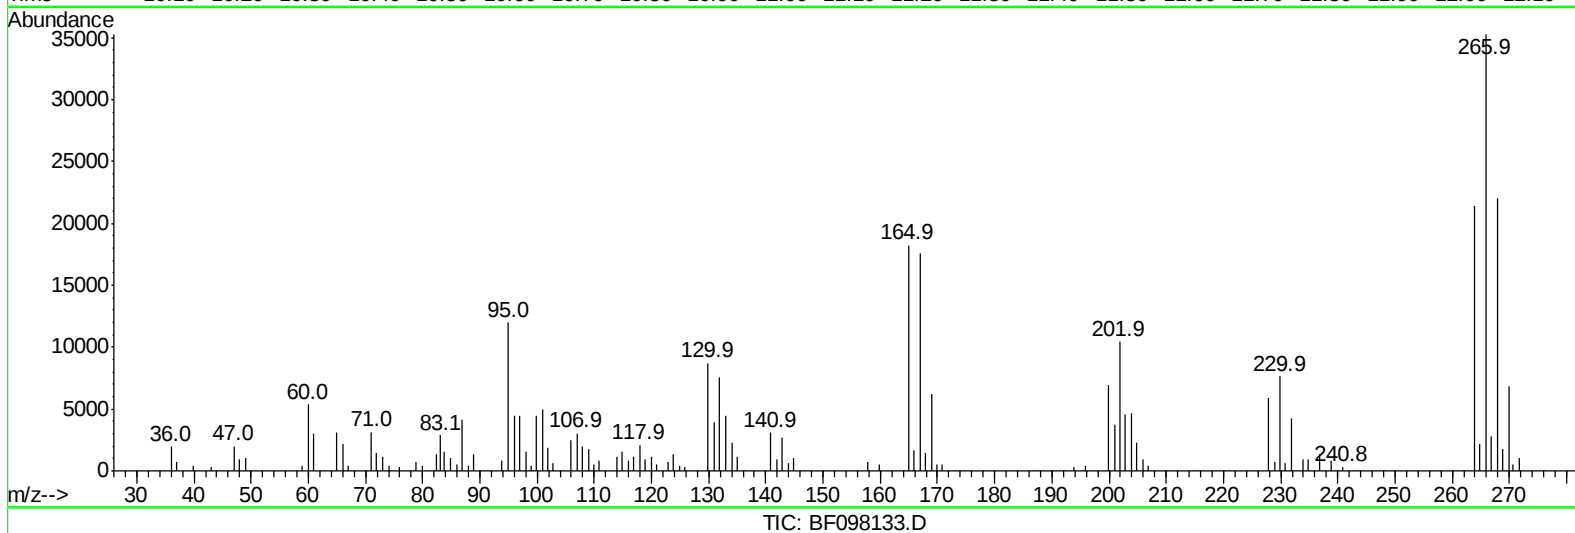


Data Path : Z:\HPCHEM1\BNA F\DATA\BF082917\
Data File : BF098133.D
Acq On : 30 Aug 2017 2:10
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 30 08:52:45 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 21 15:59:04 2017
Response via : Initial Calibration

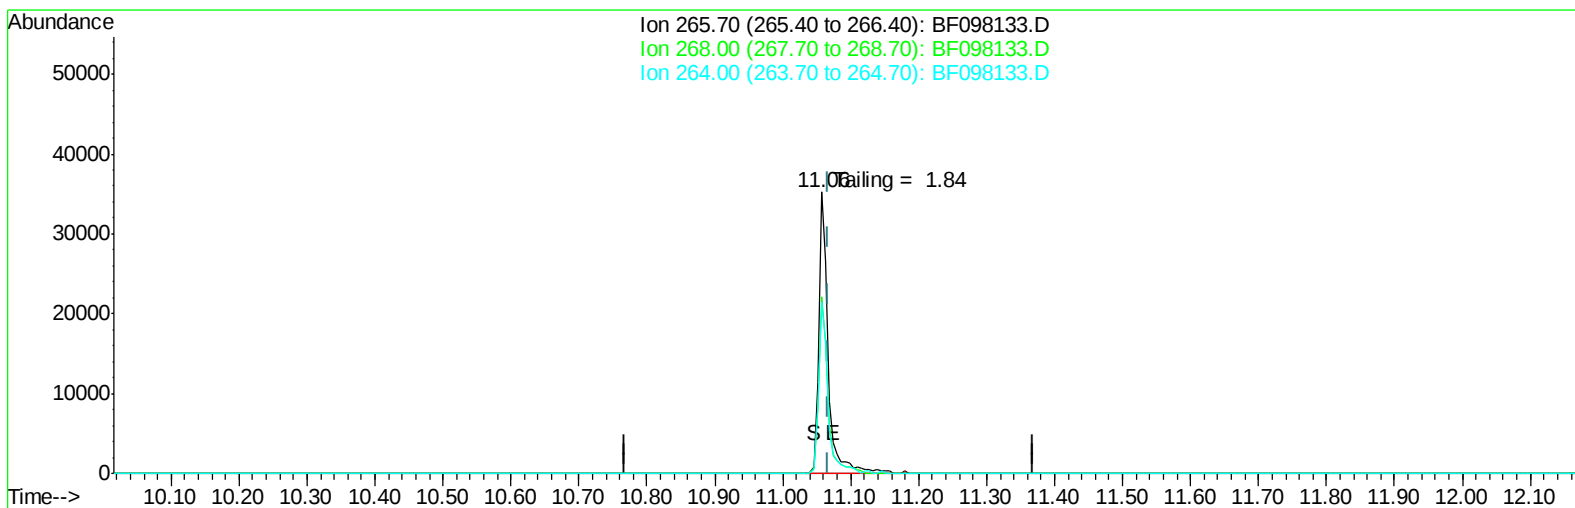

(69) Pentachlorophenol (C)



11.057min (-0.012) 46132.34ng

response 34733

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.60
264.00	64.60	60.85
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF082917\
Data File : BF098133.D
Acq On : 30 Aug 2017 2:10
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 30 08:52:45 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 21 15:59:04 2017
Response via : Initial Calibration

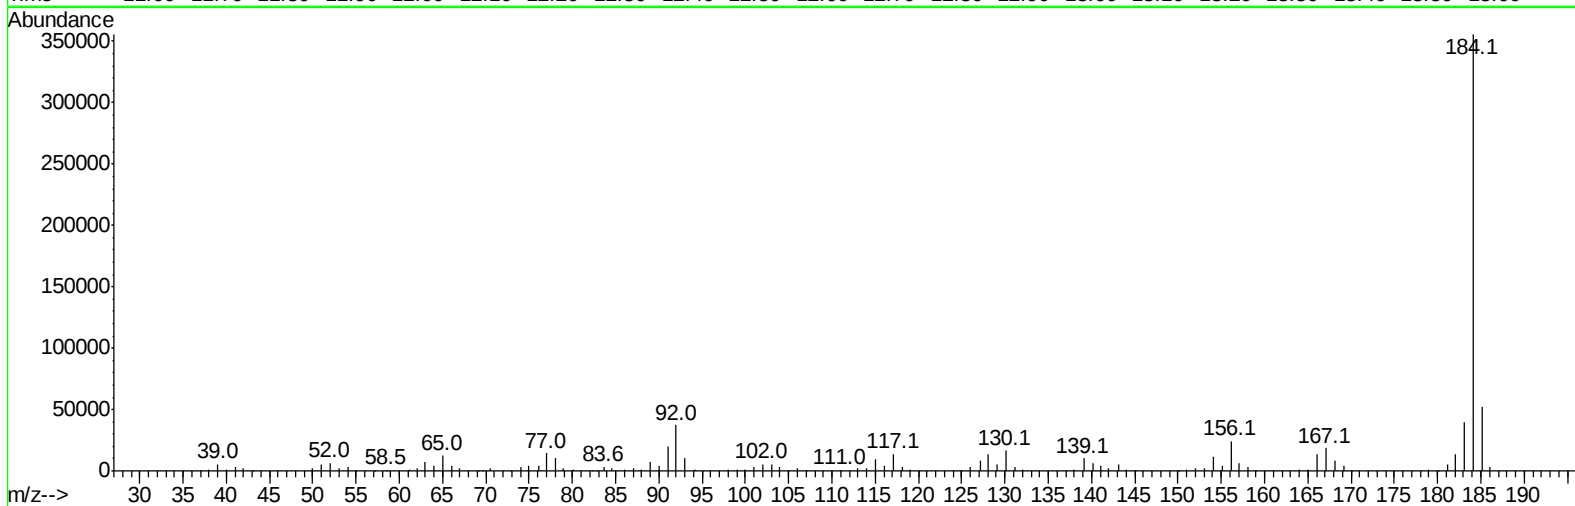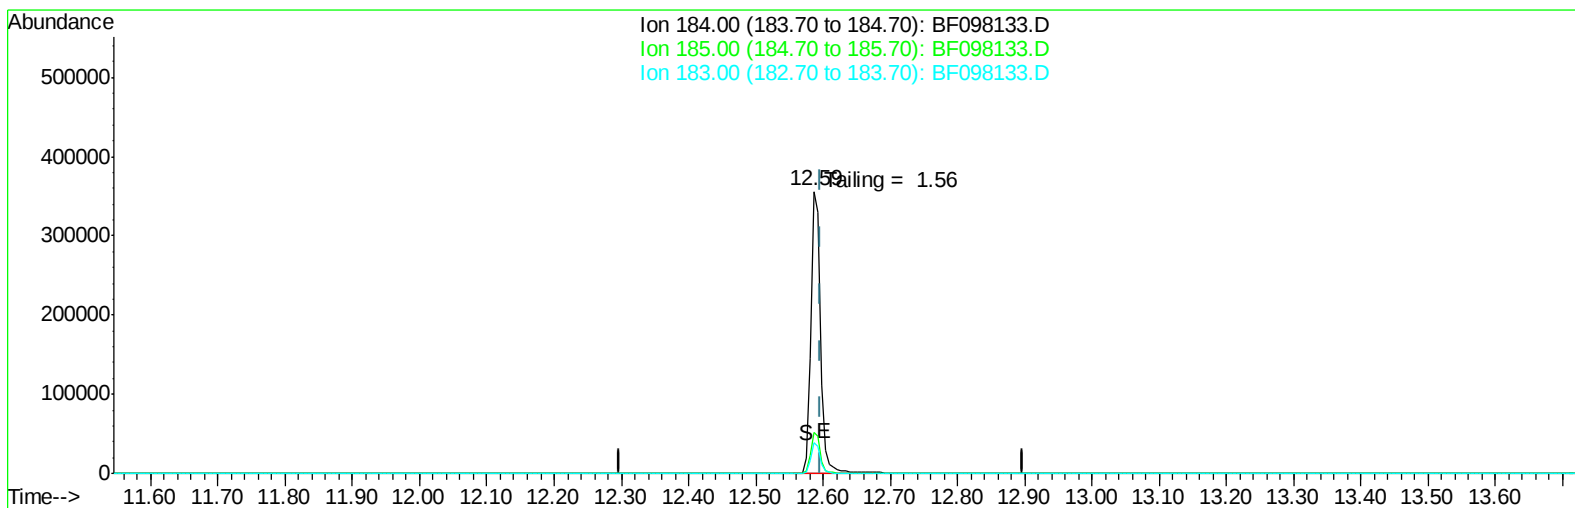

TIC: BF098133.D

(76) Benzidine

12.586min (-0.012) 0.00ng m

response 364037

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.66#
183.00	12.20	11.04
0.00	0.00	0.00