

Data Path : Z:\HPCHEM1\BNA F\DATA\BF082917\
 Data File : BF098135.D
 Acq On : 30 Aug 2017 3:52
 Operator : SJ/JU
 Sample : I4990-01 10X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 B-1

Quant Time: Aug 30 07:54:26 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 21 15:59:04 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.73	152	122299	20.00	ng	-0.02
21) Naphthalene-d8	8.02	136	474049	20.00	ng	-0.02
38) Acenaphthene-d10	9.77	164	189741	20.00	ng	-0.02
63) Phenanthrene-d10	11.25	188	308802	20.00	ng	-0.01
75) Chrysene-d12	13.89	240	268387	20.00	ng	-0.01
86) Perylene-d12	15.31	264	206625	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.33	112	95527	11.88	ng	-0.02
7) Phenol-d6	6.36	99	148921	13.63	ng	-0.02
23) Nitrobenzene-d5	7.29	82	88466	10.14	ng	-0.03
41) 2,4,6-Tribromophenol	10.56	330	11948	7.26	ng	-0.02
44) 2-Fluorobiphenyl	9.09	172	144579	11.20	ng	-0.02
78) Terphenyl-d14	12.83	244	93289	7.25	ng	-0.02


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF082917\
Data File : BF098135.D
Acq On : 30 Aug 2017 3:52
Operator : SJ/JU
Sample : I4990-01 10X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
B-1

Quant Time: Aug 30 07:54:26 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 21 15:59:04 2017
Response via : Initial Calibration

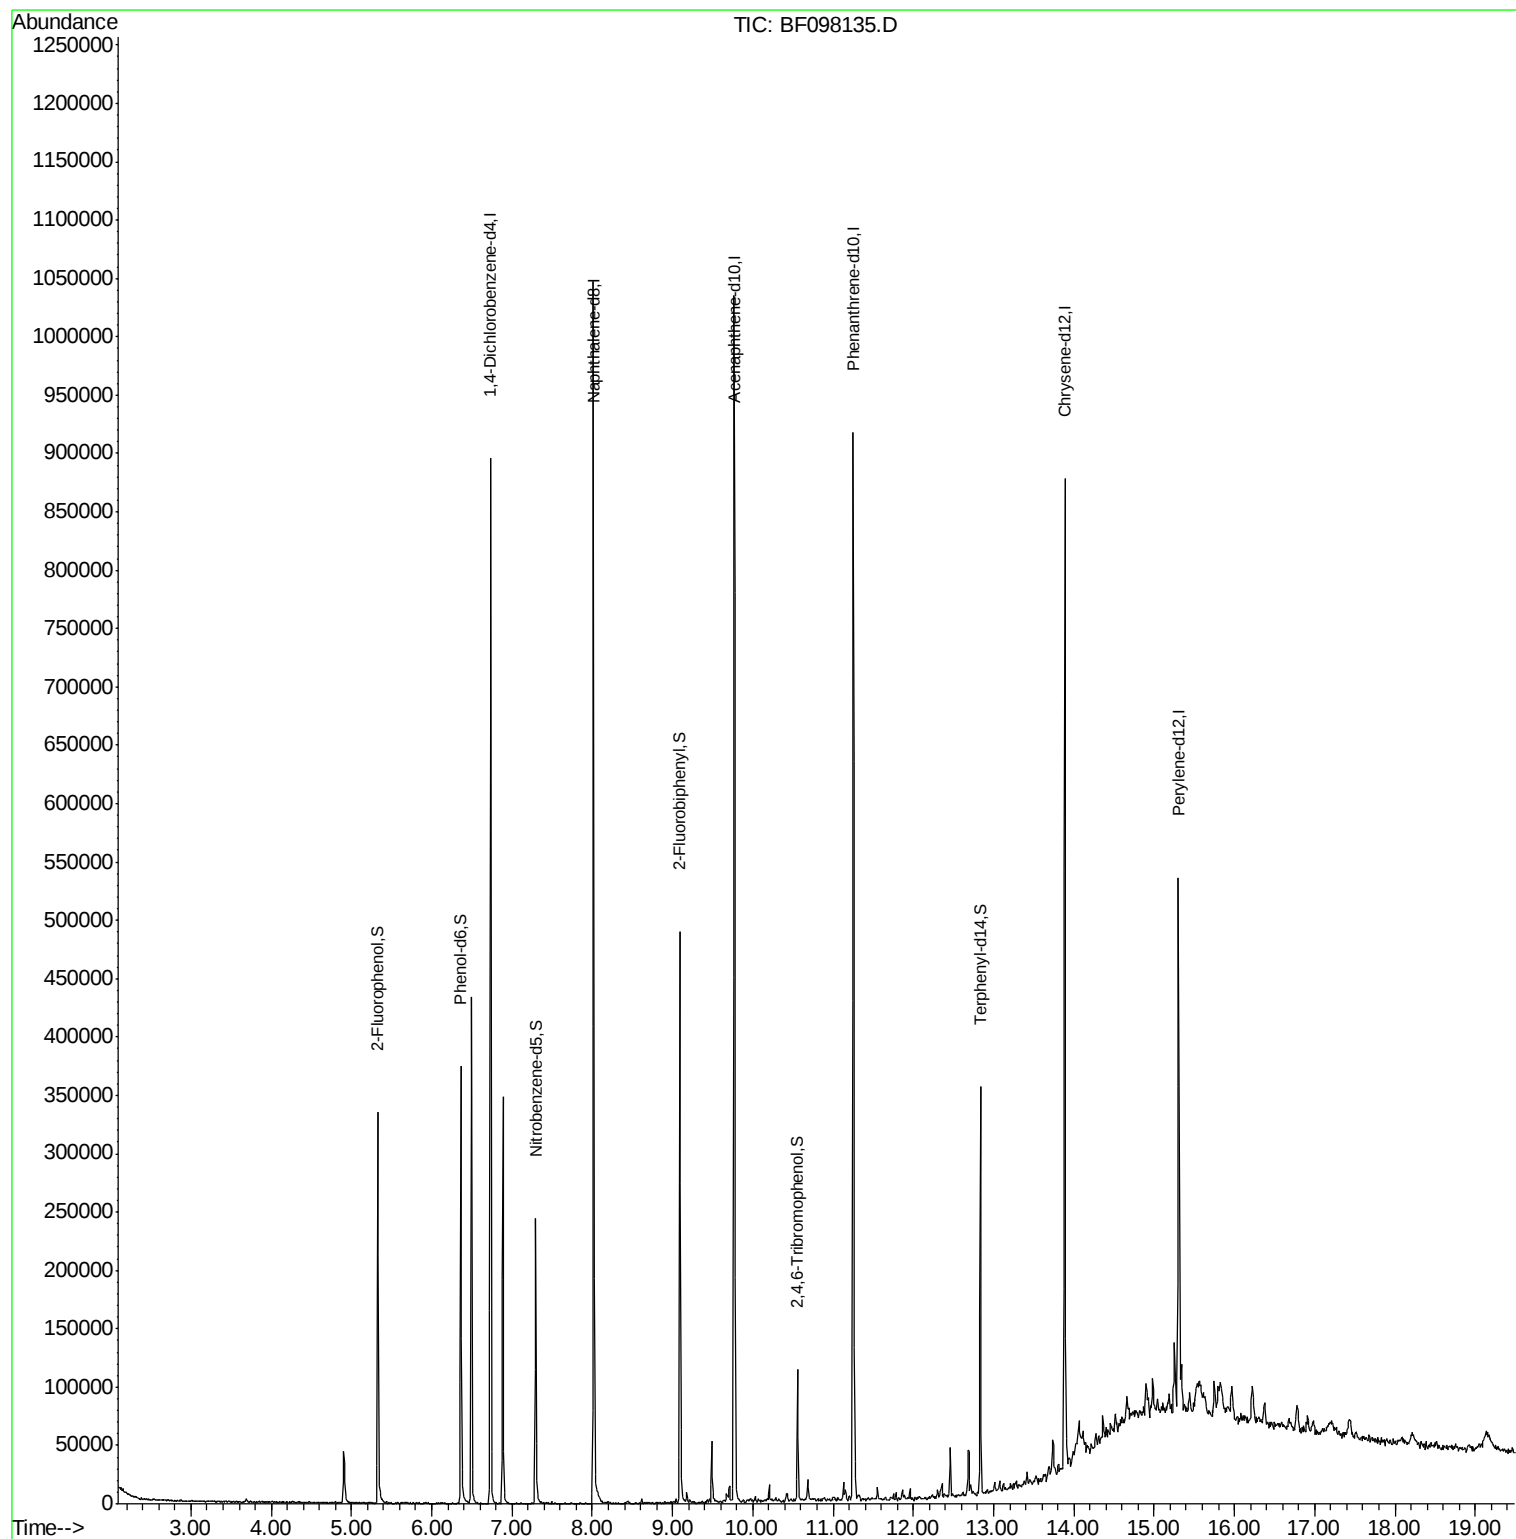







#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.73 min Scan# 790
Delta R.T. -0.02 min
Lab File: BF098135.D
Acq: 30 Aug 2017 3:52

Instrument :
BNA_F
ClientSampleId :
B-1




Tot Ion:152 Resp: 122299
Ion Ratio Lower Upper
152 100
150 158.3 126.2 189.2
115 65.3 52.2 78.2

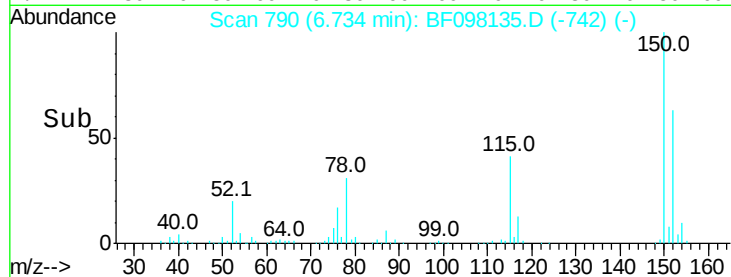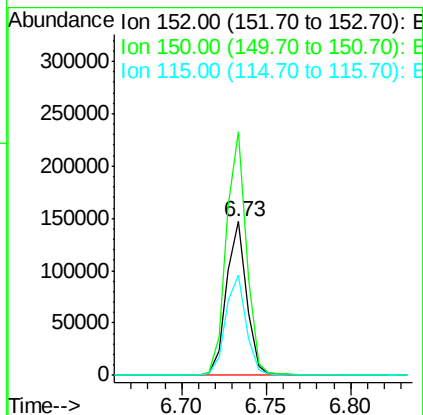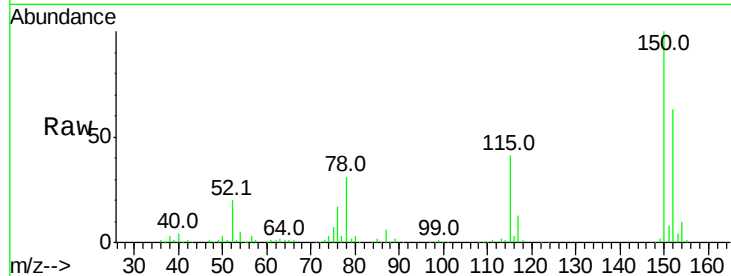


#5

2-Fluorophenol
Concen: 11.881 ng
RT: 5.33 min Scan# 551
Delta R.T. -0.02 min
Lab File: BF098135.D
Acq: 30 Aug 2017 3:52

Tgt Ion:112 Resp: 95527
Ion Ratio Lower Upper
112 100
64 59.6 46.0 69.0
63 30.8 23.4 35.0

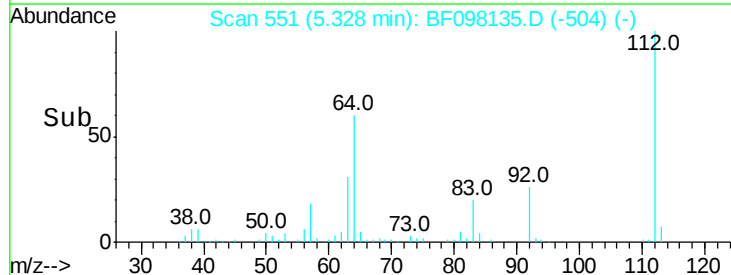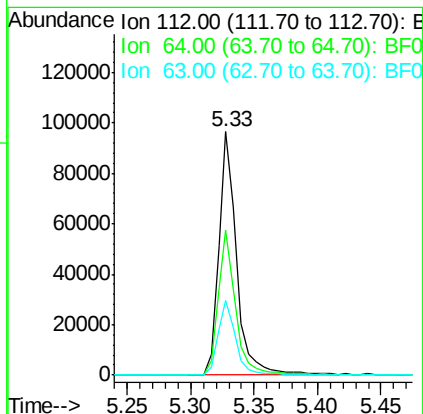

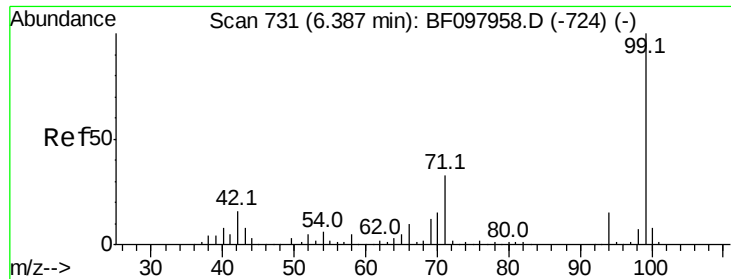

#7

Phenol-d6

Concen: 13.632 ng

RT: 6.36 min Scan# 727

Delta R.T. -0.02 min

Lab File: BF098135.D

Acq: 30 Aug 2017 3:52

Instrument :

BNA_F

ClientSampleId :

B-1


Tot Ion: 99 Resp: 148921

Ion Ratio Lower Upper

99 100

42 15.3 13.5 20.3




71 29.7 24.5 36.7

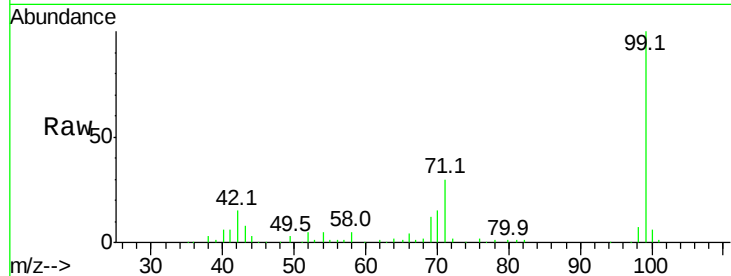

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

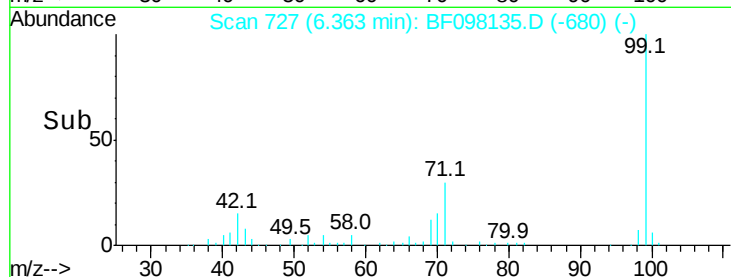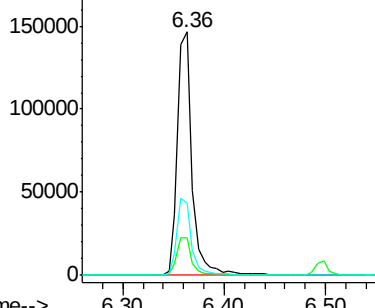

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.02 min Scan# 1008

Delta R.T. -0.02 min

Lab File: BF098135.D

Acq: 30 Aug 2017 3:52

Tgt Ion: 136 Resp: 474049


Ion Ratio Lower Upper

136 100

137 11.4 8.5 12.7

54 8.2 4.9 7.3#

68 7.7 4.1 6.1#






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



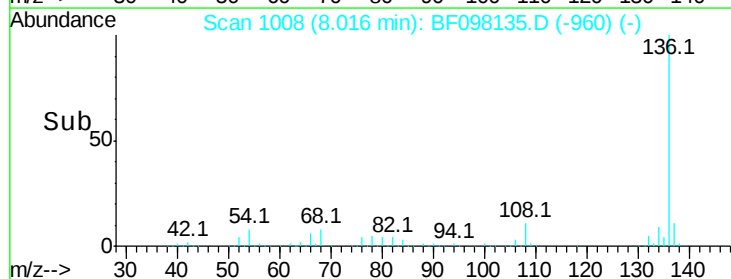
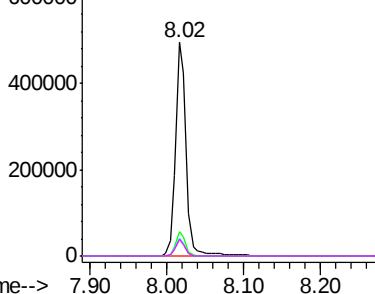


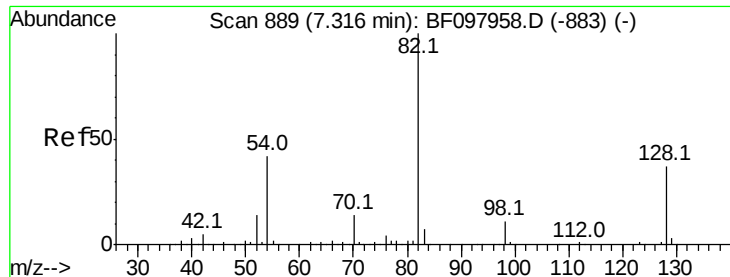

#23
Nitrobenzene-d5
Concen: 10.138 ng
RT: 7.29 min Scan# 885
Delta R.T. -0.03 min
Lab File: BF098135.D
Acq: 30 Aug 2017 3:52




Instrument :
BNA_F
ClientSampleId :
B-1

Tot Ion	82	Resp	88466
Ion Ratio	Lower	Upper	
82	100		
128	36.2	34.0	51.0
54	42.9	42.2	63.2

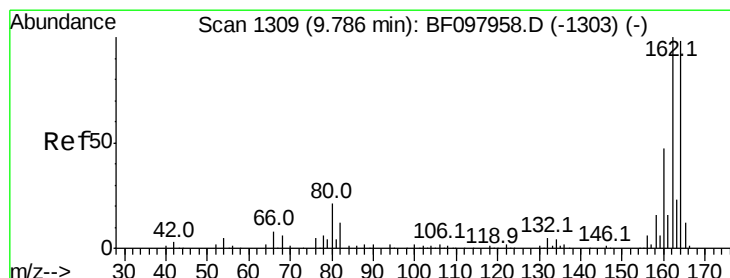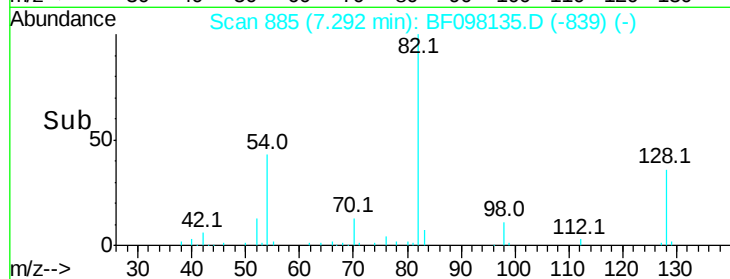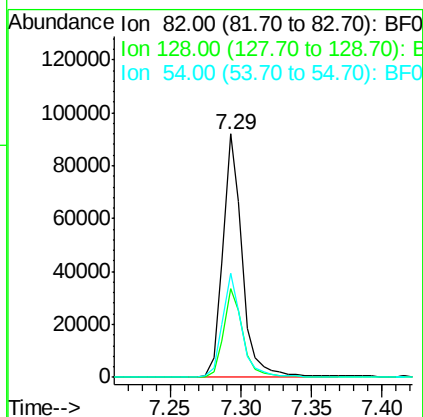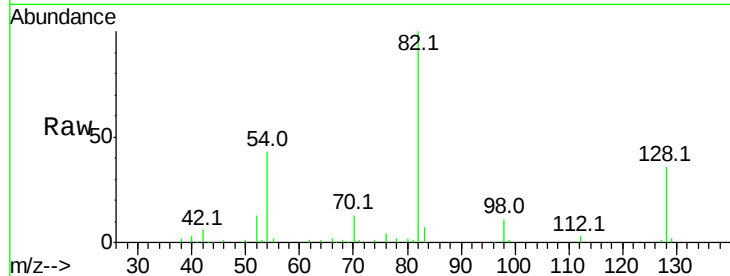

#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.77 min Scan# 1306
Delta R.T. -0.02 min
Lab File: BF098135.D
Acq: 30 Aug 2017 3:52

Tgt Ion	164	Resp	189741
Ion Ratio	Lower	Upper	
164	100		
162	100.1	82.6	123.8
160	46.7	36.2	54.2

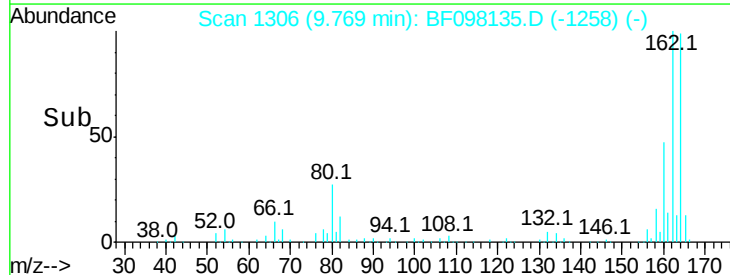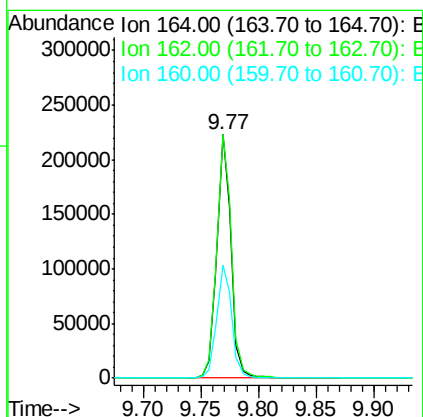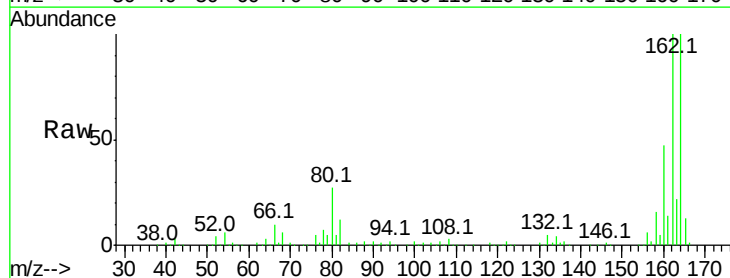







#41
 2,4,6-Tribromophenol
 Concen: 7.257 ng
 RT: 10.56 min Scan# 1440
 Delta R.T. -0.02 min
 Lab File: BF098135.D
 Acq: 30 Aug 2017 3:52

Instrument :
 BNA_F
 ClientSampleId :
 B-1

Tot Ion	Ratio	Lower	Upper
330	100		
332	97.1	76.6	115.0
141	43.0	31.4	47.2




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

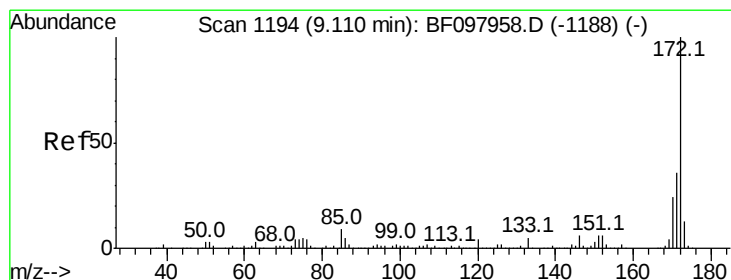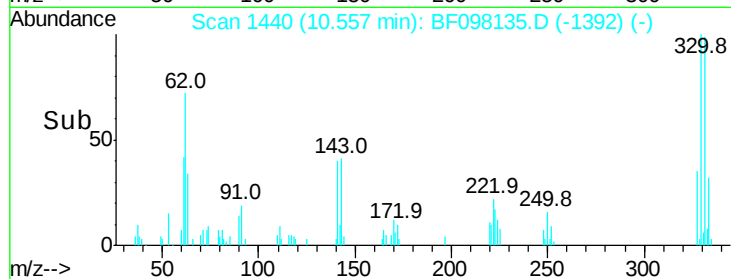
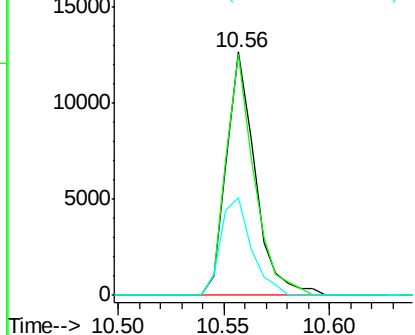



#44
 2-Fluorobiphenyl
 Concen: 11.195 ng
 RT: 9.09 min Scan# 1191
 Delta R.T. -0.02 min
 Lab File: BF098135.D
 Acq: 30 Aug 2017 3:52

Tgt Ion	Ratio	Lower	Upper
172	100		
171	34.4	29.6	44.4
170	23.4	19.8	29.8

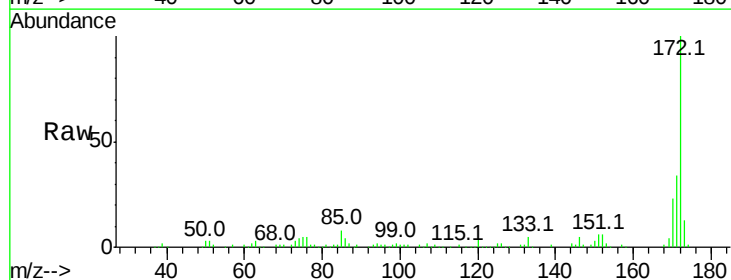

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

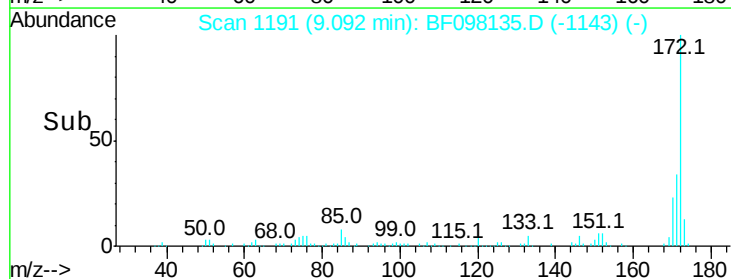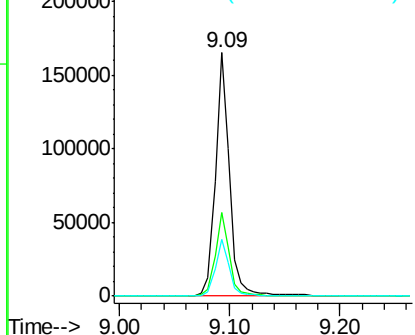


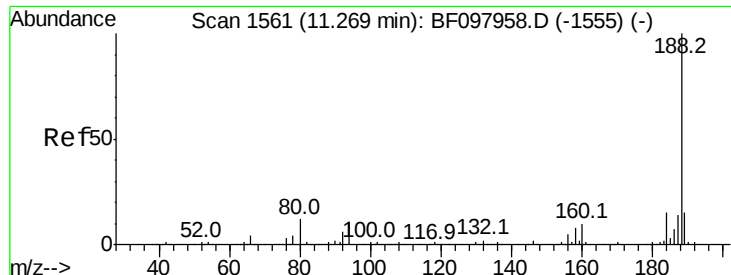




#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.25 min Scan# 1558
Delta R.T. -0.01 min
Lab File: BF098135.D
Acq: 30 Aug 2017 3:52

Instrument :
BNA_F
ClientSampled :
B-1

Tot Ion:188 Resp: 308802
Ion Ratio Lower Upper
188 100
94 11.6 9.4 14.2
80 12.5 10.2 15.2

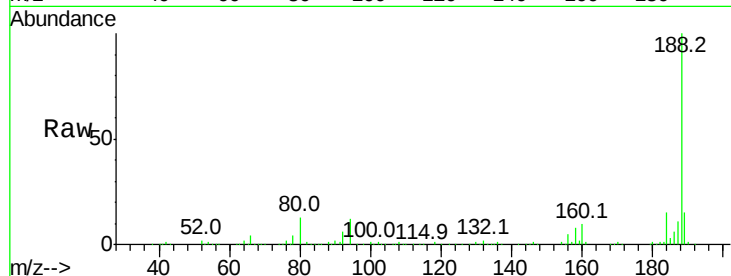


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

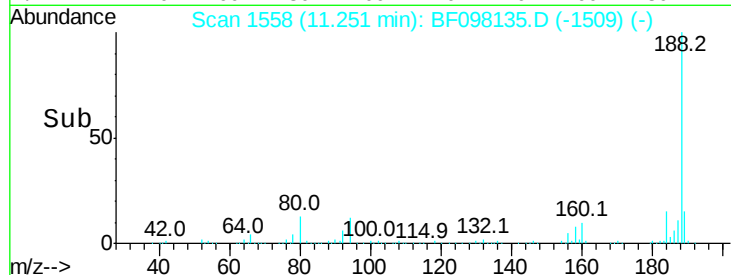
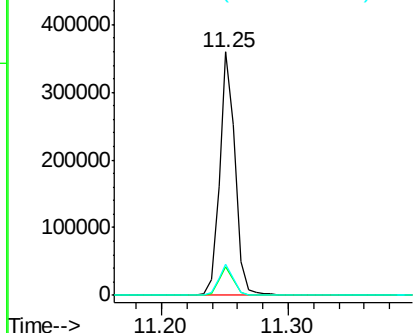



#75
Chrysene-d12
Concen: 20.000 ng
RT: 13.89 min Scan# 2006
Delta R.T. -0.01 min
Lab File: BF098135.D
Acq: 30 Aug 2017 3:52

Tgt Ion:240 Resp: 268387
Ion Ratio Lower Upper
240 100
120 14.2 5.8 8.8#
236 26.5 20.5 30.7



Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

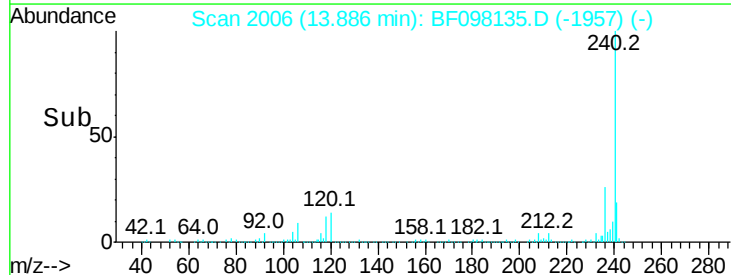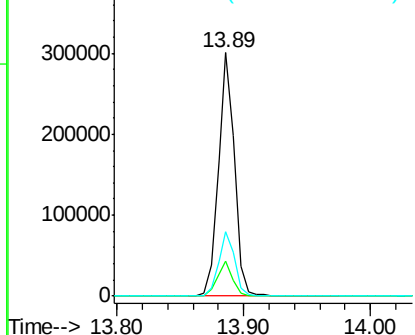

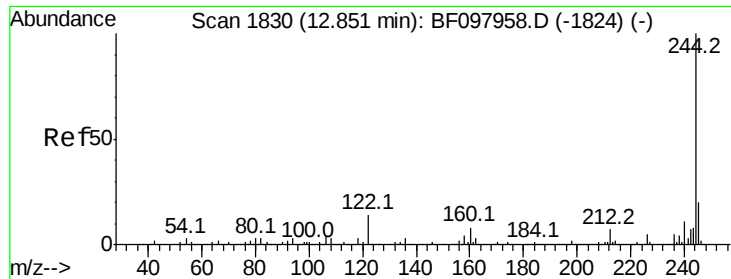

#78

Terphenyl-d14

Concen: 7.248 ng

RT: 12.83 min Scan# 1827

Delta R.T. -0.02 min

Lab File: BF098135.D

Acq: 30 Aug 2017 3:52

Instrument :

BNA_F

ClientSampled :

B-1


Tot Ion:244 Resp: 93289

Ion Ratio Lower Upper

244 100

212 7.2 6.0 9.0




122 13.5 10.3 15.5



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

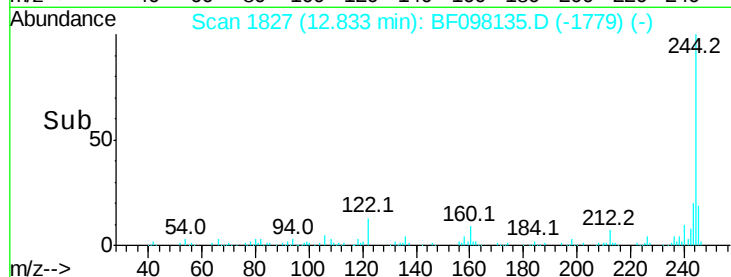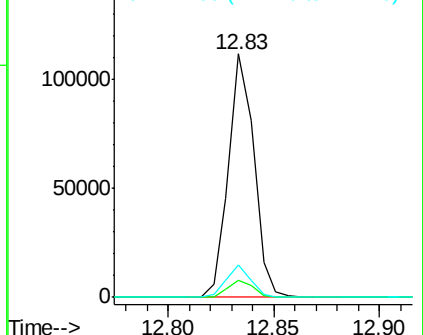

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.31 min Scan# 2248

Delta R.T. 0.00 min

Lab File: BF098135.D

Acq: 30 Aug 2017 3:52


Tgt Ion:264 Resp: 206625

Ion Ratio Lower Upper

264 100

260 24.8 19.5 29.3

265 22.1 17.2 25.8



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

