

Data Path : Z:\HPCHEM1\BNA F\DATA\BF082917\
 Data File : BF098142.D
 Acq On : 30 Aug 2017 7:06
 Operator : SJ/JU
 Sample : I4988-12
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FF4-COMP

Quant Time: Aug 30 08:14:53 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 21 15:59:04 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.73	152	124777	20.00	ng	-0.02
21) Naphthalene-d8	8.02	136	496522	20.00	ng	-0.02
38) Acenaphthene-d10	9.77	164	200250	20.00	ng	-0.02
63) Phenanthrene-d10	11.25	188	307504	20.00	ng	-0.01
75) Chrysene-d12	13.89	240	252540	20.00	ng	-0.01
86) Perylene-d12	15.30	264	207446	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.36	112	870419	106.11	ng	0.00
7) Phenol-d6	6.37	99	1080992	96.99	ng	-0.01
23) Nitrobenzene-d5	7.30	82	781548	85.51	ng	-0.02
41) 2,4,6-Tribromophenol	10.56	330	170196	97.95	ng	-0.02
44) 2-Fluorobiphenyl	9.10	172	1126478	82.65	ng	-0.01
78) Terphenyl-d14	12.84	244	709142	58.56	ng	-0.01


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF082917\
Data File : BF098142.D
Acq On : 30 Aug 2017 7:06
Operator : SJ/JU
Sample : I4988-12
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FF4-COMP

Quant Time: Aug 30 08:14:53 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 21 15:59:04 2017
Response via : Initial Calibration

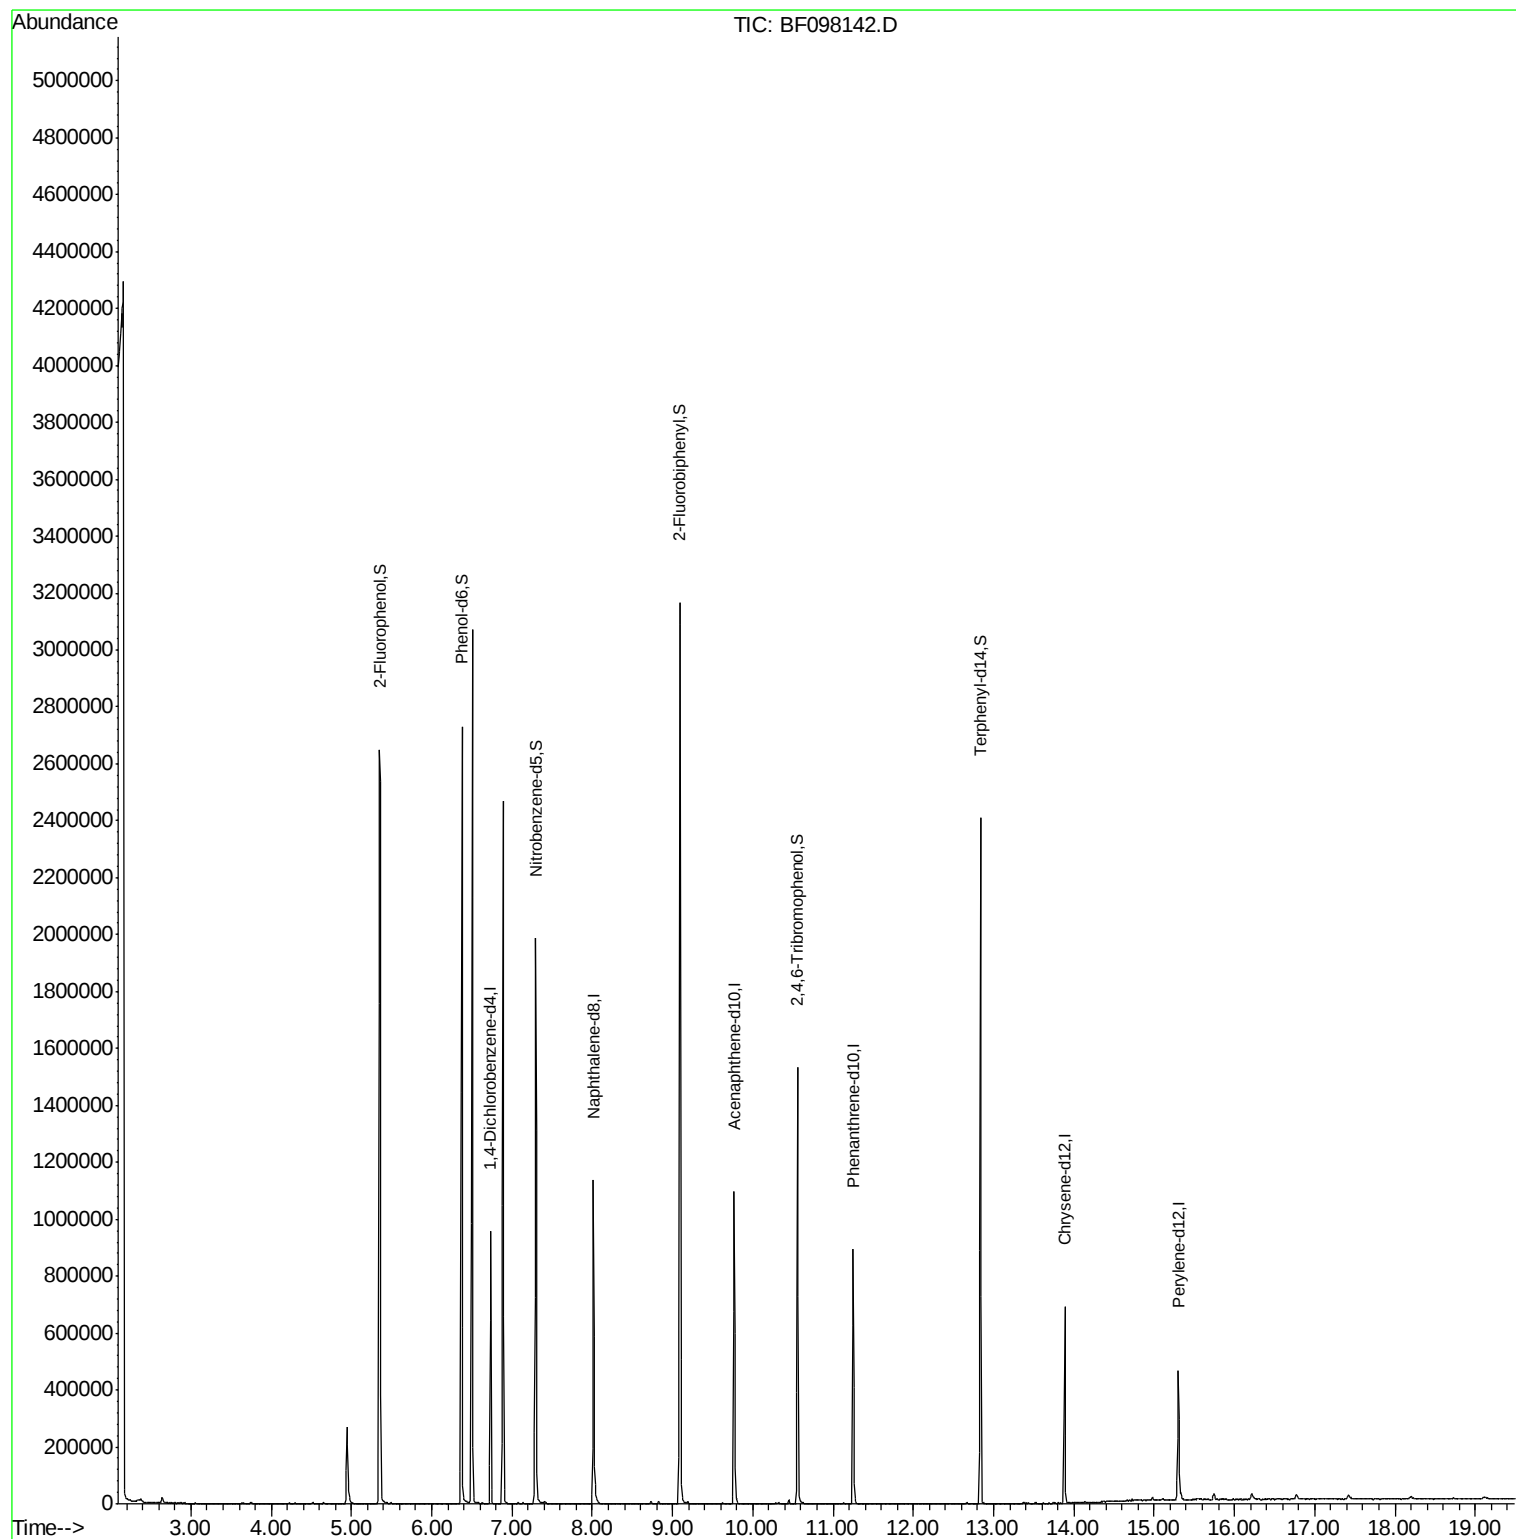

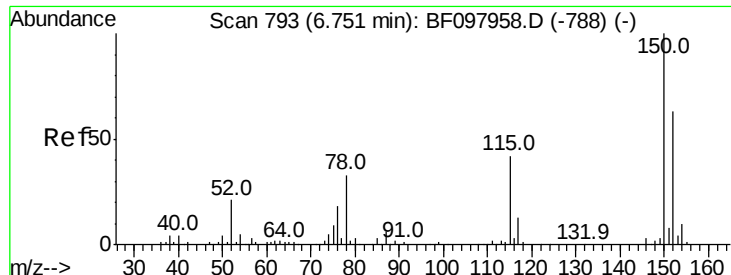


#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.73 min Scan# 790
Delta R.T. -0.02 min
Lab File: BF098142.D
Acq: 30 Aug 2017 7:06

Instrument :
BNA_F
ClientSampleId :
FF4-COMP

Tot Ion:152 Resp: 124777
Ion Ratio Lower Upper
152 100
150 160.9 126.2 189.2
115 65.1 52.2 78.2

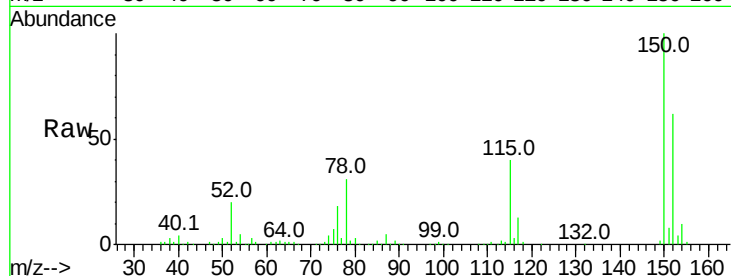


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

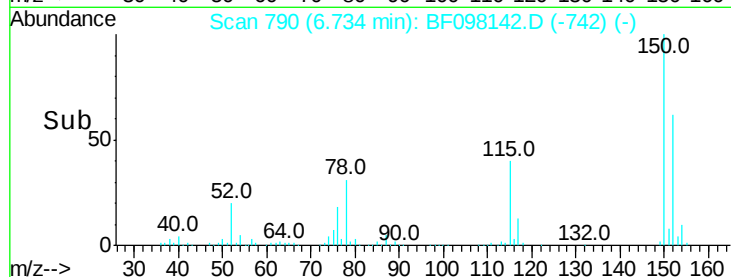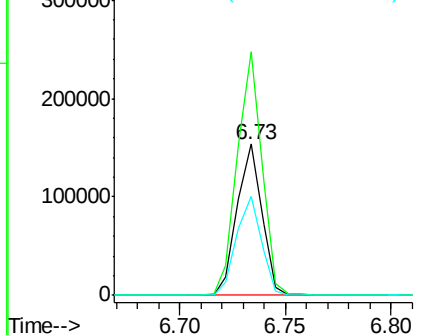



#5


2-Fluorophenol
Concen: 106.107 ng
RT: 5.36 min Scan# 556
Delta R.T. 0.01 min
Lab File: BF098142.D
Acq: 30 Aug 2017 7:06

Tgt Ion:112 Resp: 870419
Ion Ratio Lower Upper
112 100
64 54.6 46.0 69.0
63 27.4 23.4 35.0

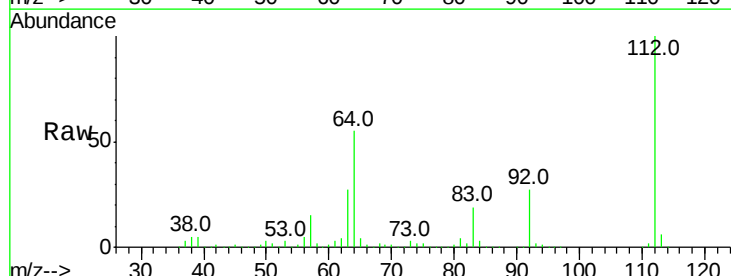

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

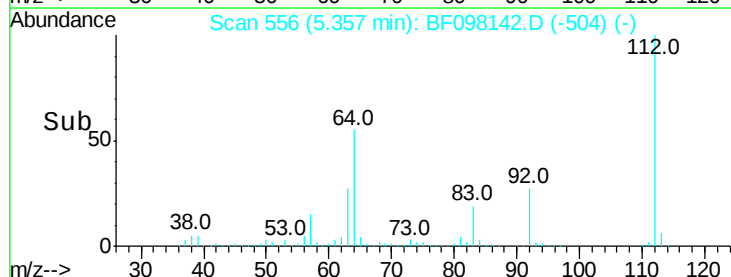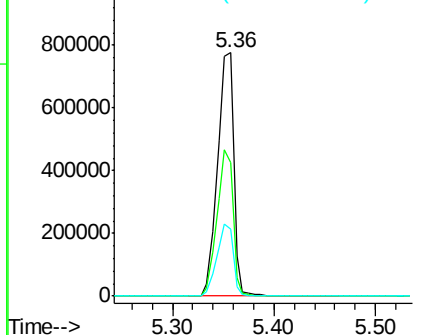

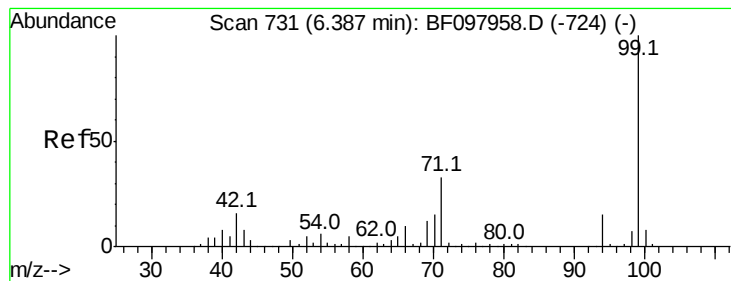

#7

Phenol-d6

Concen: 96.986 ng

RT: 6.37 min Scan# 729

Delta R.T. -0.01 min

Lab File: BF098142.D

Acq: 30 Aug 2017 7:06

Instrument :

BNA_F

ClientSampleId :

FF4-COMP


Tot Ion: 99 Resp: 1080992

Ion Ratio Lower Upper

99 100

42 14.7 13.5 20.3




71 31.8 24.5 36.7

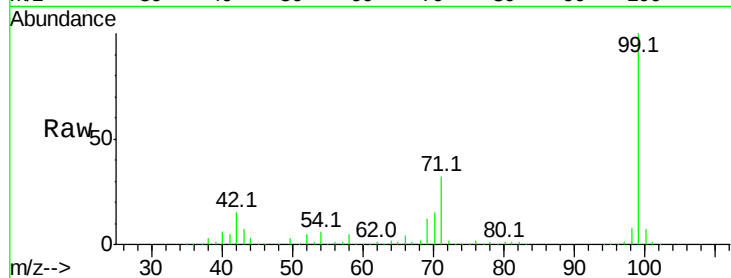

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

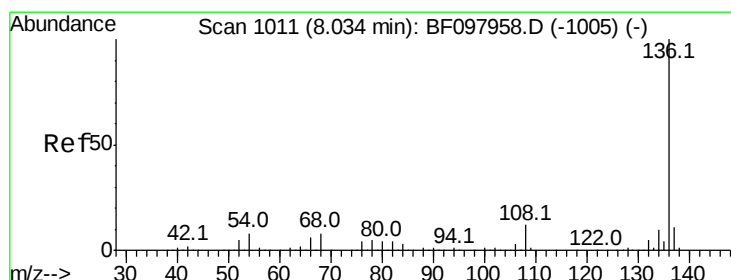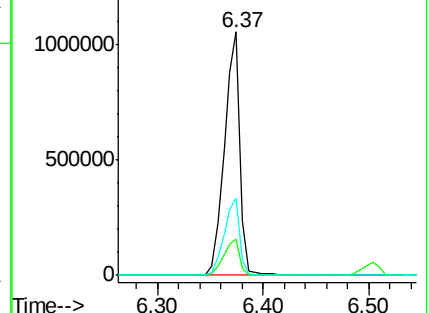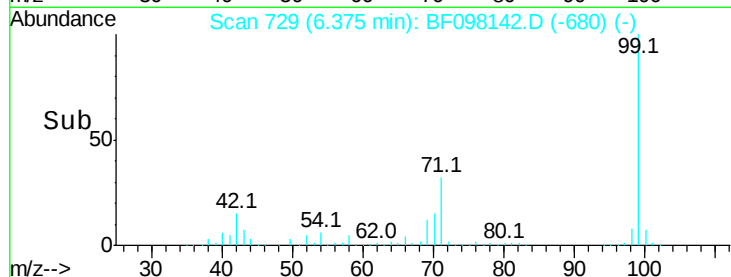

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.02 min Scan# 1008

Delta R.T. -0.02 min

Lab File: BF098142.D

Acq: 30 Aug 2017 7:06

Tgt Ion: 136 Resp: 496522


Ion Ratio Lower Upper

136 100

137 11.0 8.5 12.7

54 7.7 4.9 7.3#

68 7.2 4.1 6.1#


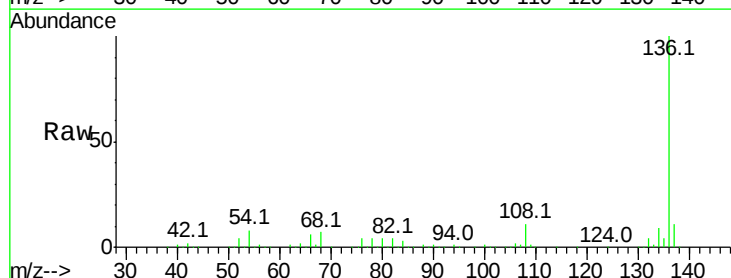



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



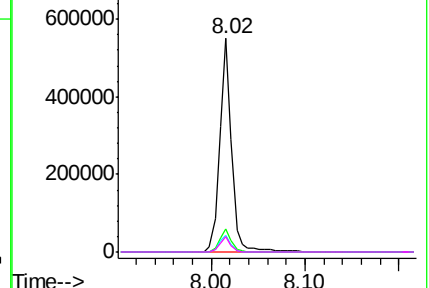
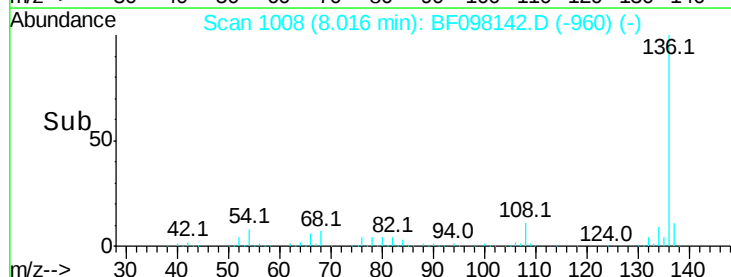


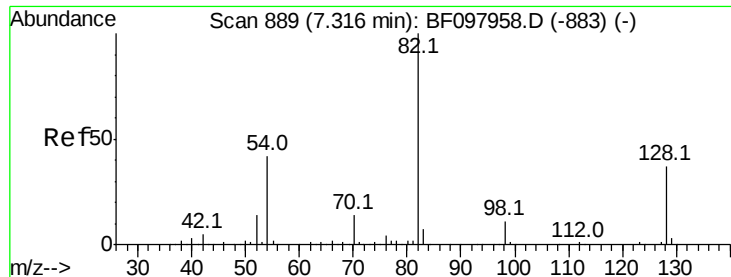

#23
 Nitrobenzene-d5
 Concen: 85.509 ng
 RT: 7.30 min Scan# 886
 Delta R.T. -0.02 min
 Lab File: BF098142.D
 Acq: 30 Aug 2017 7:06




Instrument :
 BNA_F
 ClientSampleId :
 FF4-COMP

Tot Ion	Ratio	Lower	Upper
82	100		
128	38.5	34.0	51.0
54	41.3	42.2	63.2#

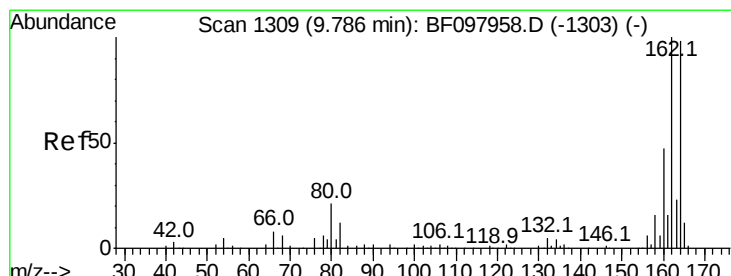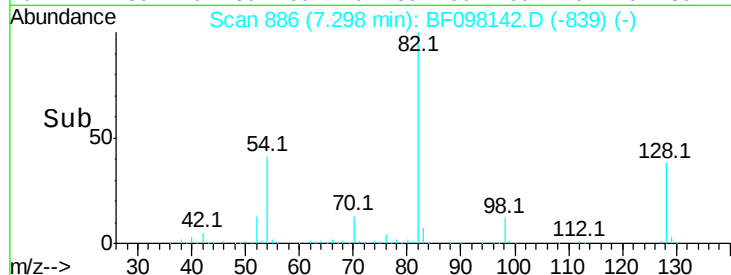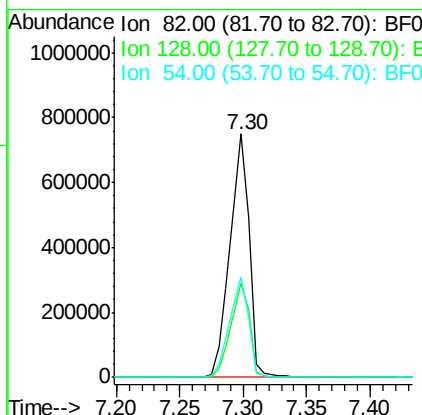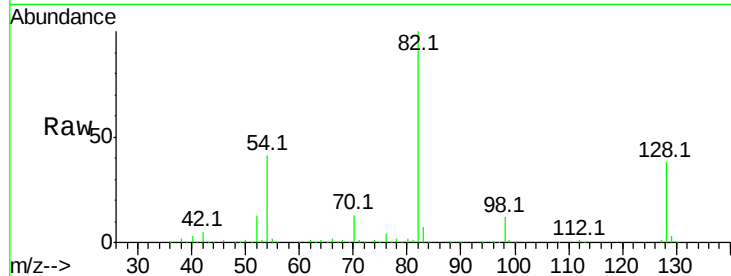

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.77 min Scan# 1306
 Delta R.T. -0.02 min
 Lab File: BF098142.D
 Acq: 30 Aug 2017 7:06

Tgt Ion	Ratio	Lower	Upper
164	100		
162	102.6	82.6	123.8
160	47.1	36.2	54.2

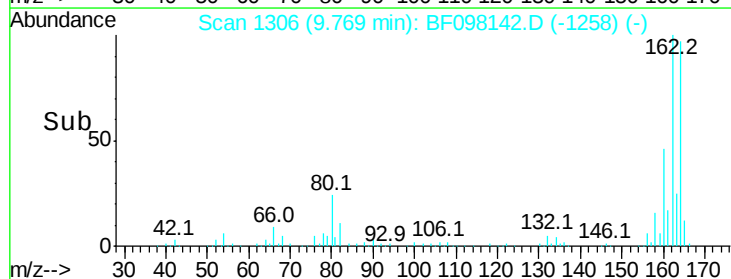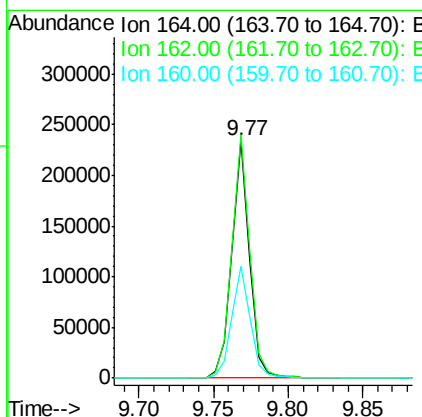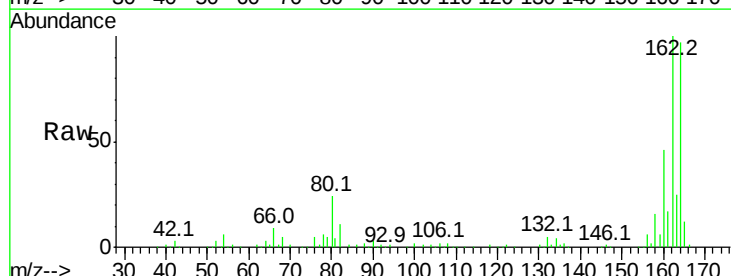







#41
 2,4,6-Tribromophenol
 Concen: 97.955 ng
 RT: 10.56 min Scan# 1440
 Delta R.T. -0.02 min
 Lab File: BF098142.D
 Acq: 30 Aug 2017 7:06

Instrument :
 BNA_F
 ClientSampleId :
 FF4-COMP

Tot Ion:330 Resp: 170196
 Ion Ratio Lower Upper
 330 100
 332 95.0 76.6 115.0
 141 38.0 31.4 47.2

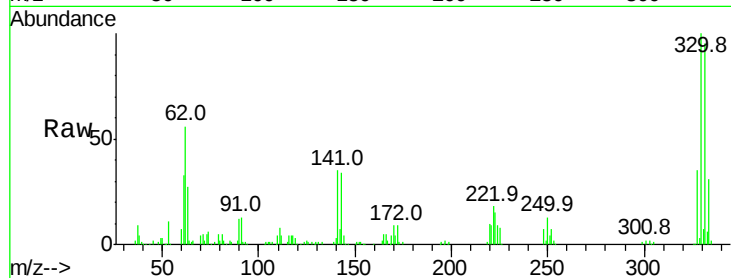


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

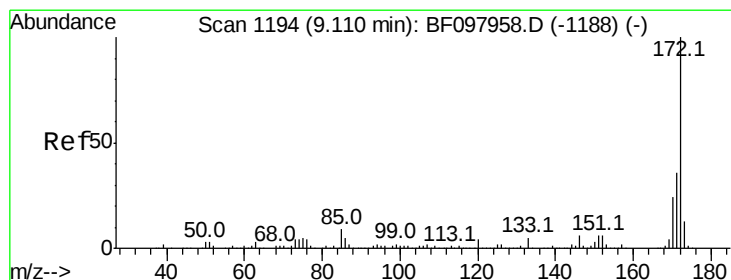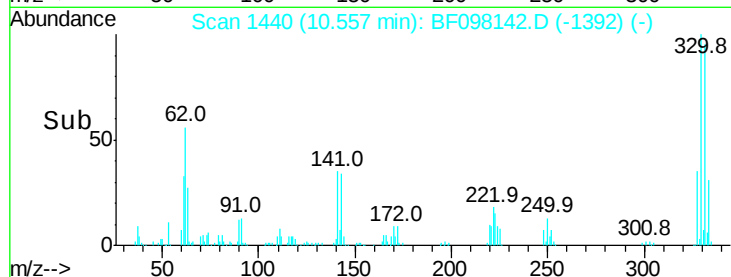
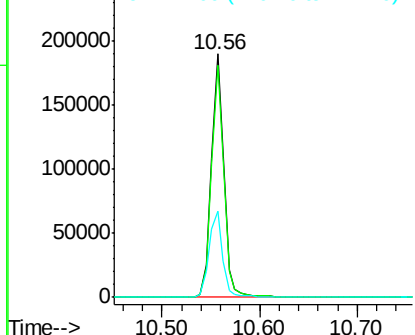



#44
 2-Fluorobiphenyl
 Concen: 82.648 ng
 RT: 9.10 min Scan# 1192
 Delta R.T. -0.01 min
 Lab File: BF098142.D
 Acq: 30 Aug 2017 7:06

Tgt Ion:172 Resp: 1126478
 Ion Ratio Lower Upper
 172 100
 171 35.7 29.6 44.4
 170 24.1 19.8 29.8

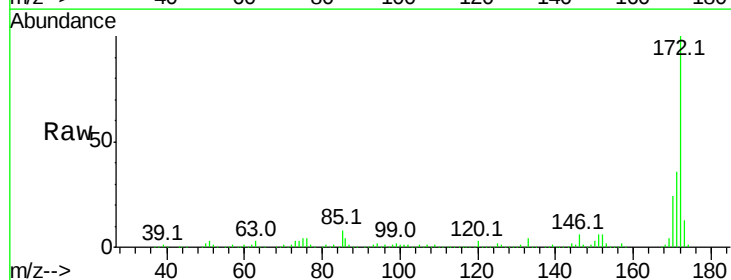

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

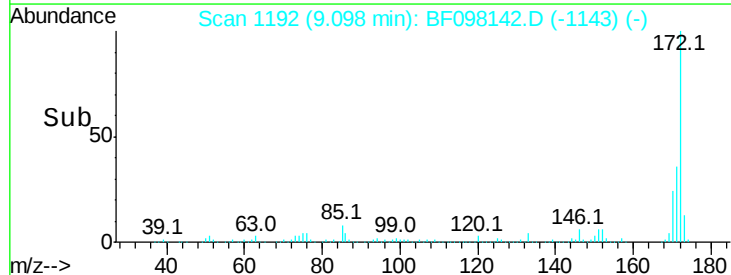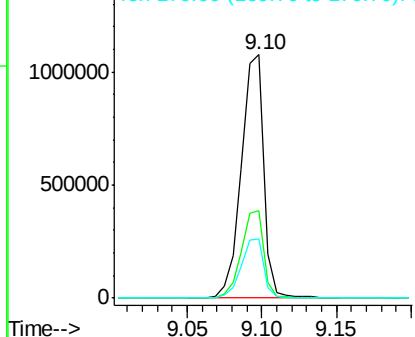

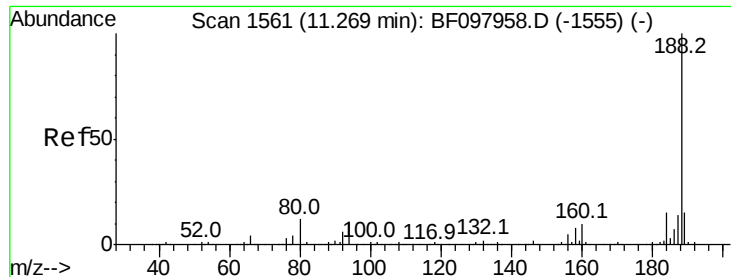

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.25 min Scan# 1558

Delta R.T. -0.01 min

Lab File: BF098142.D

Acq: 30 Aug 2017 7:06

Instrument :

BNA_F

ClientSampleId :

FF4-COMP


Tot Ion:188 Resp: 307504

Ion Ratio Lower Upper

188 100

94 10.6 9.4 14.2




80 11.7 10.2 15.2

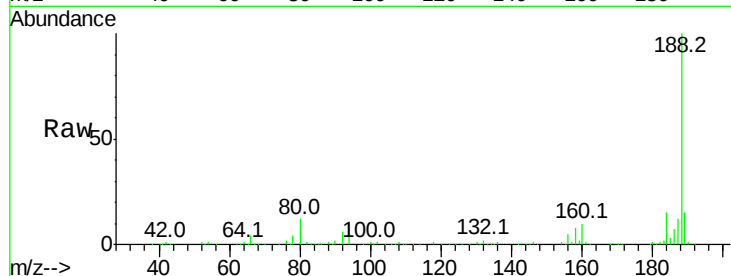

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

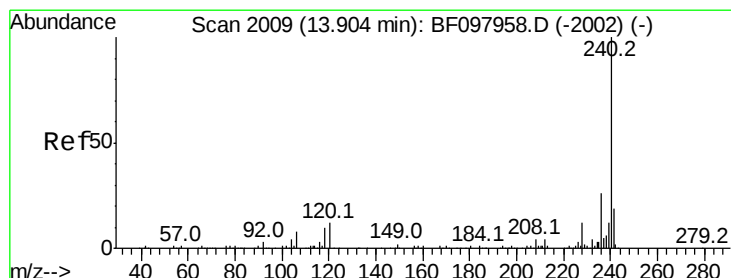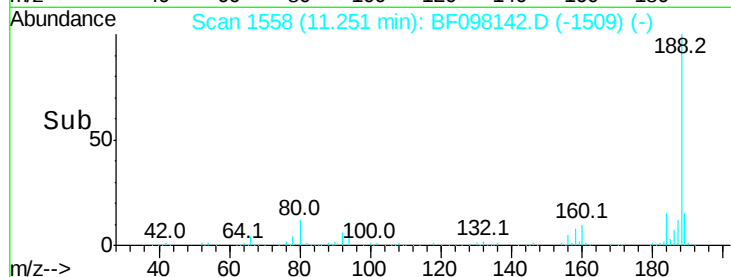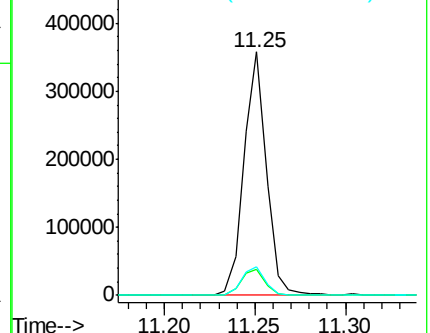

#75

Chrysene-d12

Concen: 20.000 ng

RT: 13.89 min Scan# 2006

Delta R.T. -0.01 min

Lab File: BF098142.D

Acq: 30 Aug 2017 7:06


Tgt Ion:240 Resp: 252540

Ion Ratio Lower Upper

240 100

120 11.2 5.8 8.8#



236 26.6 20.5 30.7

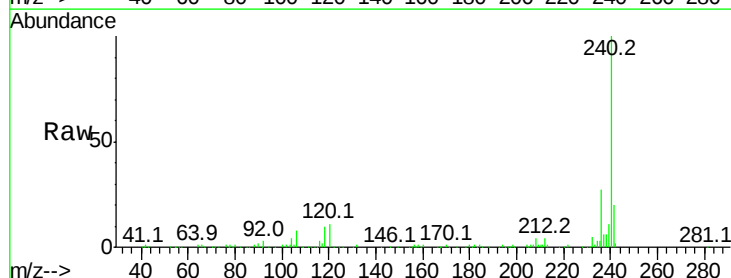


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

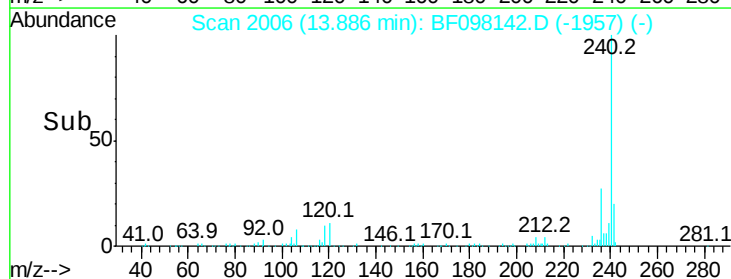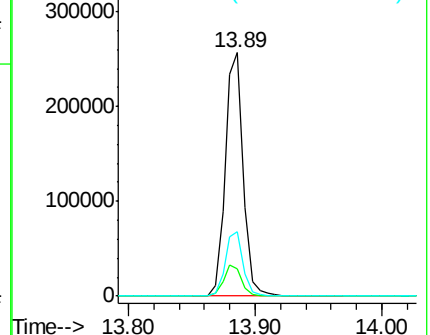

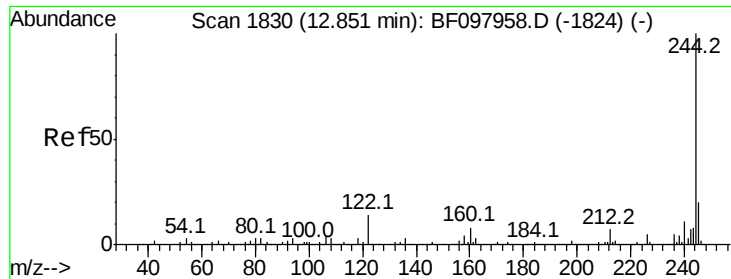

#78

Terphenyl-d14

Concen: 58.557 ng

RT: 12.84 min Scan# 1828

Delta R.T. -0.01 min

Lab File: BF098142.D

Acq: 30 Aug 2017 7:06

Instrument :

BNA_F

ClientSampleId :

FF4-COMP


Tot Ion:244 Resp: 709142

Ion Ratio Lower Upper

244 100

212 7.3 6.0 9.0




122 13.0 10.3 15.5

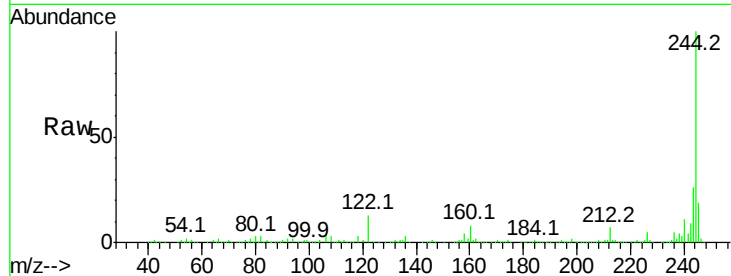

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

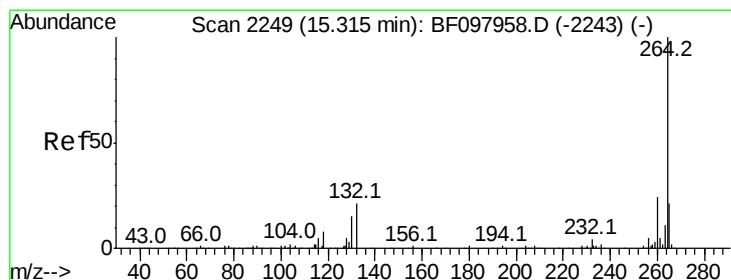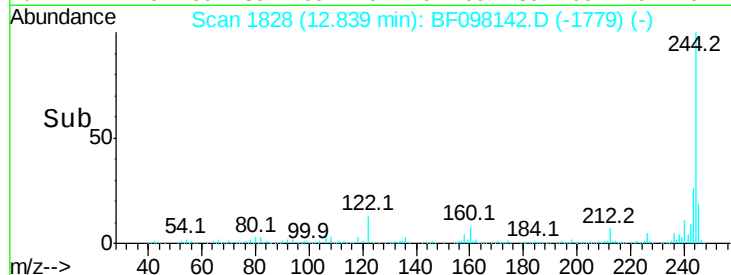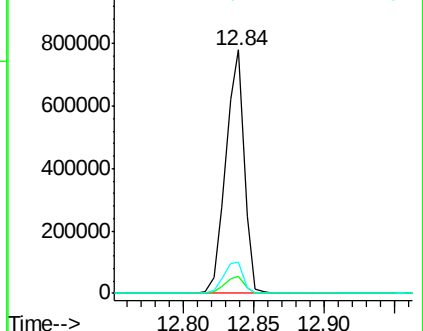

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.30 min Scan# 2247

Delta R.T. -0.01 min

Lab File: BF098142.D

Acq: 30 Aug 2017 7:06


Tgt Ion:264 Resp: 207446

Ion Ratio Lower Upper

264 100

260 24.5 19.5 29.3

265 20.7 17.2 25.8

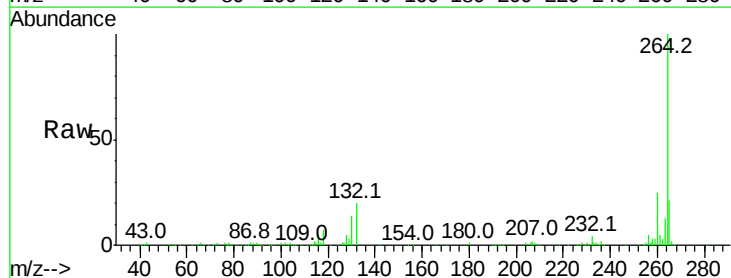

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

