

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF082917\
 Data File : BF098121.D
 Acq On : 29 Aug 2017 20:04
 Operator : SJ/JU
 Sample : I4989-10 5X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 BERGEN-GEN-S4-COMP

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.910	477	480	488	rBV	37372	44705	4.16%	0.459%
2	5.328	547	551	565	rBV	615672	568776	52.92%	5.833%
3	6.357	723	726	738	rBV	667717	626262	58.27%	6.423%
4	6.498	746	750	753	rBV	658257	607192	56.50%	6.227%
5	6.734	786	790	793	rBV	877543	796902	74.15%	8.173%
6	6.886	812	816	824	rBV	522882	442826	41.20%	4.542%
7	7.292	881	885	897	rBV	404622	355173	33.05%	3.643%
8	8.016	1004	1008	1026	rBV	1248550	1054579	98.12%	10.816%
9	9.092	1187	1191	1200	rBV	733377	626213	58.27%	6.423%
10	9.486	1255	1258	1267	rBV	94243	88118	8.20%	0.904%
11	9.769	1302	1306	1317	rVB	1280084	1074738	100.00%	11.023%
12	10.204	1378	1380	1383	rVB	16494	12440	1.16%	0.128%
13	10.551	1436	1439	1445	rBV	350866	302717	28.17%	3.105%
14	10.674	1456	1460	1468	rBV	21811	29251	2.72%	0.300%
15	11.127	1533	1537	1539	rBV2	13975	14438	1.34%	0.148%
16	11.251	1554	1558	1561	rBV	1137104	938260	87.30%	9.623%
17	12.457	1759	1763	1766	rBV	46895	42437	3.95%	0.435%
18	12.686	1799	1802	1805	rVB	42040	35759	3.33%	0.367%
19	12.739	1808	1811	1817	rVB	23816	21457	2.00%	0.220%
20	12.833	1824	1827	1830	rBV	514491	424441	39.49%	4.353%
21	13.733	1977	1980	1988	rVB6	36359	46692	4.34%	0.479%
22	13.880	2001	2005	2009	rBV	779104	767825	71.44%	7.875%
23	14.362	2084	2087	2090	rBV4	13616	18728	1.74%	0.192%
24	14.898	2174	2178	2181	rBV2	28733	42748	3.98%	0.438%
25	15.239	2233	2236	2242	rBV2	22119	27303	2.54%	0.280%
26	15.304	2242	2247	2251	rBV	570390	688172	64.03%	7.058%
27	15.745	2319	2322	2327	rVB3	17410	25132	2.34%	0.258%
28	16.215	2398	2402	2407	rVB6	16956	26918	2.50%	0.276%


Sum of corrected areas: 9750202

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF082917\
Data File : BF098121.D
Acq On : 29 Aug 2017 20:04
Operator : SJ/JU
Sample : I4989-10 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BERGEN-GEN-S4-COMP

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

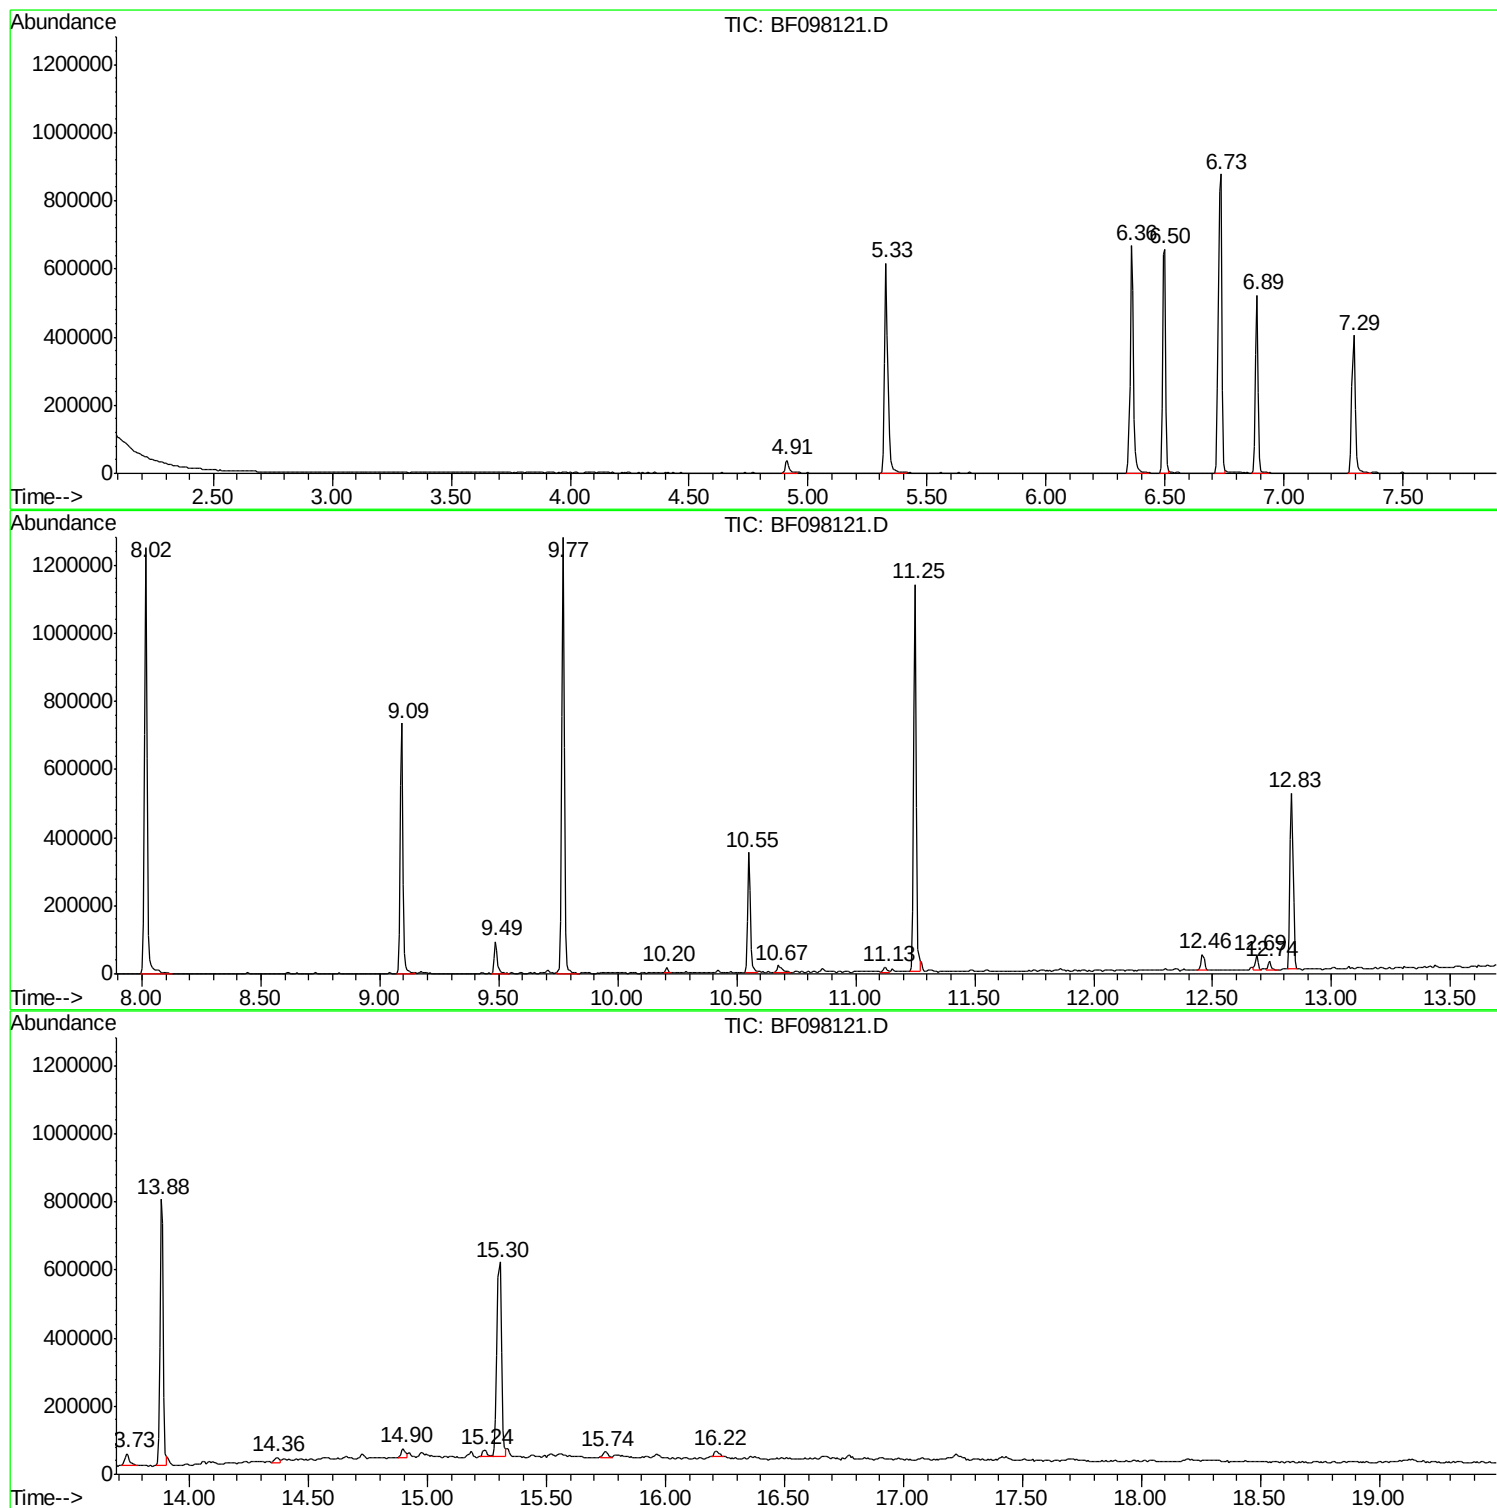

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF082917\
Data File : BF098121.D
Acq On : 29 Aug 2017 20:04
Operator : SJ/JU
Sample : I4989-10 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BERGEN-GEN-S4-COMP










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.50 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.50	15.24 ng	607192	1,4-Dichlorobenzene-d4	6.73

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
3		5-Aminoindole	132	C8H8N2	005192-03-0	10
4		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
5		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9

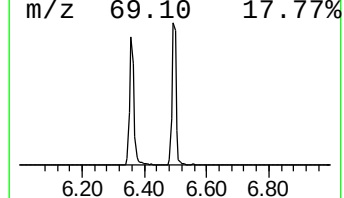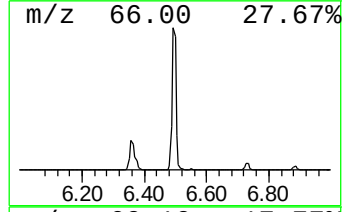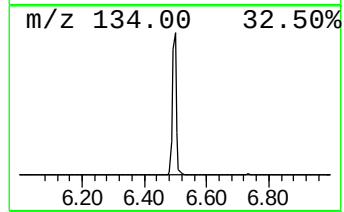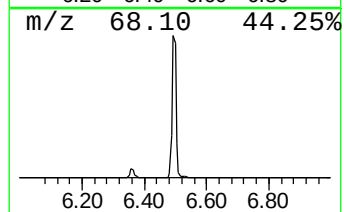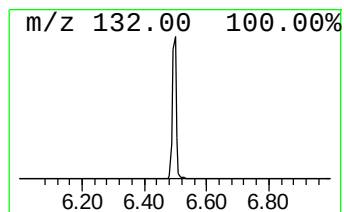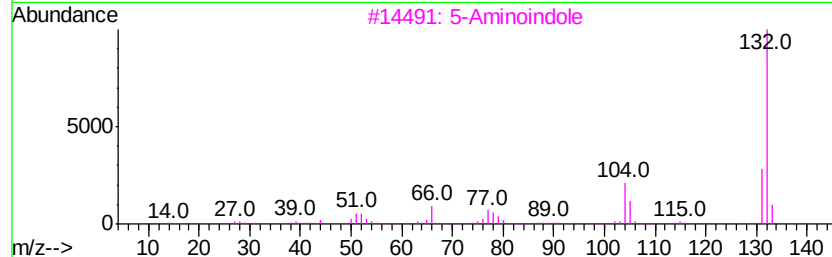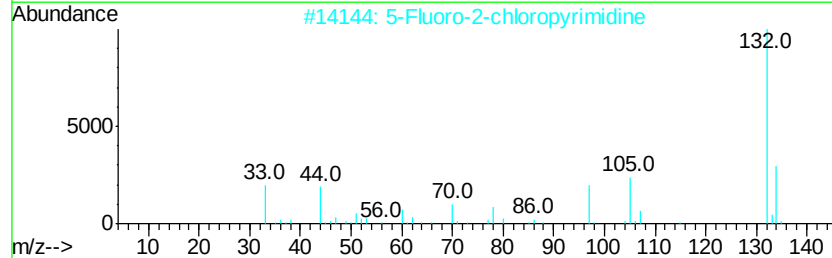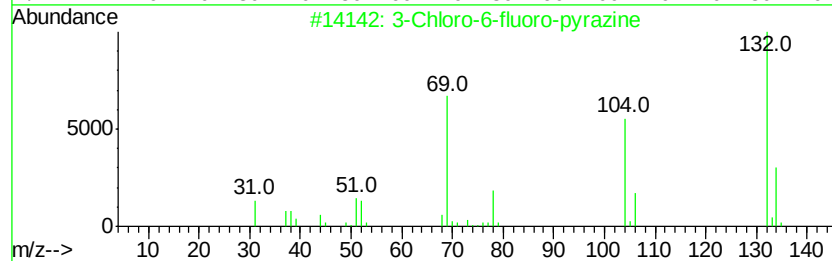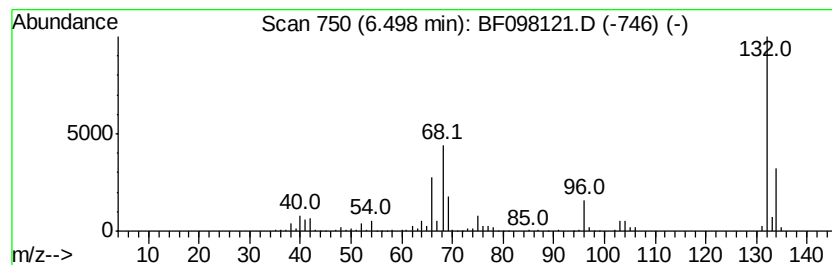

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF082917\
Data File : BF098121.D
Acq On : 29 Aug 2017 20:04
Operator : SJ/JU
Sample : I4989-10 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BERGEN-GEN-S4-COMP

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.50	6.50	15.2	ng	607192	1	6.73	796902	20.0