

Data Path : Z:\HPCHEM1\BNA F\DATA\BF082917\
 Data File : BF098126.D
 Acq On : 29 Aug 2017 22:25
 Operator : SJ/JU
 Sample : I4986-01 10X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SU-01-82517

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.910	477	480	486	rBV	23690	27322	2.88%	0.392%
2	5.328	547	551	562	rBV	318226	299272	31.55%	4.295%
3	6.357	723	726	741	rBV	356314	343274	36.19%	4.927%
4	6.498	746	750	760	rVB	361497	335837	35.41%	4.820%
5	6.734	786	790	793	rBV	891822	754568	79.56%	10.830%
6	6.886	812	816	823	rVB	303947	257931	27.20%	3.702%
7	7.292	881	885	896	rBV	213945	197485	20.82%	2.834%
8	8.016	1004	1008	1015	rBV	1125305	948435	100.00%	13.613%
9	9.092	1187	1191	1203	rBV	405223	353971	37.32%	5.081%
10	9.486	1255	1258	1263	rBV	61419	53171	5.61%	0.763%
11	9.769	1302	1306	1316	rVB	1069411	893086	94.16%	12.818%
12	10.551	1436	1439	1447	rBV	145026	136129	14.35%	1.954%
13	10.674	1458	1460	1462	rBV	13008	13027	1.37%	0.187%
14	11.127	1534	1537	1539	rBV2	11932	11025	1.16%	0.158%
15	11.251	1554	1558	1565	rBV	877295	748301	78.90%	10.740%
16	12.457	1760	1763	1766	rBV	16305	15450	1.63%	0.222%
17	12.686	1799	1802	1805	rBV	24887	19560	2.06%	0.281%
18	12.833	1824	1827	1835	rVB	301478	260598	27.48%	3.740%
19	13.015	1854	1858	1860	rBV5	10754	15409	1.62%	0.221%
20	13.068	1865	1867	1870	rVV4	12197	12789	1.35%	0.184%
21	13.739	1979	1981	1984	rBV4	17571	16761	1.77%	0.241%
22	13.886	2002	2006	2011	rBV	778269	740928	78.12%	10.635%
23	15.304	2243	2247	2251	rBV	431257	512871	54.08%	7.361%


Sum of corrected areas: 6967200

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF082917\
Data File : BF098126.D
Acq On : 29 Aug 2017 22:25
Operator : SJ/JU
Sample : I4986-01 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SU-01-82517

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

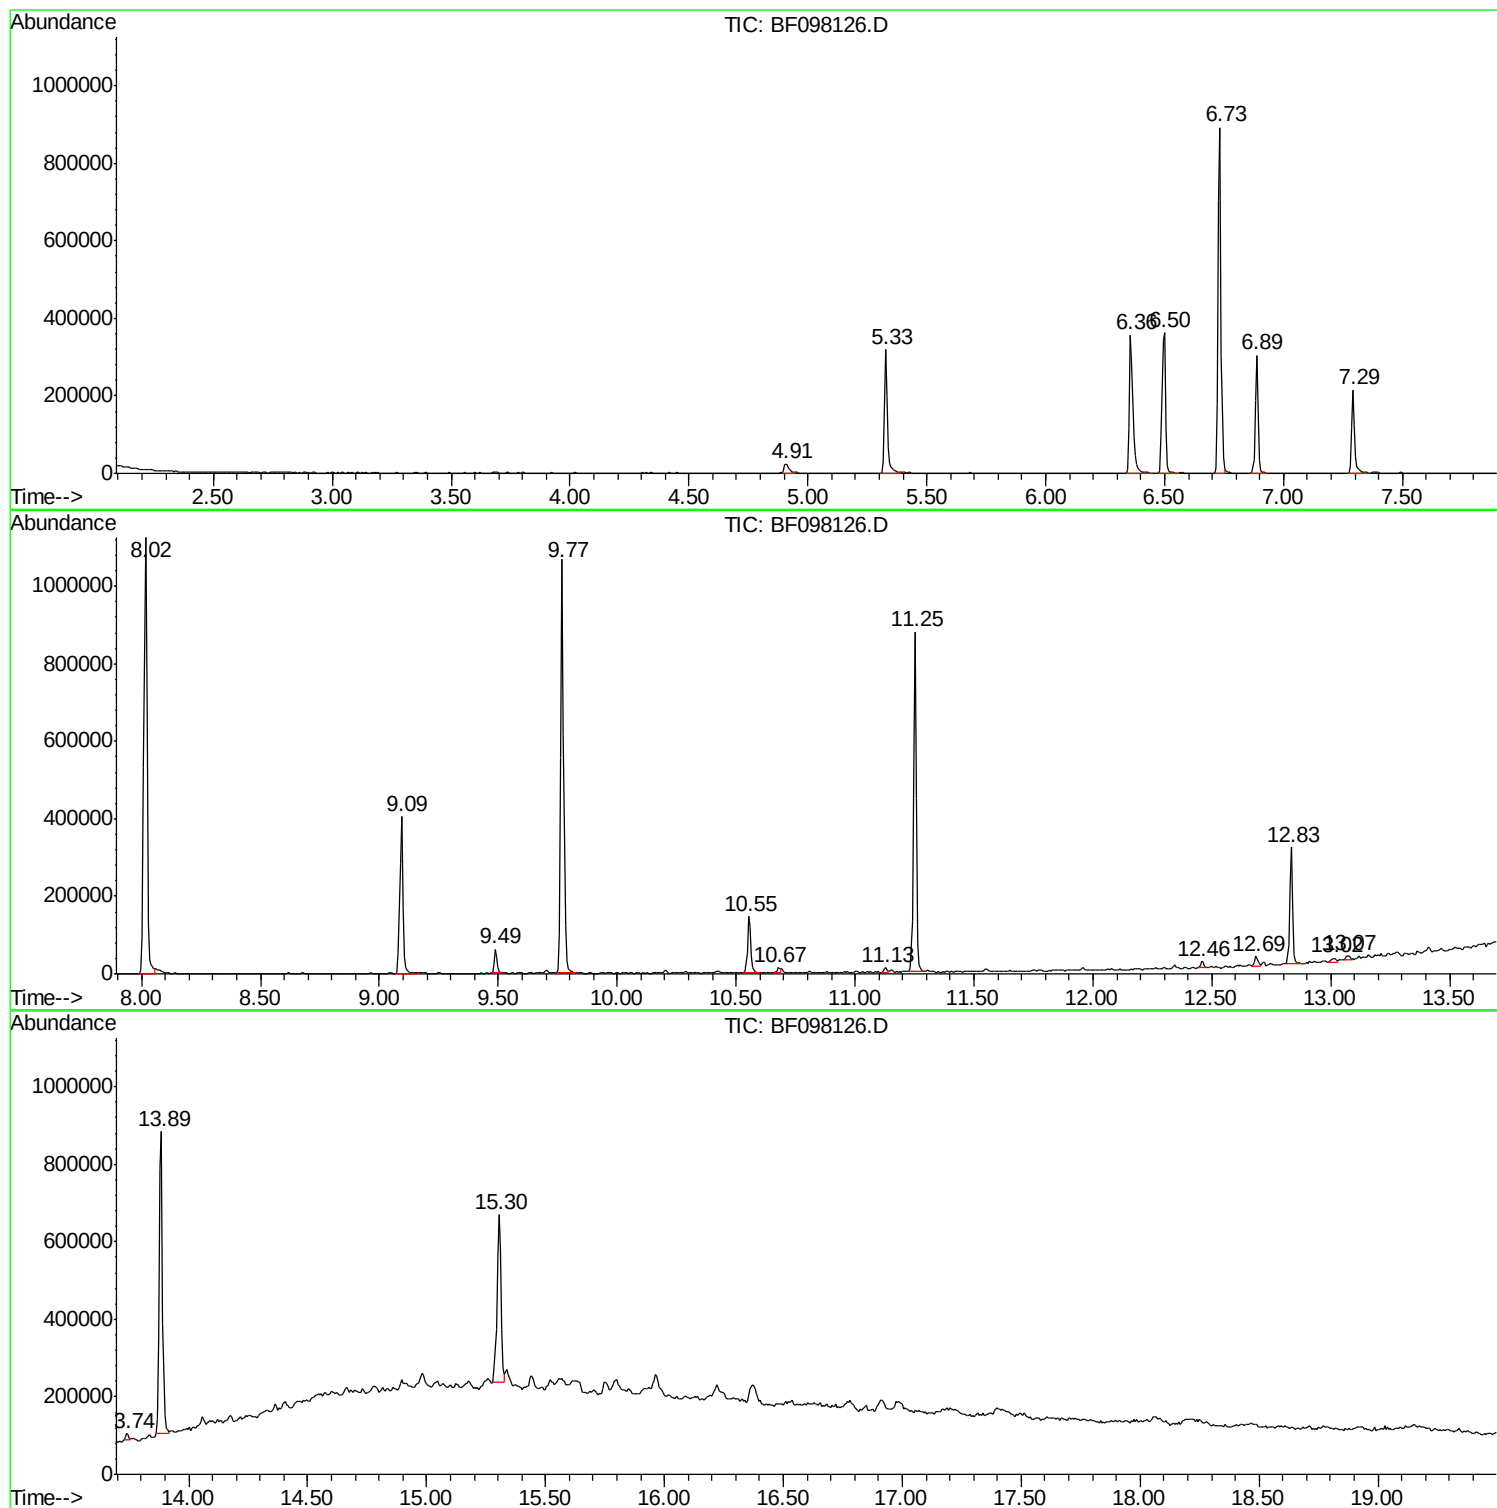

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF082917\
Data File : BF098126.D
Acq On : 29 Aug 2017 22:25
Operator : SJ/JU
Sample : I4986-01 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SU-01-82517










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.50 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.50	8.90 ng	335837	1,4-Dichlorobenzene-d4	6.73

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
2			Xenon	132	Xe	007440-63-3	9
3			(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9
4			Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
5			Benzene, 1-ethenyl-3,5-dimethyl-	132	C10H12	005379-20-4	9

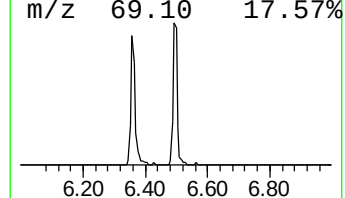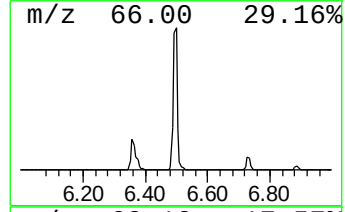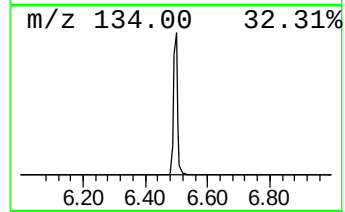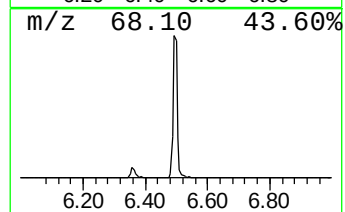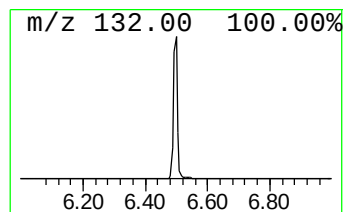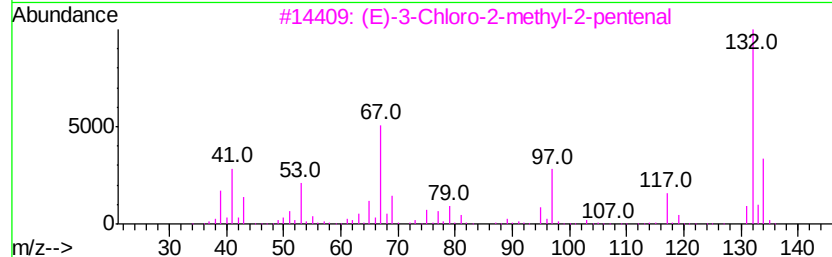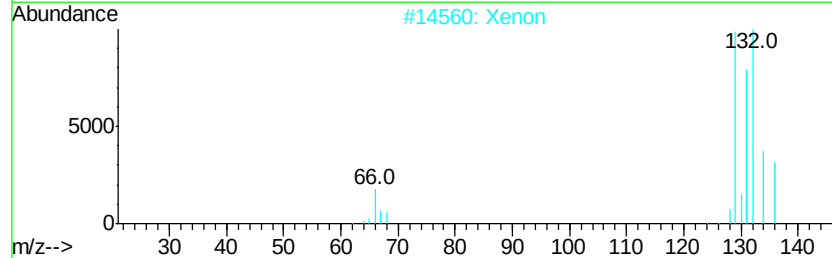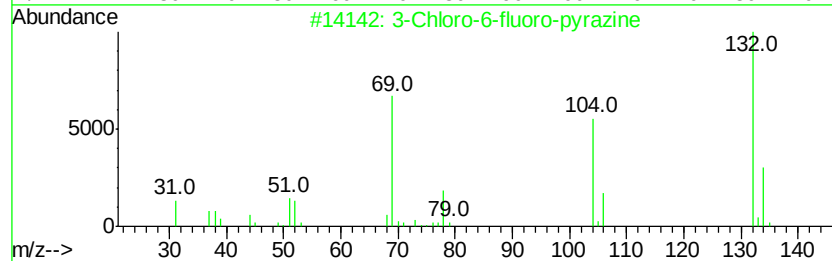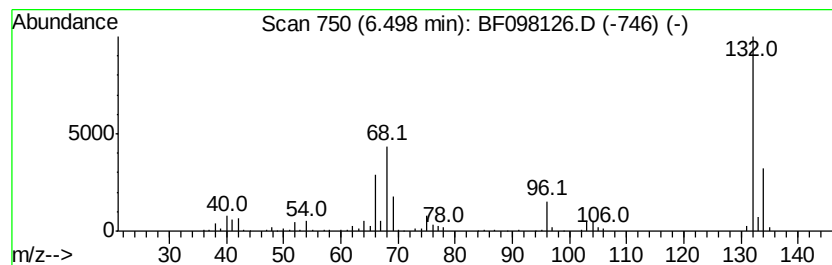

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF082917\
Data File : BF098126.D
Acq On : 29 Aug 2017 22:25
Operator : SJ/JU
Sample : I4986-01 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SU-01-82517

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.50	6.50	8.9	ng	335837	1	6.73	754568	20.0