


Data Path : Z:\HPCHEM1\BNA F\DATA\BF082917\
 Data File : BF098107.D
 Acq On : 29 Aug 2017 13:27
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 21 15:59:04 2017

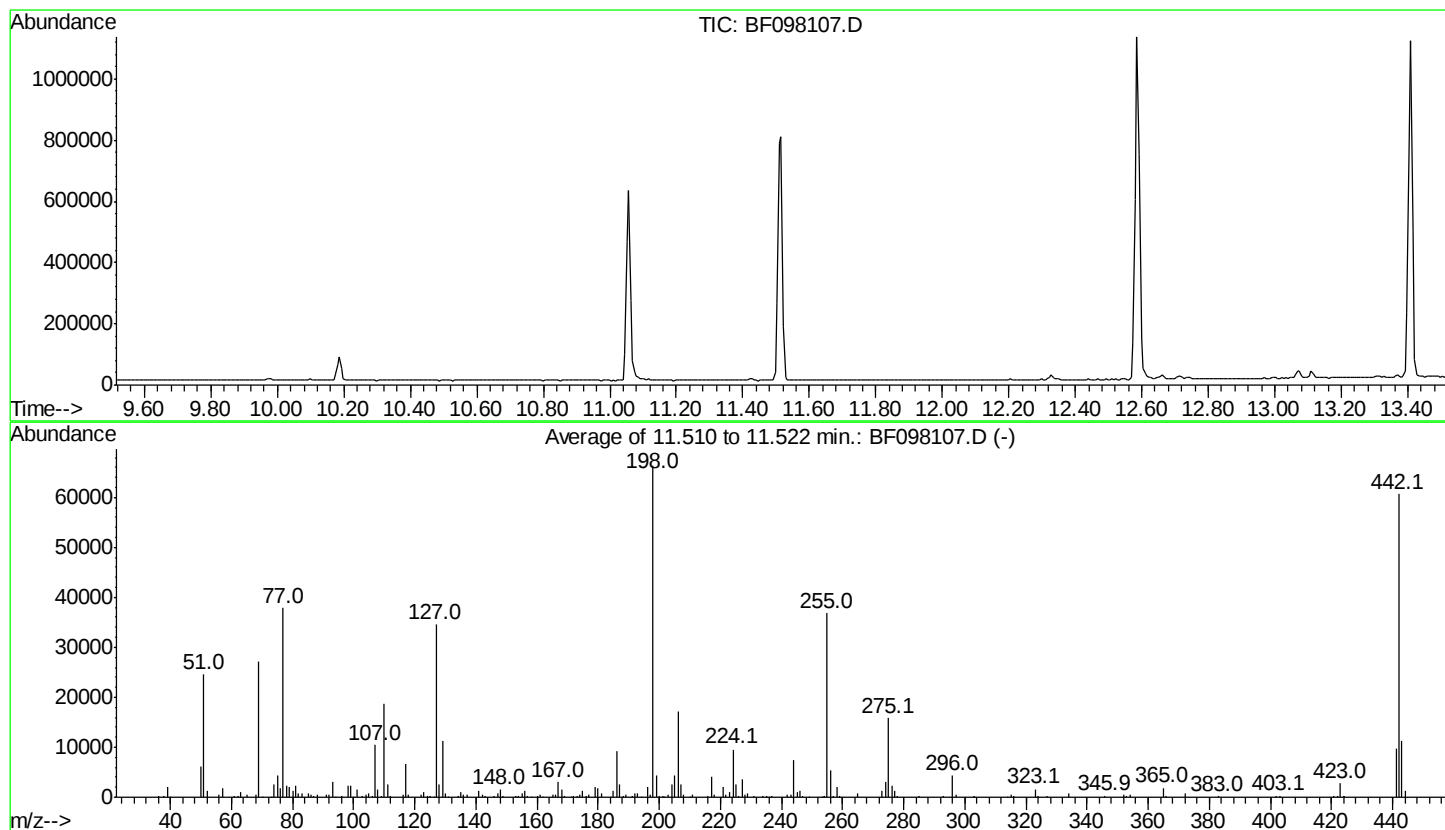

AutoFind: Scans 1602, 1603, 1604; Background Corrected with Scan 1597

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.0	24520	PASS
68	69	0.00	2	1.8	499	PASS
69	198	0.00	100	40.8	27062	PASS
70	69	0.00	2	0.5	127	PASS
127	198	10	80	52.0	34504	PASS
197	198	0.00	2	1.0	632	PASS
198	198	100	100	100.0	66357	PASS
199	198	5	9	6.5	4345	PASS
275	198	10	60	23.8	15809	PASS
365	198	1	100	2.9	1900	PASS
441	442	0.01	24	15.9	9617	PASS
442	198	50	100	91.4	60629	PASS
443	442	15	24	18.5	11239	PASS