

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082922\
 Data File : BF130033.D
 Acq On : 29 Aug 2022 14:10
 Operator : CG\JU
 Sample : PB147234BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB147234BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF130033.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.345	516	520	546	rBV	3941177	4038061	66.90%	12.674%
2	6.369	690	694	718	rBV	4055178	4040157	66.94%	12.681%
3	6.698	747	750	764	rBV	911622	786235	13.03%	2.468%
4	7.275	843	848	851	rBV	2701196	2611454	43.27%	8.196%
5	7.981	964	968	978	rBV	1181861	1076846	17.84%	3.380%
6	9.057	1146	1151	1154	rBV	5248994	5159998	85.49%	16.195%
7	9.733	1261	1266	1270	rBV	1582304	1278369	21.18%	4.012%
8	10.533	1398	1402	1405	rBV	3836781	3340567	55.35%	10.485%
9	11.222	1516	1519	1523	rBV	1663977	1378266	22.83%	4.326%
10	12.810	1784	1789	1792	rBV	5642819	6035879	100.00%	18.944%
11	13.868	1966	1969	1976	rBV	1399471	1185691	19.64%	3.721%
12	15.298	2209	2212	2222	rVB2	714158	861256	14.27%	2.703%
13	16.133	2349	2354	2361	rVB	38482	68329	1.13%	0.214%




Sum of corrected areas: 31861108

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082922\
Data File : BF130033.D
Acq On : 29 Aug 2022 14:10
Operator : CG\JU
Sample : PB147234BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB147234BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

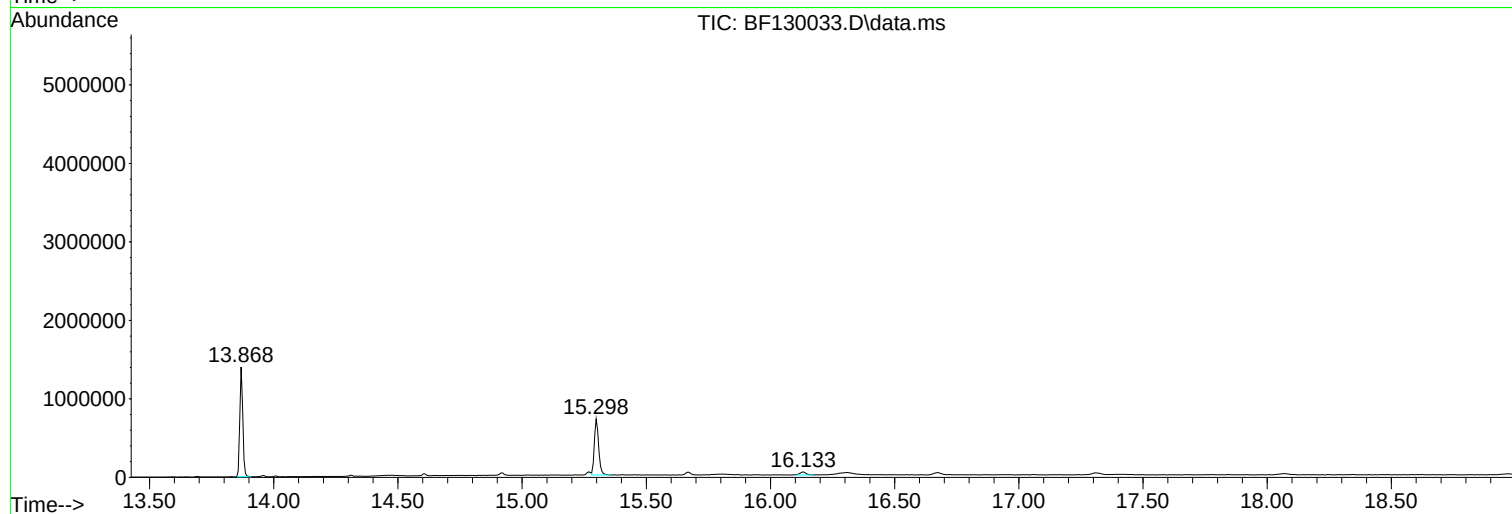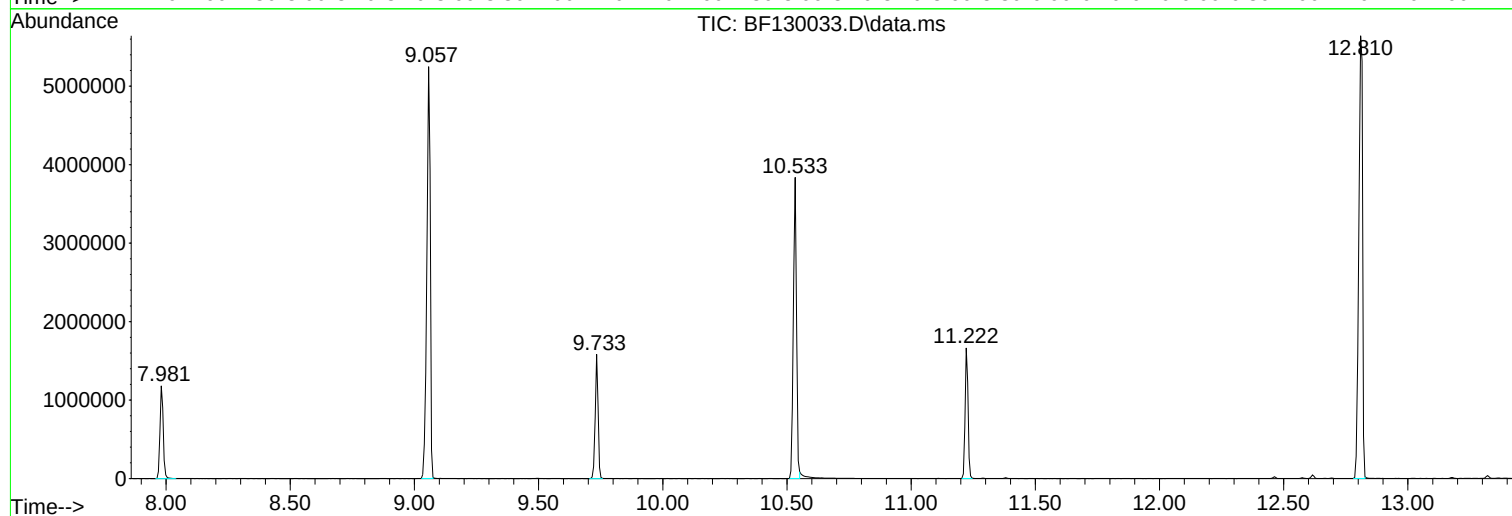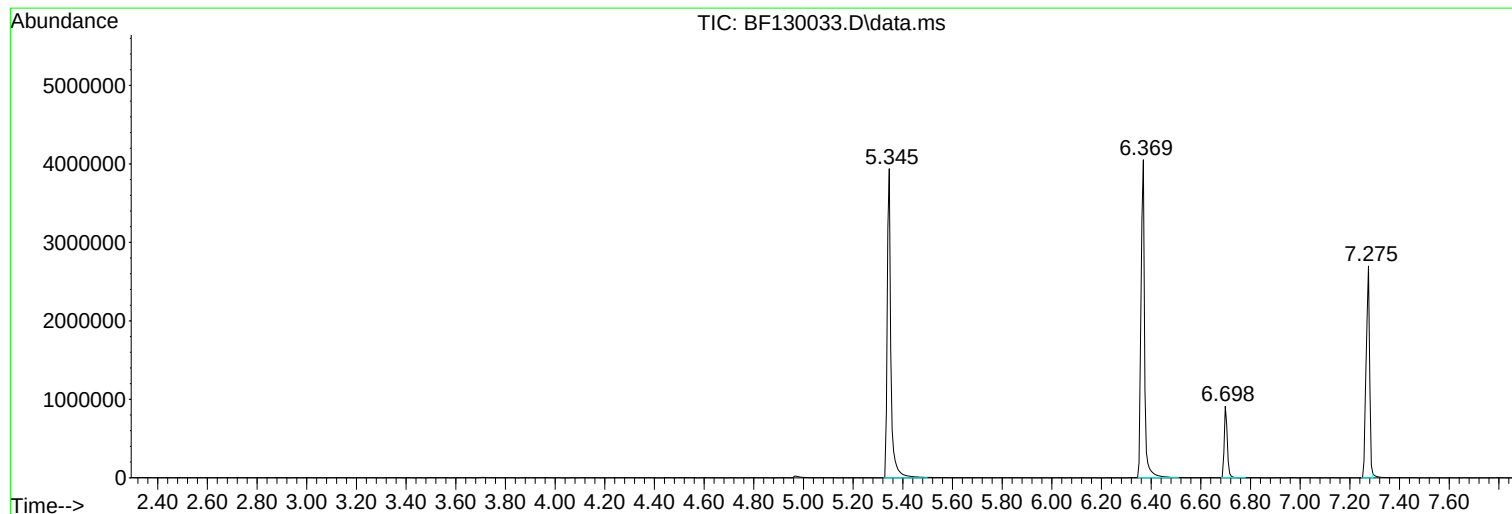

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082922\
Data File : BF130033.D
Acq On : 29 Aug 2022 14:10
Operator : CG\JU
Sample : PB147234BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB147234BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082922\
Data File : BF130033.D
Acq On : 29 Aug 2022 14:10
Operator : CG\JU
Sample : PB147234BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB147234BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------