

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082922\
 Data File : BF130039.D
 Acq On : 29 Aug 2022 17:39
 Operator : CG\JU
 Sample : N4379-21
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 EQUIP-BLANK

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF130039.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.910	442	446	466	rBV	855945	1062503	21.32%	4.272%
2	5.346	517	520	536	rBV	1518332	1806090	36.24%	7.262%
3	6.369	691	694	711	rBV	1040464	1269963	25.48%	5.106%
4	6.698	747	750	765	rVB	825532	742762	14.90%	2.987%
5	7.275	844	848	851	rBV	2813991	2571776	51.60%	10.341%
6	7.981	965	968	983	rVB	1177653	1001658	20.10%	4.028%
7	9.057	1146	1151	1154	rBV	5237595	4984294	100.00%	20.042%
8	9.734	1262	1266	1270	rBV	1453670	1163607	23.35%	4.679%
9	10.533	1398	1402	1405	rBV	3415636	2956296	59.31%	11.887%
10	11.222	1516	1519	1527	rVB	1417619	1153390	23.14%	4.638%
11	12.810	1784	1789	1792	rBV	5516656	4810239	96.51%	19.342%
12	13.869	1966	1969	1977	rBV	777861	671374	13.47%	2.700%
13	15.298	2208	2212	2223	rVB	563503	675656	13.56%	2.717%




Sum of corrected areas: 24869608

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082922\
Data File : BF130039.D
Acq On : 29 Aug 2022 17:39
Operator : CG\JU
Sample : N4379-21
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
EQUIP-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

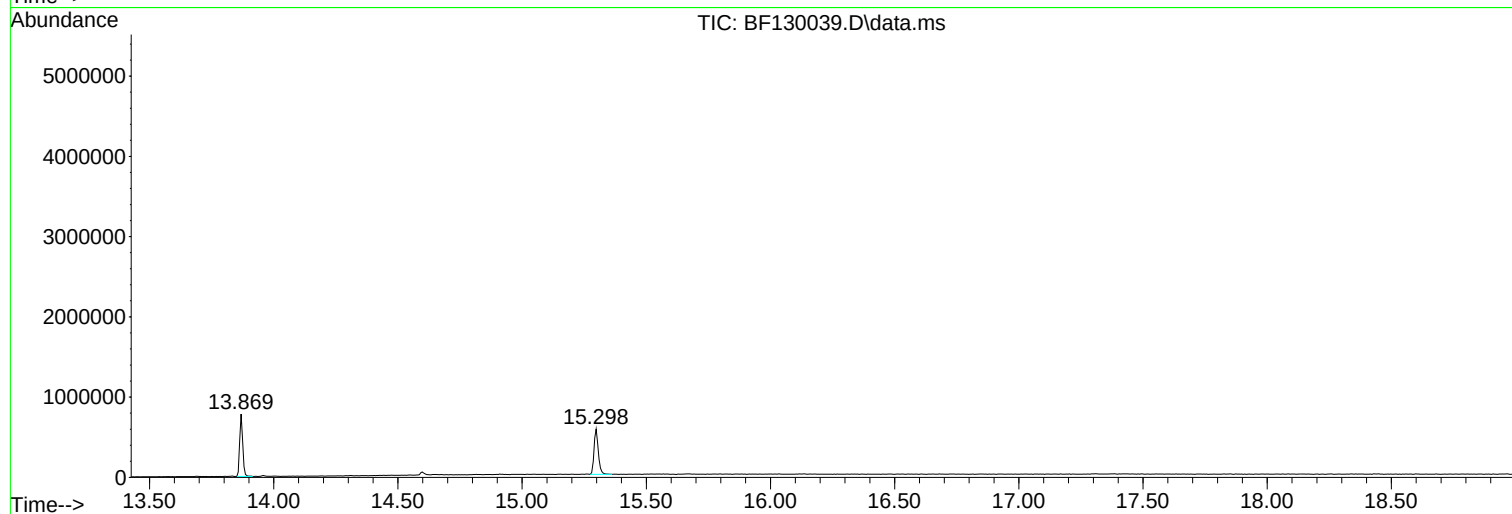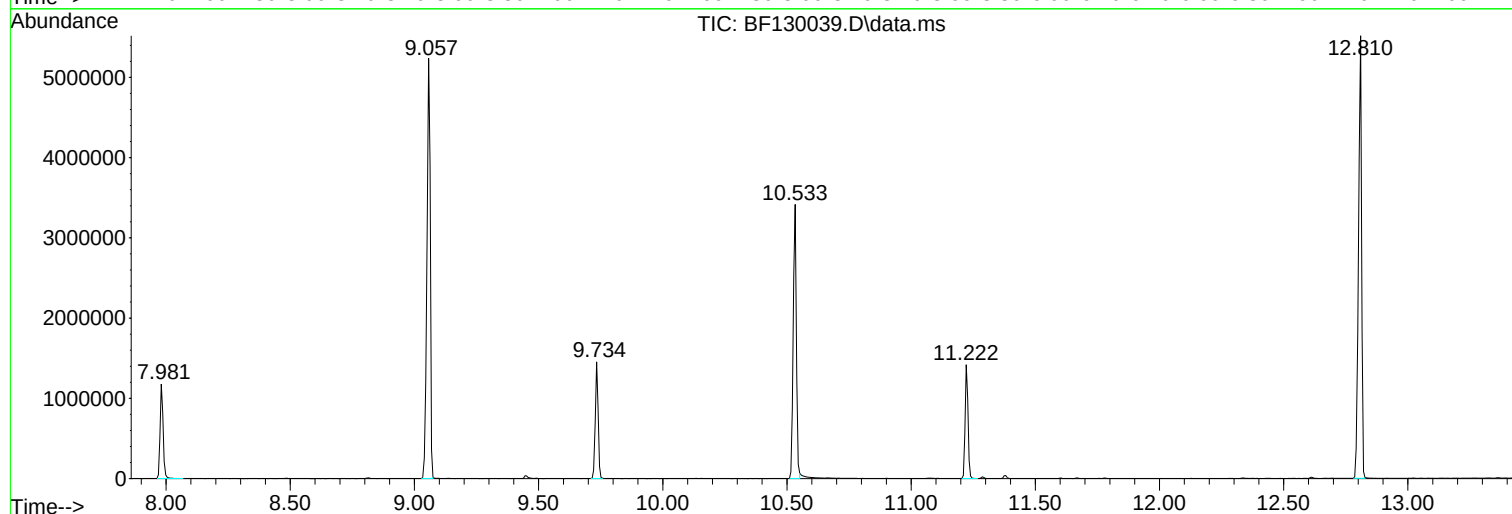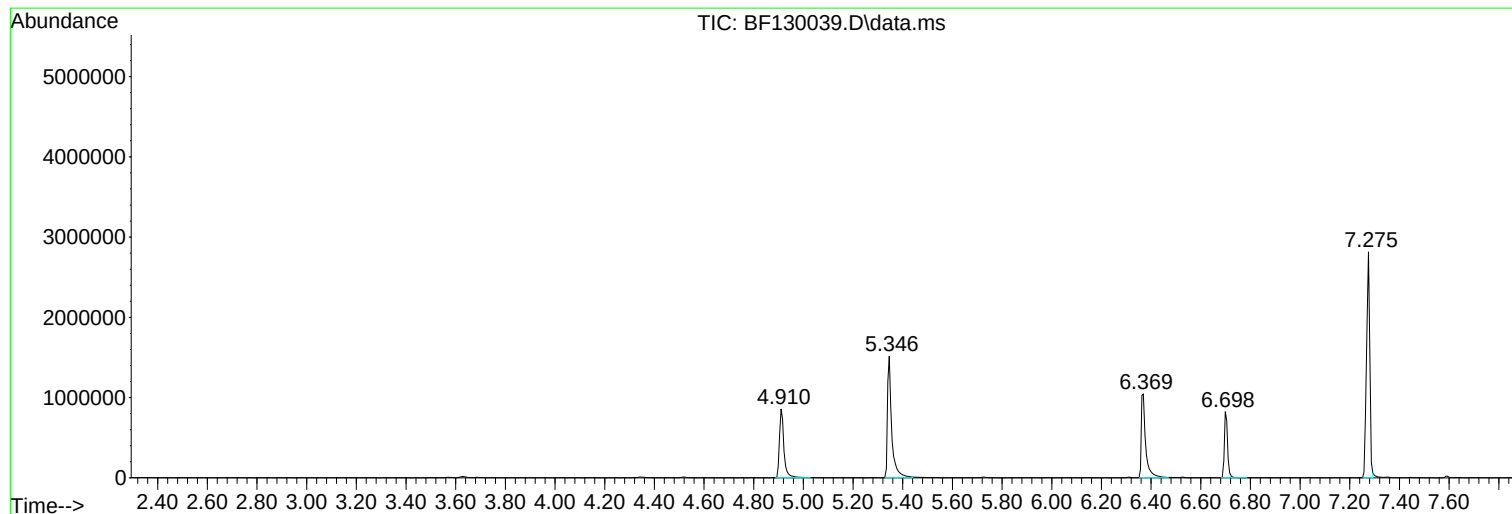

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082922\
Data File : BF130039.D
Acq On : 29 Aug 2022 17:39
Operator : CG\JU
Sample : N4379-21
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
EQUIP-BLANK










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.910	28.61 ng	1062500	1,4-Dichlorobenzene-d4	6.698

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56		
2	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	23		
3	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	12		
4	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10		
5	Butane, 1-ethoxy-	102	C6H14O	000628-81-9	9		

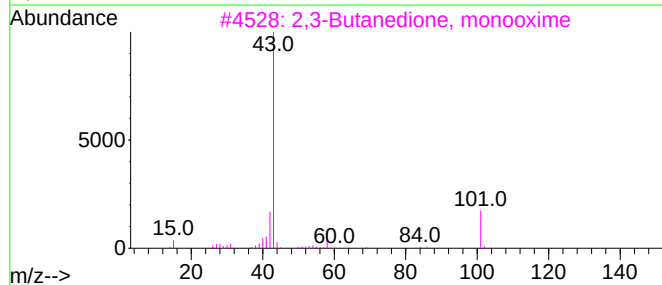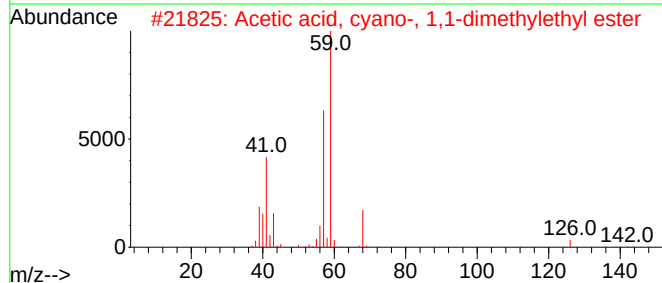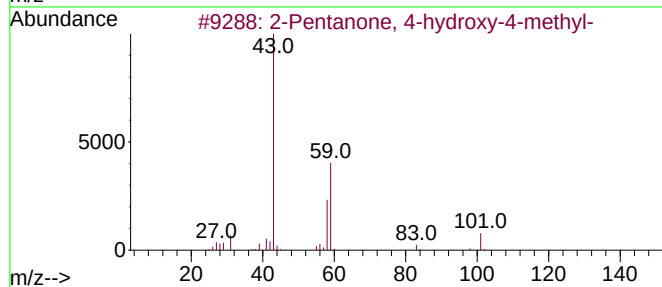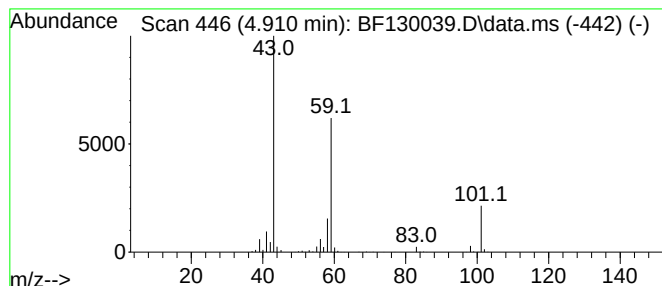

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082922\
Data File : BF130039.D
Acq On : 29 Aug 2022 17:39
Operator : CG\JU
Sample : N4379-21
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
EQUIP-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.910	28.6	ng	1062500	1	6.698	742762	20.0