


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082922\
 Data File : BF130031.D
 Acq On : 29 Aug 2022 11:53
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 30 01:22:56 2022

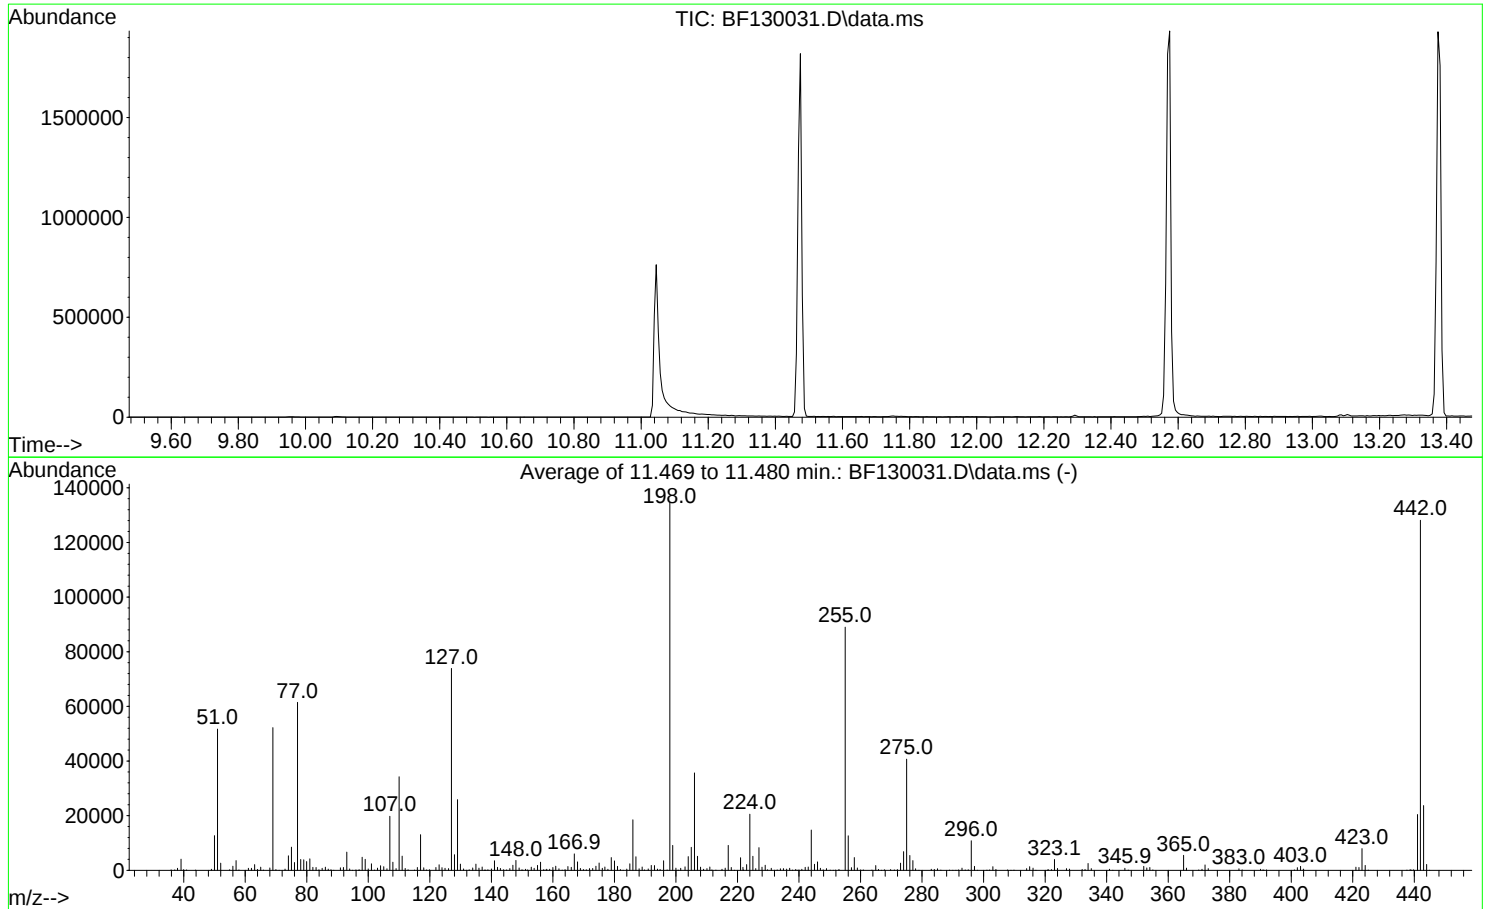




AutoFind: Scans 1561, 1562, 1563; Background Corrected with Scan 1556

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.4	51686	PASS
68	69	0.00	2	1.6	850	PASS
69	198	0.00	100	38.8	52235	PASS
70	69	0.00	2	0.5	265	PASS
127	198	10	80	54.9	73859	PASS
197	198	0.00	2	0.1	180	PASS
198	198	100	100	100.0	134645	PASS
199	198	5	9	6.8	9089	PASS
275	198	10	60	30.2	40707	PASS
365	198	1	100	4.1	5464	PASS
441	198	0.01	100	15.1	20390	PASS
442	442	50	100	100.0	128115	PASS
443	442	15	24	18.5	23686	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082922\
Data File : BF130031.D
Acq On : 29 Aug 2022 11:53
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 30 05:26:23 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 30 01:22:56 2022
Response via : Initial Calibration

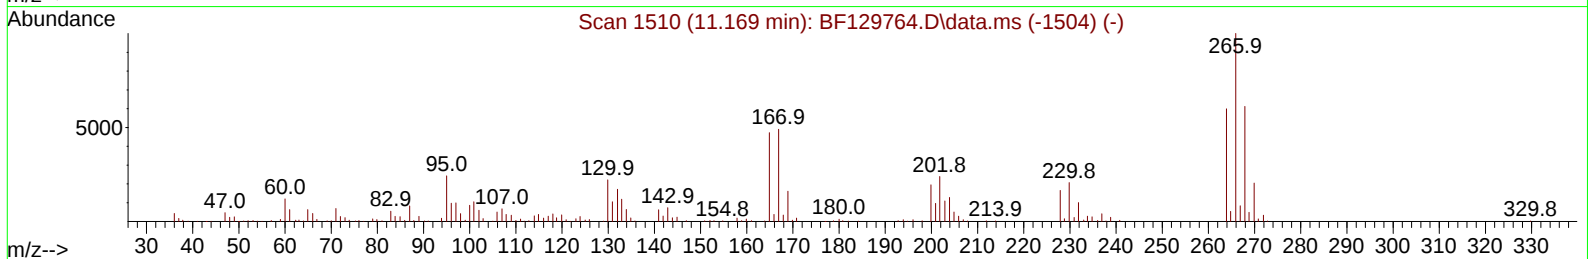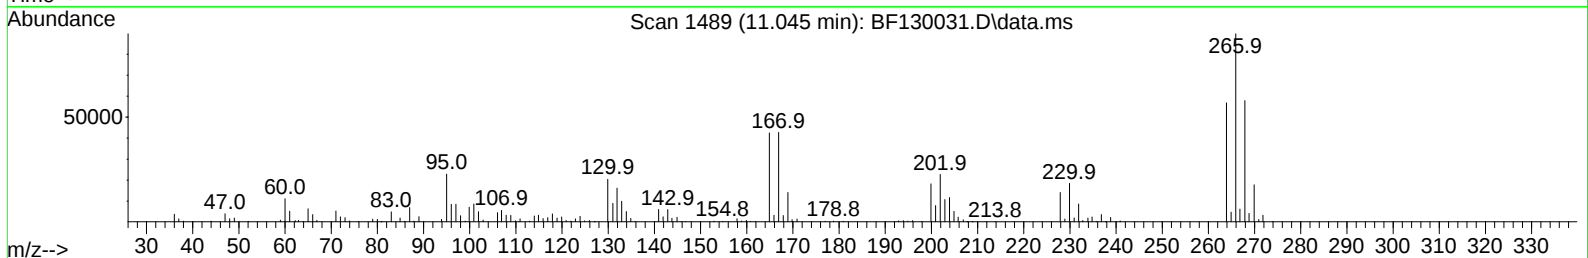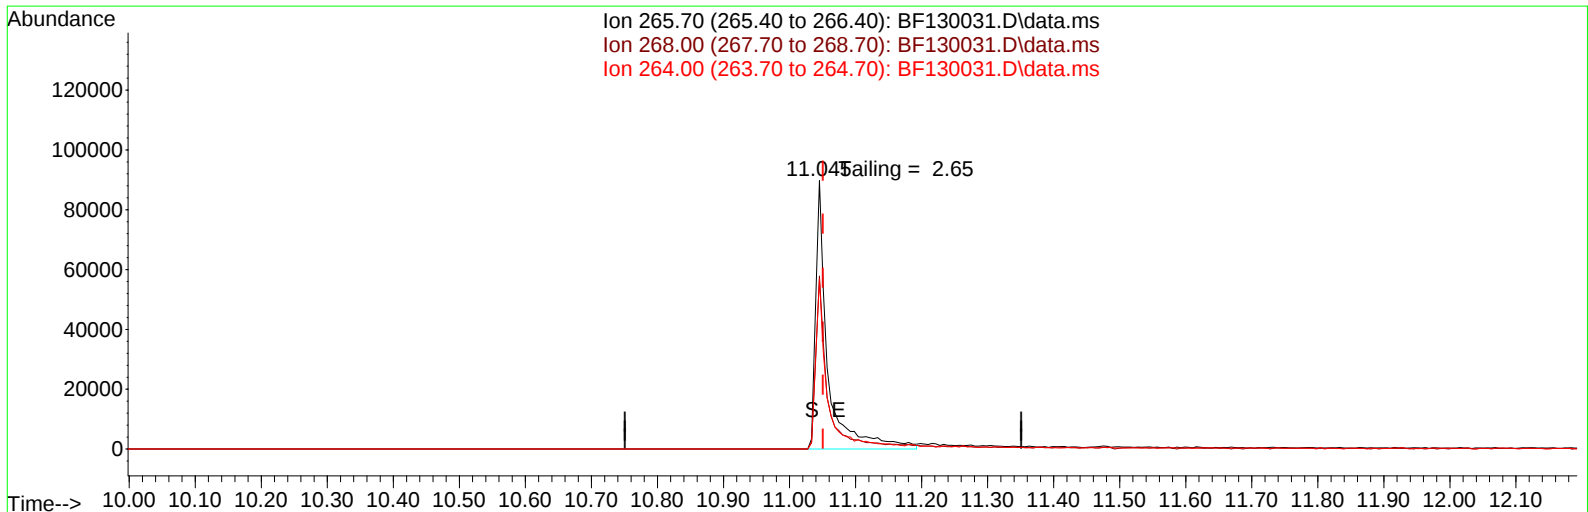

TIC: BF130031.D\data.ms

(70) Pentachlorophenol (C)

11.045min (-0.006) 521209.48 ng




response 116571

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	64.47
264.00	59.90	63.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082922\
Data File : BF130031.D
Acq On : 29 Aug 2022 11:53
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 30 05:26:23 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 30 01:22:56 2022
Response via : Initial Calibration

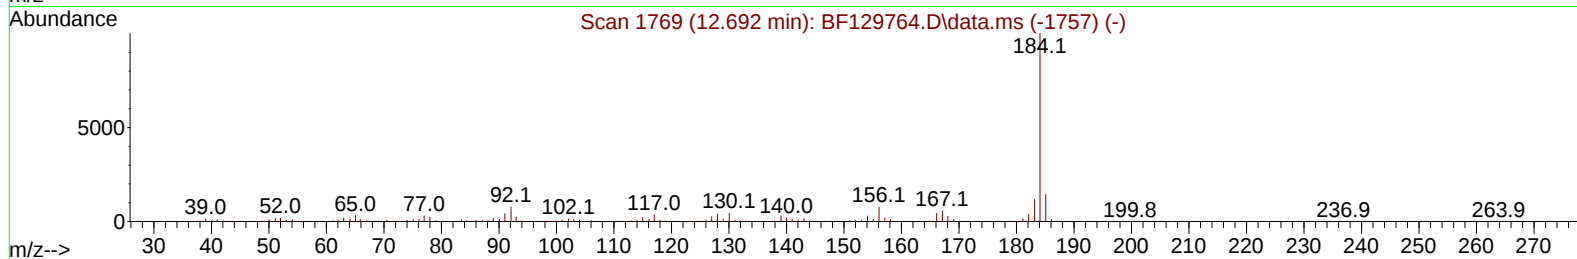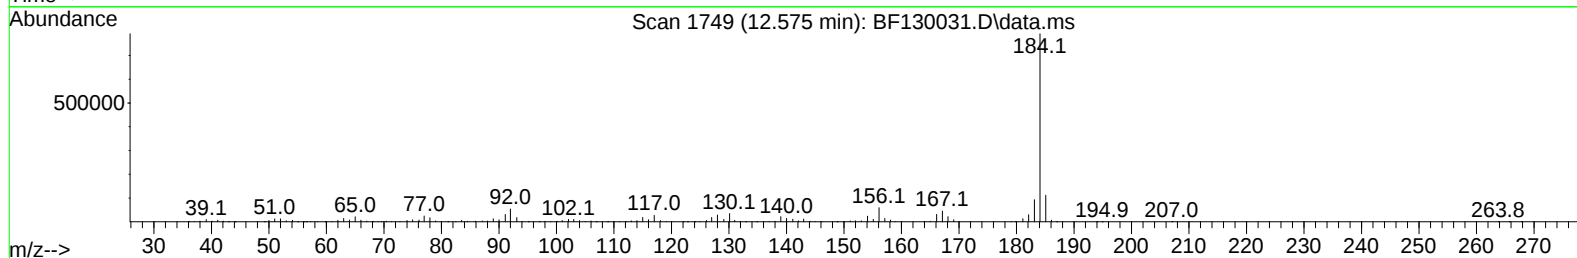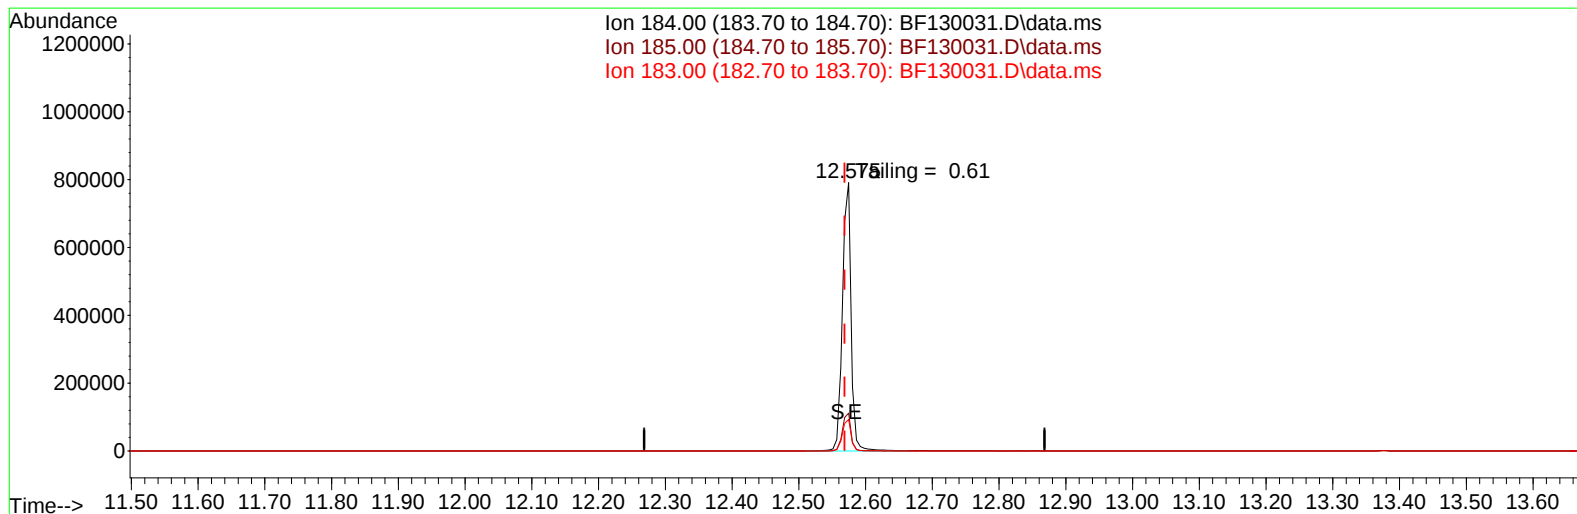

TIC: BF130031.D\data.ms

(77) Benzidine

12.575min (+ 0.006) 0.00 ng

response 718960

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.14
183.00	11.80	11.77
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/29/2022	BNA_F	<u>BF130031.D</u>
Compound Name	Response	Retention Time
DDT	325747	13.38
DDD	3661	13.104
DDE	1511	12.745
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5172	330919	1.56

Instrument :
BNA_F
ClientSampleId :
DFTPP