
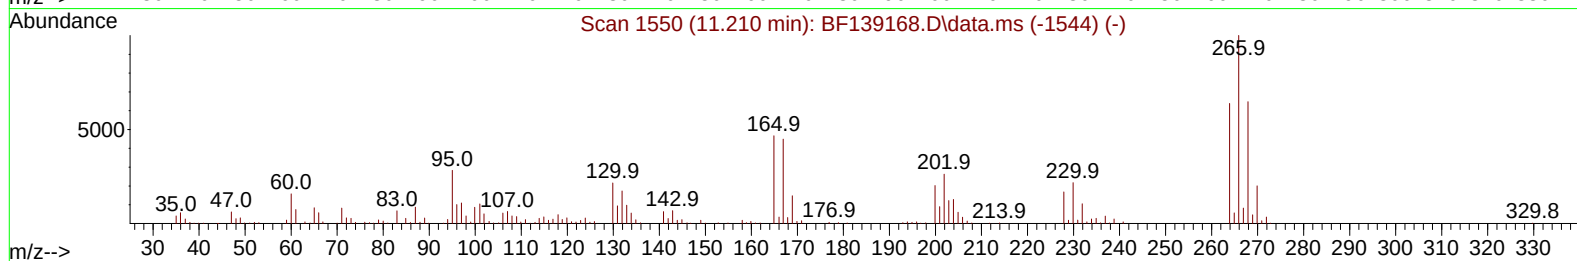
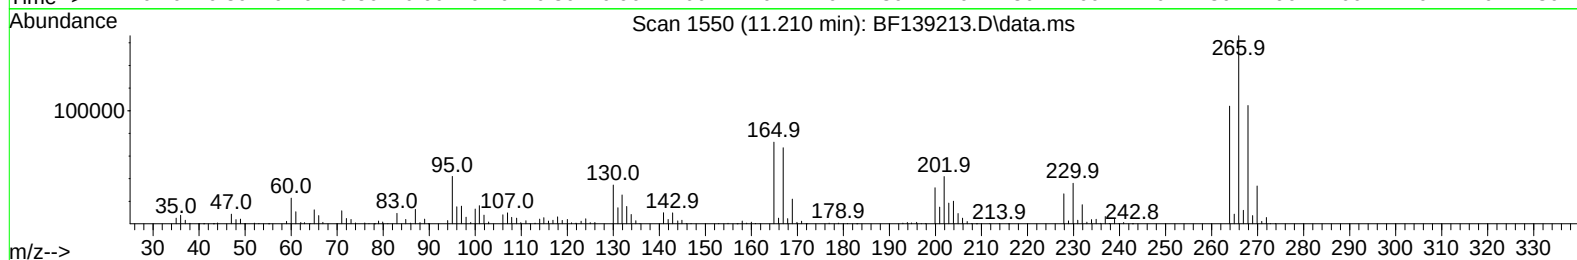


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082924\
Data File : BF139213.D
Acq On : 29 Aug 2024 08:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 29 12:09:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 27 02:51:47 2024
Response via : Initial Calibration

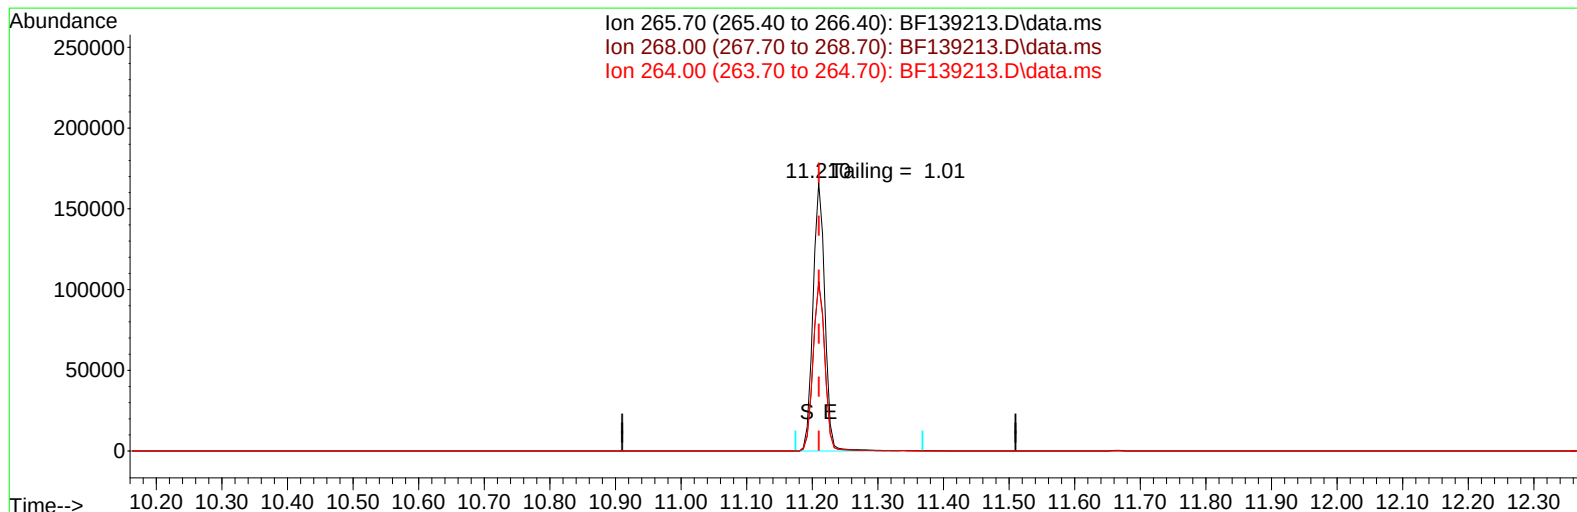

TIC: BF139213.D\data.ms

(70) Pentachlorophenol (C)




11.210min (-0.000) 35146.67 ng

response 210464

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.80	62.95
264.00	63.80	62.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082924\
Data File : BF139213.D
Acq On : 29 Aug 2024 08:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 29 12:09:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 27 02:51:47 2024
Response via : Initial Calibration

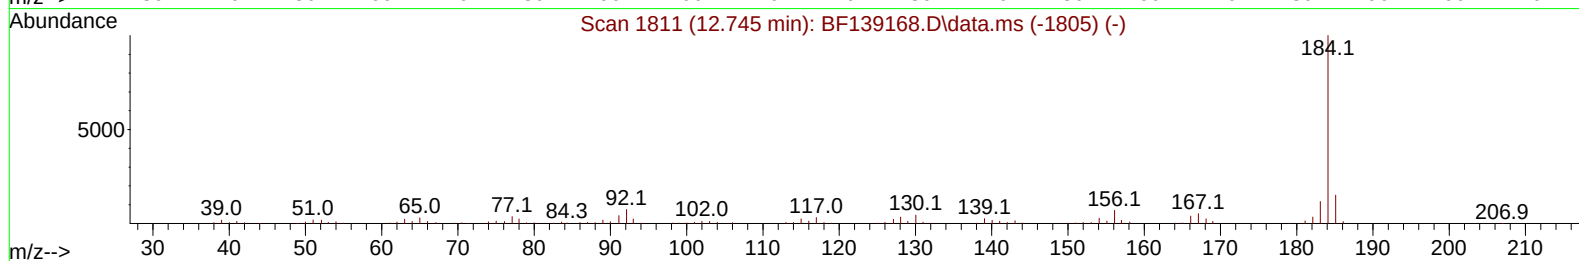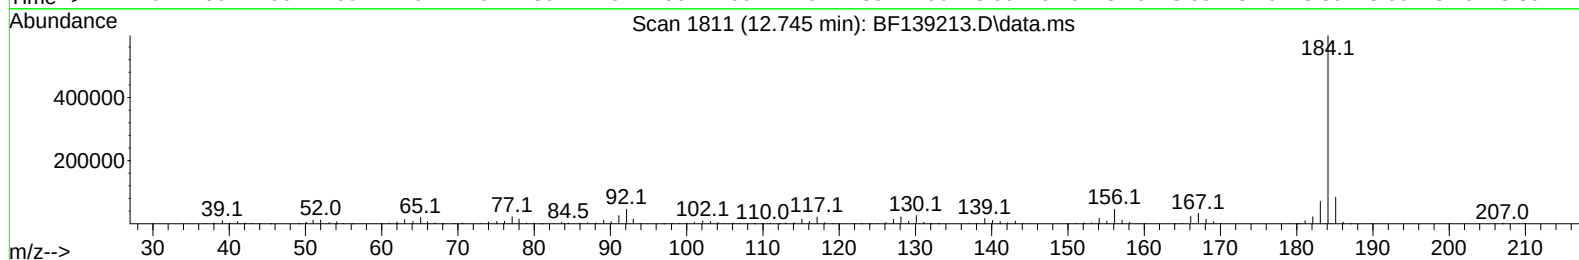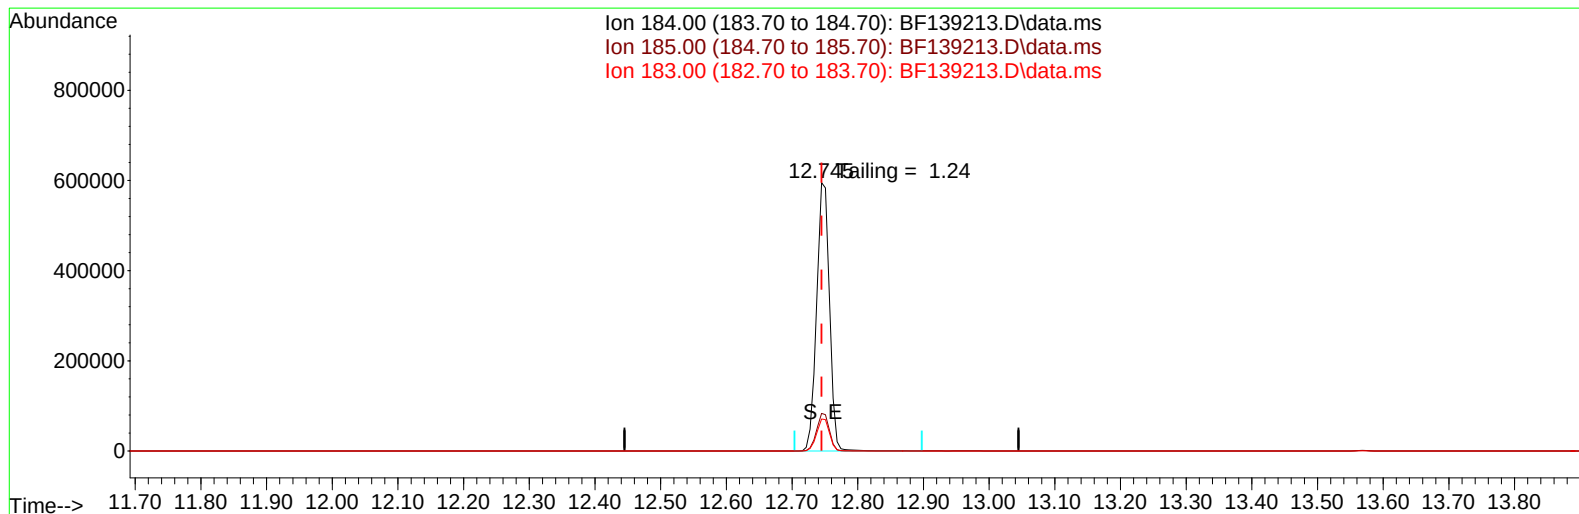

TIC: BF139213.D\data.ms

(77) Benzidine

12.745min (0.000) 0.00 ng

response 816411

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.04
183.00	11.70	11.95
0.00	0.00	0.00