

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082924\
 Data File : BF139224.D
 Acq On : 29 Aug 2024 16:36
 Operator : RC/JU
 Sample : PB163024BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB163024BL

Quant Time: Aug 29 17:02:46 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 29 15:46:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.887	152	98348	20.000	ng	0.00
21) Naphthalene-d8	8.169	136	380318	20.000	ng	0.00
39) Acenaphthene-d10	9.922	164	220485	20.000	ng	0.00
64) Phenanthrene-d10	11.410	188	397900	20.000	ng	0.00
76) Chrysene-d12	14.045	240	241971	20.000	ng	0.00
86) Perylene-d12	15.516	264	188854	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.516	112	860866	140.319	ng	0.01
7) Phenol-d6	6.516	99	1124148	138.127	ng	0.00
23) Nitrobenzene-d5	7.446	82	759495	95.997	ng	0.00
42) 2,4,6-Tribromophenol	10.710	330	326929	147.821	ng	0.00
45) 2-Fluorobiphenyl	9.245	172	1313313	92.745	ng	0.00
79) Terphenyl-d14	12.998	244	1571927	93.642	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082924\
Data File : BF139224.D
Acq On : 29 Aug 2024 16:36
Operator : RC/JU
Sample : PB163024BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB163024BL


Quant Time: Aug 29 17:02:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 29 15:46:29 2024
Response via : Initial Calibration

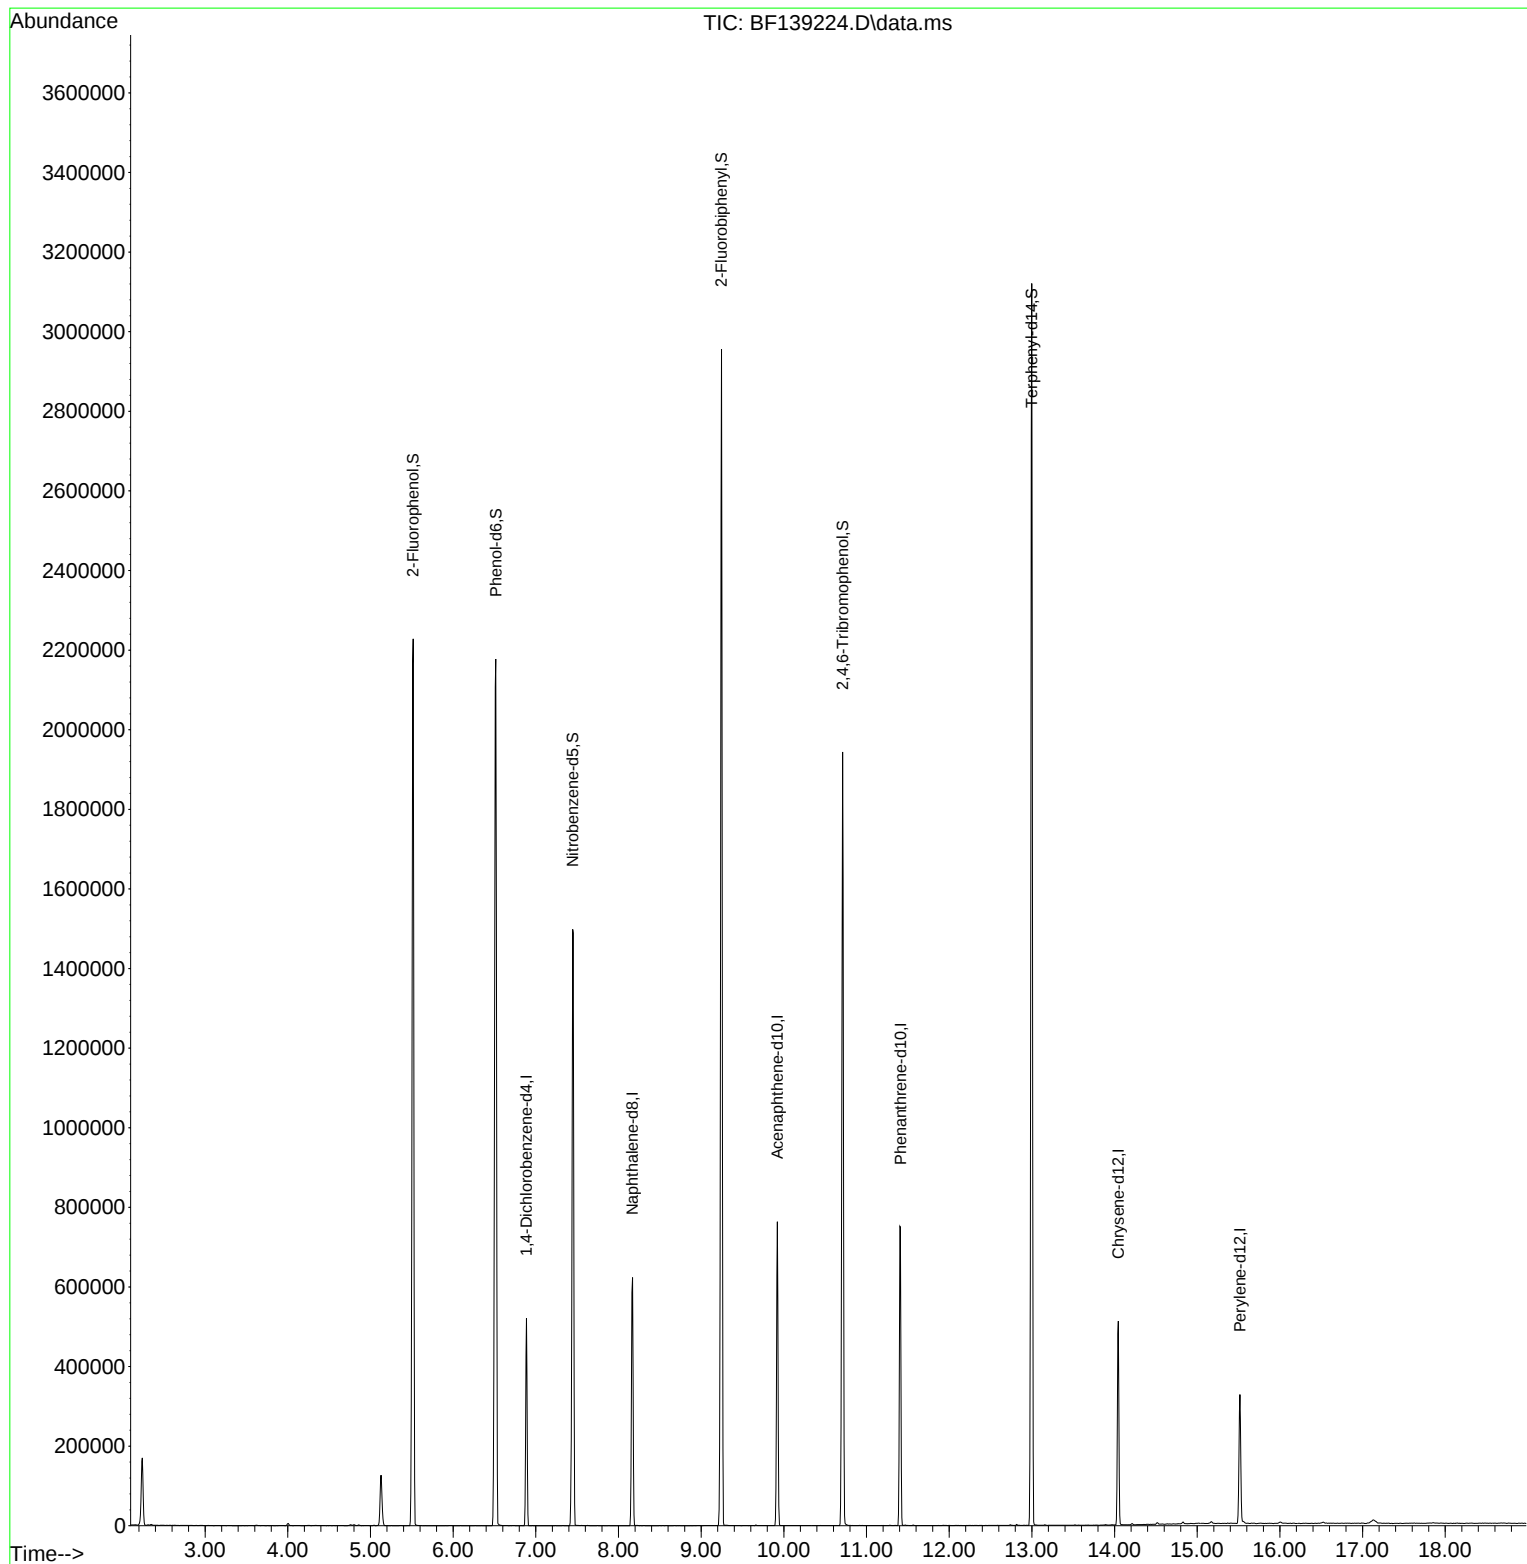



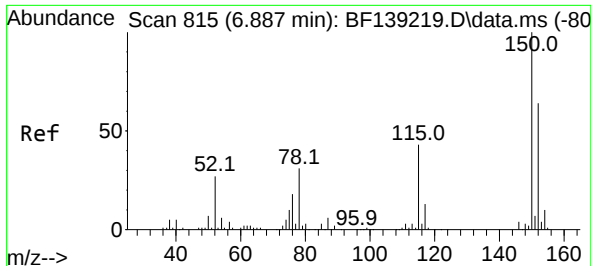


#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.887 min Scan# 815
Delta R.T. -0.000 min
Lab File: BF139224.D
Acq: 29 Aug 2024 16:36

Instrument :
BNA_F
ClientSampleId :
PB163024BL



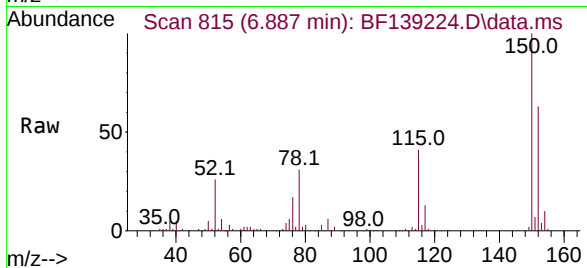



Tgt Ion:152 Resp: 98348
Ion Ratio Lower Upper
152 100
150 159.2 125.6 188.4
115 66.0 54.2 81.4

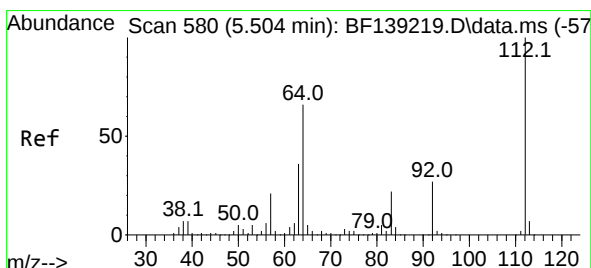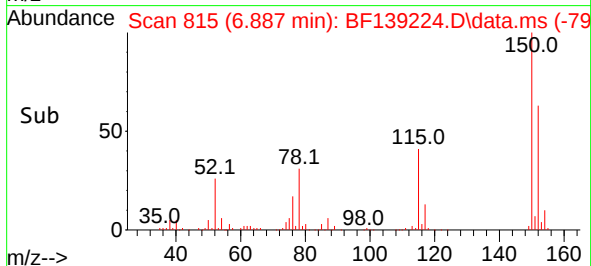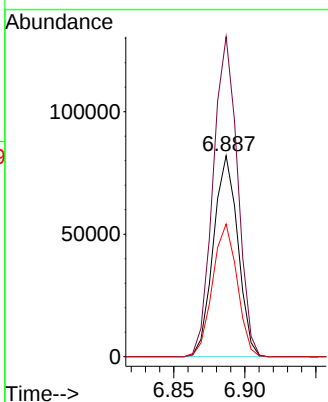

#5
2-Fluorophenol
Concen: 140.319 ng
RT: 5.516 min Scan# 582
Delta R.T. 0.012 min
Lab File: BF139224.D
Acq: 29 Aug 2024 16:36

Tgt Ion:112 Resp: 860866
Ion Ratio Lower Upper
112 100
64 65.0 52.5 78.7
63 35.2 28.5 42.7


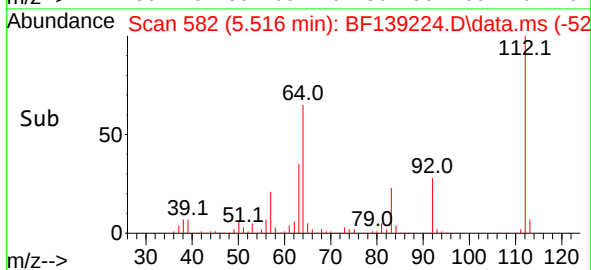
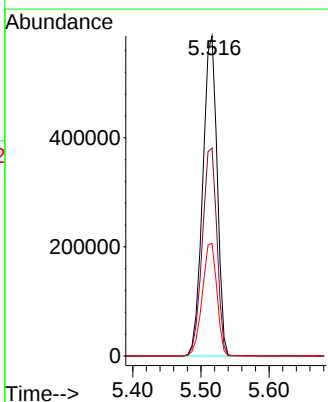
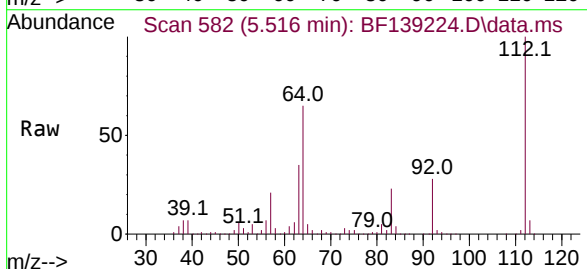


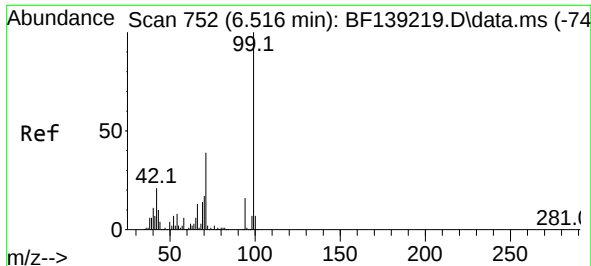

#7
Phenol-d6
Concen: 138.127 ng
RT: 6.516 min Scan# 71
Delta R.T. 0.000 min
Lab File: BF139224.D
Acq: 29 Aug 2024 16:36




Instrument :
BNA_F
ClientSampleId :
PB163024BL


Tgt Ion: 99 Resp: 1124148
Ion Ratio Lower Upper
99 100
42 21.0 16.8 25.2
71 39.6 31.3 46.9

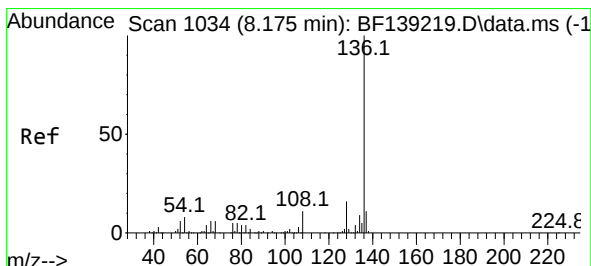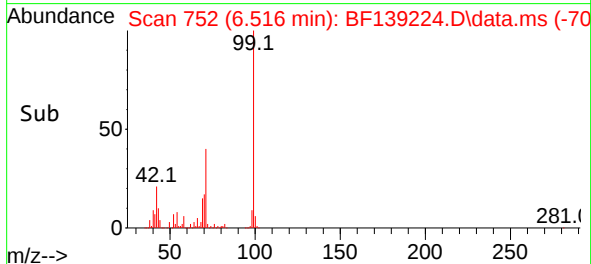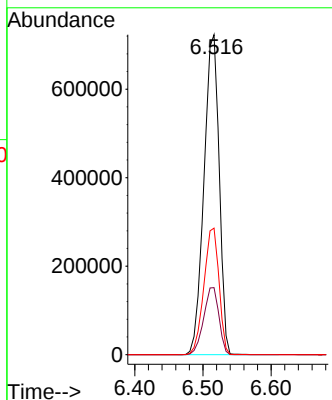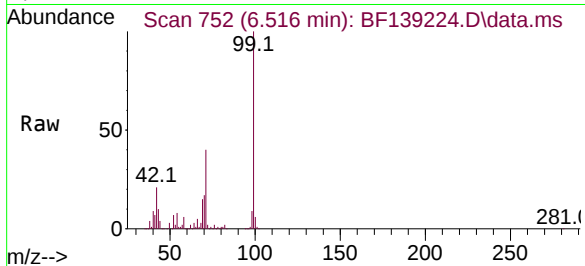

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.169 min Scan# 1033
Delta R.T. -0.006 min
Lab File: BF139224.D
Acq: 29 Aug 2024 16:36

Tgt Ion: 136 Resp: 380318
Ion Ratio Lower Upper
136 100
137 10.8 8.7 13.1
54 8.6 6.9 10.3
68 6.1 4.8 7.2

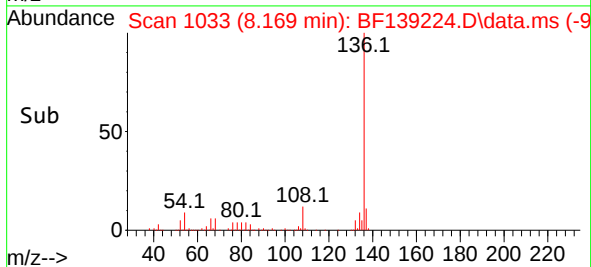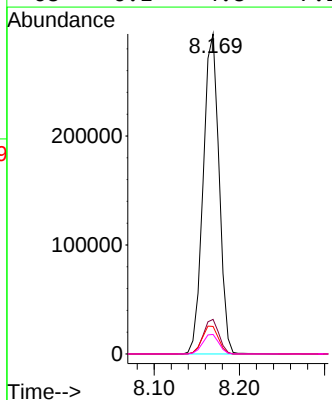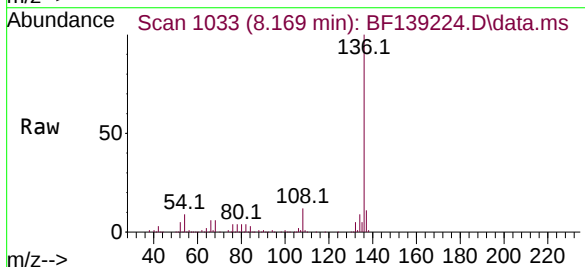

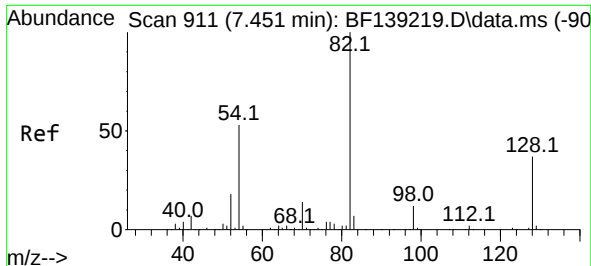

#23

Nitrobenzene-d5

Concen: 95.997 ng

RT: 7.446 min Scan# 911

Delta R.T. -0.006 min

Lab File: BF139224.D

Acq: 29 Aug 2024 16:36

Instrument :

BNA_F

ClientSampleId :

PB163024BL





Tgt Ion: 82 Resp: 759495

Ion Ratio Lower Upper

82 100

128 36.9 29.4 44.2

54 53.2 42.4 63.6

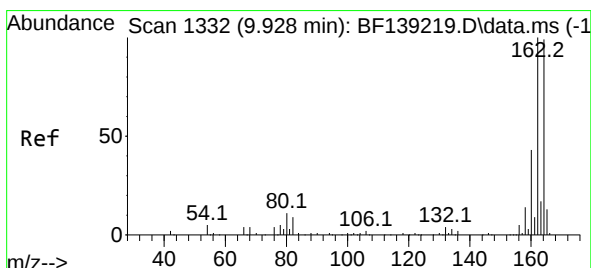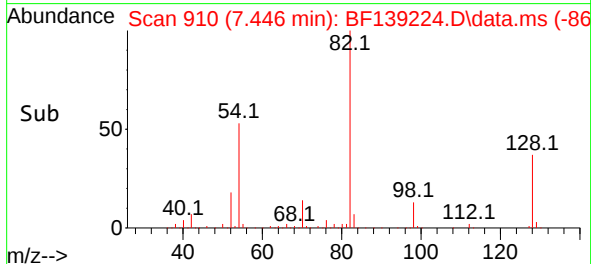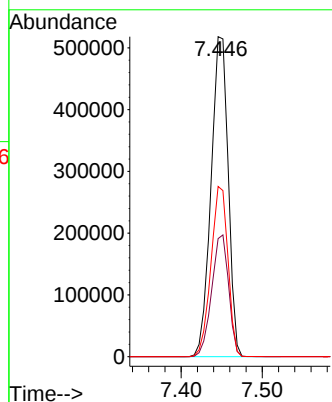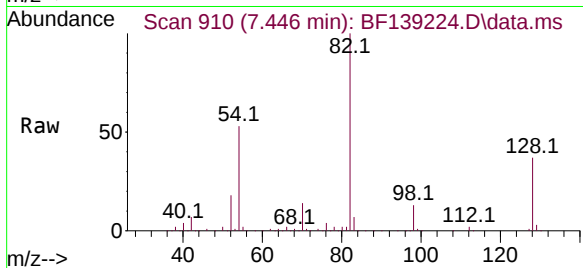

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.922 min Scan# 1331

Delta R.T. -0.006 min

Lab File: BF139224.D

Acq: 29 Aug 2024 16:36




Tgt Ion:164 Resp: 220485


Ion Ratio Lower Upper

164 100

162 99.2 80.8 121.2

160 43.1 34.4 51.6

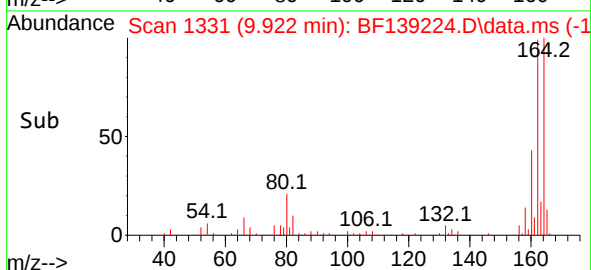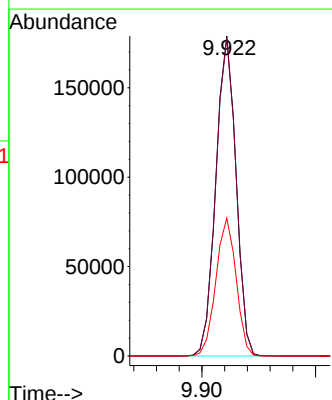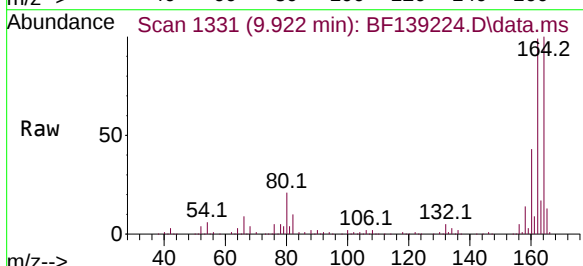

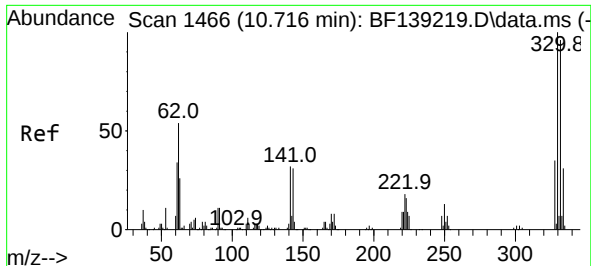

#42

2,4,6-Tribromophenol

Concen: 147.821 ng

RT: 10.710 min Scan# 1466

Delta R.T. -0.006 min

Lab File: BF139224.D


Acq: 29 Aug 2024 16:36

Instrument :

BNA_F

ClientSampleId :

PB163024BL

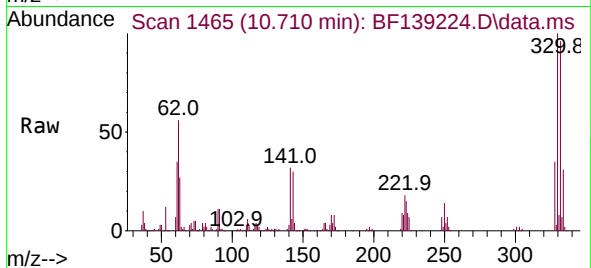




Tgt Ion:330 Resp: 326929

Ion Ratio Lower Upper

330 100

332 96.4 76.6 114.8

141 31.3 26.9 40.3

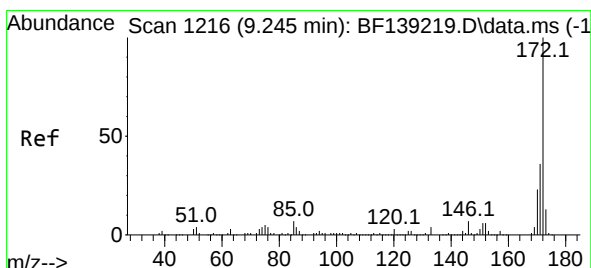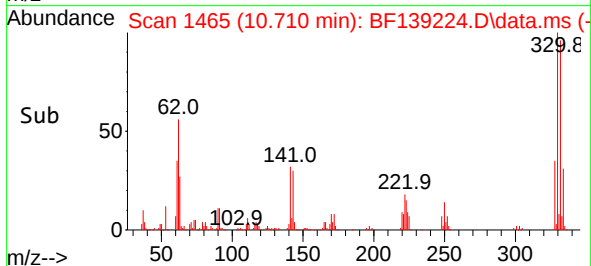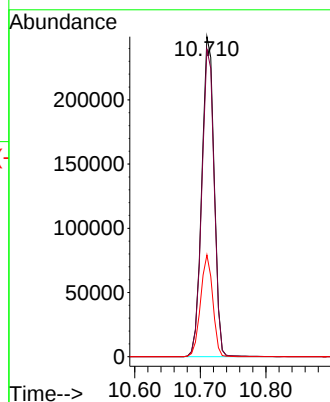

#45

2-Fluorobiphenyl

Concen: 92.745 ng

RT: 9.245 min Scan# 1216

Delta R.T. 0.000 min

Lab File: BF139224.D

Acq: 29 Aug 2024 16:36




Tgt Ion:172 Resp: 1313313


Ion Ratio Lower Upper

172 100

171 35.6 28.7 43.1

170 23.6 18.7 28.1

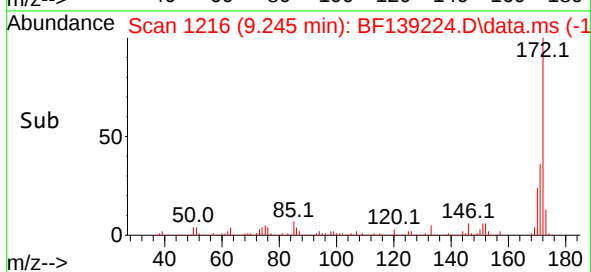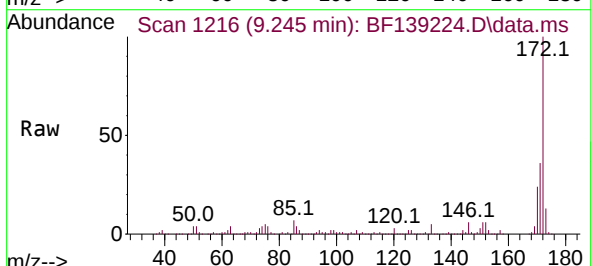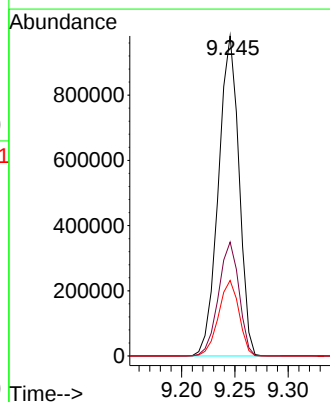

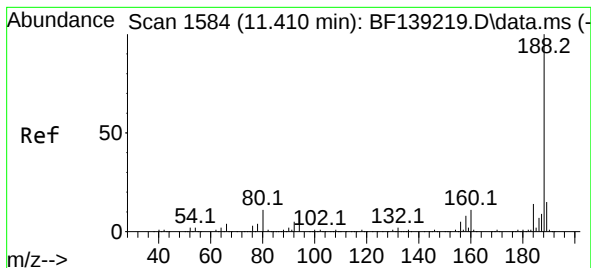

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.410 min Scan# 1

Delta R.T. 0.000 min

Lab File: BF139224.D


Acq: 29 Aug 2024 16:36

Instrument :

BNA_F

ClientSampleId :

PB163024BL

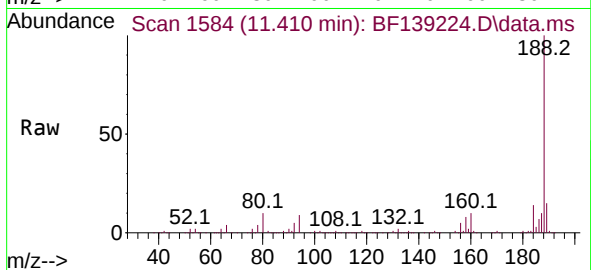




Tgt Ion:188 Resp: 397900

Ion Ratio Lower Upper

188 100

94 8.7 7.4 11.2

80 10.1 8.6 12.8

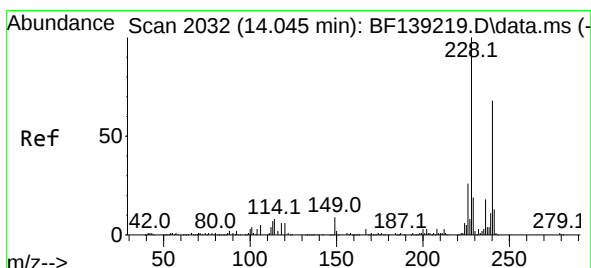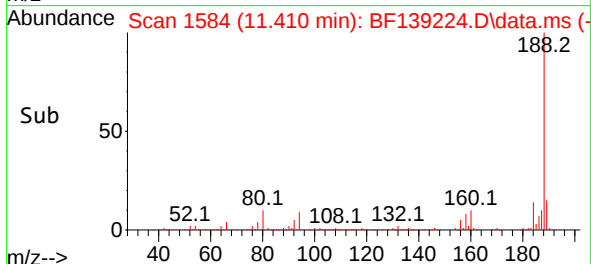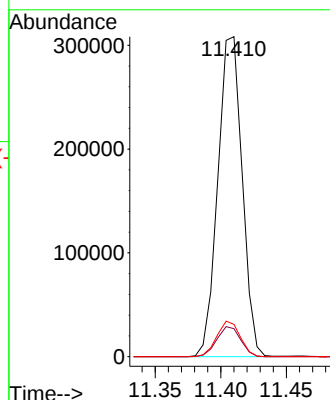

#76

Chrysene-d12

Concen: 20.000 ng

RT: 14.045 min Scan# 2032

Delta R.T. 0.000 min

Lab File: BF139224.D

Acq: 29 Aug 2024 16:36




Tgt Ion:240 Resp: 241971


Ion Ratio Lower Upper

240 100

120 8.5 7.4 11.2


236 25.3 20.9 31.3

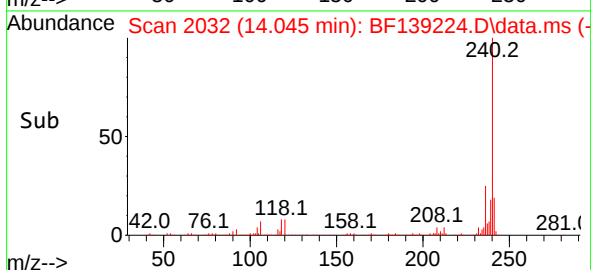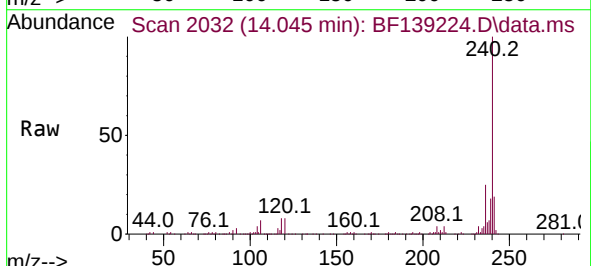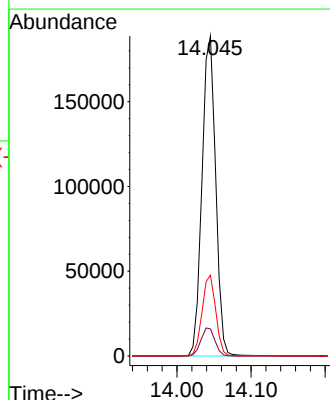



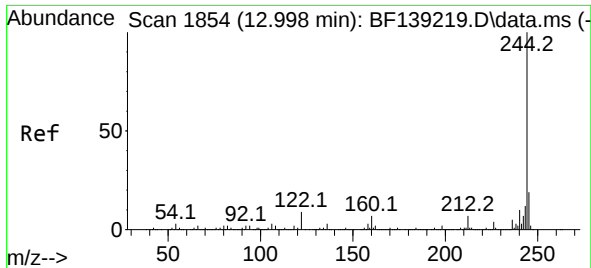


#79
Terphenyl-d14
Concen: 93.642 ng
RT: 12.998 min Scan# 11
Delta R.T. 0.000 min
Lab File: BF139224.D
Acq: 29 Aug 2024 16:36

Instrument :
BNA_F
ClientSampleId :
PB163024BL

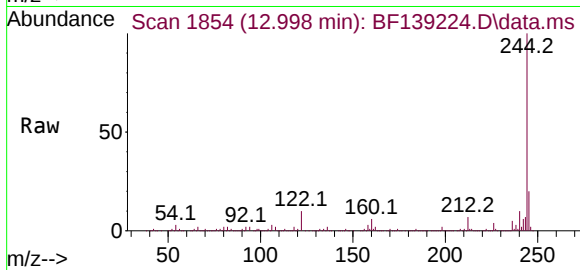

Tgt Ion:244 Resp: 1571927
Ion Ratio Lower Upper
244 100
212 7.0 5.7 8.5
122 9.6 7.4 11.2

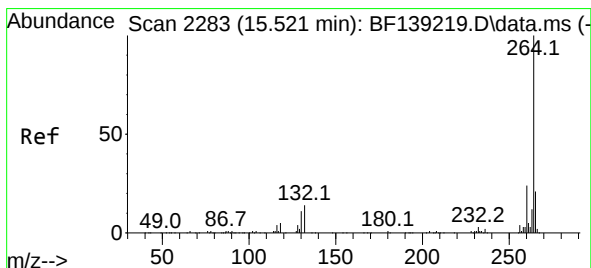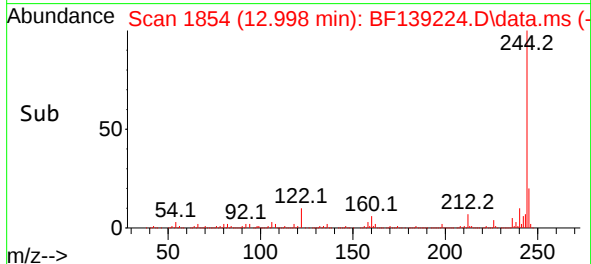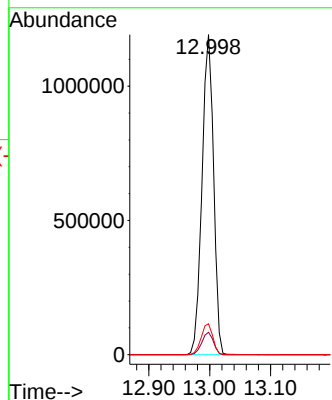

#86
Perylene-d12
Concen: 20.000 ng
RT: 15.516 min Scan# 2282
Delta R.T. -0.006 min
Lab File: BF139224.D
Acq: 29 Aug 2024 16:36

Tgt Ion:264 Resp: 188854
Ion Ratio Lower Upper
264 100
260 22.7 18.8 28.2
265 21.2 16.9 25.3

