
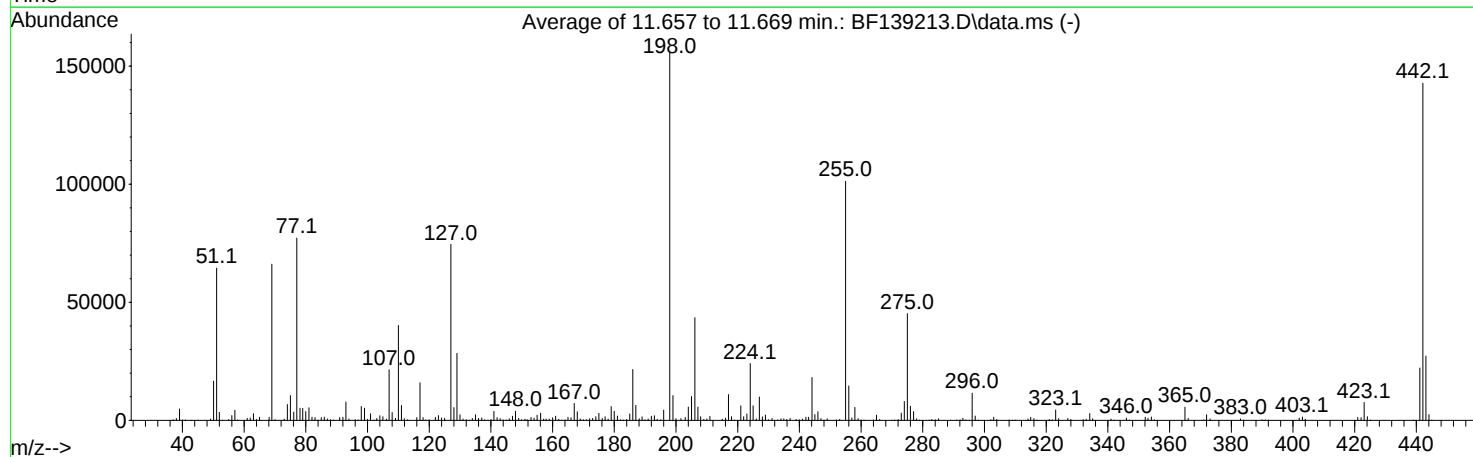


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082924\
Data File : BF139213.D
Acq On : 29 Aug 2024 08:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 29 15:46:29 2024

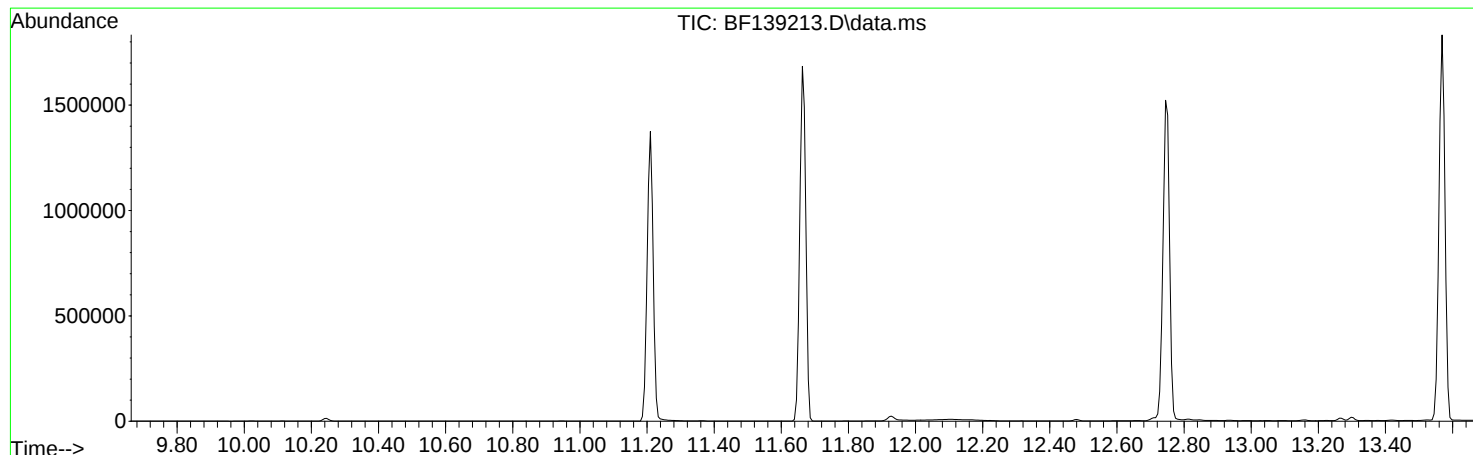

AutoFind: Scans 1626, 1627, 1628; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.4	64421	PASS
68	69	0.00	2	1.9	1267	PASS
69	198	0.00	100	42.4	66112	PASS
70	69	0.00	2	0.5	330	PASS
127	198	10	80	47.8	74515	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	155787	PASS
199	198	5	9	6.7	10497	PASS
275	198	10	60	29.0	45184	PASS
365	198	1	100	3.6	5659	PASS
441	198	0.01	100	14.2	22184	PASS
442	442	50	100	100.0	142744	PASS
443	442	15	24	19.1	27272	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/29/2024	BNA_F	<u>BF139213.D</u>
Compound Name	Response	Retention Time
DDT	442999	13.568
DDD	8352	13.298
DDE	858	12.933
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9210	452209	2.04

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082924\
Data File : BF139213.D
Acq On : 29 Aug 2024 08:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 29 12:09:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 27 02:51:47 2024
Response via : Initial Calibration

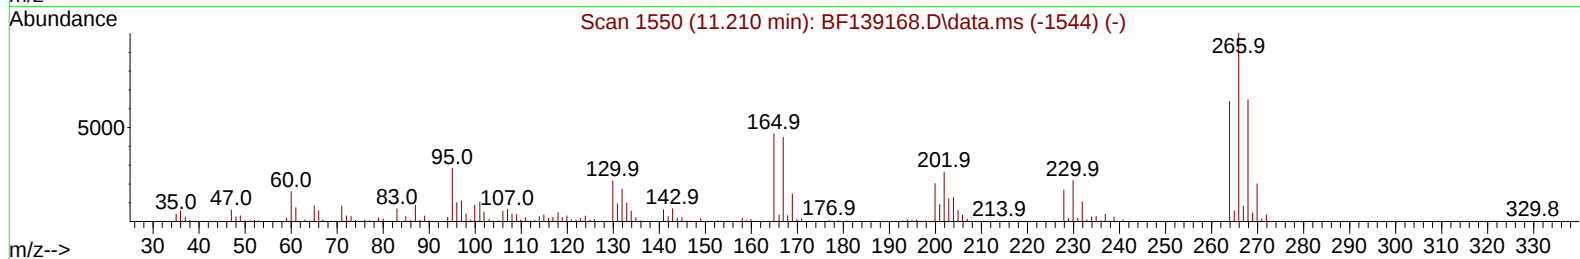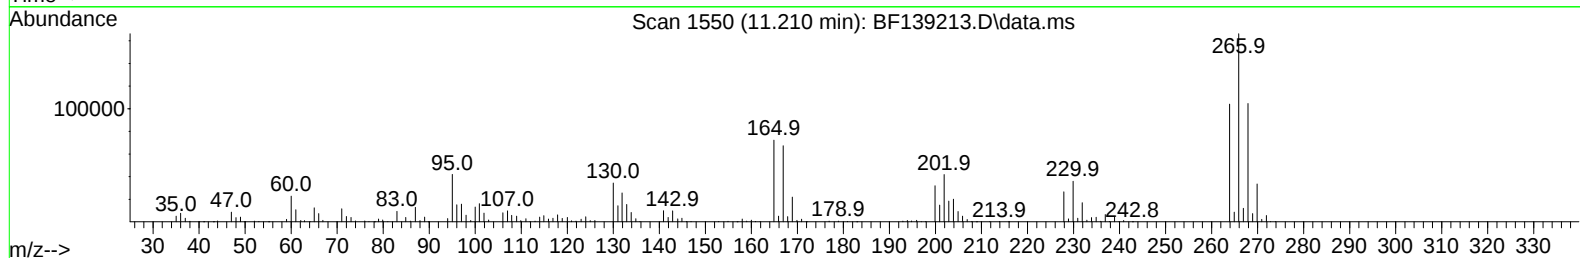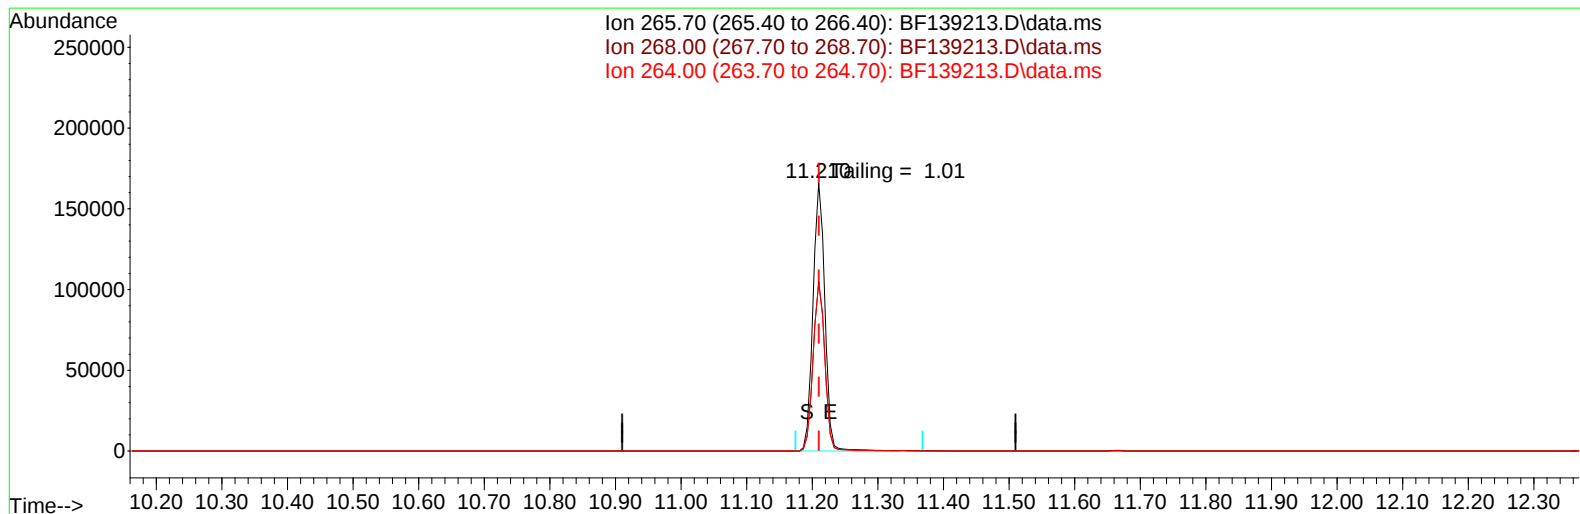

TIC: BF139213.D\data.ms

(70) Pentachlorophenol (C)

11.210min (-0.000) 35146.67 ng




response 210464

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.80	62.95
264.00	63.80	62.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082924\
Data File : BF139213.D
Acq On : 29 Aug 2024 08:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 29 12:09:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 27 02:51:47 2024
Response via : Initial Calibration

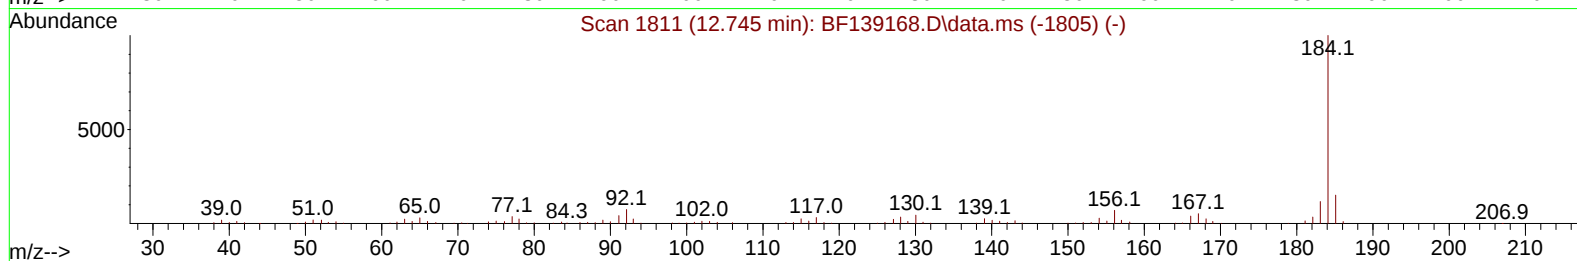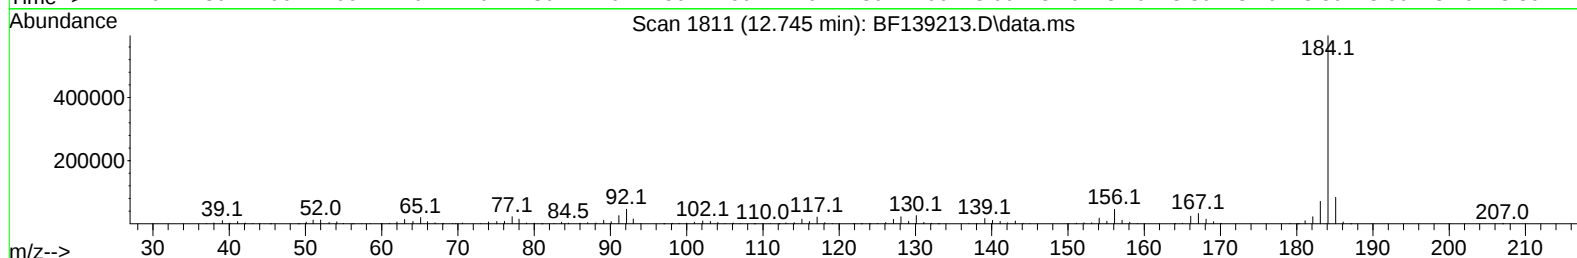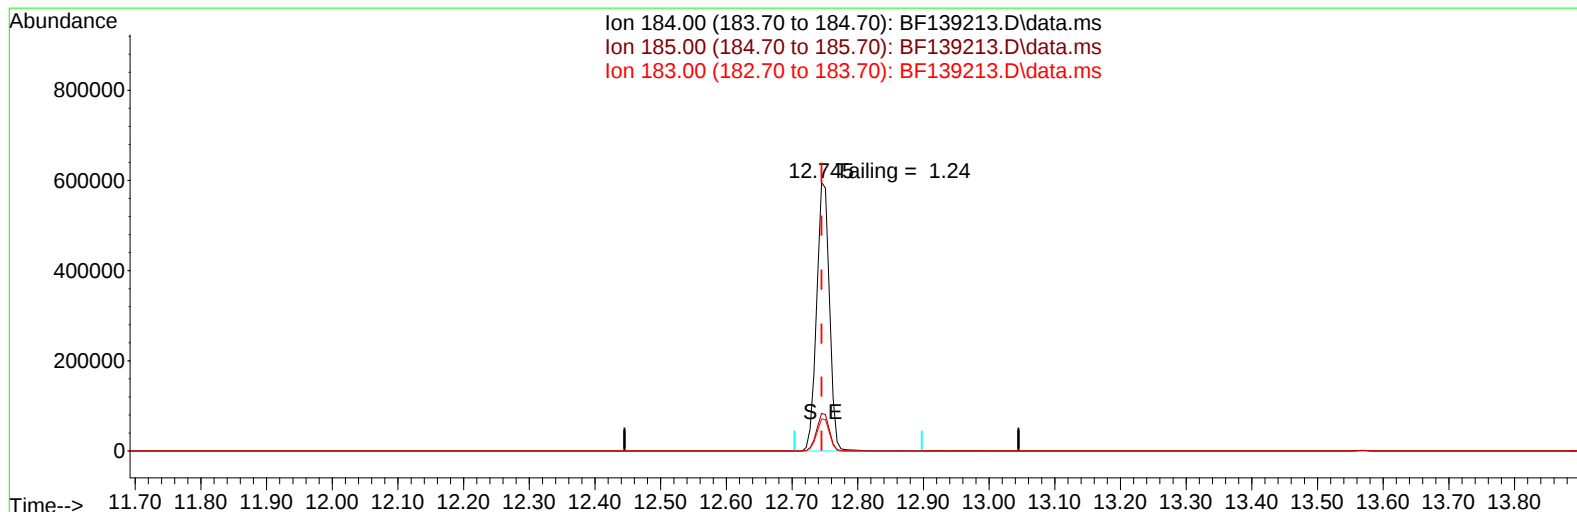

TIC: BF139213.D\data.ms

(77) Benzidine

12.745min (0.000) 0.00 ng

response 816411

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.04
183.00	11.70	11.95
0.00	0.00	0.00