

Data Path : Z:\HPCHEM1\BNA F\DATA\BF083017\
 Data File : BF08178.D
 Acq On : 31 Aug 2017 1:42
 Operator : SJ/JU
 Sample : I4979-02
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Aug 31 06:51:40 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 21 15:59:04 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.73	152	124687	20.00	ng	-0.02
21) Naphthalene-d8	8.01	136	454273	20.00	ng	-0.02
38) Acenaphthene-d10	9.76	164	170637	20.00	ng	-0.03
63) Phenanthrene-d10	11.24	188	277213	20.00	ng	-0.02
75) Chrysene-d12	13.87	240	260652	20.00	ng	-0.02
86) Perylene-d12	15.29	264	178818	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.34	112	933742	113.91	ng	-0.01
7) Phenol-d6	6.37	99	1235560	110.93	ng	-0.02
23) Nitrobenzene-d5	7.29	82	708674	84.75	ng	-0.03
41) 2,4,6-Tribromophenol	10.55	330	138965	93.86	ng	-0.02
44) 2-Fluorobiphenyl	9.09	172	722795	62.23	ng	-0.02
78) Terphenyl-d14	12.83	244	452169	36.18	ng	-0.02
Target Compounds						Qvalue
10) Phenol	6.38	94	52910	4.062	ng	87
17) 2-Methylphenol	7.15	107	18006	2.364	ng	87
19) n-Nitroso-di-n-propylamine	7.29	70	94456	12.389	ng	# 72
25) Isophorone	7.29	82	698609	40.178	ng	# 67
26) 2-Nitrophenol	7.70	139	266	5.328	ng	# 1
31) Naphthalene	8.03	128	401523	17.026	ng	99
32) Benzoic acid	7.80	122	9923	8.032	ng	# 26
33) 4-Chloroaniline	8.03	127	53113	5.340	ng	# 31
37) 2-Methylnaphthalene	8.72	142	46833	3.239	ng	97
49) Dimethylphthalate	9.48	163	225693	18.094	ng	99
51) Acenaphthene	9.79	154	162991	14.314	ng	98
53) 2,4-Dinitrophenol	10.05	184	241	10.320	ng	# 40
54) Dibenzofuran	9.96	168	157351	10.311	ng	# 98
57) Fluorene	10.30	166	152056	12.887	ng	99
64) 4,6-Dinitro-2-methylphenol	10.55	198	419	8.586	ng	# 1
66) 4-Bromophenyl-phenylether	10.55	248	9079	3.154	ng	# 1
70) Phenanthrene	11.26	178	185402	12.551	ng	99
71) Anthracene	11.32	178	87324	5.828	ng	99
74) Fluoranthene	12.45	202	114409	7.420	ng	99
77) Pvrene	12.68	202	91772	4.305	ng	98
88) Benzo(k)fluoranthene	14.89	252	21576	2.037	ng	# 86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF083017\
Data File : BF098178.D
Acq On : 31 Aug 2017 1:42
Operator : SJ/JU
Sample : I4979-02
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Aug 31 06:51:40 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 21 15:59:04 2017
Response via : Initial Calibration

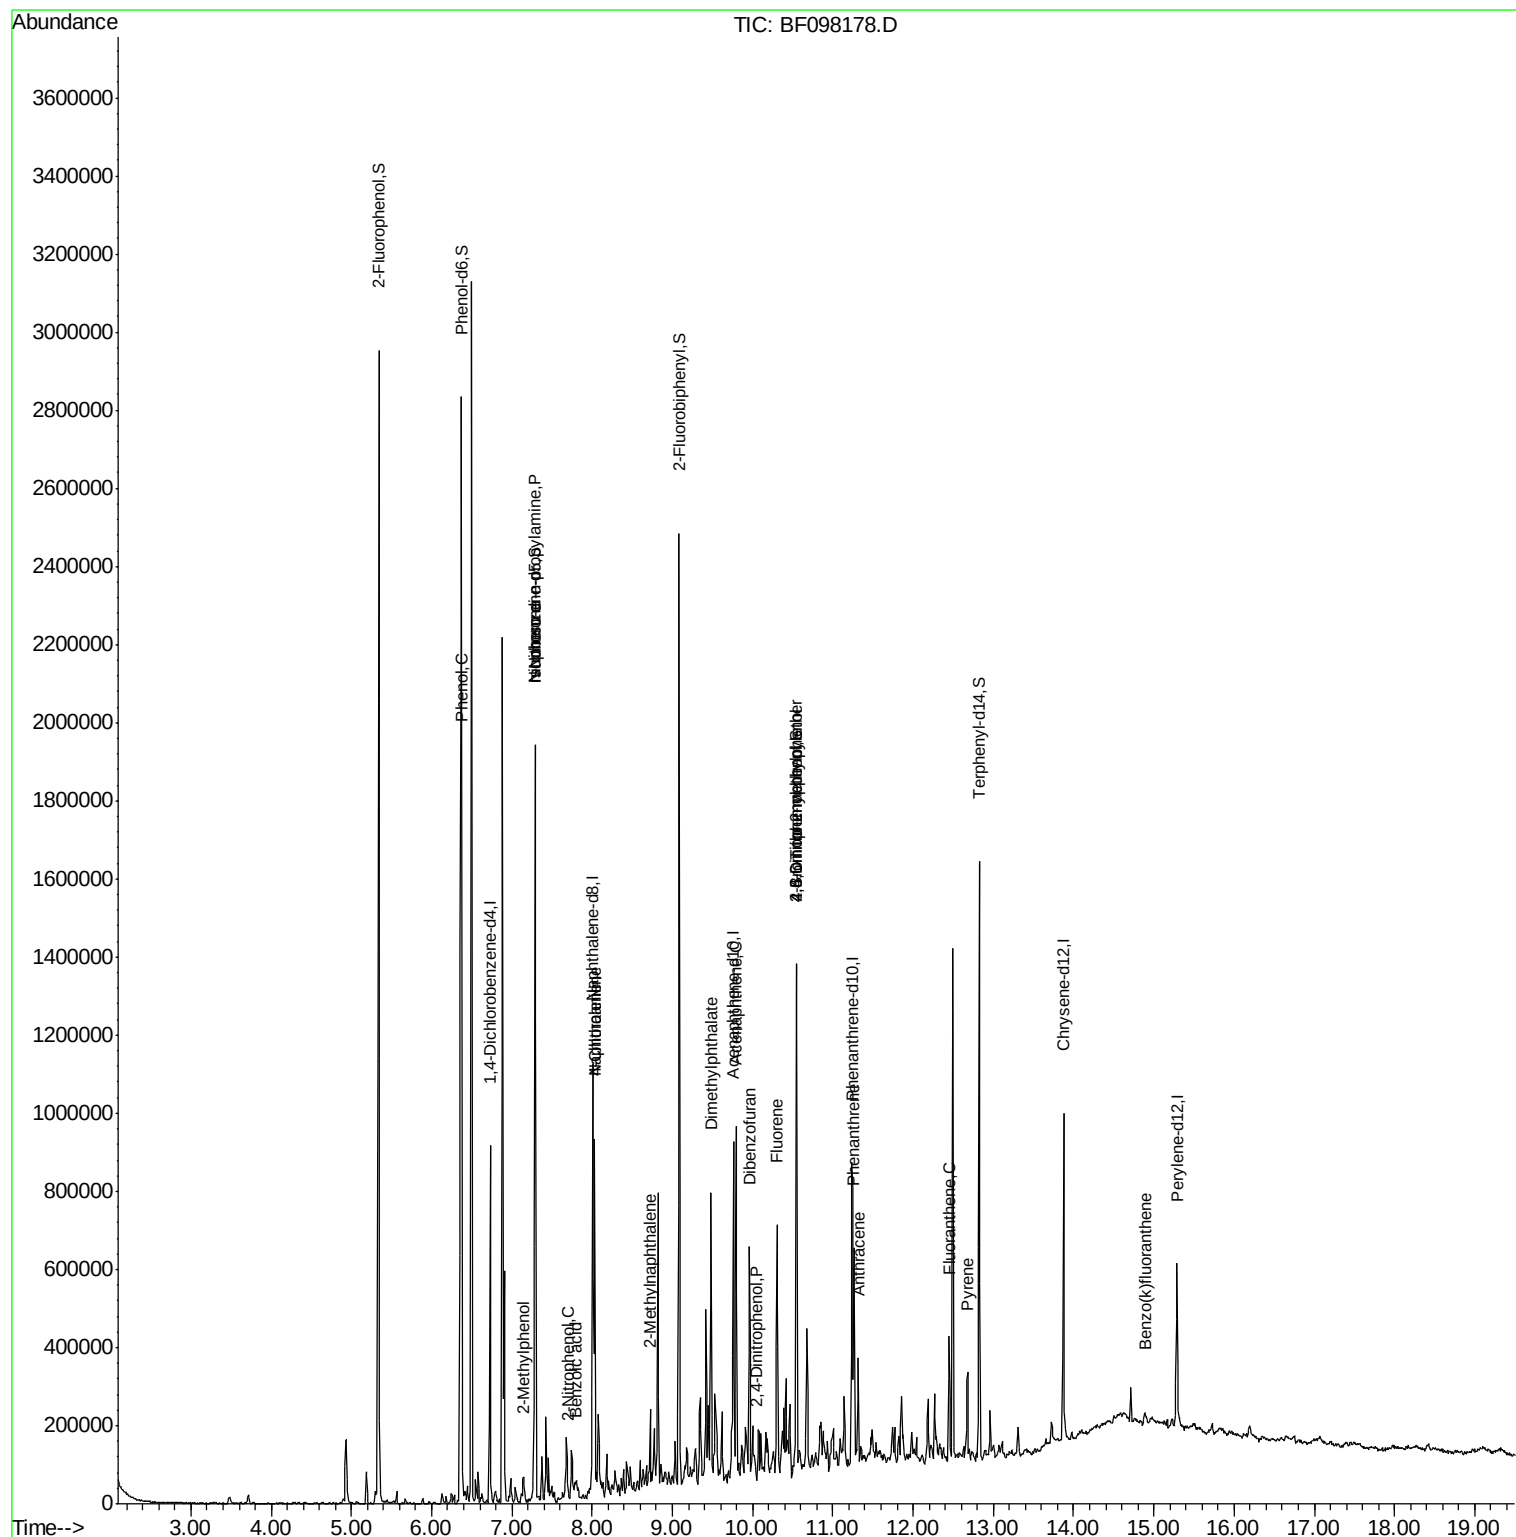

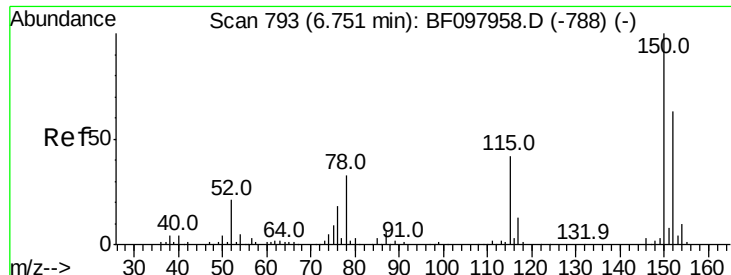


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.73 min Scan# 789
Delta R.T. -0.02 min
Lab File: BF098178.D
Acq: 31 Aug 2017 1:42

Instrument :
BNA_F
ClientSampleId :

Tot Ion:152 Resp: 124687
Ion Ratio Lower Upper
152 100
150 158.4 126.2 189.2
115 62.0 52.2 78.2




Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

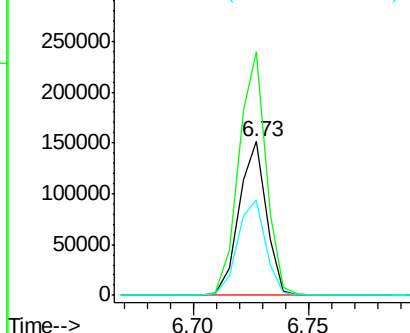



#5


2-Fluorophenol
Concen: 113.908 ng
RT: 5.34 min Scan# 553
Delta R.T. -0.01 min
Lab File: BF098178.D
Acq: 31 Aug 2017 1:42

Tgt Ion:112 Resp: 933742
Ion Ratio Lower Upper
112 100
64 59.4 46.0 69.0
63 29.4 23.4 35.0



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

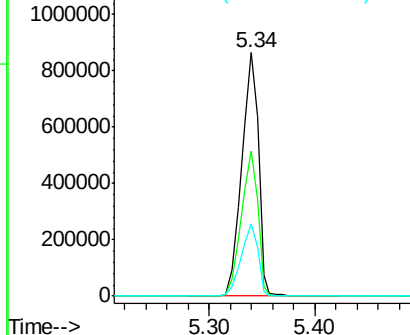



#7

Phenol-d6

Concen: 110.934 ng

RT: 6.37 min Scan# 728

Delta R.T. -0.02 min

Lab File: BF098178.D

Acq: 31 Aug 2017 1:42

Instrument :

BNA_F

ClientSampled :


Tot Ion: 99 Resp: 1235560

Ion Ratio Lower Upper




99 100

42 14.5 13.5 20.3

71 31.8 24.5 36.7



Abundance Ion 99.00 (98.70 to 99.70): BF0
Ion 42.00 (41.70 to 42.70): BF0
Ion 71.00 (70.70 to 71.70): BF0

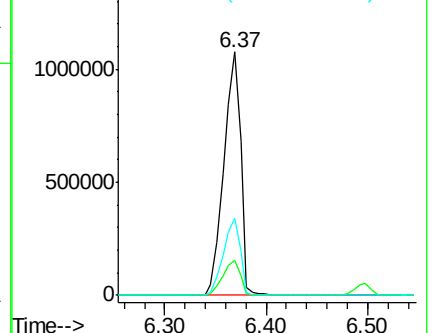

#10

Phenol

Concen: 4.062 ng

RT: 6.38 min Scan# 730

Delta R.T. -0.02 min

Lab File: BF098178.D

Acq: 31 Aug 2017 1:42


Tgt Ion: 94 Resp: 52910

Ion Ratio Lower Upper



94 100


65 25.7 9.9 49.9

66 32.8 23.1 63.1



Abundance Ion 94.00 (93.70 to 94.70): BF0
Ion 65.00 (64.70 to 65.70): BF0
Ion 66.00 (65.70 to 66.70): BF0

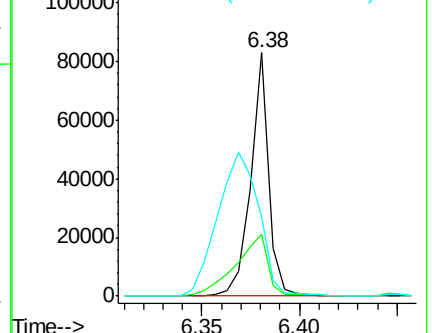

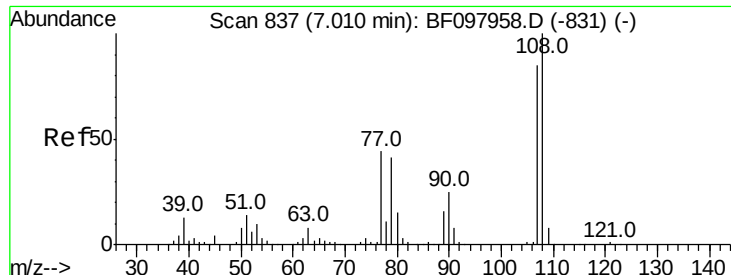

#17

2-Methylphenol

Concen: 2.364 ng

RT: 7.15 min Scan# 860


Delta R.T. 0.14 min

Lab File: BF098178.D




Acq: 31 Aug 2017 1:42

Instrument :
BNA_F
ClientSampleId :

Tot Ion:	107	Resp:	18006
Ion	Ratio	Lower	Upper
107	100		
108	98.4	93.4	140.0
77	42.4	35.8	53.6
79	35.1	34.8	52.2



Abundance Ion 107.00 (106.70 to 107.70): E
Ion 108.00 (107.70 to 108.70): E
Ion 77.00 (76.70 to 77.70): BF0
Ion 79.00 (78.70 to 79.70): BF0

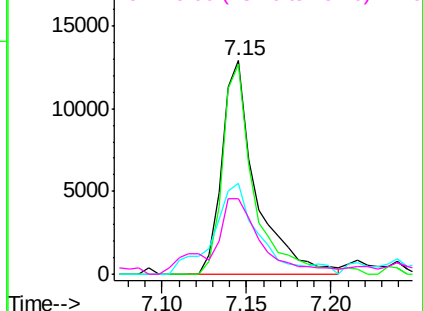

#19

n-Nitroso-di-n-propylamine

Concen: 12.389 ng


RT: 7.29 min Scan# 885

Delta R.T. 0.12 min



Lab File: BF098178.D


Acq: 31 Aug 2017 1:42

Tgt Ion:	70	Resp:	94456
Ion	Ratio	Lower	Upper
70	100		
42	40.5	47.2	70.8#
101	0.0	7.2	10.8#
130	2.1	15.9	23.9#



Abundance Ion 70.00 (69.70 to 70.70): BF0
Ion 42.00 (41.70 to 42.70): BF0
Ion 101.00 (100.70 to 101.70): E
Ion 130.00 (129.70 to 130.70): E

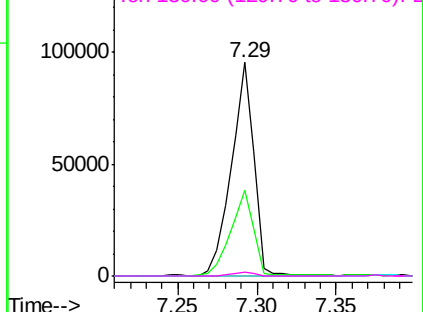

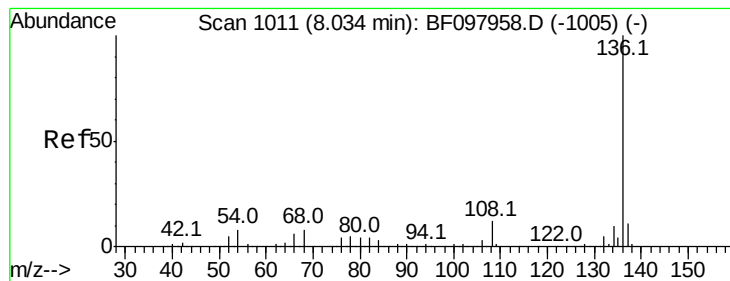

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.01 min Scan# 1007

Delta R.T. -0.02 min

Lab File: BF098178.D

Acq: 31 Aug 2017 1:42

Instrument :

BNA_F

ClientSampleId :

Tot Ion:136 Resp: 454273



Ion Ratio Lower Upper

136 100

137 10.6 8.5 12.7

54 7.0 4.9 7.3

68 7.2 4.1 6.1#

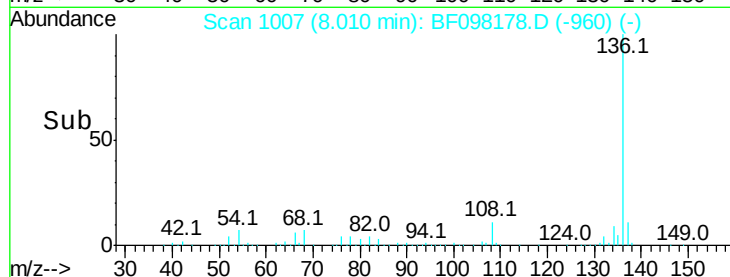
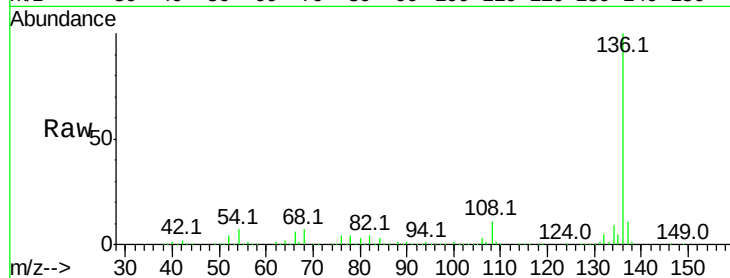


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

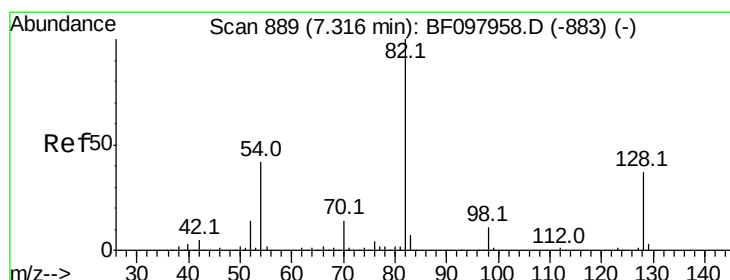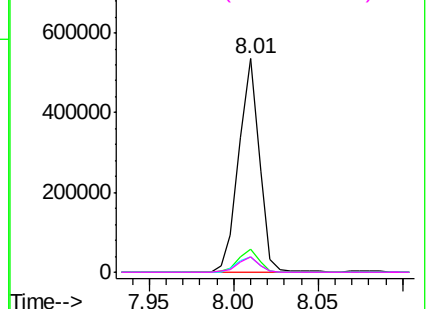

#23

Nitrobenzene-d5

Concen: 84.747 ng

RT: 7.29 min Scan# 885

Delta R.T. -0.03 min

Lab File: BF098178.D

Acq: 31 Aug 2017 1:42



Tgt Ion: 82 Resp: 708674

Ion Ratio Lower Upper

82 100

128 39.4 34.0 51.0


54 41.3 42.2 63.2#

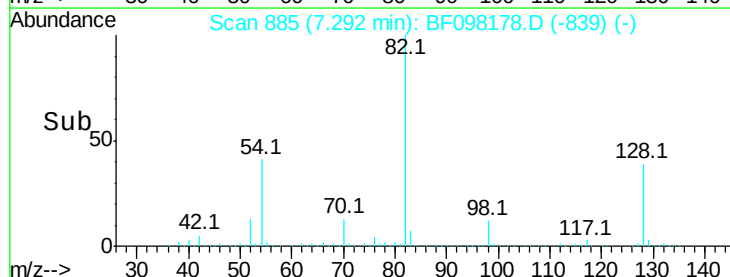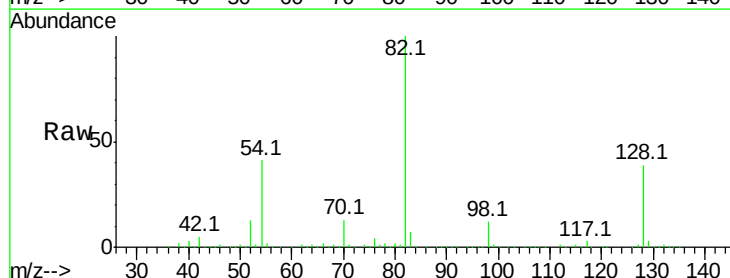


Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF0

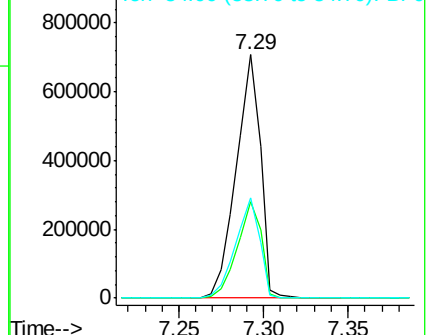



#25

Isophorone

Concen: 40.178 ng

RT: 7.29 min Scan# 885





Delta R.T. -0.29 min

Lab File: BF098178.D

Acq: 31 Aug 2017 1:42

Instrument :
BNA_F
ClientSampled :

Tot Ion:	82	Resp:	698609
Ion Ratio	Lower	Upper	
82	100		
95	0.1	5.3	7.9#
138	0.0	13.1	19.7#

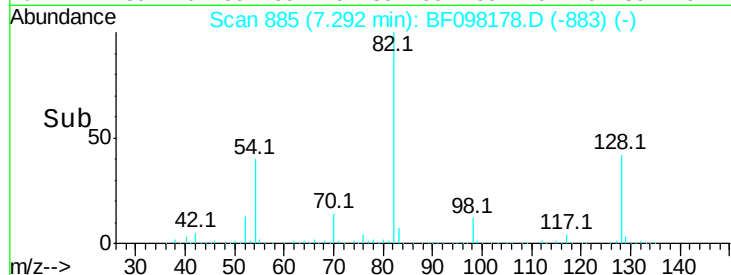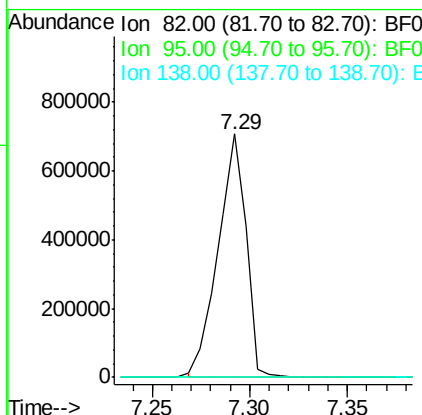

#26

2-Nitrophenol

Concen: 5.328 ng




RT: 7.70 min Scan# 954


Delta R.T. 0.05 min

Lab File: BF098178.D

Acq: 31 Aug 2017 1:42

Tgt Ion:	139	Resp:	266
Ion Ratio	Lower	Upper	
139	100		
109	0.0	21.0	31.6#
65	168.2	33.0	49.6#

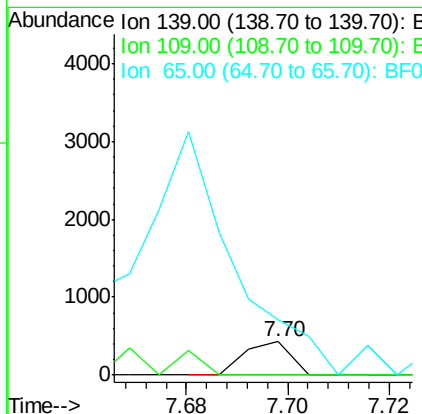

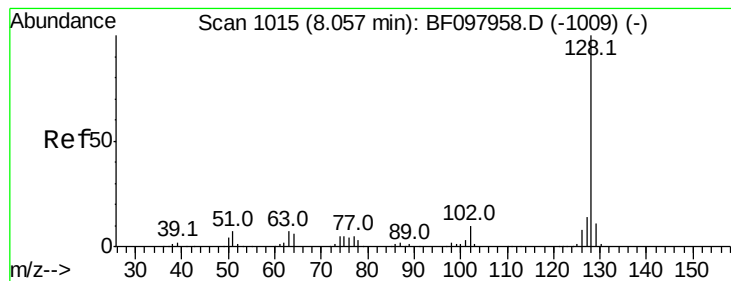

#31

Naphthalene

Concen: 17.026 ng

RT: 8.03 min Scan# 1011

Delta R.T. -0.02 min

Lab File: BF098178.D

Acq: 31 Aug 2017 1:42

Instrument :

BNA_F

ClientSampleId :


Tot Ion:128 Resp: 401523

Ion Ratio Lower Upper

128 100

129 11.2 9.0 13.6




127 12.9 10.8 16.2



Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

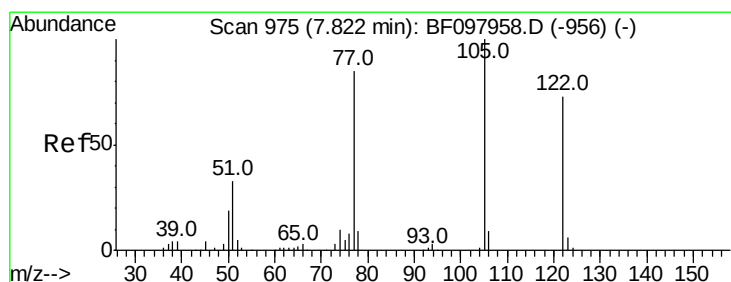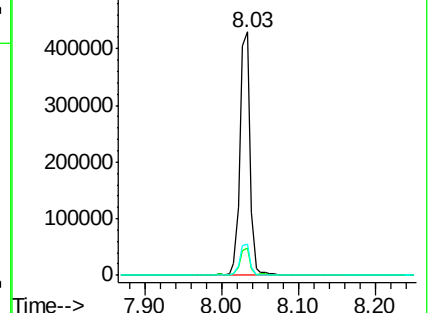

#32

Benzoic acid

Concen: 8.032 ng

RT: 7.80 min Scan# 972

Delta R.T. -0.03 min

Lab File: BF098178.D

Acq: 31 Aug 2017 1:42


Tgt Ion:122 Resp: 9923

Ion Ratio Lower Upper

122 100

105 11.2 103.3 143.3#



77 54.5 73.7 113.7#

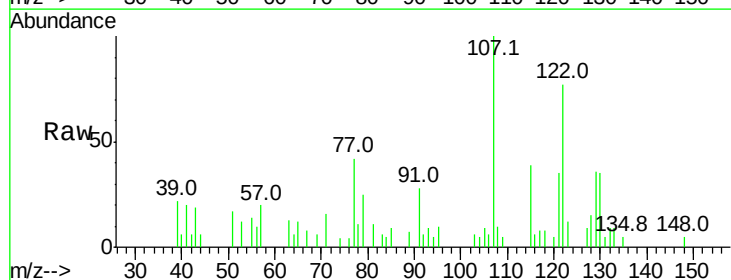


Abundance Ion 122.00 (121.70 to 122.70): E

Ion 105.00 (104.70 to 105.70): E

Ion 77.00 (76.70 to 77.70): BF0



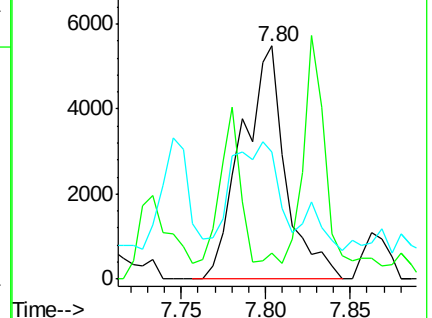



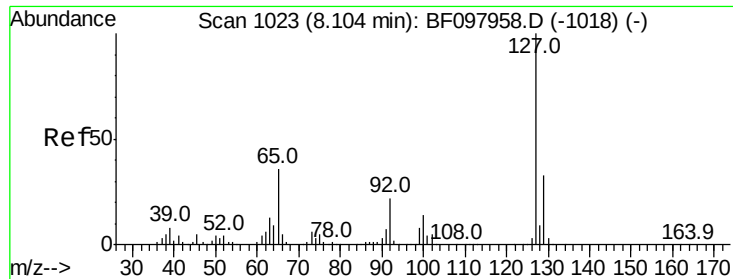

#33
 4-Chloroaniline
 Concen: 5.340 ng
 RT: 8.03 min Scan# 1011
 Delta R.T. -0.07 min
 Lab File: BF098178.D
 Acq: 31 Aug 2017 1:42




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion:	127	Resp:	53113
Ion	Ratio	Lower	Upper
127	100		
129	86.6	26.2	39.2#
65	0.0	27.8	41.8#
92	0.8	16.8	25.2#

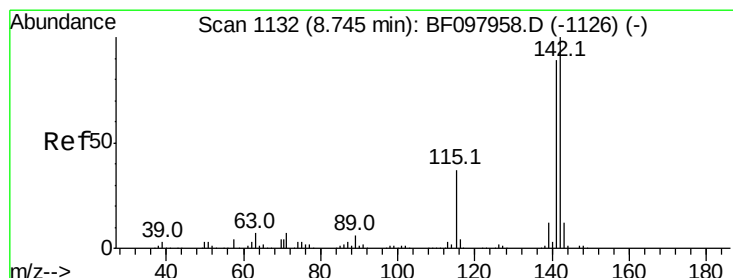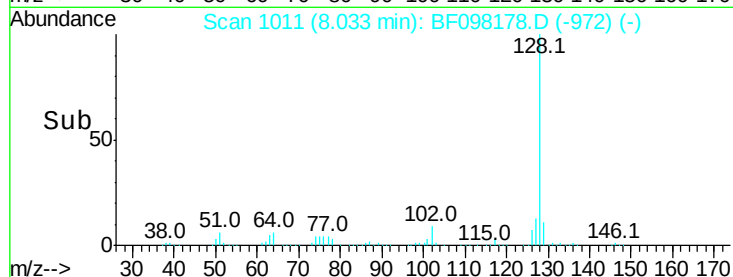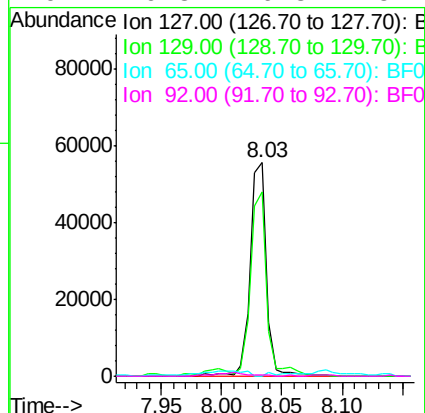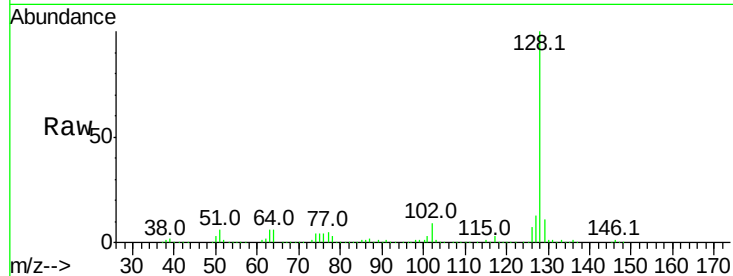

#37
 2-Methylnaphthalene
 Concen: 3.239 ng
 RT: 8.72 min Scan# 1128
 Delta R.T. -0.02 min
 Lab File: BF098178.D
 Acq: 31 Aug 2017 1:42

Tgt Ion:	142	Resp:	46833
Ion	Ratio	Lower	Upper
142	100		
141	90.6	71.3	106.9
115	38.8	27.1	40.7

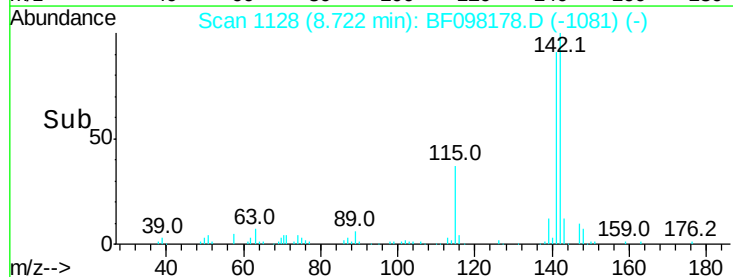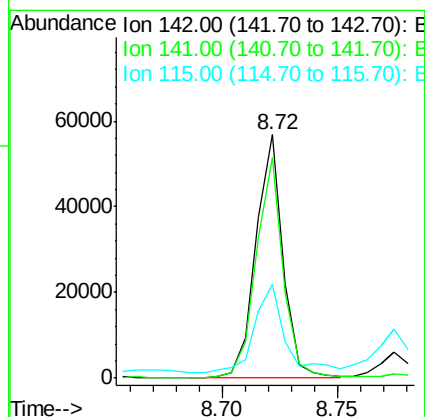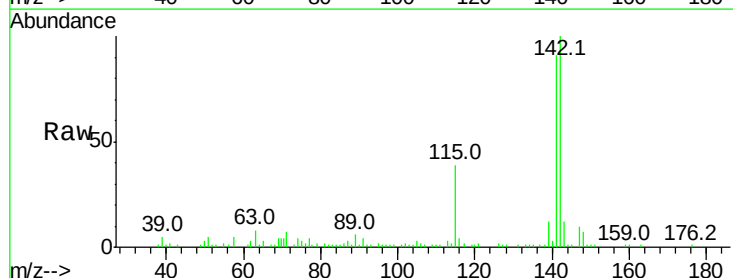







#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.76 min Scan# 1304
 Delta R.T. -0.03 min
 Lab File: BF098178.D
 Acq: 31 Aug 2017 1:42

Instrument :
 BNA_F
 ClientSampled :

Tot Ion	Ratio	Lower	Upper
164	100		
162	99.5	82.6	123.8
160	45.8	36.2	54.2




Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E


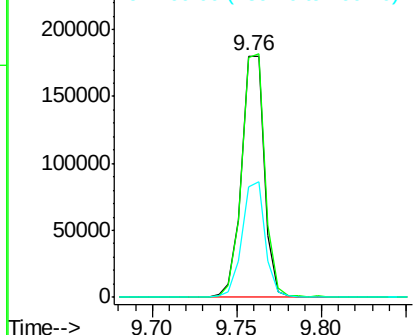



#41
 2,4,6-Tribromophenol
 Concen: 93.860 ng
 RT: 10.55 min Scan# 1439
 Delta R.T. -0.02 min
 Lab File: BF098178.D
 Acq: 31 Aug 2017 1:42

Tgt Ion	Ratio	Lower	Upper
330	100		
332	95.4	76.6	115.0
141	38.5	31.4	47.2



Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E




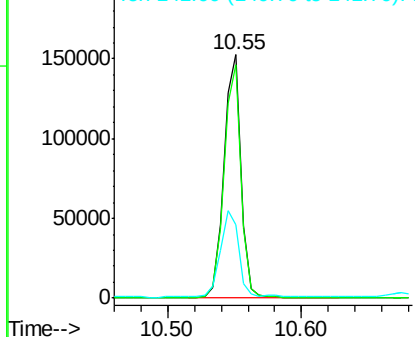




#44
2-Fluorobiphenyl
Concen: 62.234 ng
RT: 9.09 min Scan# 1190
Delta R.T. -0.02 min
Lab File: BF098178.D
Acq: 31 Aug 2017 1:42




Instrument :
BNA_F
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
172	100		
171	36.0	29.6	44.4
170	23.9	19.8	29.8

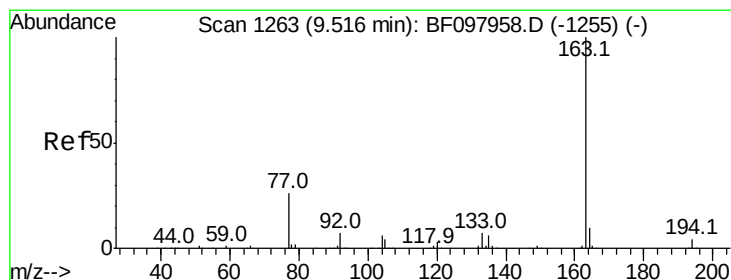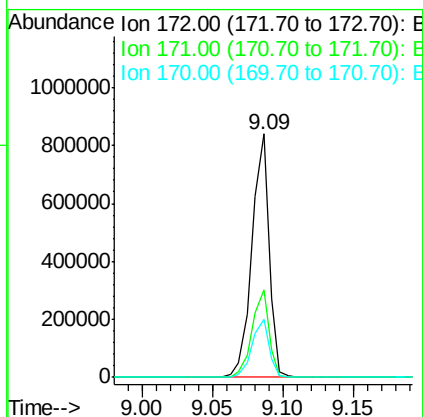

#49
Dimethylphthalate
Concen: 18.094 ng
RT: 9.48 min Scan# 1257
Delta R.T. -0.04 min
Lab File: BF098178.D
Acq: 31 Aug 2017 1:42

Tgt Ion	Ratio	Lower	Upper
163	100		
194	3.5	2.6	4.0
164	10.0	8.4	12.6

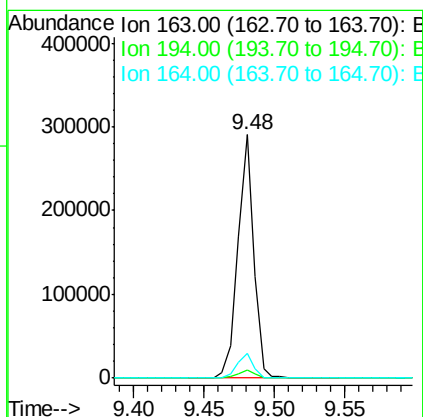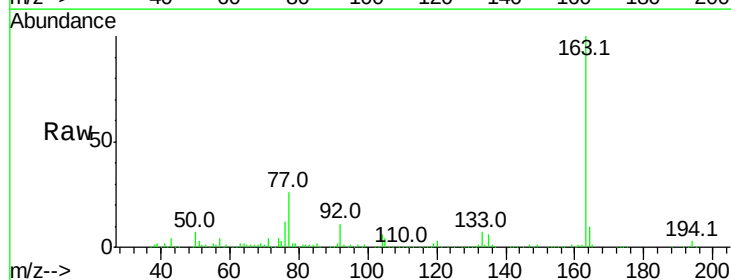



#51

Acenaphthene

Concen: 14.314 ng

RT: 9.79 min Scan# 1310

Delta R.T. -0.03 min

Lab File: BF098178.D

Acq: 31 Aug 2017 1:42

Instrument :

BNA_F

ClientSampleId :


Tot Ion:154 Resp: 162991

Ion Ratio Lower Upper

154 100

153 111.2 90.5 135.7

152 55.4 43.6 65.4



Abundance Ion 154.00 (153.70 to 154.70): E

Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

300000

250000

200000

150000

100000

50000

0



9.79

9.70

9.75

9.80

Time-->

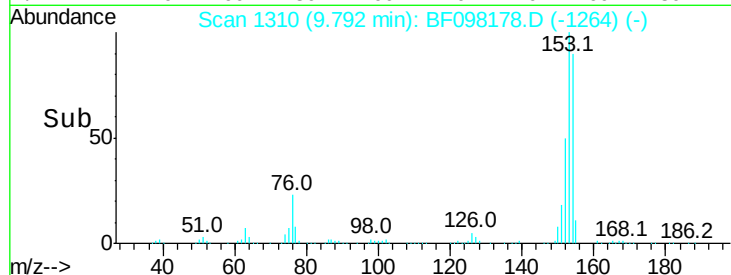

#53

2,4-Dinitrophenol

Concen: 10.320 ng

RT: 10.05 min Scan# 1353

Delta R.T. 0.20 min

Lab File: BF098178.D

Acq: 31 Aug 2017 1:42


Tgt Ion:184 Resp: 241

Ion Ratio Lower Upper

184 100

63 85.1 62.7 94.1

154 0.0 81.1 121.7#



Abundance Ion 184.00 (183.70 to 184.70): E

Ion 63.00 (62.70 to 63.70): BF0

Ion 154.00 (153.70 to 154.70): E

4000

3000

2000

1000

0


10.05


10.02

10.04

10.06

Time-->









#54
Dibenzofuran
Concen: 10.311 ng
RT: 9.96 min Scan# 1339
Delta R.T. -0.03 min
Lab File: BF098178.D
Acq: 31 Aug 2017 1:42




Instrument :
BNA_F
ClientSampled :


Tot Ion:168 Resp: 157351
Ion Ratio Lower Upper
168 100
139 38.1 30.6 45.8
169 16.4 10.8 16.2#

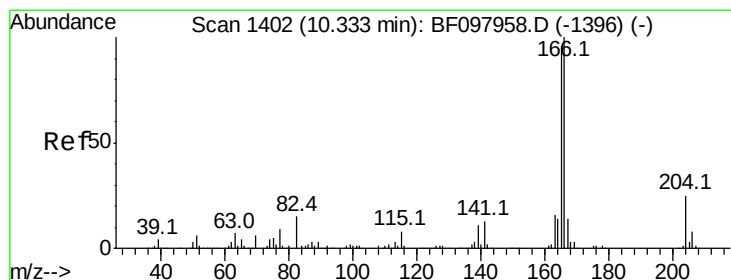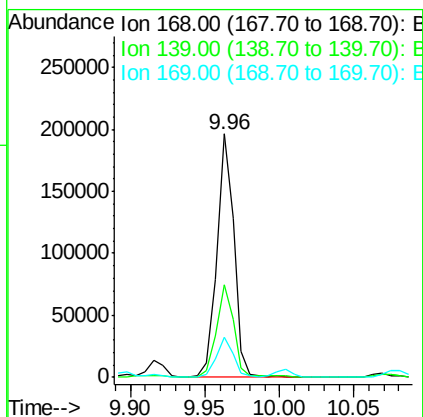

#57
Fluorene
Concen: 12.887 ng
RT: 10.30 min Scan# 1397
Delta R.T. -0.03 min
Lab File: BF098178.D
Acq: 31 Aug 2017 1:42

Tgt Ion:166 Resp: 152056
Ion Ratio Lower Upper
166 100
165 97.6 78.8 118.2
167 14.5 10.6 16.0



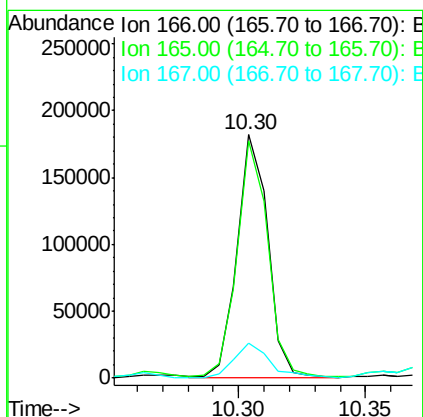
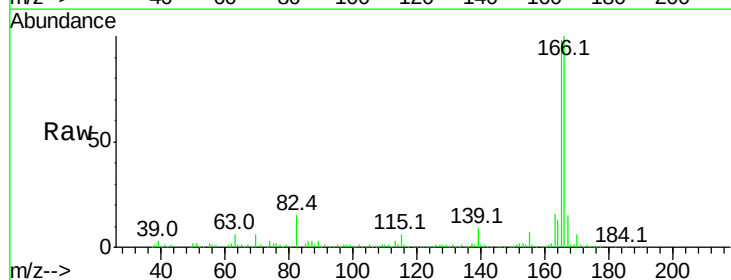


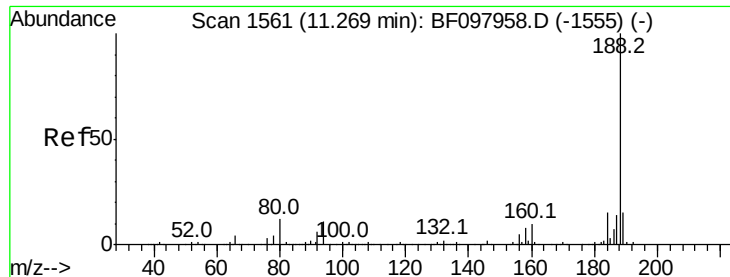

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.24 min Scan# 1556
Delta R.T. -0.02 min
Lab File: BF098178.D
Acq: 31 Aug 2017 1:42




Instrument :
BNA_F
ClientSampleId :


Tot Ion:188 Resp: 277213
Ion Ratio Lower Upper
188 100
94 13.6 9.4 14.2
80 14.5 10.2 15.2

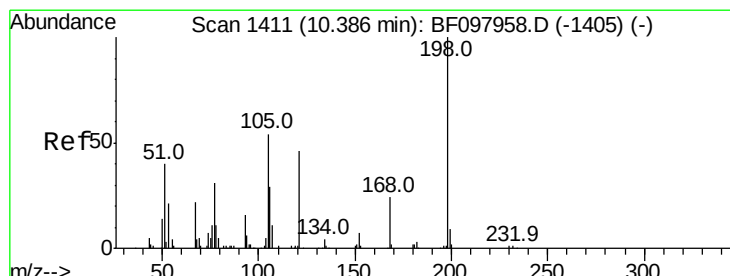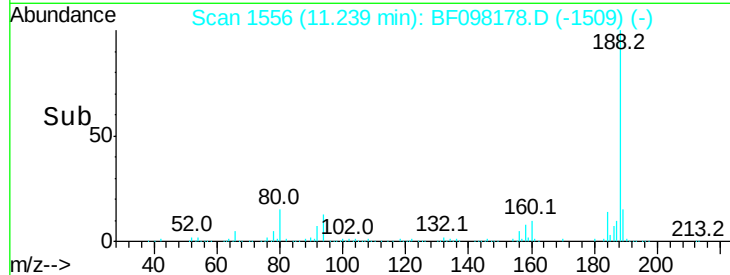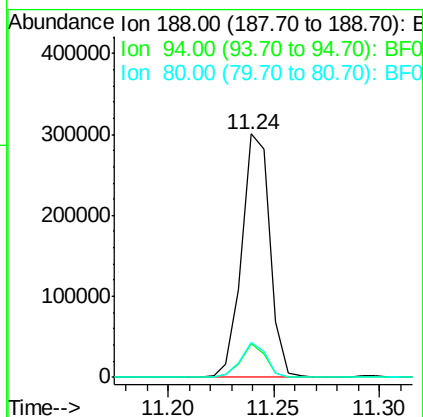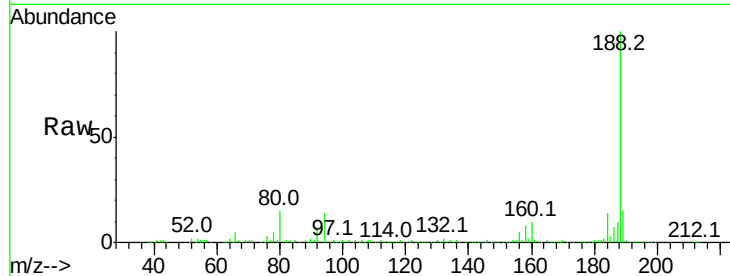

#64
4,6-Dinitro-2-methylphenol
Concen: 8.586 ng
RT: 10.55 min Scan# 1439
Delta R.T. 0.17 min
Lab File: BF098178.D
Acq: 31 Aug 2017 1:42

Tgt Ion:198 Resp: 419
Ion Ratio Lower Upper
198 100
51 452.5 53.2 93.2#
105 302.3 45.8 85.8#

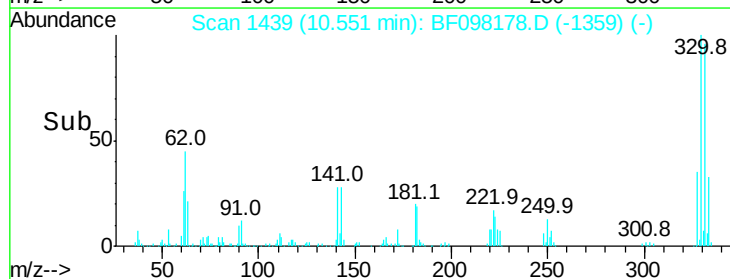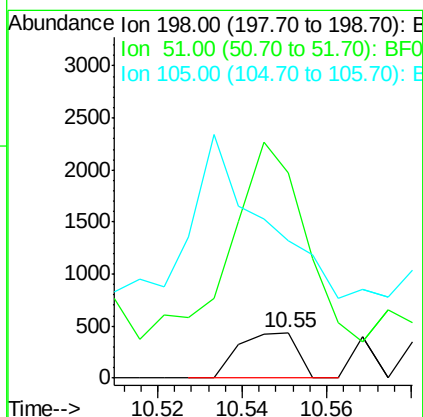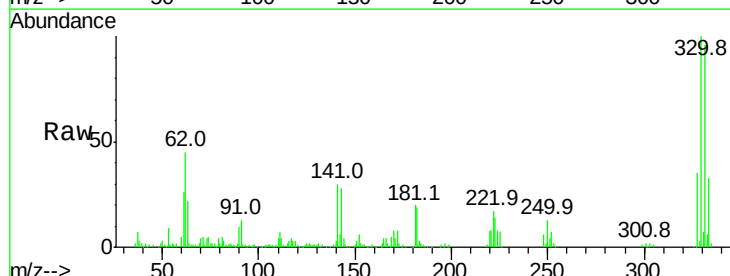


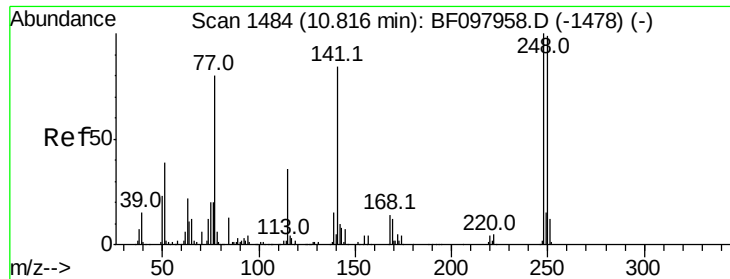




#66
 4-Bromophenyl-phenylether
 Concen: 3.154 ng
 RT: 10.55 min Scan# 1439
 Delta R.T. -0.26 min
 Lab File: BF098178.D
 Acq: 31 Aug 2017 1:42

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:248 Resp: 9079
 Ion Ratio Lower Upper
 248 100
 250 208.5 76.8 115.2#
 141 484.4 68.6 103.0#

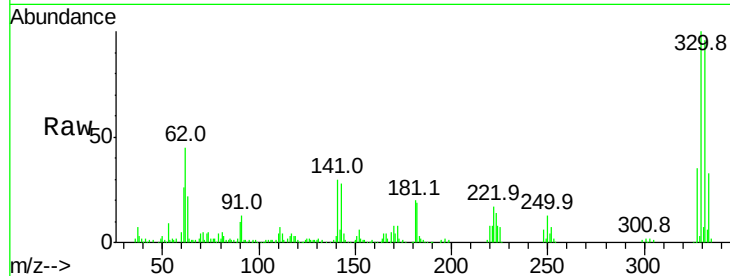


Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

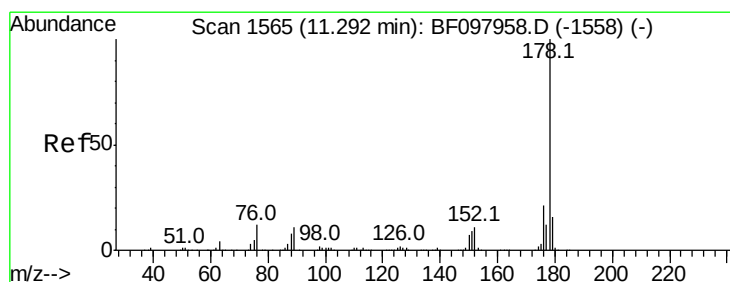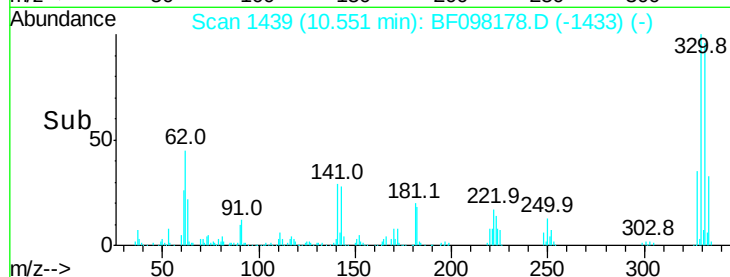
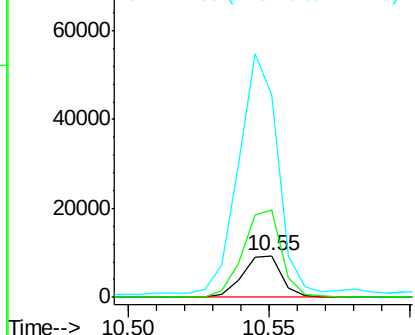



#70
 Phenanthrene
 Concen: 12.551 ng
 RT: 11.26 min Scan# 1560
 Delta R.T. -0.03 min
 Lab File: BF098178.D
 Acq: 31 Aug 2017 1:42

Tgt Ion:178 Resp: 185402
 Ion Ratio Lower Upper
 178 100
 176 19.5 16.2 24.4
 179 15.7 12.6 19.0

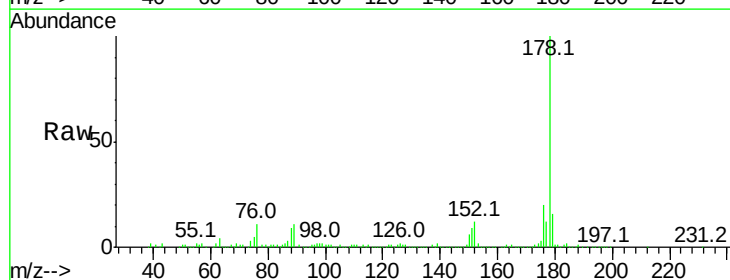

Abundance Ion 178.00 (177.70 to 178.70): E
 Ion 176.00 (175.70 to 176.70): E
 Ion 179.00 (178.70 to 179.70): E



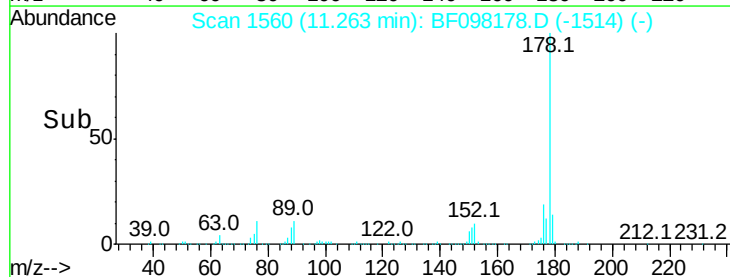
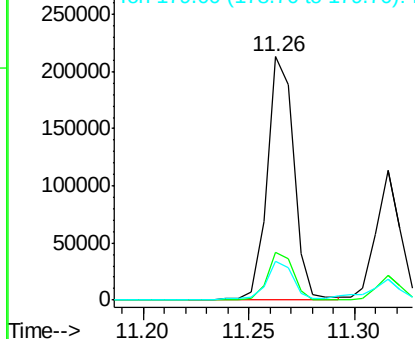




#71
 Anthracene
 Concen: 5.828 ng
 RT: 11.32 min Scan# 1569
 Delta R.T. -0.03 min
 Lab File: BF098178.D
 Acq: 31 Aug 2017 1:42




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion:178 Resp: 87324
 Ion Ratio Lower Upper
 178 100
 176 18.9 15.8 23.8
 179 16.2 12.7 19.1

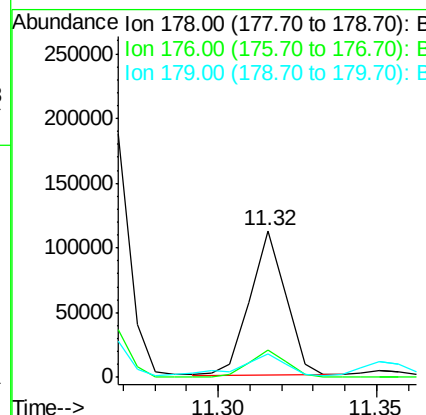

#74
 Fluoranthene
 Concen: 7.420 ng
 RT: 12.45 min Scan# 1762
 Delta R.T. -0.02 min
 Lab File: BF098178.D
 Acq: 31 Aug 2017 1:42

Tgt Ion:202 Resp: 114409
 Ion Ratio Lower Upper
 202 100
 101 12.8 0.0 33.2
 203 17.7 0.0 38.1

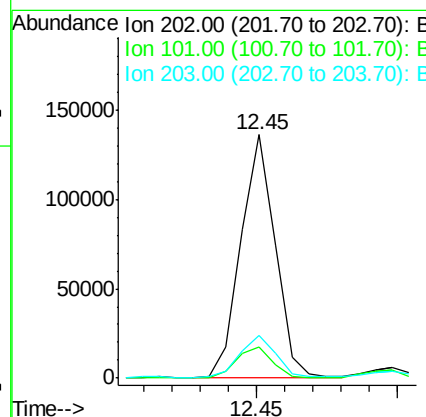

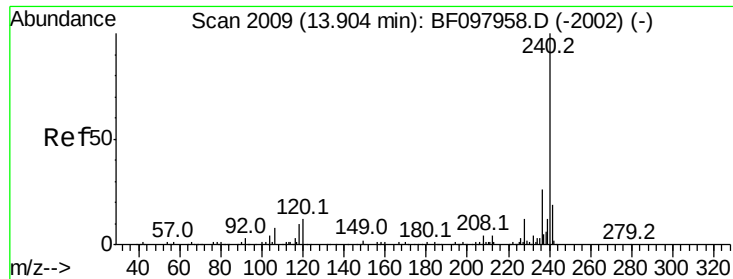

#75

Chrysene-d12

Concen: 20.000 ng

RT: 13.87 min Scan# 2004

Delta R.T. -0.02 min

Lab File: BF098178.D

Acq: 31 Aug 2017 1:42

Instrument :

BNA_F

ClientSampleId :


Tot Ion:240 Resp: 260652

Ion Ratio Lower Upper

240 100

120 13.3 5.8 8.8#




236 26.2 20.5 30.7

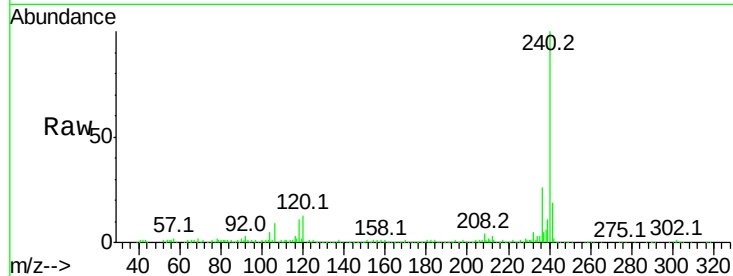

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

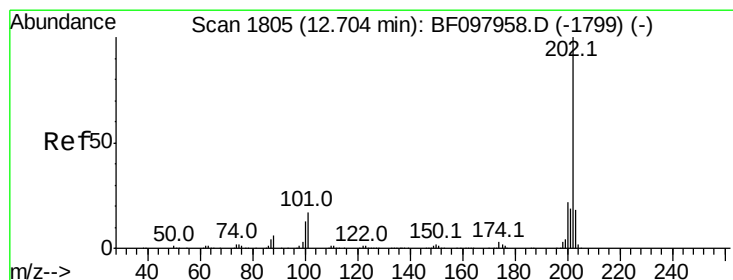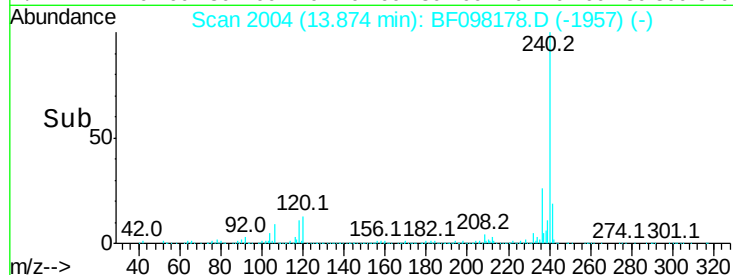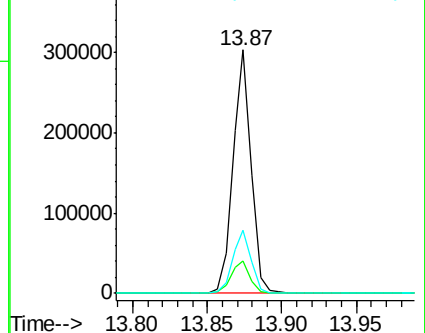

#77

Pyrene

Concen: 4.305 ng

RT: 12.68 min Scan# 1801

Delta R.T. -0.02 min

Lab File: BF098178.D

Acq: 31 Aug 2017 1:42


Tgt Ion:202 Resp: 91772

Ion Ratio Lower Upper

202 100

200 20.1 17.6 26.4



203 17.9 14.4 21.6

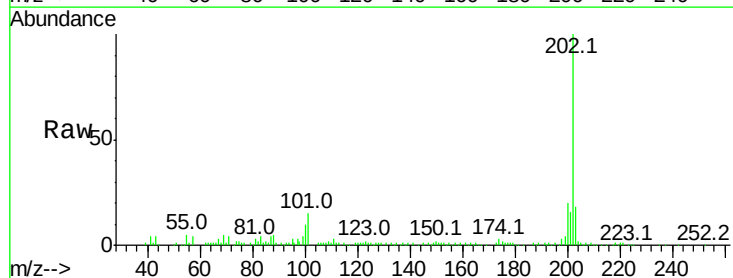


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E



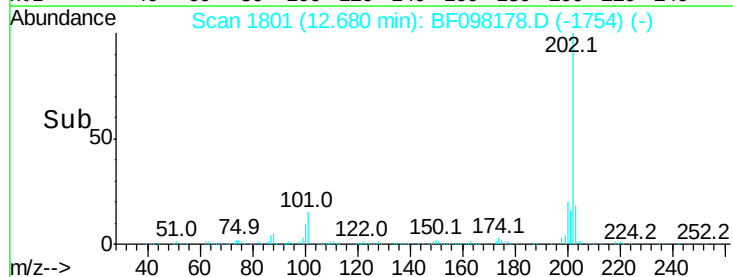
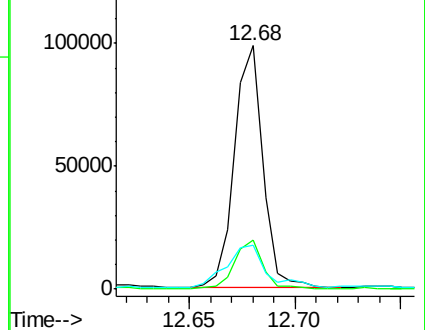




#78
 Terphenyl-d14
 Concen: 36.176 ng
 RT: 12.83 min Scan# 1826
 Delta R.T. -0.02 min
 Lab File: BF098178.D
 Acq: 31 Aug 2017 1:42




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion:244 Resp: 452169
 Ion Ratio Lower Upper
 244 100
 212 7.1 6.0 9.0
 122 12.4 10.3 15.5

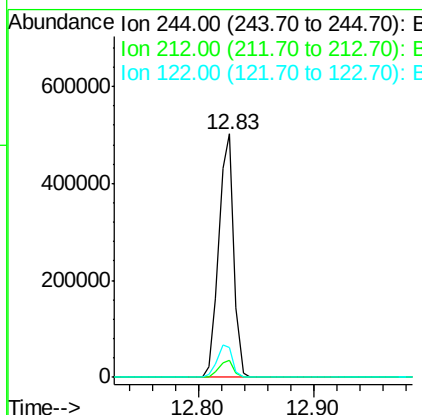

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.29 min Scan# 2244
 Delta R.T. -0.02 min
 Lab File: BF098178.D
 Acq: 31 Aug 2017 1:42

Tgt Ion:264 Resp: 178818
 Ion Ratio Lower Upper
 264 100
 260 23.9 19.5 29.3
 265 22.4 17.2 25.8

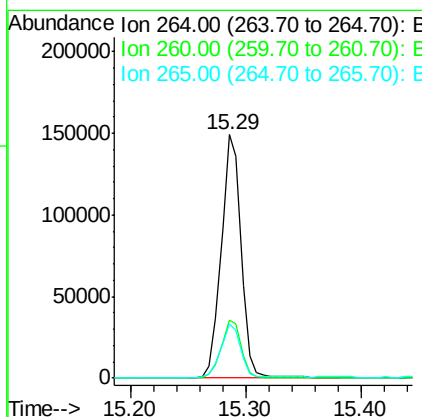



#88

Benzo(k)fluoranthene

Concen: 2.037 ng

RT: 14.89 min Scan# 2176

Delta R.T. -0.05 min

Lab File: BF098178.D

Acq: 31 Aug 2017 1:42

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 252 Resp: 21576

Ion Ratio Lower Upper

252 100

253 25.7 18.4 27.6

125 27.2 13.1 19.7#



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

