
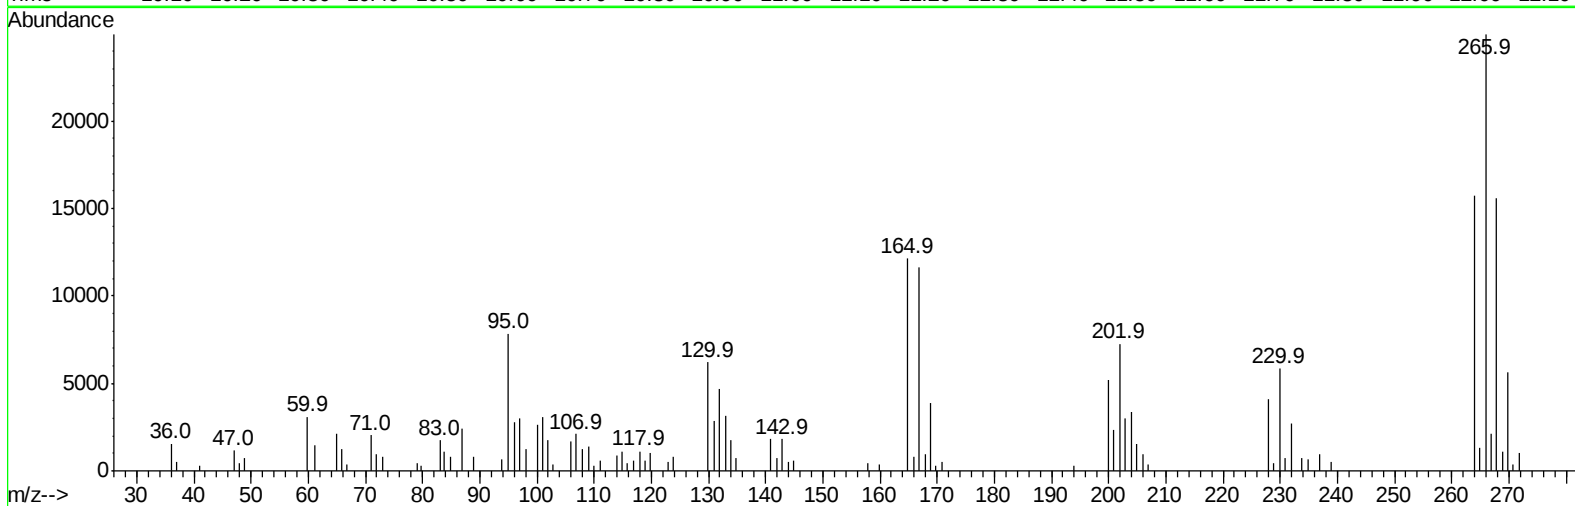


Data Path : Z:\HPCHEM1\BNA F\DATA\BF083017\
Data File : BF098183.D
Acq On : 31 Aug 2017 4:30
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 31 09:17:20 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 21 15:59:04 2017
Response via : Initial Calibration

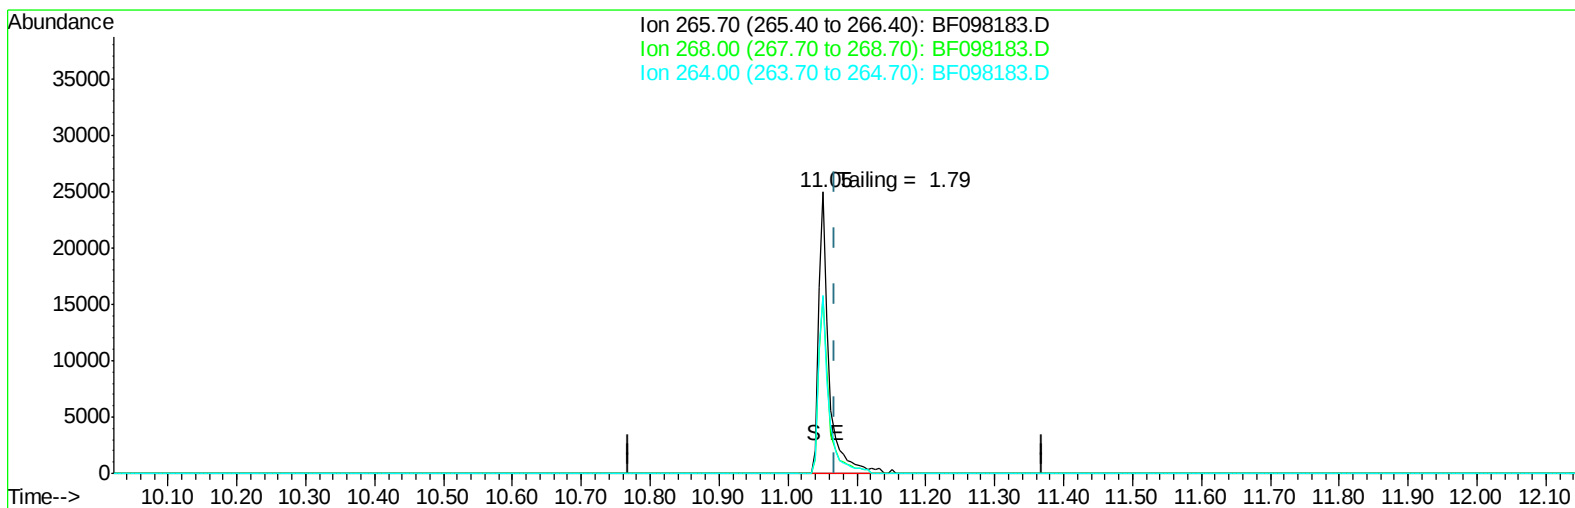

TIC: BF098183.D

(69) Pentachlorophenol (C)



11.051min (-0.018) 15936.96ng

response 26555

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.53
264.00	64.60	63.16
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF083017\
Data File : BF098183.D
Acq On : 31 Aug 2017 4:30
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 31 09:17:20 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 21 15:59:04 2017
Response via : Initial Calibration

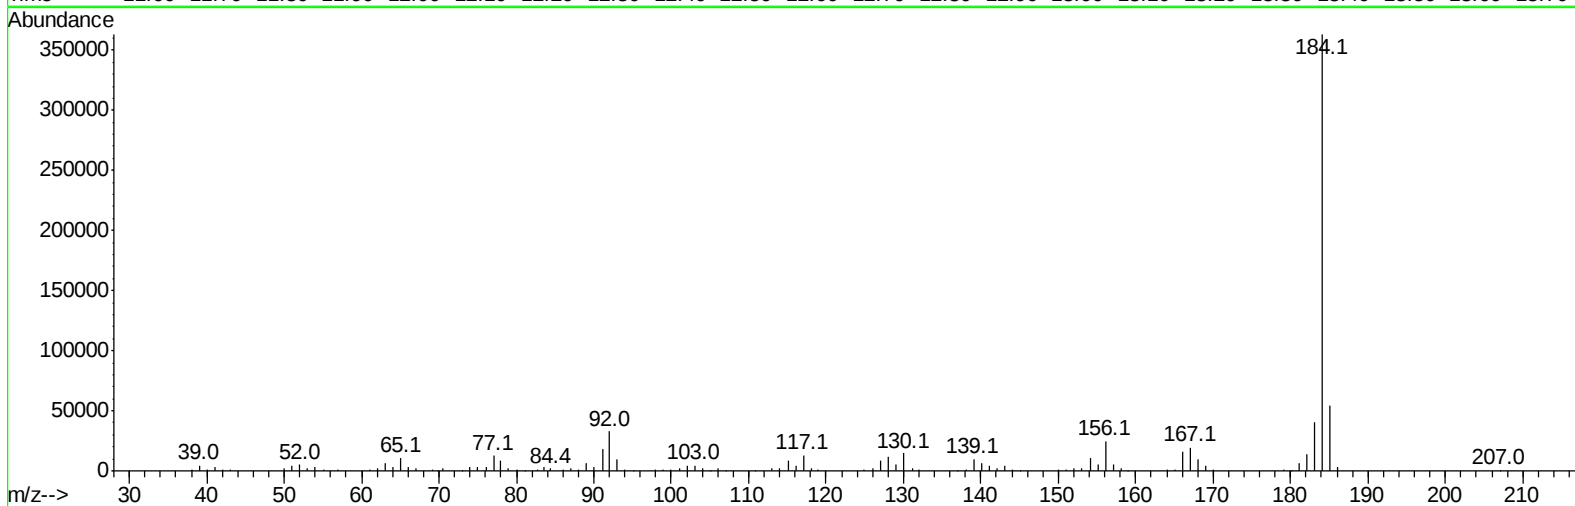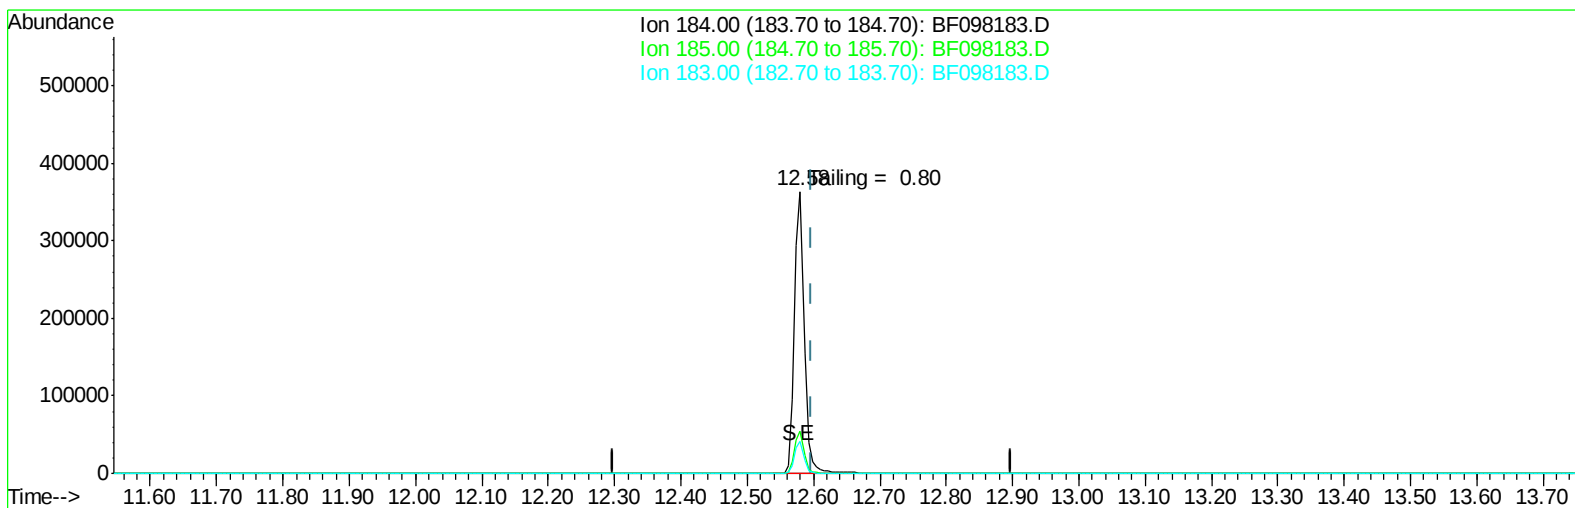

TIC: BF098183.D

(76) Benzidine

12.580min (-0.018) 0.00ng

response 356121

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.93#
183.00	12.20	11.21
0.00	0.00	0.00