

Data Path : Z:\HPCHEM1\BNA F\DATA\BF083017\
 Data File : BF098179.D
 Acq On : 31 Aug 2017 2:09
 Operator : SJ/JU
 Sample : I5024-04 5X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CL-01-082917-B

Manual Integrations
 APPROVED

Sohil
 8/31/2017 7:13:05 PM

Quant Time: Aug 31 08:29:42 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 21 15:59:04 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.72	152	118236	20.00	ng	-0.03
21) Naphthalene-d8	8.01	136	422166	20.00	ng	-0.02
38) Acenaphthene-d10	9.76	164	154807	20.00	ng	-0.03
63) Phenanthrene-d10	11.25	188	269486	20.00	ng	-0.02
75) Chrysene-d12	13.88	240	234798	20.00	ng	-0.02
86) Perylene-d12	15.29	264	168605	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.32	112	182666	23.50	ng	-0.03
7) Phenol-d6	6.36	99	253030	23.96	ng	-0.03
23) Nitrobenzene-d5	7.29	82	137878	17.74	ng	-0.04
41) 2,4,6-Tribromophenol	10.55	330	28542	21.25	ng	-0.03
44) 2-Fluorobiphenyl	9.08	172	223514	21.21	ng	-0.03
78) Terphenyl-d14	12.82	244	171843	15.26	ng	-0.03
Target Compounds						
31) Naphthalene	8.03	128	277939	12.682	ng	Qvalue 100
37) 2-Methylnaphthalene	8.72	142	85782	6.384	ng	97
48) Acenaphthylene	9.62	152	122951	7.506	ng	98
49) Dimethylphthalate	9.47	163	33135	2.928	ng	99
51) Acenaphthene	9.79	154	93235	9.025	ng	99
54) Dibenzofuran	9.96	168	164393	11.874	ng	98
57) Fluorene	10.30	166	263225	24.590	ng	96
70) Phenanthrene	11.27	178	1373816	95.669	ng	100
71) Anthracene	11.32	178	398220	27.341	ng	99
72) Carbazole	11.47	167	247719	17.918	ng	98
74) Fluoranthene	12.46	202	1390618	92.778	ng	100
77) Pyrene	12.69	202	1171927	61.026	ng	99
80) Benzo(a)anthracene	13.87	228	593268	42.158	ng	96
82) Chrysene	13.90	228	474041	33.863	ng	97
85) Indeno(1,2,3-cd)pyrene	16.66	276	159509	15.489	ng	# 90
87) Benzo(b)fluoranthene	14.89	252	468028m	44.038	ng	
88) Benzo(k)fluoranthene	14.92	252	145536m	14.576	ng	
89) Benzo(a)pyrene	15.24	252	321428	34.164	ng	98
90) Dibenzo(a,h)anthracene	16.67	278	41225	5.382	ng	# 92
91) Benzo(a,h,i)perylene	17.08	276	145416	18.195	ng	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA F\DATA\BF083017\
Data File : BF098179.D
Acq On : 31 Aug 2017 2:09
Operator : SJ/JU
Sample : I5024-04 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1


Instrument :
BNA_F
ClientSampleId :
CL-01-082917-B

Manual Integrations
APPROVED

Sohil
8/31/2017 7:13:05 PM

Quant Time: Aug 31 08:29:42 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 21 15:59:04 2017
Response via : Initial Calibration

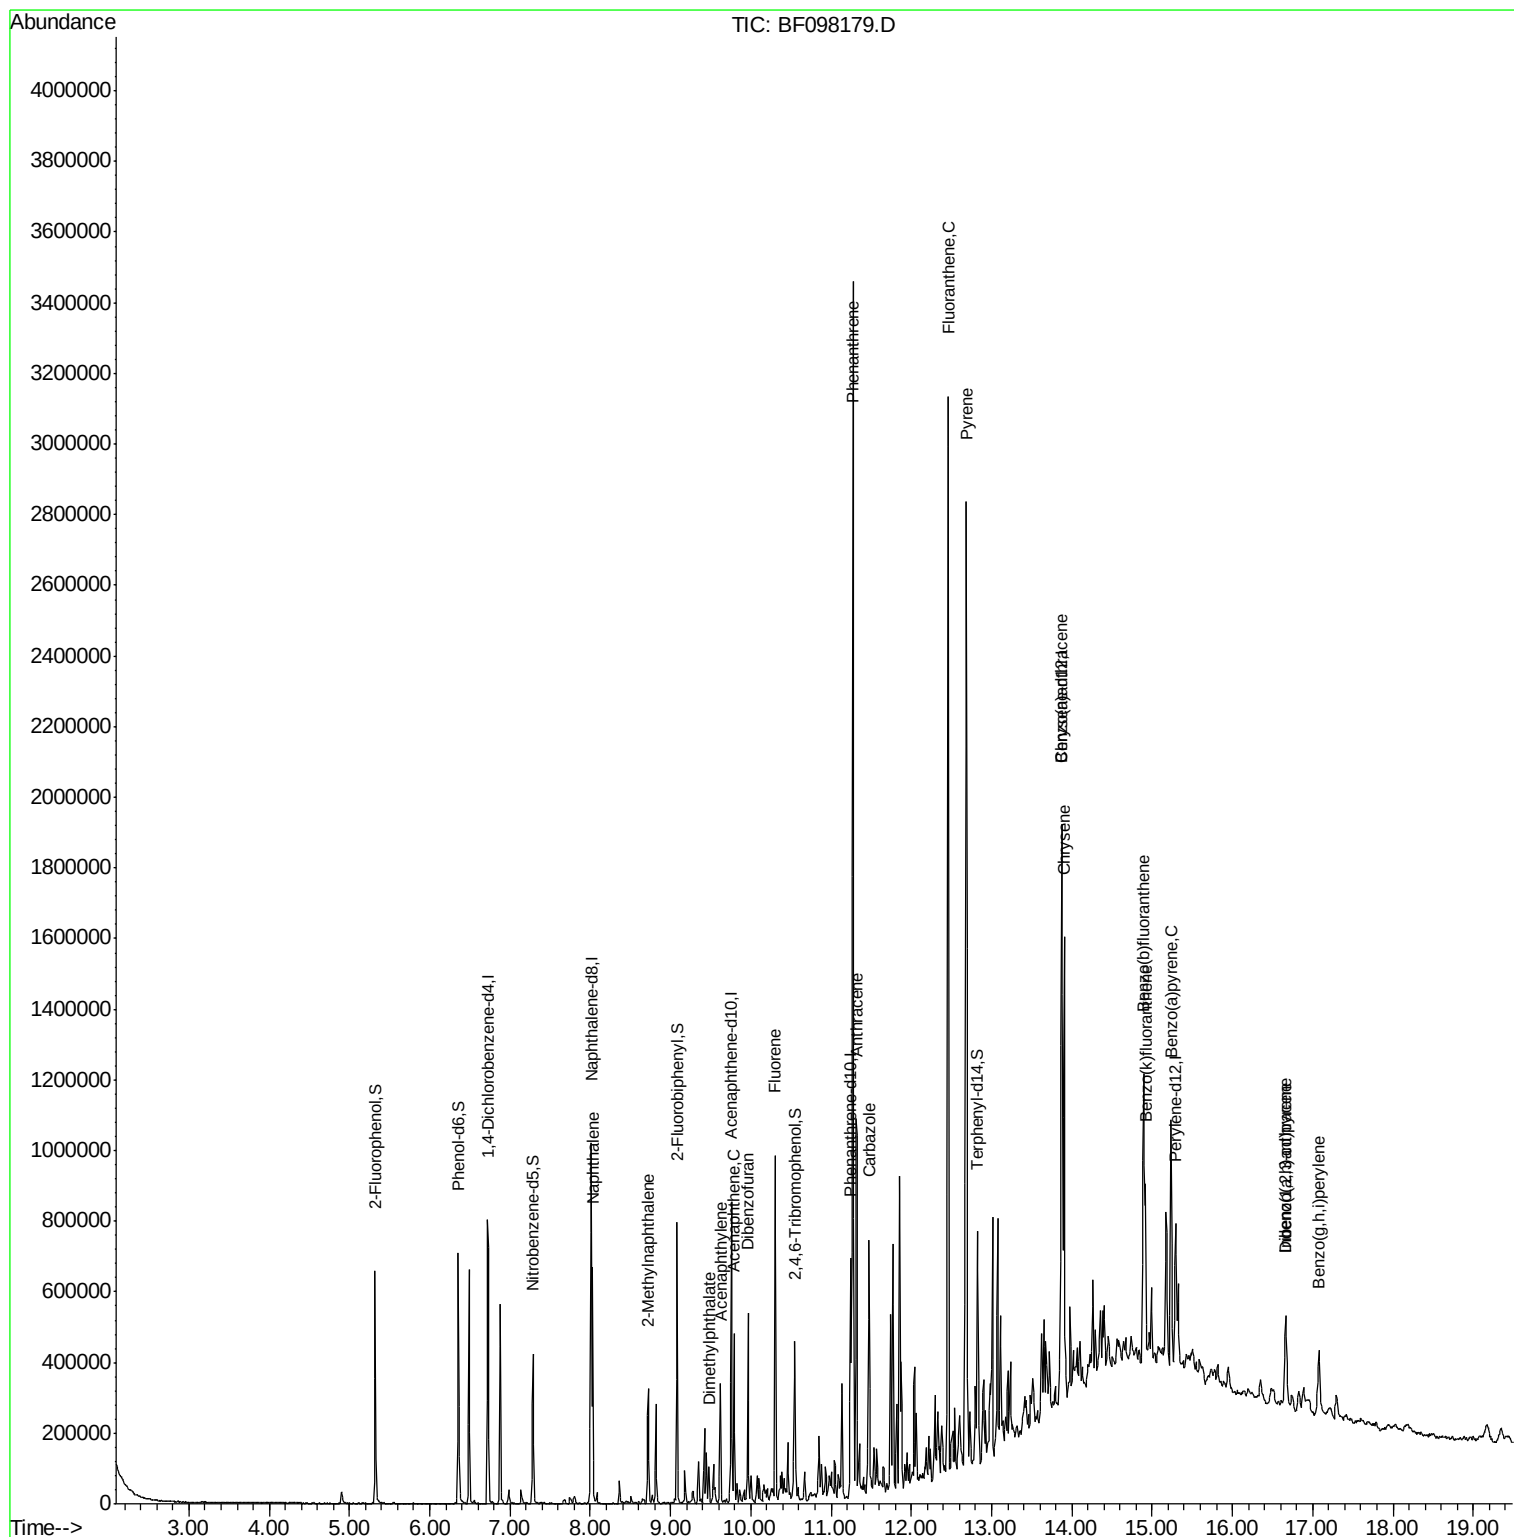

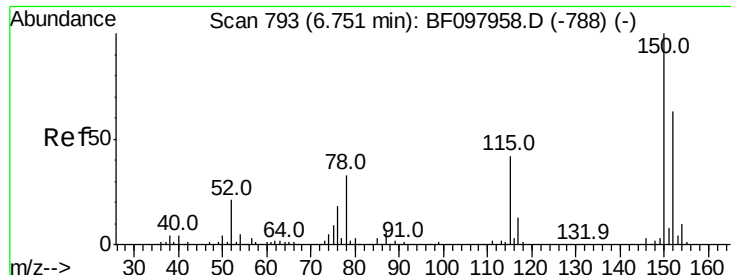

#1





1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.72 min Scan# 788
Delta R.T. -0.03 min
Lab File: BF098179.D
Acq: 31 Aug 2017 2:09

Instrument :
BNA_F
ClientSampleId :
CL-01-082917-B

Tot Ion	Ratio	Lower	Upper
152	100		
150	160.5	126.2	189.2
115	67.3	52.2	78.2

Manual Integrations
APPROVED




Sohil
8/31/2017 7:13:05 PM

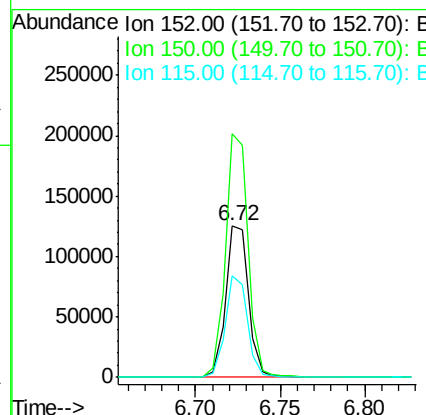


#5

2-Fluorophenol
Concen: 23.499 ng
RT: 5.32 min Scan# 550
Delta R.T. -0.03 min
Lab File: BF098179.D
Acq: 31 Aug 2017 2:09

Tgt Ion	Ratio	Lower	Upper
112	100		
64	59.6	46.0	69.0
63	30.5	23.4	35.0

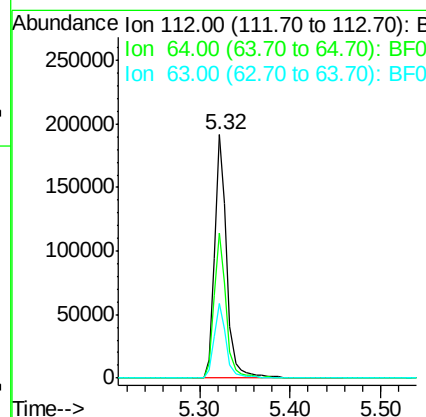



#7

Phenol-d6

Concen: 23.958 ng

RT: 6.36 min Scan# 726

Delta R.T. -0.03 min

Lab File: BF098179.D

Acq: 31 Aug 2017 2:09

Instrument :

BNA_F


ClientSampled :

CL-01-082917-B




Tot Ion:	99	Resp:	253030
Ion Ratio	Lower	Upper	
99	100		
42	14.8	13.5	20.3
71	31.0	24.5	36.7

Manual Integrations
APPROVED

Sohil
8/31/2017 7:13:05 PM



Abundance Ion 99.00 (98.70 to 99.70): BF0
Ion 42.00 (41.70 to 42.70): BF0
Ion 71.00 (70.70 to 71.70): BF0

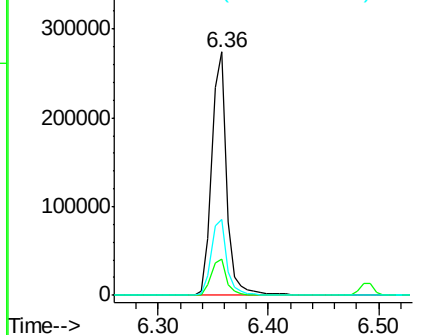

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.01 min Scan# 1007




Delta R.T. -0.02 min


Lab File: BF098179.D

Acq: 31 Aug 2017 2:09

Tgt Ion:	136	Resp:	422166
Ion Ratio	Lower	Upper	
136	100		
137	10.8	8.5	12.7
54	6.9	4.9	7.3
68	6.8	4.1	6.1#

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0

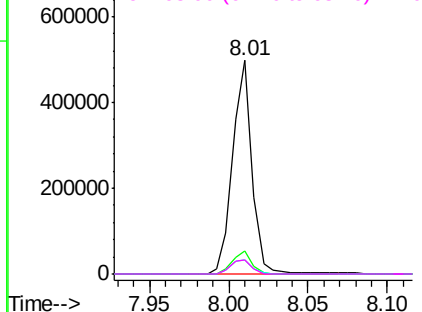

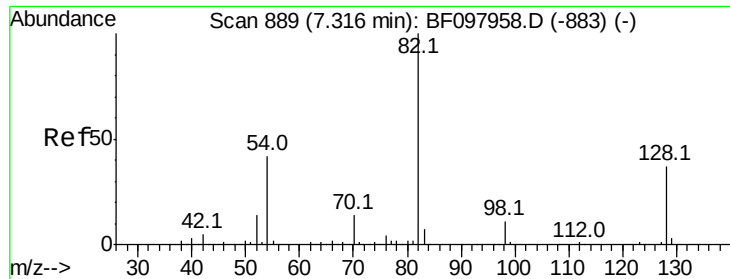

#23

Nitrobenzene-d5

Concen: 17.742 ng

RT: 7.29 min Scan# 884

Delta R.T. -0.04 min

Lab File: BF098179.D

Acq: 31 Aug 2017 2:09

Instrument :

BNA_F

ClientSampleId :

CL-01-082917-B

Tot Ion: 82 Resp: 137878

Ion Ratio Lower Upper

82 100





128 39.9 34.0 51.0

54 40.8 42.2 63.2#

Manual Integrations
APPROVED

Sohil

8/31/2017 7:13:05 PM

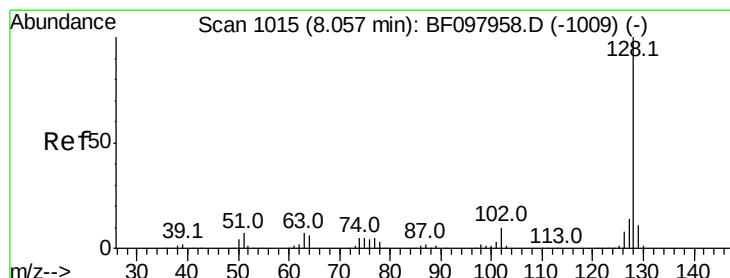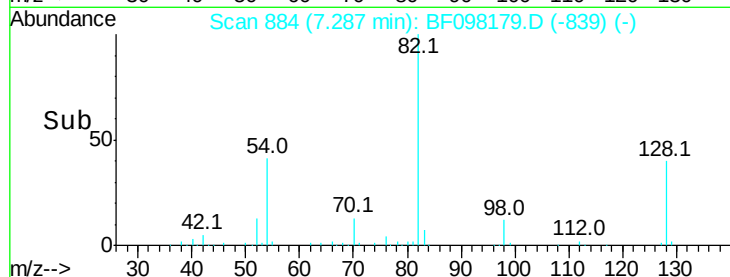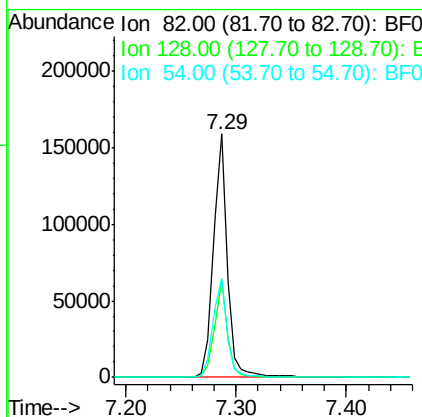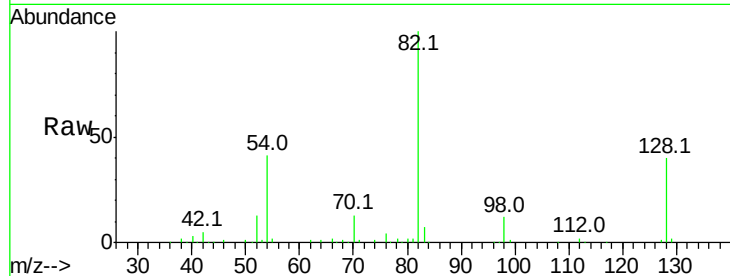

#31

Naphthalene

Concen: 12.682 ng

RT: 8.03 min Scan# 1010

Delta R.T. -0.03 min

Lab File: BF098179.D

Acq: 31 Aug 2017 2:09




Tgt Ion: 128 Resp: 277939


Ion Ratio Lower Upper

128 100

129 11.2 9.0 13.6

127 13.3 10.8 16.2

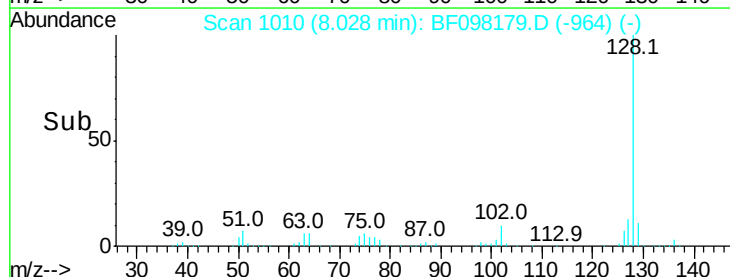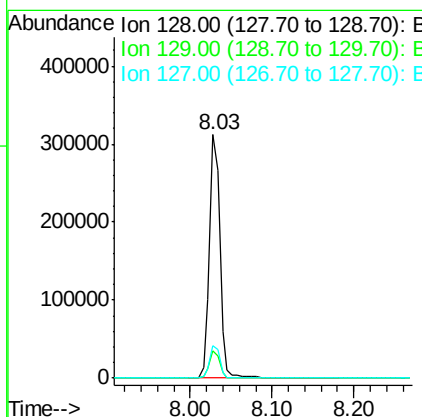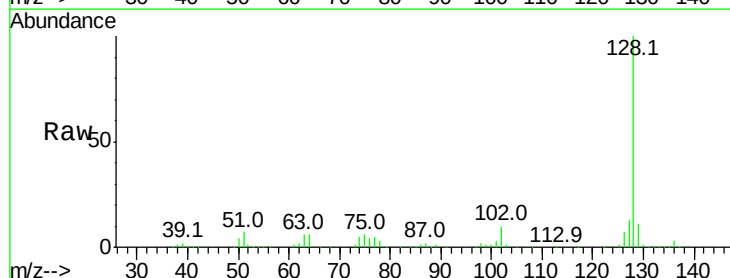

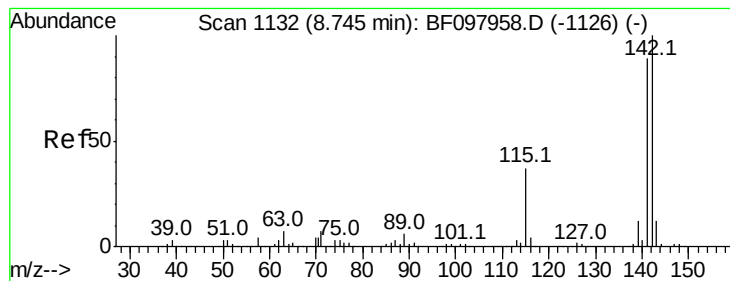

#37

2-Methylnaphthalene

Concen: 6.384 ng

RT: 8.72 min Scan# 1128

Delta R.T. -0.02 min

Lab File: BF098179.D

Acq: 31 Aug 2017 2:09

Instrument :

BNA_F


ClientSampleId :

CL-01-082917-B




Tot Ion:	142	Resp:	85782
Ion Ratio	Lower	Upper	
142	100		
141	85.9	71.3	106.9
115	35.2	27.1	40.7

Manual Integrations
APPROVED

Sohil
8/31/2017 7:13:05 PM

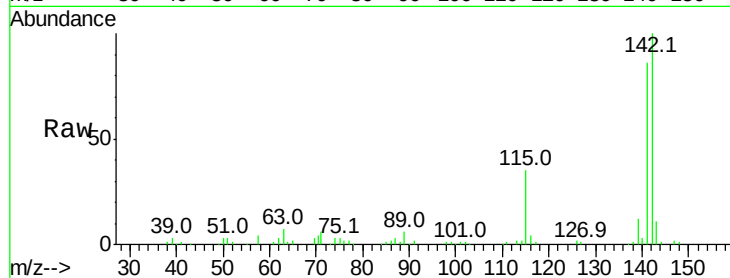

Abundance Ion 142.00 (141.70 to 142.70): E
Ion 141.00 (140.70 to 141.70): E
Ion 115.00 (114.70 to 115.70): E

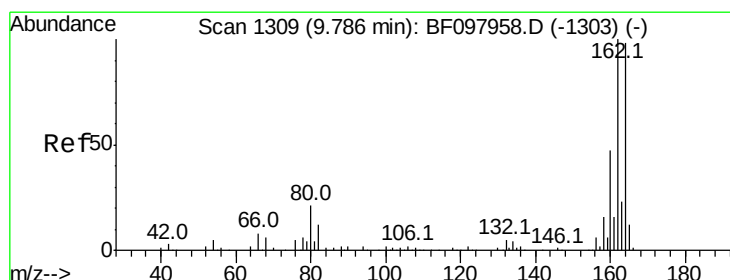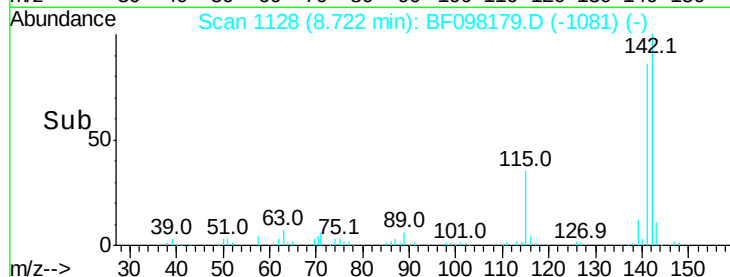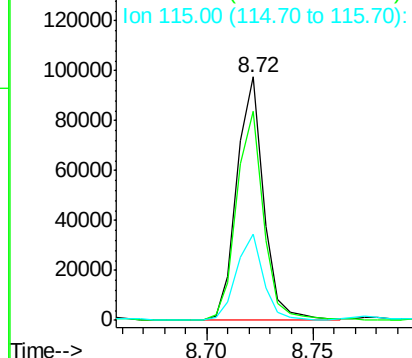

#38

Acenaphthene-d10

Concen: 20.000 ng


RT: 9.76 min Scan# 1304

Delta R.T. -0.03 min



Lab File: BF098179.D


Acq: 31 Aug 2017 2:09

Tgt Ion:	164	Resp:	154807
Ion Ratio	Lower	Upper	
164	100		
162	101.3	82.6	123.8
160	46.9	36.2	54.2

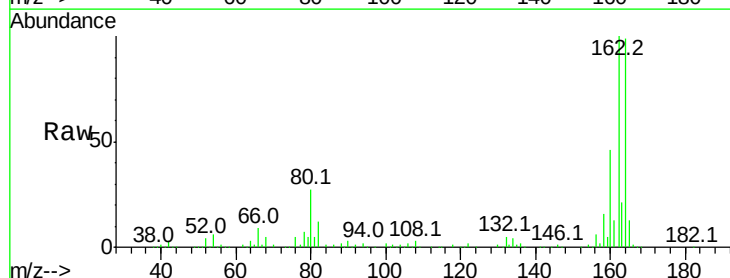

Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

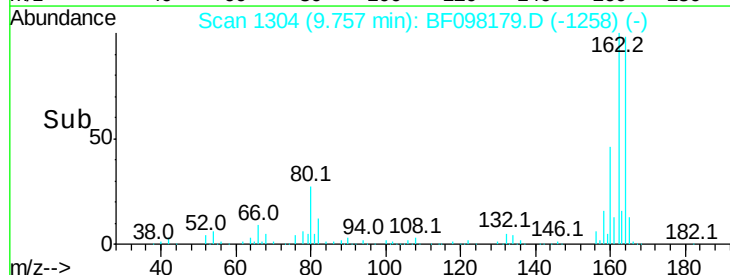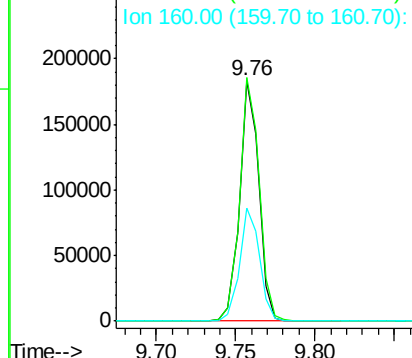



#41

2,4,6-Tribromophenol

Concen: 21.249 ng

RT: 10.55 min Scan# 1438

Delta R.T. -0.03 min

Lab File: BF098179.D

Acq: 31 Aug 2017 2:09

Instrument :

BNA_F


ClientSampleId :

CL-01-082917-B




Tot Ion:	330	Resp:	28542
Ion Ratio	Lower	Upper	
330	100		
332	98.5	76.6	115.0
141	46.2	31.4	47.2

Manual Integrations
APPROVED

Sohil
8/31/2017 7:13:05 PM



Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

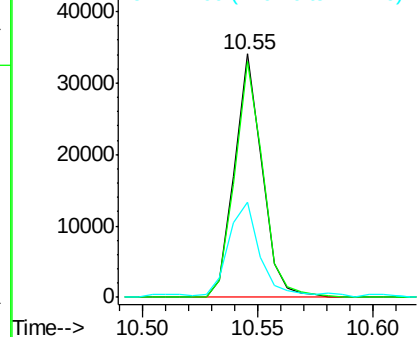

#44

2-Fluorobiphenyl

Concen: 21.213 ng


RT: 9.08 min Scan# 1189

Delta R.T. -0.03 min



Lab File: BF098179.D


Acq: 31 Aug 2017 2:09

Tgt Ion:	172	Resp:	223514
Ion Ratio	Lower	Upper	
172	100		
171	35.3	29.6	44.4
170	23.7	19.8	29.8



Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

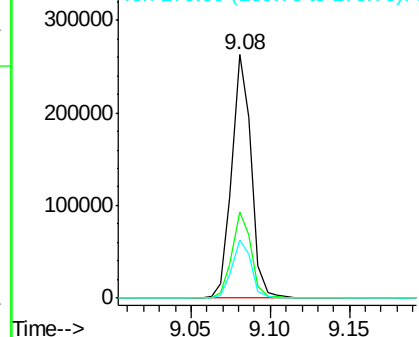







#48
Acenaphthylene
Concen: 7.506 ng
RT: 9.62 min Scan# 1281
Delta R.T. -0.03 min
Lab File: BF098179.D
Acq: 31 Aug 2017 2:09

Instrument :
BNA_F
ClientSampled :
CL-01-082917-B

Tot Ion	Ratio	Resp	Lower	Upper
152	100	122951		
151	20.3		16.8	25.2
153	14.1		10.8	16.2




Manual Integrations
APPROVED


Sohil
8/31/2017 7:13:05 PM

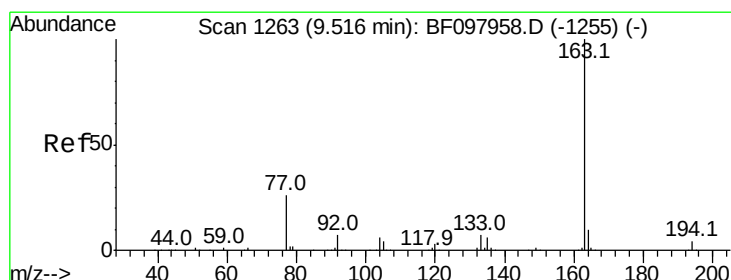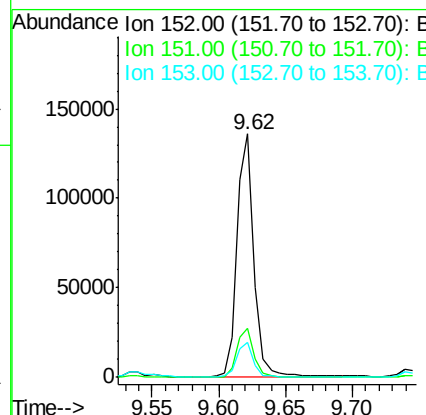

#49
Dimethylphthalate
Concen: 2.928 ng
RT: 9.47 min Scan# 1256
Delta R.T. -0.04 min
Lab File: BF098179.D
Acq: 31 Aug 2017 2:09

Tgt Ion	Ratio	Resp	Lower	Upper
163	100	33135		
194	3.2		2.6	4.0
164	11.2		8.4	12.6

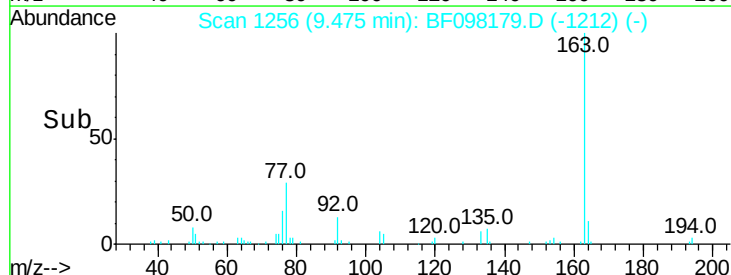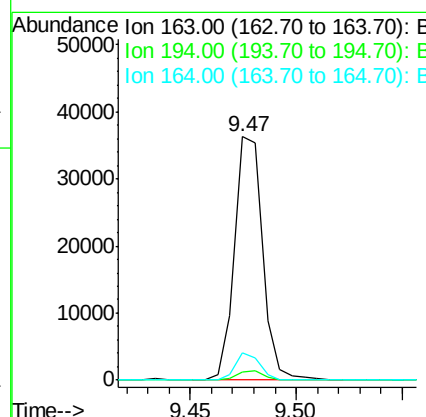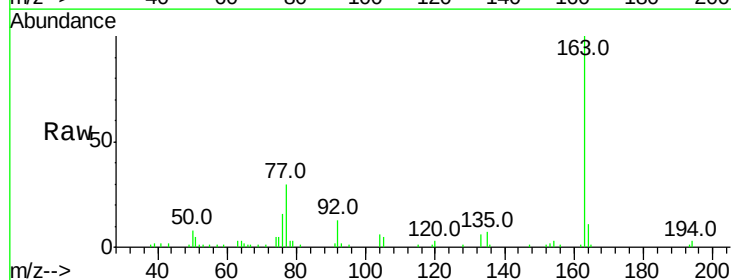



#51

Acenaphthene

Concen: 9.025 ng

RT: 9.79 min Scan# 1310

Delta R.T. -0.03 min

Lab File: BF098179.D

Acq: 31 Aug 2017 2:09

Instrument :

BNA_F


ClientSampleId :

CL-01-082917-B




Tot Ion:	154	Resp:	93235
Ion Ratio	Lower	Upper	
154	100		
153	112.2	90.5	135.7
152	54.9	43.6	65.4

Manual Integrations
APPROVED

Sohil
8/31/2017 7:13:05 PM



Abundance Ion 154.00 (153.70 to 154.70): E
Ion 153.00 (152.70 to 153.70): E
Ion 152.00 (151.70 to 152.70): E

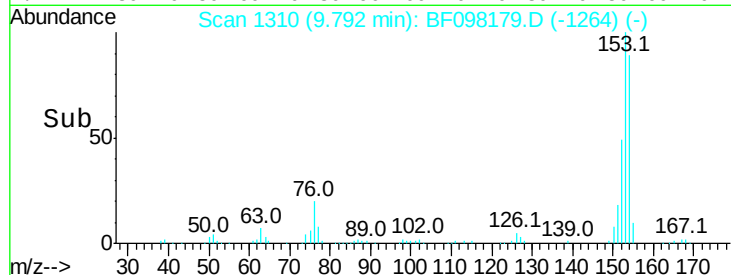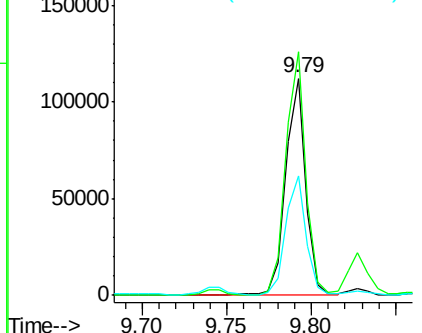

#54

Dibenzofuran

Concen: 11.874 ng

RT: 9.96 min Scan# 1339




Delta R.T. -0.03 min


Lab File: BF098179.D

Acq: 31 Aug 2017 2:09

Tgt Ion:	168	Resp:	164393
Ion Ratio	Lower	Upper	
168	100		
139	39.2	30.6	45.8
169	14.7	10.8	16.2

Abundance Ion 168.00 (167.70 to 168.70): E
Ion 139.00 (138.70 to 139.70): E
Ion 169.00 (168.70 to 169.70): E

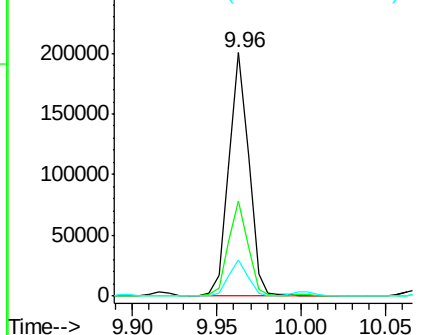

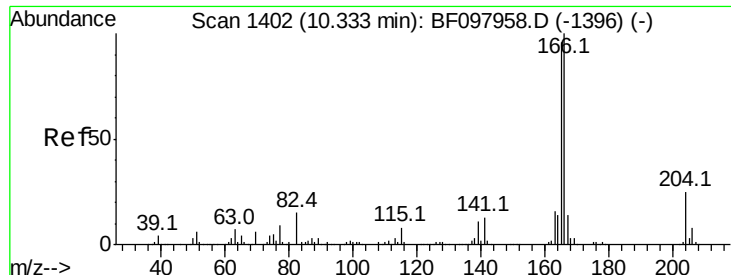





#57
Fluorene
 Concen: 24.590 ng
 RT: 10.30 min Scan# 1397
 Delta R.T. -0.03 min
 Lab File: BF098179.D
 Acq: 31 Aug 2017 2:09

Instrument :
 BNA_F
 ClientSampleId :
 CL-01-082917-B

Tot Ion	Ratio	Resp	Lower	Upper
166	100	263225		
165	93.8	78.8	118.2	
167	13.8	10.6	16.0	




Manual Integrations
 APPROVED


Sohil
 8/31/2017 7:13:05 PM

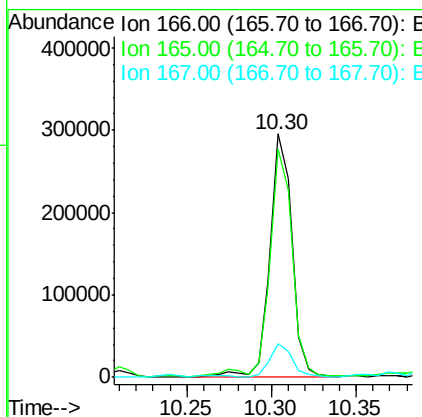

#63
Phenanthrene-d10
 Concen: 20.000 ng
 RT: 11.25 min Scan# 1557
 Delta R.T. -0.02 min
 Lab File: BF098179.D
 Acq: 31 Aug 2017 2:09

Tgt Ion	Ratio	Resp	Lower	Upper
188	100	269486		
94	10.7	9.4	14.2	
80	10.8	10.2	15.2	

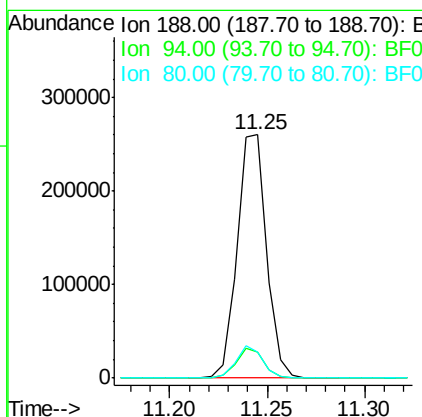

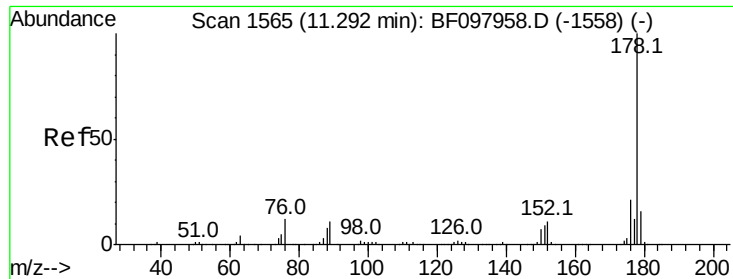

#70

Phenanthrene

Concen: 95.669 ng

RT: 11.27 min Scan# 1562

Delta R.T. -0.02 min

Lab File: BF098179.D

Acq: 31 Aug 2017 2:09

Instrument :

BNA_F

ClientSampleId :

CL-01-082917-B

Tot Ion:178 Resp: 1373816

Ion Ratio Lower Upper

178 100

176 20.6 16.2 24.4


179 15.7 12.6 19.0

Manual Integrations

APPROVED

Sohil




8/31/2017 7:13:05 PM

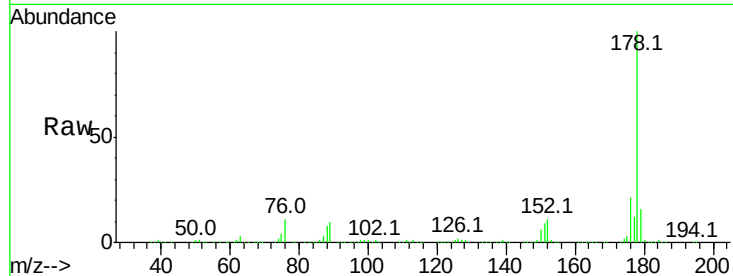

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

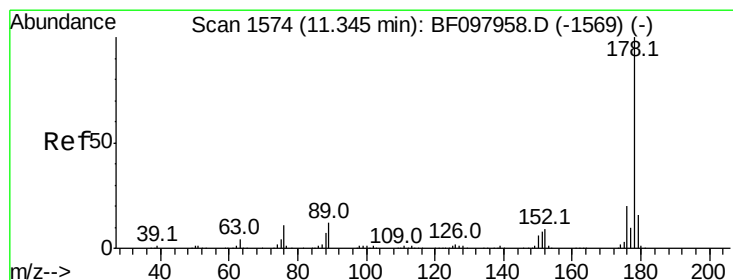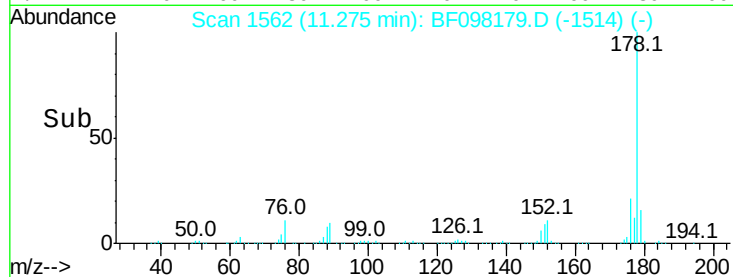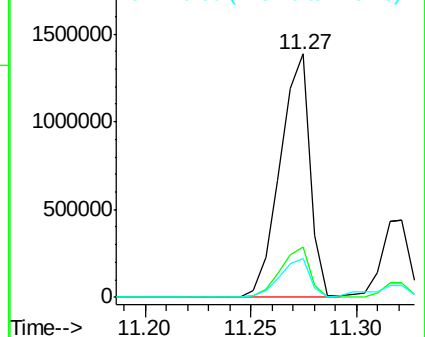

#71

Anthracene

Concen: 27.341 ng

RT: 11.32 min Scan# 1570

Delta R.T. -0.02 min

Lab File: BF098179.D

Acq: 31 Aug 2017 2:09

Tgt Ion:178 Resp: 398220

Ion Ratio Lower Upper

178 100




176 19.4 15.8 23.8


179 15.3 12.7 19.1

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

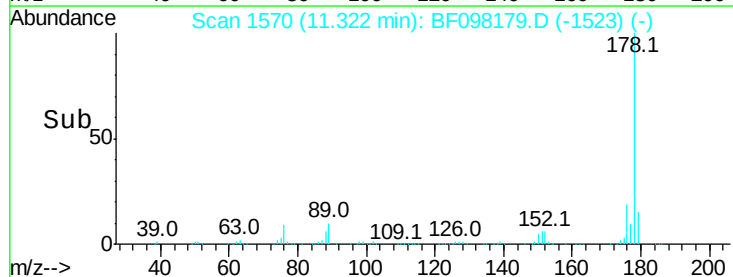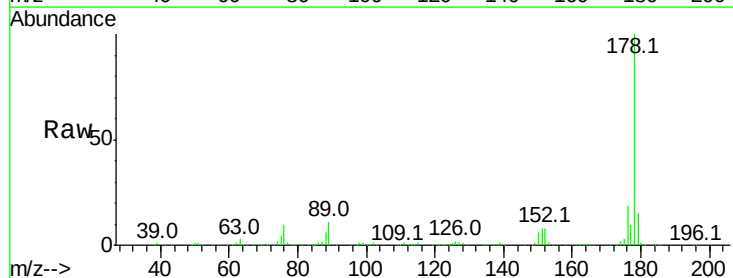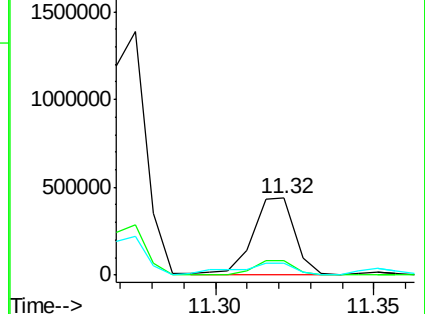



#72

Carbazole

Concen: 17.918 ng

RT: 11.47 min Scan# 1596

Delta R.T. -0.02 min

Lab File: BF098179.D

Acq: 31 Aug 2017 2:09

Instrument :

BNA_F





ClientSampleId :

CL-01-082917-B

Tot Ion:	167	Resp:	247719
Ion Ratio	Lower	Upper	
167	100		
166	21.9	18.1	27.1
139	13.3	11.7	17.5

Manual Integrations
APPROVED

Sohil
8/31/2017 7:13:05 PM

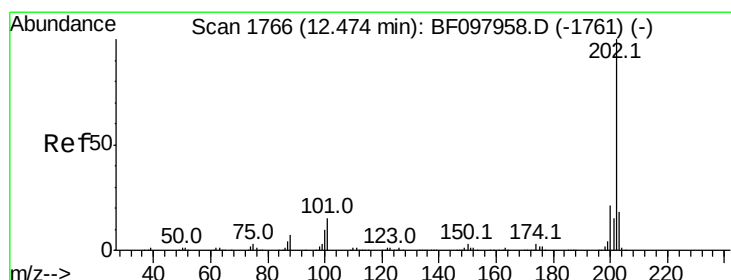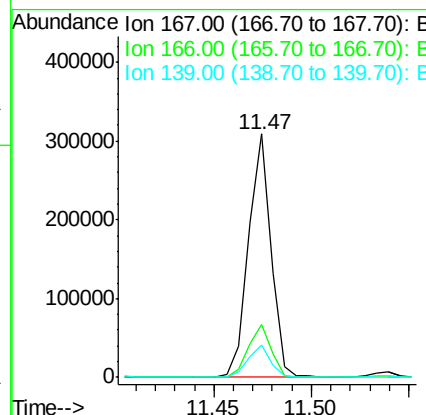

#74

Fluoranthene

Concen: 92.778 ng




RT: 12.46 min Scan# 1764


Delta R.T. -0.01 min

Lab File: BF098179.D

Acq: 31 Aug 2017 2:09

Tgt Ion:	202	Resp:	1390618
Ion Ratio	Lower	Upper	
202	100		
101	13.3	0.0	33.2
203	17.9	0.0	38.1

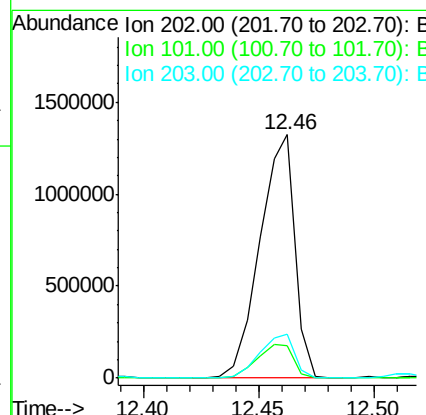



#75

Chrysene-d12

Concen: 20.000 ng

RT: 13.88 min Scan# 2005

Delta R.T. -0.02 min

Lab File: BF098179.D

Acq: 31 Aug 2017 2:09

Instrument :

BNA_F


ClientSampled :

CL-01-082917-B

Tot Ion	Ratio	Resp	Lower	Upper
240	100			
120	12.6	5.8	8.8#	
236	25.7	20.5	30.7	

Manual Integrations
APPROVED




Sohil
8/31/2017 7:13:05 PM



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

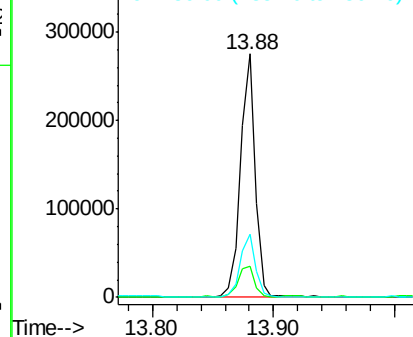

#77

Pyrene

Concen: 61.026 ng

RT: 12.69 min Scan# 1802

Delta R.T. -0.02 min

Lab File: BF098179.D




Acq: 31 Aug 2017 2:09


Tgt Ion	Ratio	Resp	Lower	Upper
202	100			
200	21.2	17.6	26.4	
203	18.0	14.4	21.6	

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

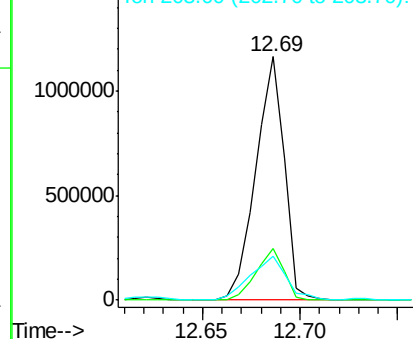







#78
 Terphenyl-d14
 Concen: 15.262 ng
 RT: 12.82 min Scan# 1825
 Delta R.T. -0.03 min
 Lab File: BF098179.D
 Acq: 31 Aug 2017 2:09

Instrument :
 BNA_F
 ClientSampled :
 CL-01-082917-B

Tot Ion	Ratio	Lower	Upper
244	100		
212	7.2	6.0	9.0
122	13.6	10.3	15.5




Manual Integrations
 APPROVED


Sohil
 8/31/2017 7:13:05 PM

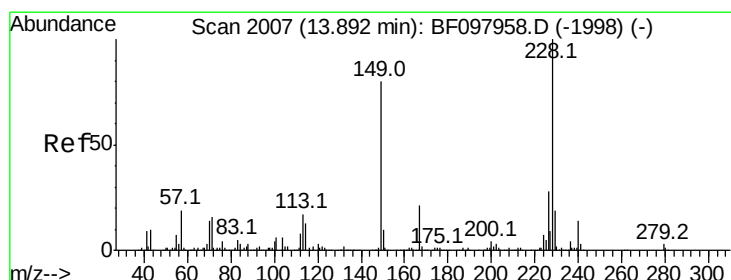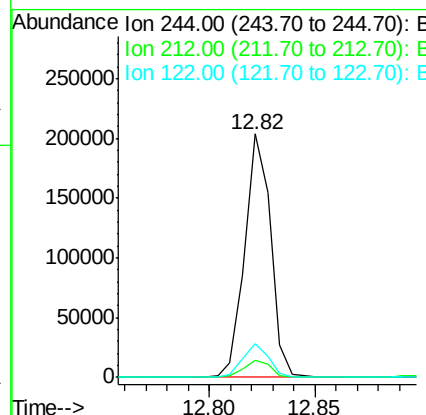

#80
 Benzo(a)anthracene
 Concen: 42.158 ng
 RT: 13.87 min Scan# 2003
 Delta R.T. -0.02 min
 Lab File: BF098179.D
 Acq: 31 Aug 2017 2:09

Tgt Ion	Ratio	Lower	Upper
228	100		
226	31.8	22.6	33.8
229	20.2	16.3	24.5

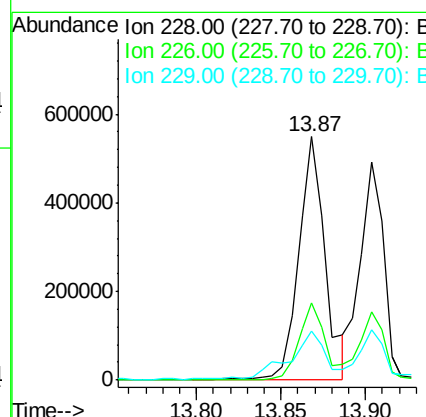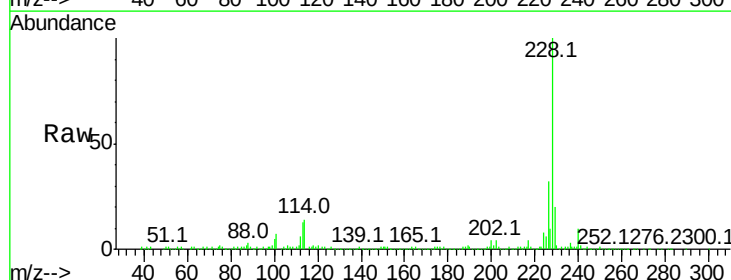

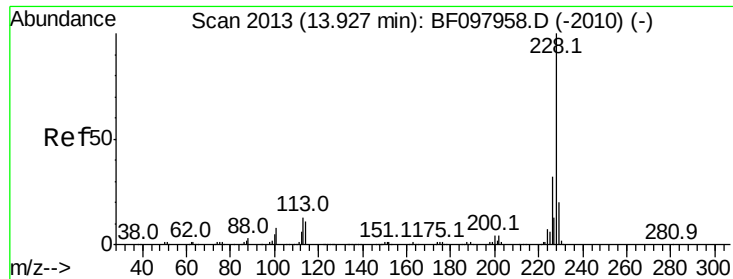





#82
 Chrysene
 Concen: 33.863 ng
 RT: 13.90 min Scan# 2009
 Delta R.T. -0.02 min
 Lab File: BF098179.D
 Acq: 31 Aug 2017 2:09

Instrument :
 BNA_F
 ClientSampled :
 CL-01-082917-B

Tot Ion:	228	Resp:	474041
Ion Ratio	Lower	Upper	
228	100		
226	31.2	24.9	37.3
229	23.0	15.8	23.6




Manual Integrations
 APPROVED


Sohil
 8/31/2017 7:13:05 PM

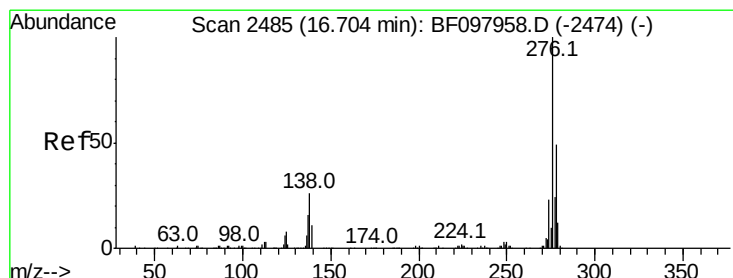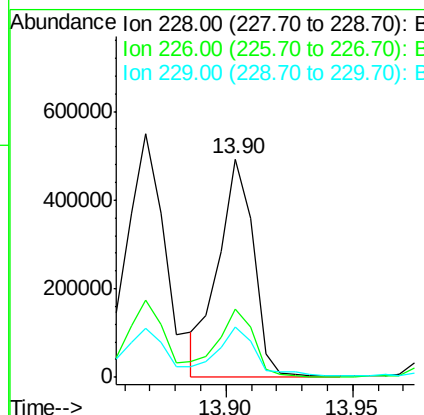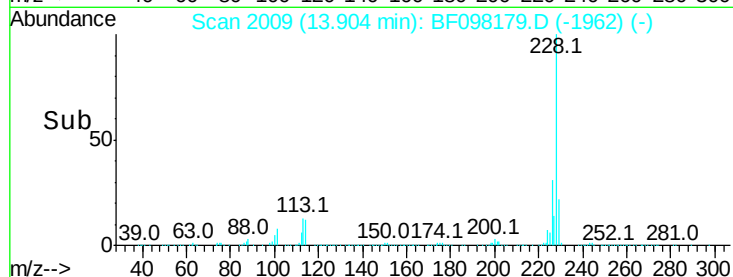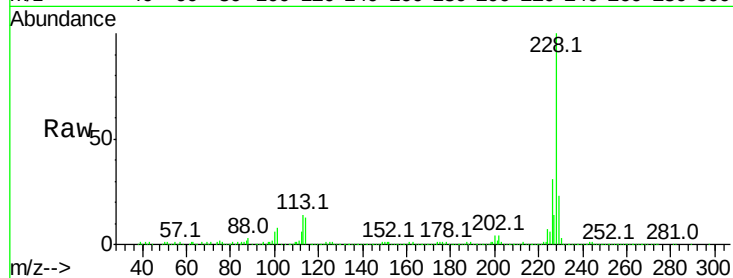

#85
 Indeno(1,2,3-cd)pyrene
 Concen: 15.489 ng
 RT: 16.66 min Scan# 2478
 Delta R.T. -0.02 min
 Lab File: BF098179.D
 Acq: 31 Aug 2017 2:09

Tgt Ion:	276	Resp:	159509
Ion Ratio	Lower	Upper	
276	100		
138	24.7	27.8	41.6#
277	24.9	20.2	30.4

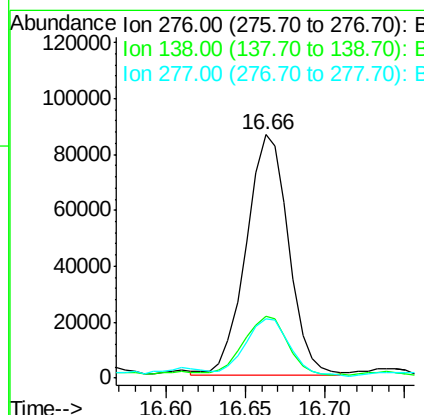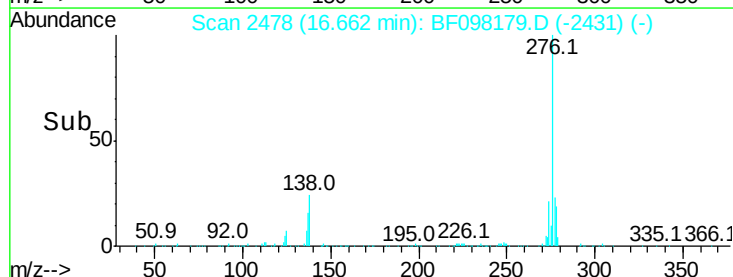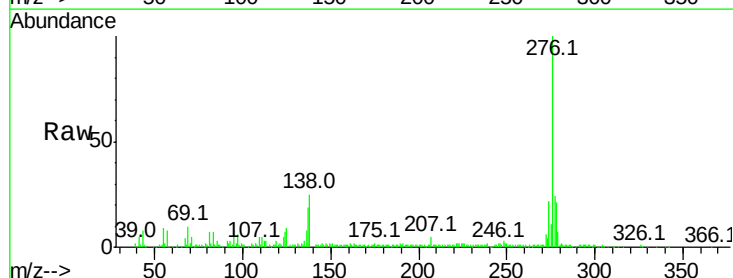



#86

Pervlene-d12

Concen: 20.000 ng

RT: 15.29 min Scan# 2245

Delta R.T. -0.02 min

Lab File: BF098179.D

Acq: 31 Aug 2017 2:09

Instrument :

BNA_F





ClientSampleId :

CL-01-082917-B

Tot Ion:	264	Resp:	168605
Ion Ratio		Lower	Upper
264	100		
260	24.4	19.5	29.3
265	24.0	17.2	25.8

Manual Integrations
APPROVED

Sohil
8/31/2017 7:13:05 PM

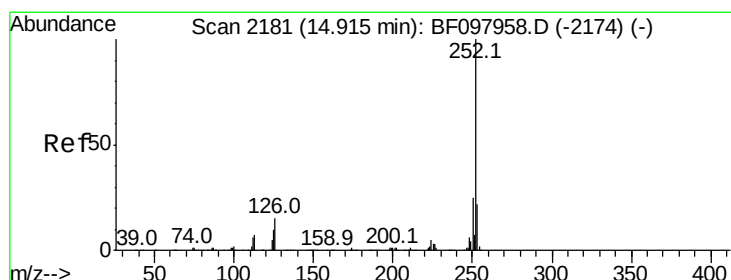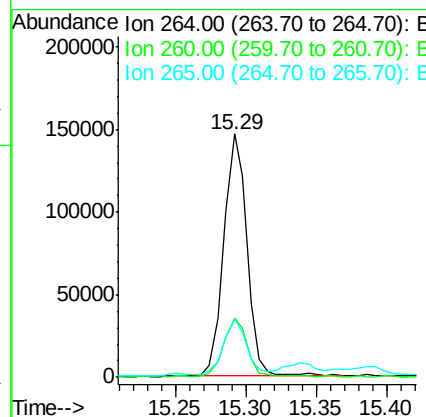

#87

Benzo(b)fluoranthene

Concen: 44.038 ng m




RT: 14.89 min Scan# 2177


Delta R.T. -0.02 min

Lab File: BF098179.D

Acq: 31 Aug 2017 2:09

Tgt Ion:	252	Resp:	468028
Ion Ratio		Lower	Upper
252	100		
253	22.6	18.1	27.1
125	13.0	9.8	14.8

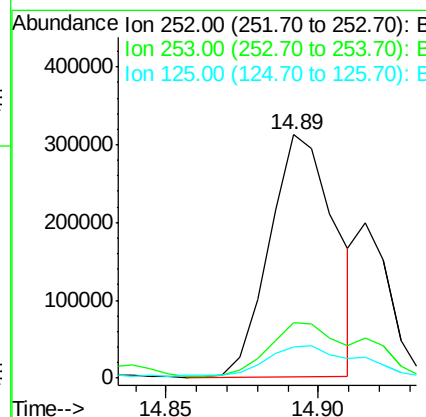

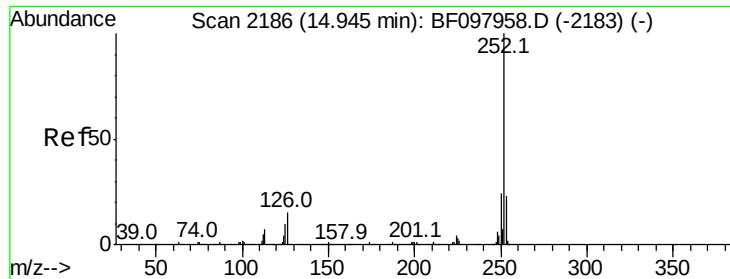

#88

Benzo(k)fluoranthene

Concen: 14.576 ng

RT: 14.92 min Scan# 2181

Delta R.T. -0.02 min

Lab File: BF098179.D

Acq: 31 Aug 2017 2:09

Instrument :

BNA_F





ClientSampleId :

CL-01-082917-B

Tot Ion	Ratio	Resp	Lower	Upper
252	100	145536		
253	26.2		18.4	27.6
125	13.2		13.1	19.7

Manual Integrations
APPROVED

Sohil
8/31/2017 7:13:05 PM

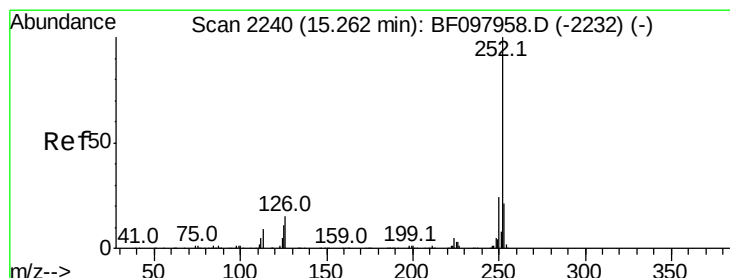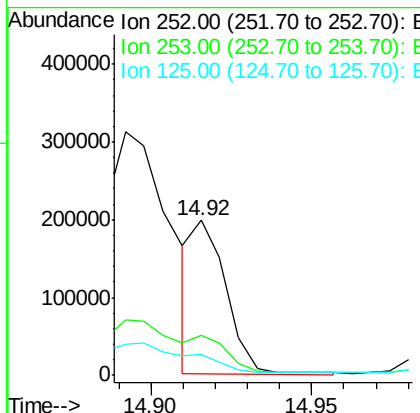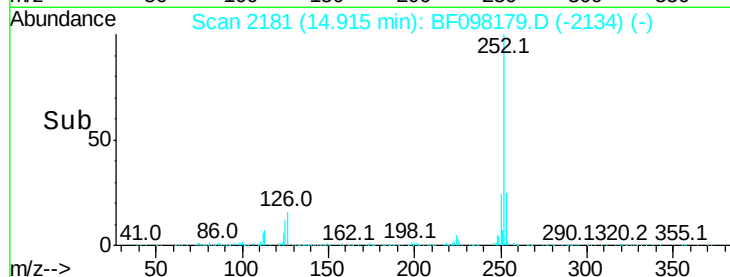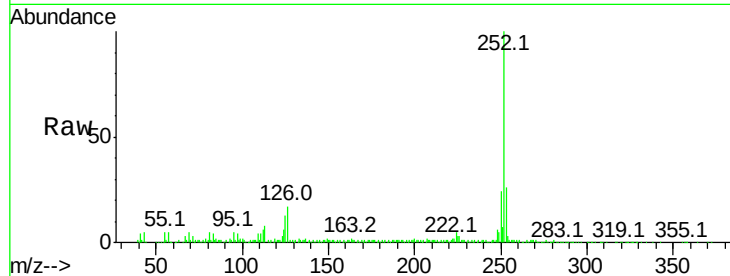

#89

Benzo(a)pyrene

Concen: 34.164 ng




RT: 15.24 min Scan# 2236


Delta R.T. -0.02 min

Lab File: BF098179.D

Acq: 31 Aug 2017 2:09

Tgt Ion	Ratio	Resp	Lower	Upper
252	100	321428		
253	22.7		17.5	26.3
125	12.8		11.0	16.4

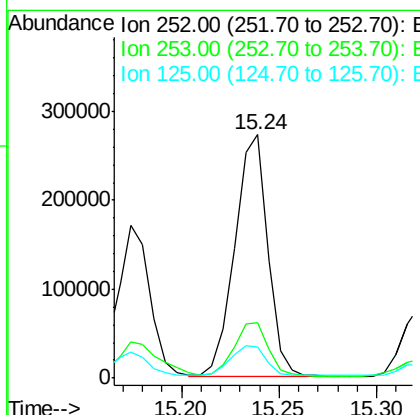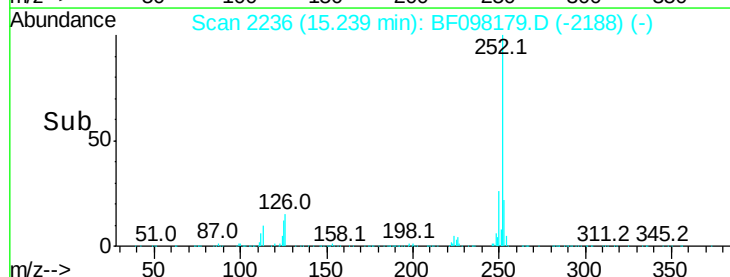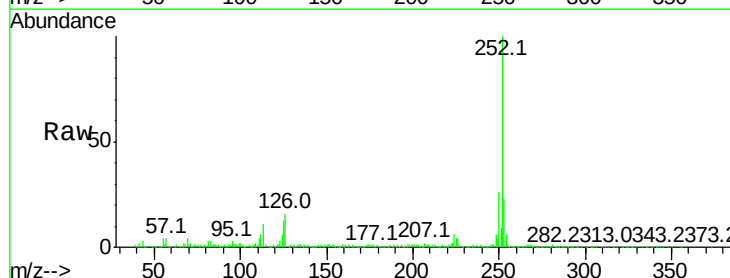







#90
Dibenzo(a,h)anthracene
Concen: 5.382 ng
RT: 16.67 min Scan# 2480
Delta R.T. -0.04 min
Lab File: BF098179.D
Acq: 31 Aug 2017 2:09

Instrument :
BNA_F
ClientSampleId :
CL-01-082917-B

Tot Ion	Ratio	Lower	Upper
278	100		
139	22.8	16.6	24.8
279	29.2	19.3	28.9

Manual Integrations
APPROVED

Sohil
8/31/2017 7:13:05 PM

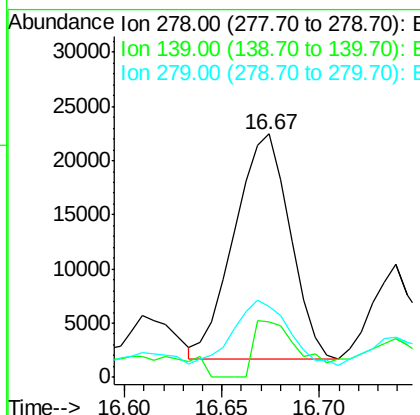

#91
Benzo(g,h,i)perylene
Concen: 18.195 ng
RT: 17.08 min Scan# 2549
Delta R.T. -0.03 min
Lab File: BF098179.D
Acq: 31 Aug 2017 2:09

Tgt Ion	Ratio	Lower	Upper
276	100		
277	26.6	18.6	28.0
138	25.8	25.4	38.0

