


Data Path : Z:\HPCHEM1\BNA F\Data\BF083017\
 Data File : BF098158.D
 Acq On : 30 Aug 2017 16:16
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 21 15:59:04 2017

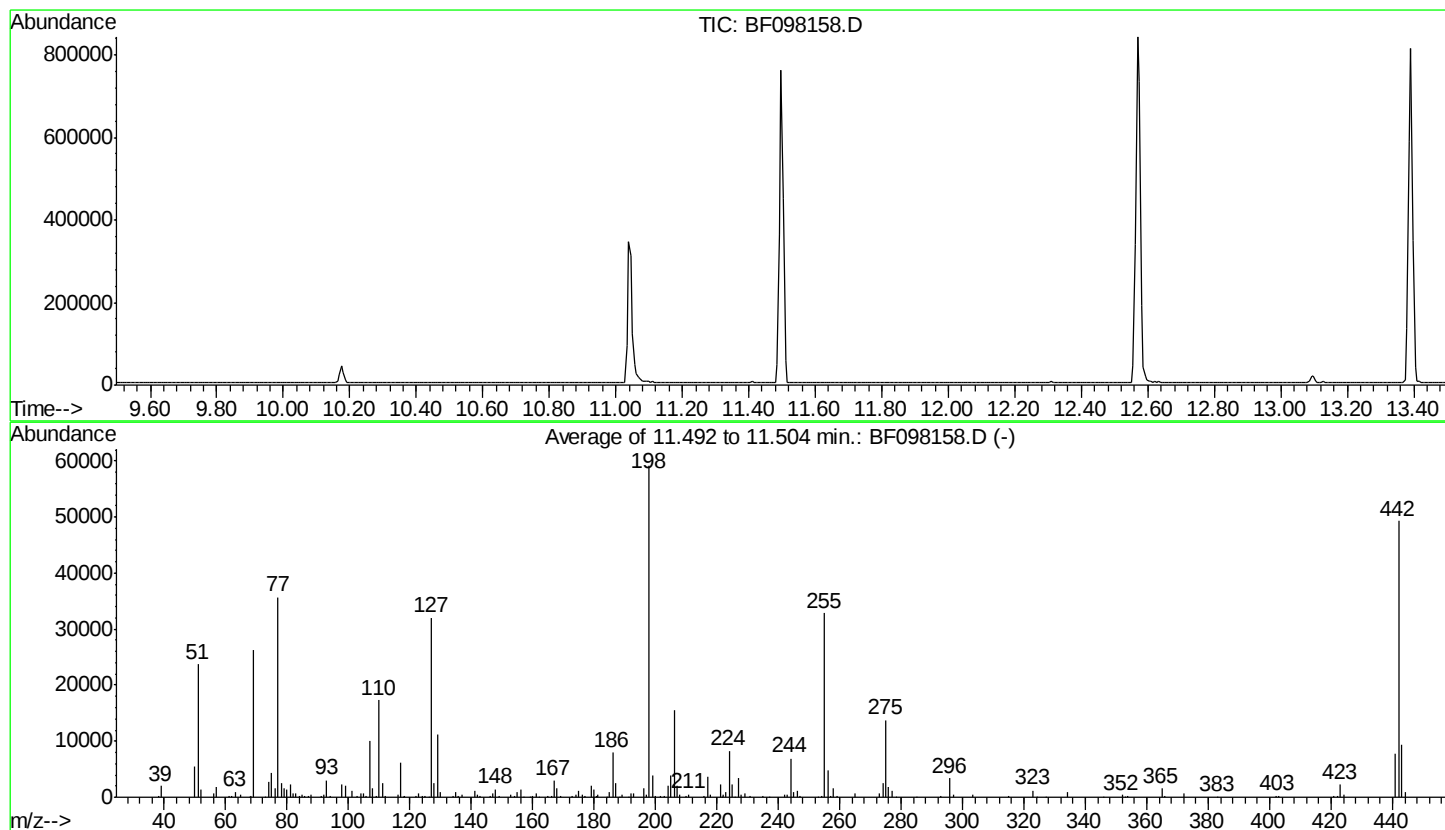

AutoFind: Scans 1599, 1600, 1601; Background Corrected with Scan 1595

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.1	23755	PASS
68	69	0.00	2	1.3	340	PASS
69	198	0.00	100	44.3	26194	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.2	32064	PASS
197	198	0.00	2	0.7	391	PASS
198	198	100	100	100.0	59186	PASS
199	198	5	9	6.7	3976	PASS
275	198	10	60	23.3	13816	PASS
365	198	1	100	2.7	1594	PASS
441	442	0.01	24	15.8	7813	PASS
442	198	50	100	83.4	49347	PASS
443	442	15	24	19.0	9376	PASS