


Data Path : Z:\HPCHEM1\BNA F\Data\BF083017\
 Data File : BF098183.D
 Acq On : 31 Aug 2017 4:30
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 21 15:59:04 2017

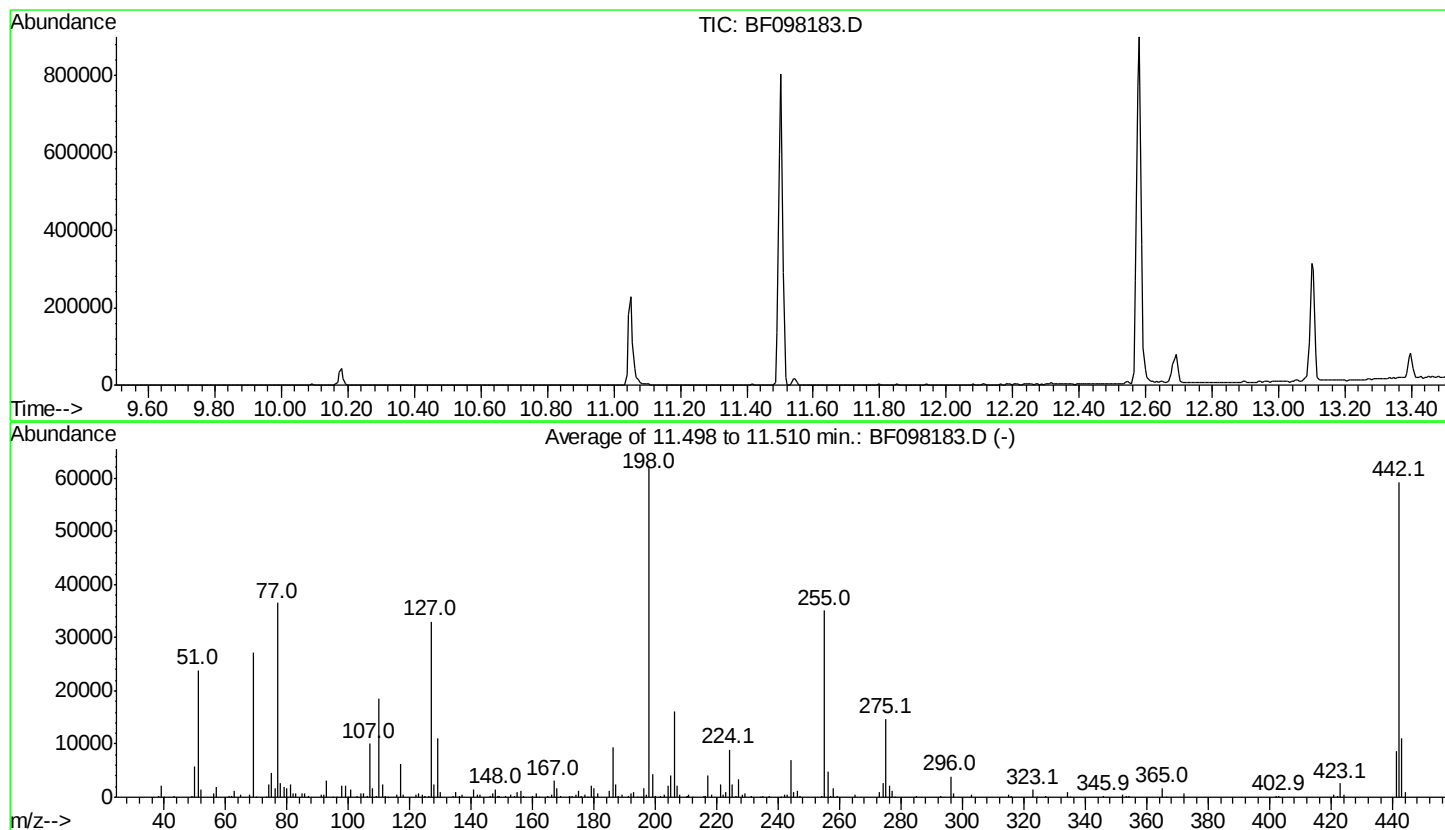

AutoFind: Scans 1600, 1601, 1602; Background Corrected with Scan 1595

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.3	23900	PASS
68	69	0.00	2	1.6	429	PASS
69	198	0.00	100	43.7	27223	PASS
70	69	0.00	2	0.4	100	PASS
127	198	10	80	52.9	32998	PASS
197	198	0.00	2	0.9	563	PASS
198	198	100	100	100.0	62362	PASS
199	198	5	9	7.0	4338	PASS
275	198	10	60	23.6	14740	PASS
365	198	1	100	2.8	1769	PASS
441	442	0.01	24	14.8	8784	PASS
442	198	50	100	95.1	59304	PASS
443	442	15	24	18.8	11157	PASS