
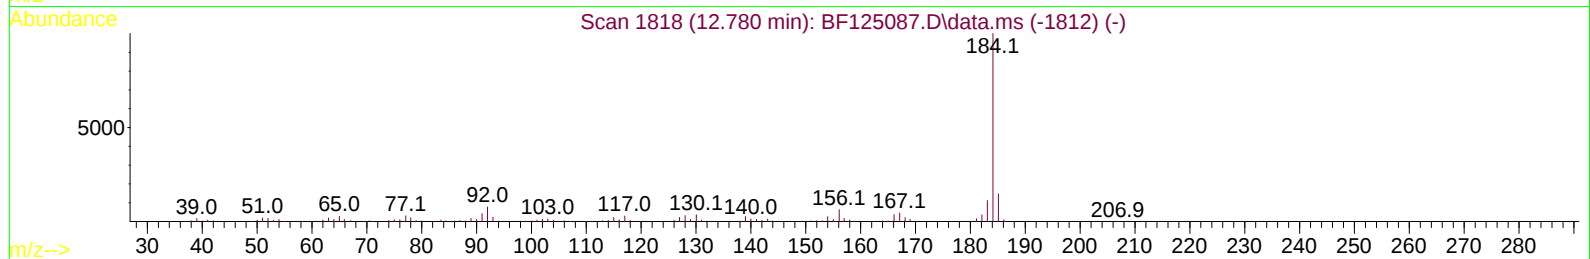
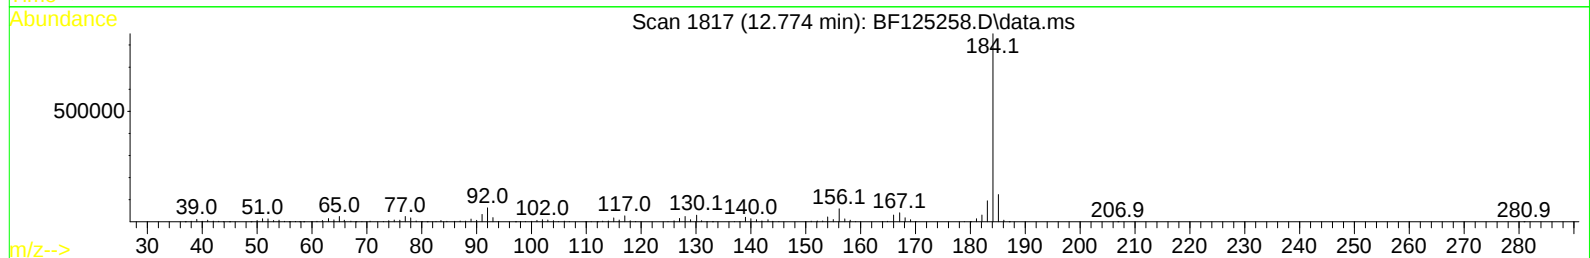


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF083021\  
Data File : BF125258.D  
Acq On : 30 Aug 2021 12:16  
Operator : JU/CG  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 30 12:41:55 2021  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF081821.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Aug 24 12:39:21 2021  
Response via : Initial Calibration

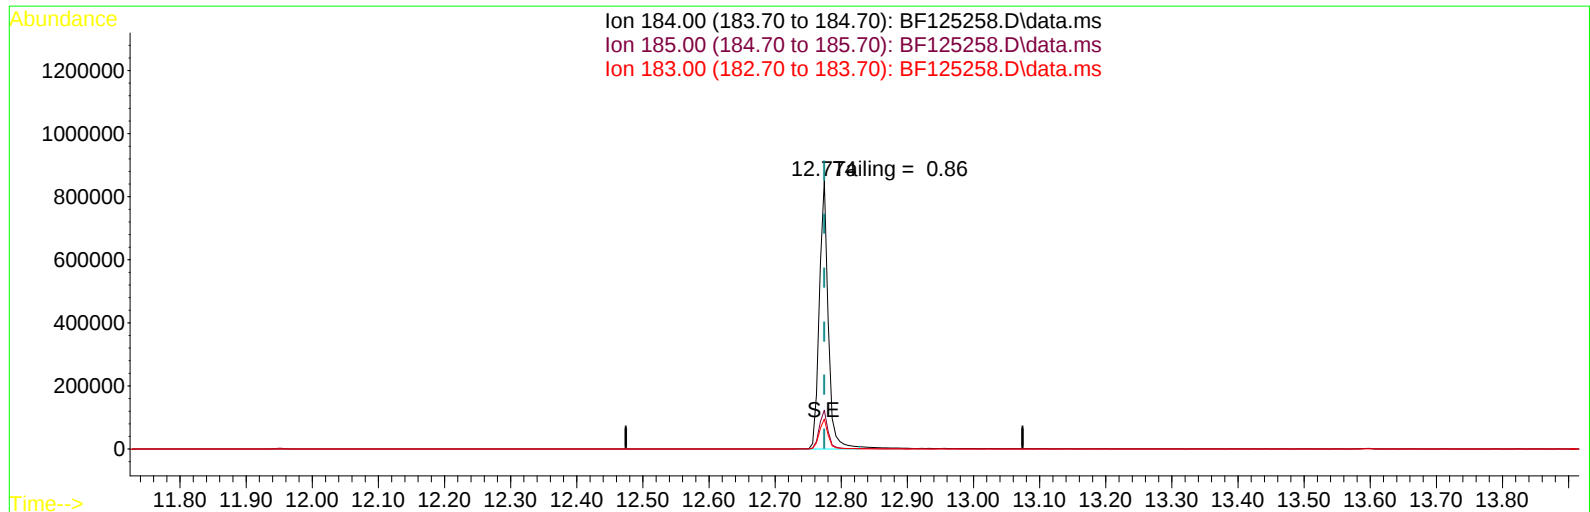

TIC: BF125258.D\data.ms

**(77) Benzidine**




**12.774min (-0.000) 18992.26 ng**

**response 815860**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 13.50  | 14.49  |
| 183.00 | 10.10  | 11.21  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF083021\  
Data File : BF125258.D  
Acq On : 30 Aug 2021 12:16  
Operator : JU/CG  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 30 12:41:55 2021  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF081821.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Aug 24 12:39:21 2021  
Response via : Initial Calibration

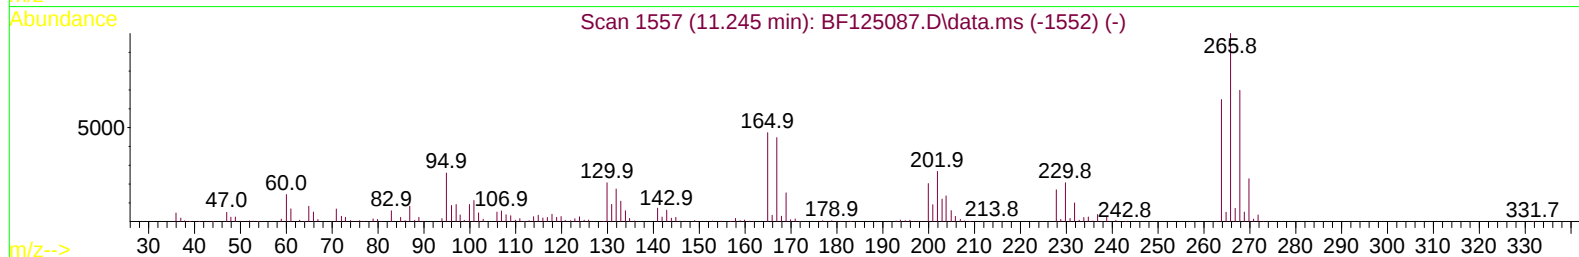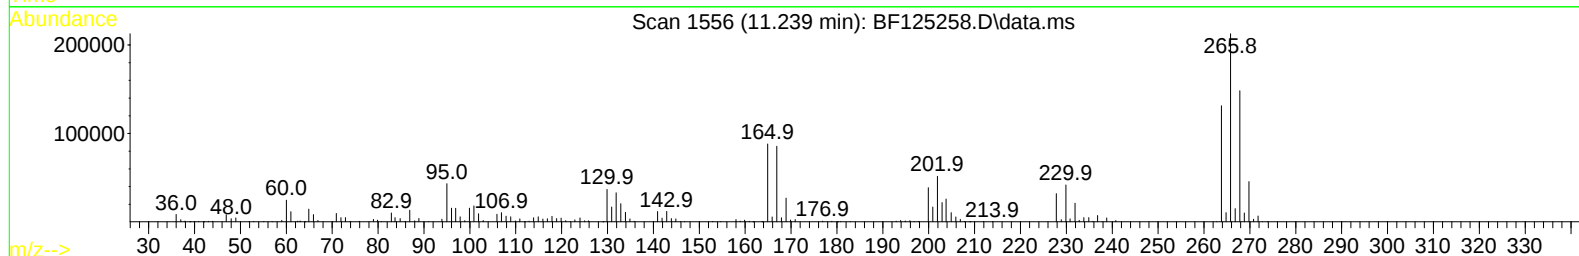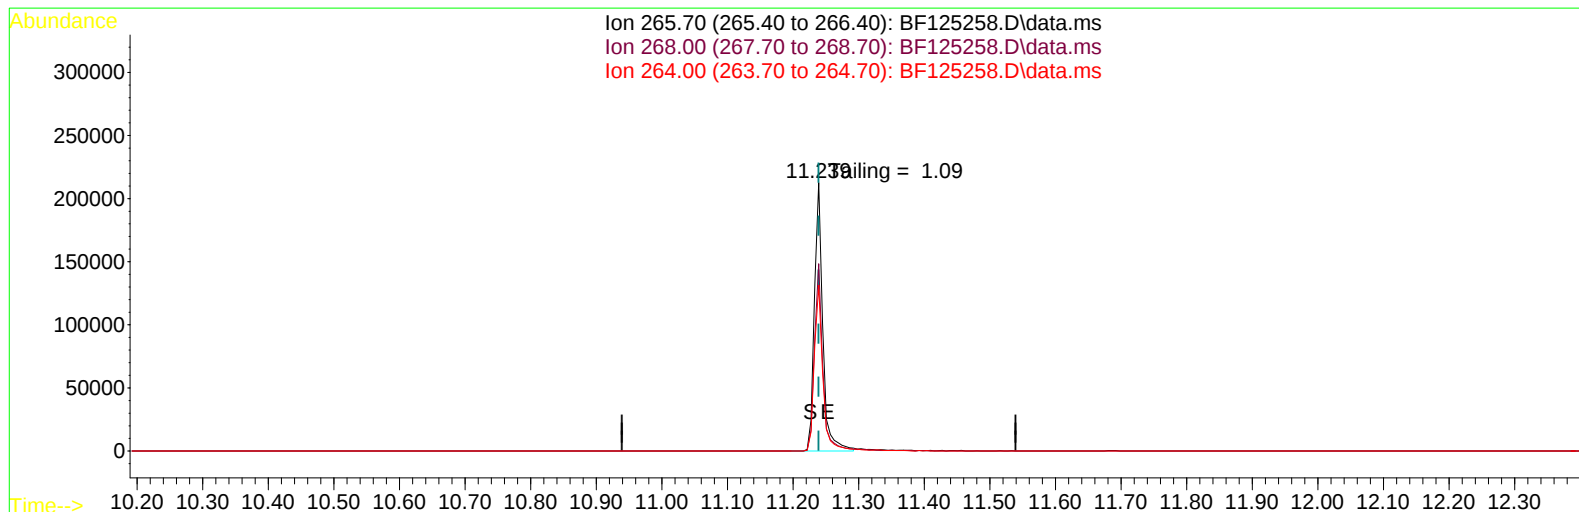

TIC: BF125258.D\data.ms

**(70) Pentachlorophenol (C)**

**11.239min (-0.000) 242144.34 ng**

**response 195619**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 61.10  | 69.76  |
| 264.00 | 69.90  | 61.78  |
| 0.00   | 0.00   | 0.00   |