

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF083021\
 Data File : BF125260.D
 Acq On : 30 Aug 2021 13:20
 Operator : JU/CG
 Sample : PB138793BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB138793BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF125260.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.269	22	31	37	rVB	112648	163422	2.15%	0.361%
2	5.545	582	588	591	rBV	5574220	6328382	83.28%	13.964%
3	6.539	751	757	760	rBV	4929195	6215072	81.78%	13.714%
4	6.916	817	821	824	rBV	1369727	1225176	16.12%	2.703%
5	7.481	911	917	920	rBV	3649998	4116240	54.17%	9.082%
6	8.198	1034	1039	1042	rBV	1633390	1589843	20.92%	3.508%
7	9.275	1216	1222	1225	rBV	6762812	7008094	92.22%	15.463%
8	9.951	1332	1337	1347	rBV	2026915	1832497	24.11%	4.043%
9	10.739	1466	1471	1485	rBV	4587835	4707898	61.95%	10.388%
10	11.439	1586	1590	1597	rBV	2091659	1872333	24.64%	4.131%
11	13.027	1855	1860	1863	rBV	7719461	7599317	100.00%	16.768%
12	14.080	2035	2039	2047	rVB	1448300	1432751	18.85%	3.161%
13	15.574	2288	2293	2306	rVB	822236	1229574	16.18%	2.713%




Sum of corrected areas: 45320599

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF083021\
Data File : BF125260.D
Acq On : 30 Aug 2021 13:20
Operator : JU/CG
Sample : PB138793BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB138793BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

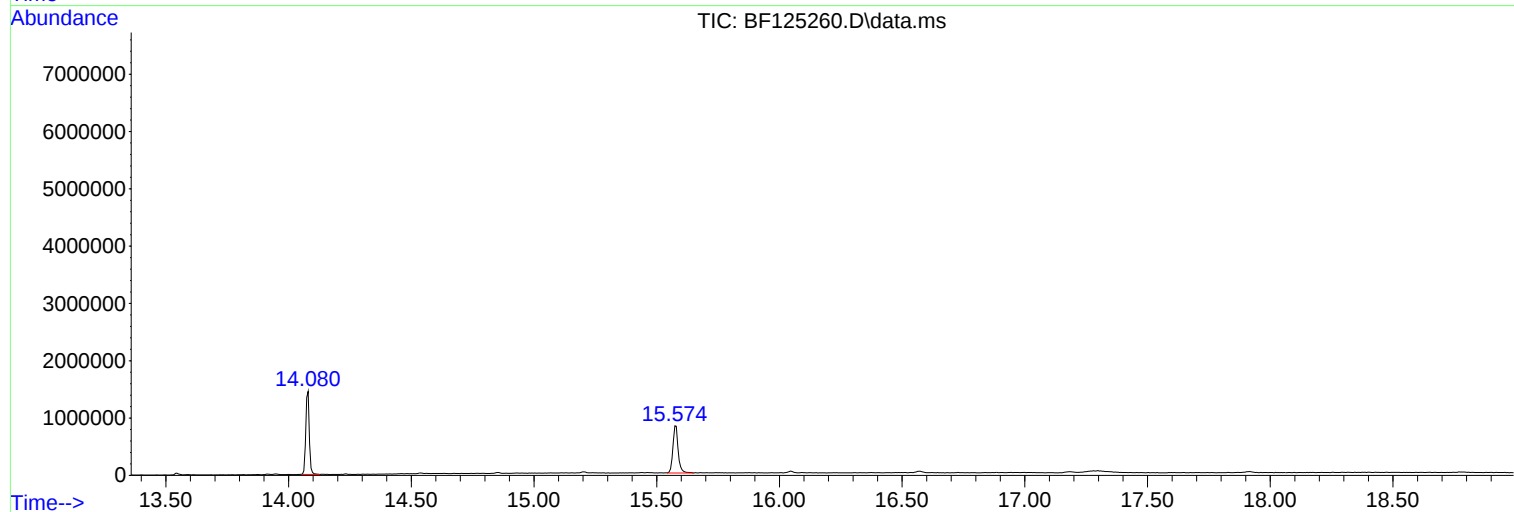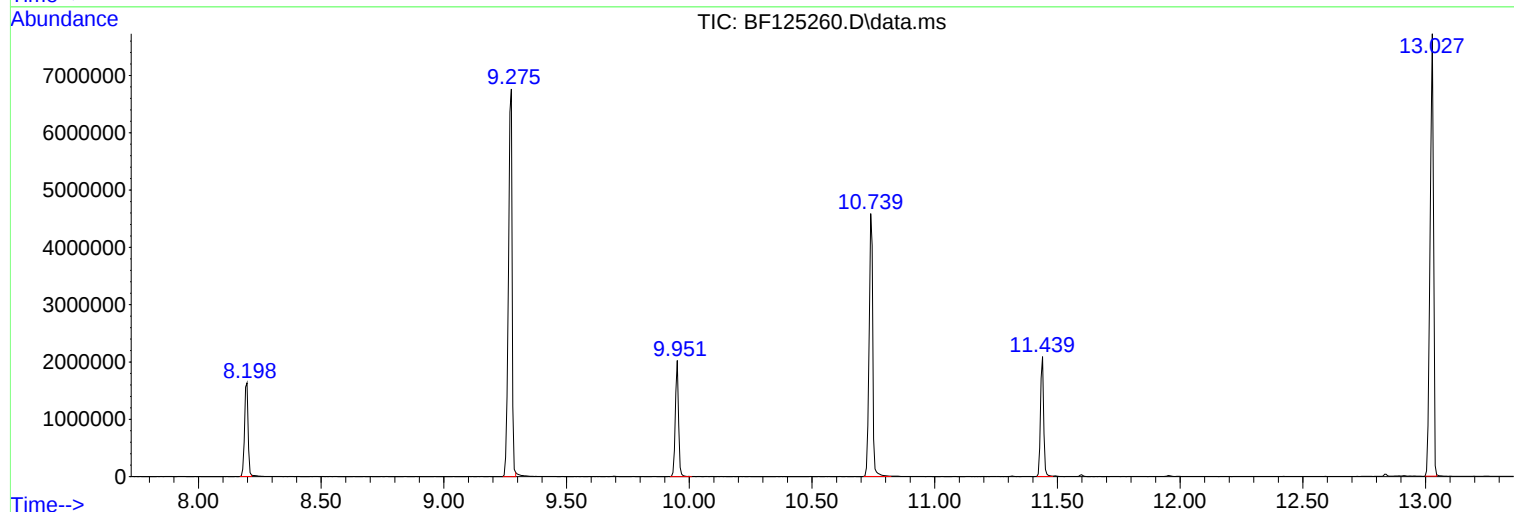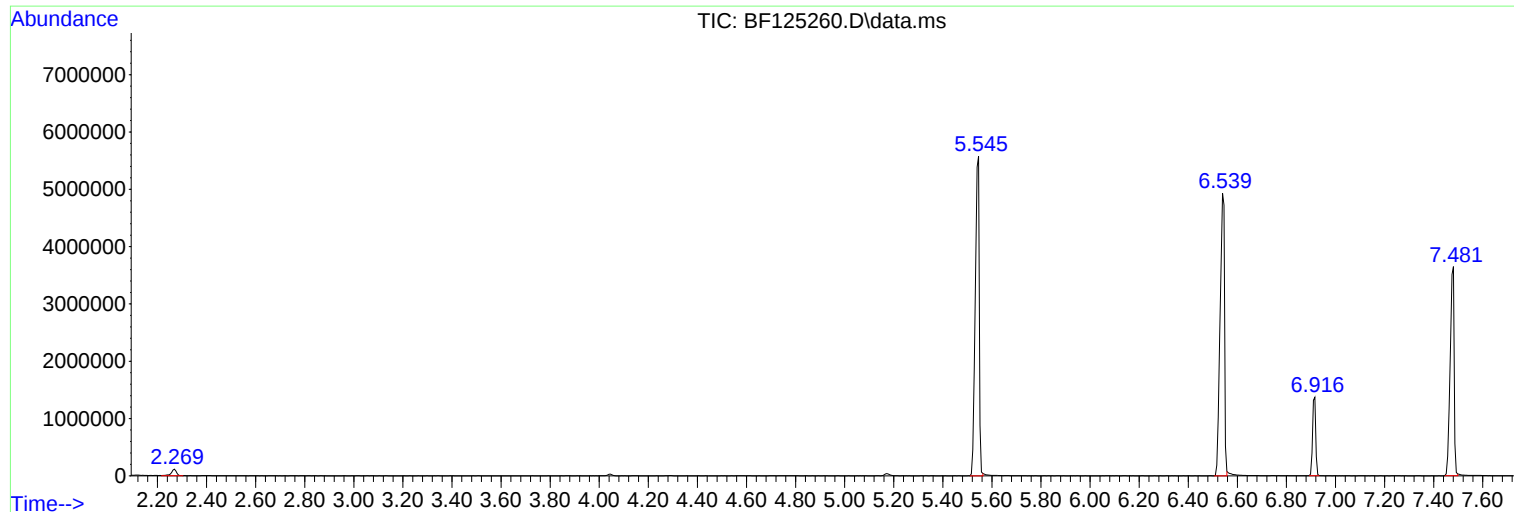

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF083021\
Data File : BF125260.D
Acq On : 30 Aug 2021 13:20
Operator : JU/CG
Sample : PB138793BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB138793BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.269	2.67 ng	163422	1,4-Dichlorobenzene-d4	6.916

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	38
3			2-Methyl-5-hexen-3-ol	114	C7H14O	032815-70-6	25
4			3-Hexanol, 2-methyl-	116	C7H16O	000617-29-8	25
5			3-Pentanol, 3-methyl-	102	C6H14O	000077-74-7	17

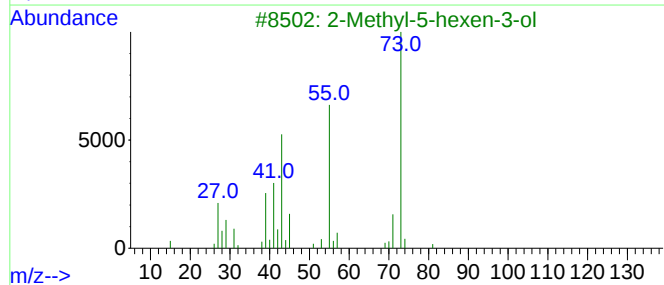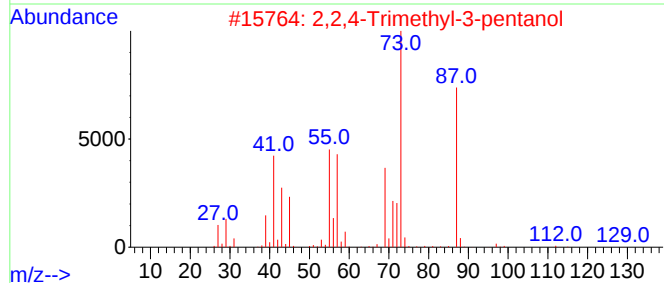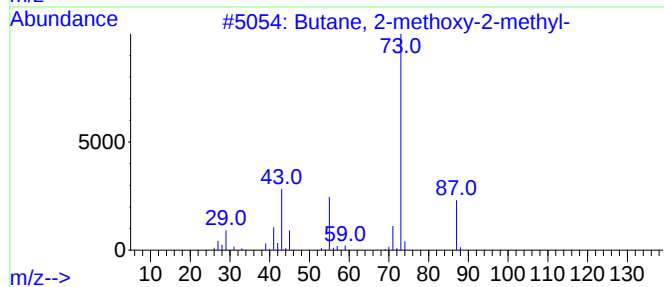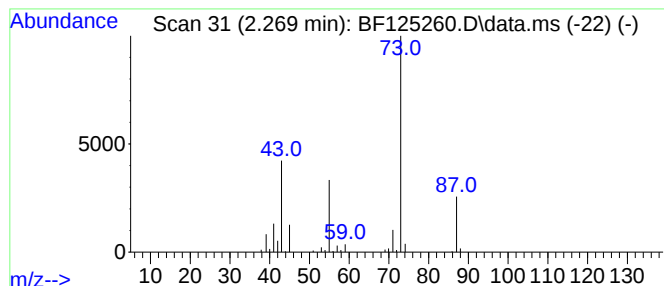

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF083021\
Data File : BF125260.D
Acq On : 30 Aug 2021 13:20
Operator : JU/CG
Sample : PB138793BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB138793BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.269	2.7	ng	163422	1	6.916	1225180	20.0