
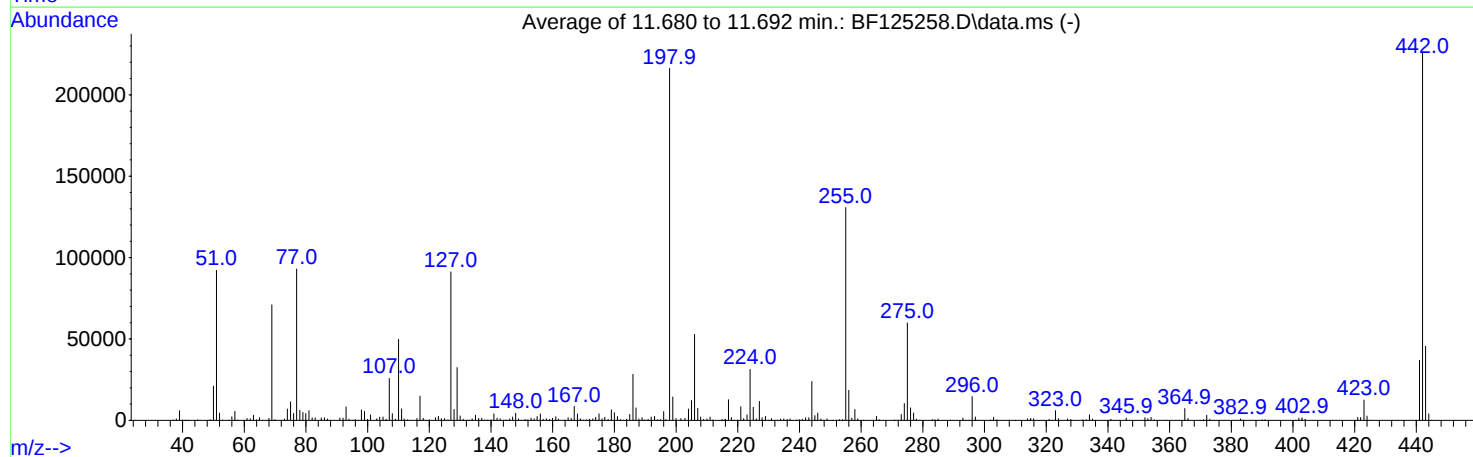


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF083021\  
 Data File : BF125258.D  
 Acq On : 30 Aug 2021 12:16  
 Operator : JU/CG  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF081821.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Tue Aug 24 12:39:21 2021

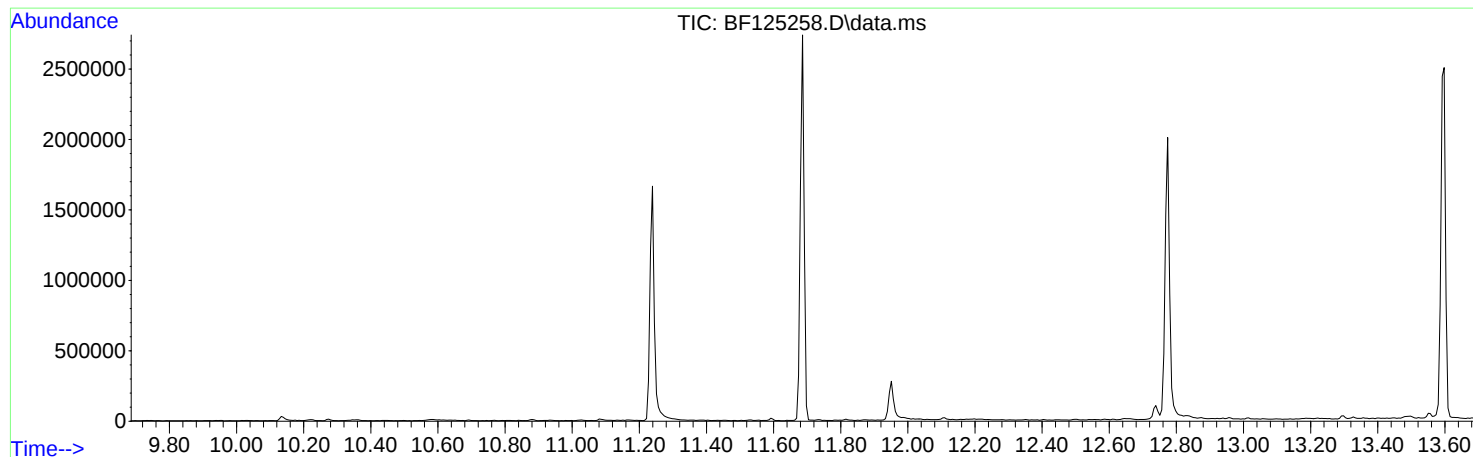




AutoFind: Scans 1631, 1632, 1633; Background Corrected with Scan 1626

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 42.6         | 92128      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.7          | 1227       | PASS                |
| 69             | 198             | 0.00            | 100             | 32.8         | 70974      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.5          | 356        | PASS                |
| 127            | 198             | 10              | 80              | 42.2         | 91237      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.3          | 541        | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 216237     | PASS                |
| 199            | 198             | 5               | 9               | 6.6          | 14322      | PASS                |
| 275            | 198             | 10              | 60              | 27.7         | 59837      | PASS                |
| 365            | 198             | 1               | 100             | 3.4          | 7321       | PASS                |
| 441            | 198             | 0.01            | 100             | 17.0         | 36840      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 226016     | PASS                |
| 443            | 442             | 15              | 24              | 20.1         | 45475      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF083021\  
Data File : BF125258.D  
Acq On : 30 Aug 2021 12:16  
Operator : JU/CG  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Aug 30 12:41:55 2021  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF081821.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Aug 24 12:39:21 2021  
Response via : Initial Calibration

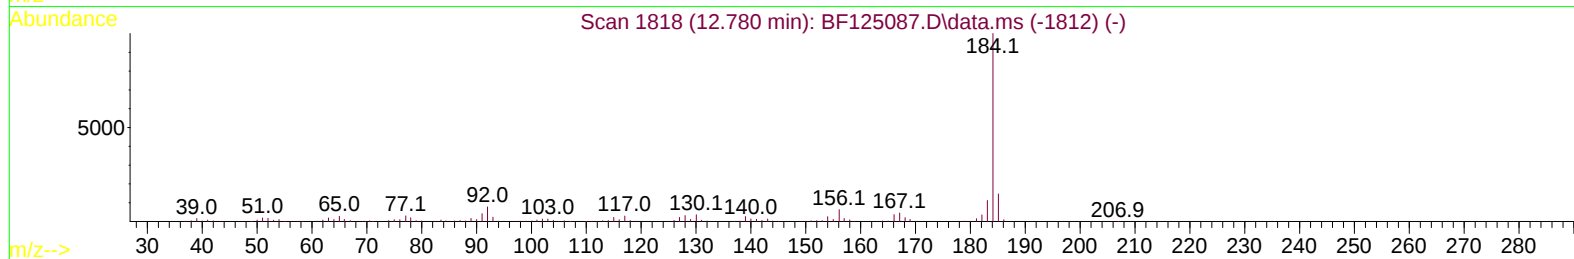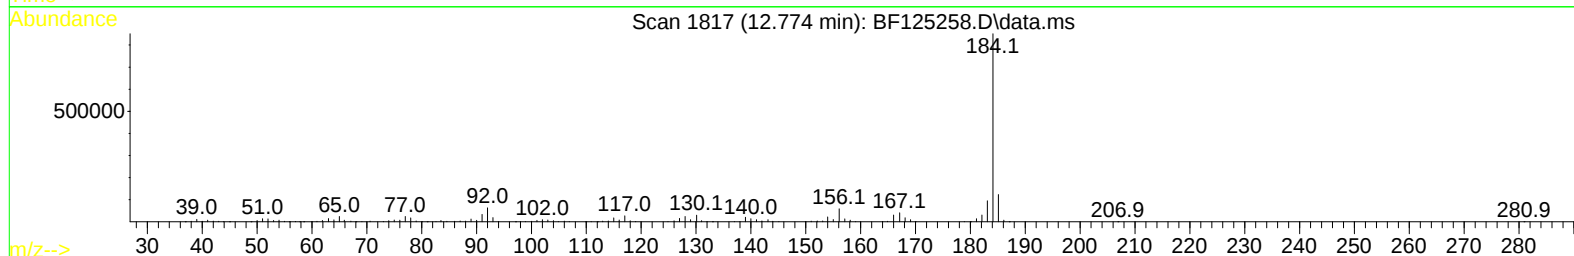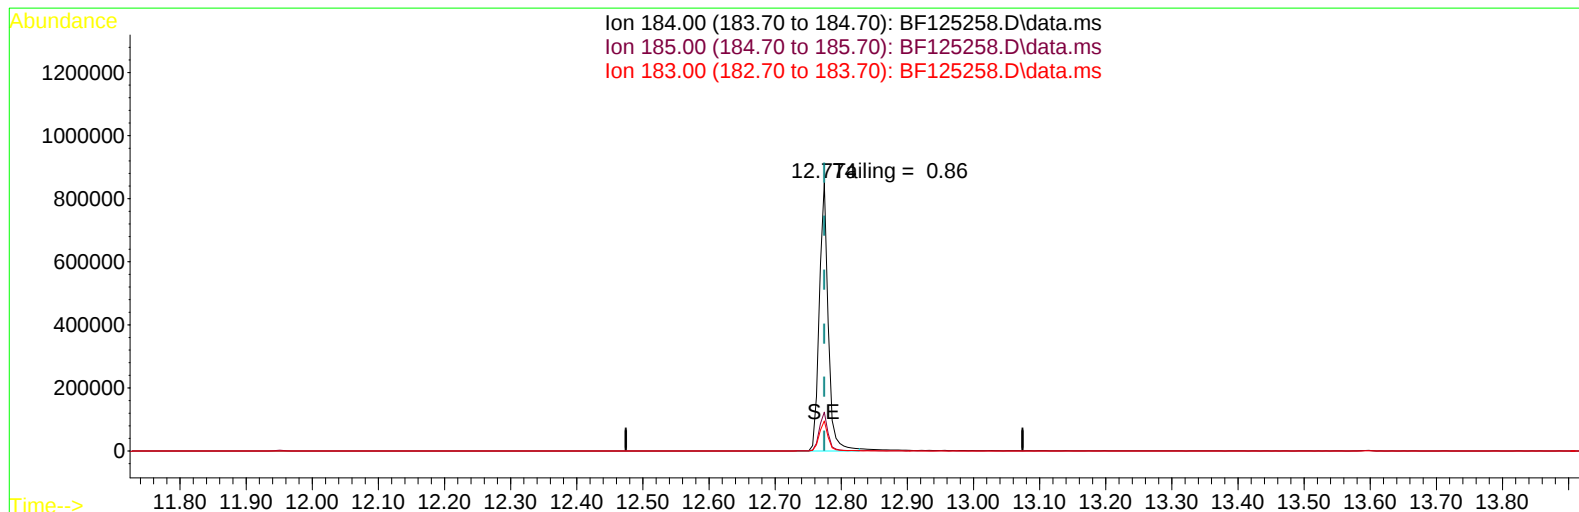

TIC: BF125258.D\data.ms

(77) Benzidine

12.774min (-0.000) 18992.26 ng




response 815860

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 13.50  | 14.49  |
| 183.00 | 10.10  | 11.21  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF083021\  
Data File : BF125258.D  
Acq On : 30 Aug 2021 12:16  
Operator : JU/CG  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Aug 30 12:41:55 2021  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF081821.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Aug 24 12:39:21 2021  
Response via : Initial Calibration

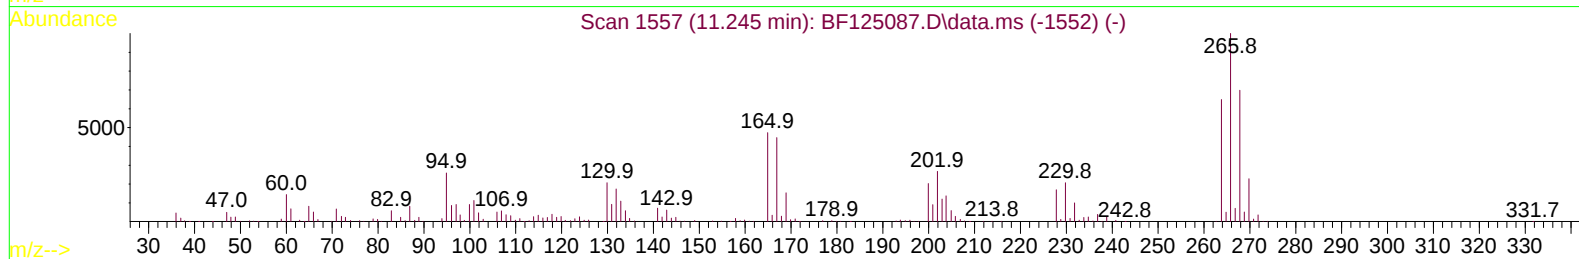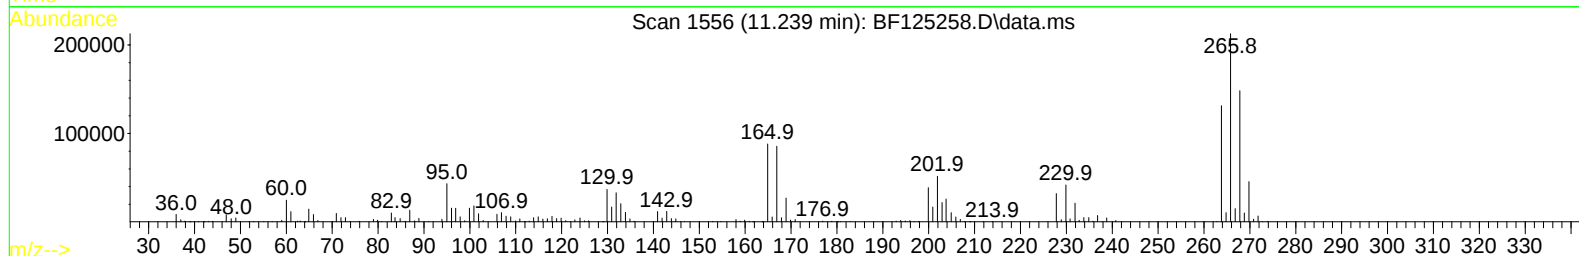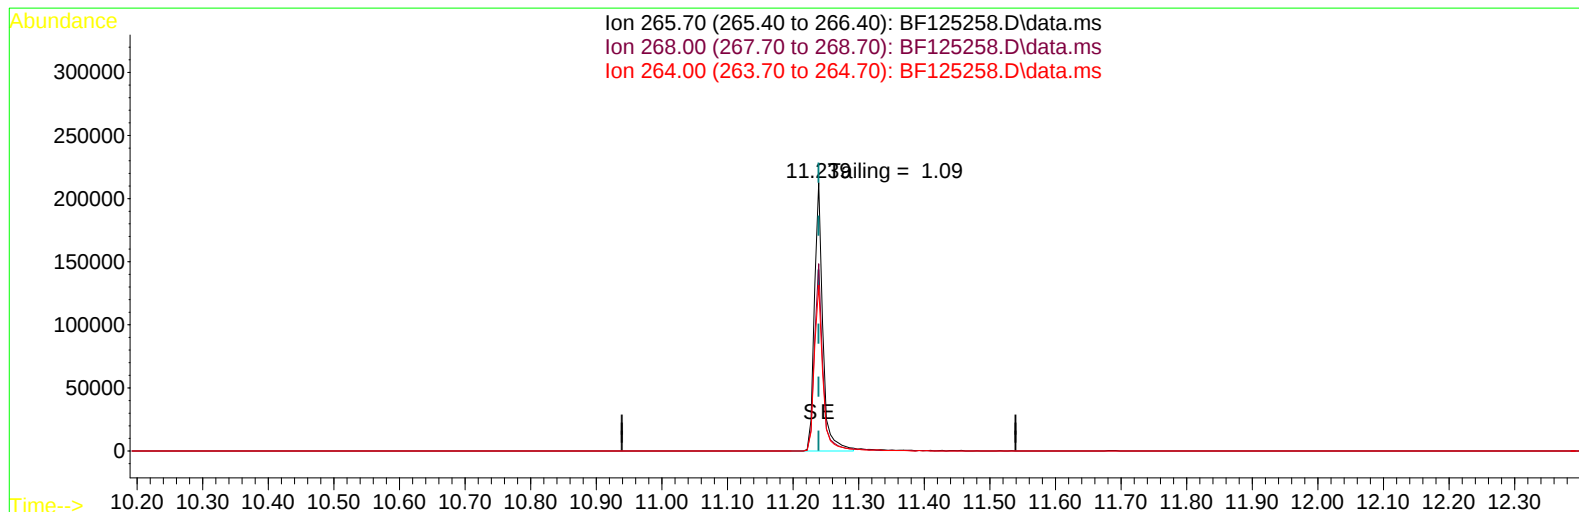

TIC: BF125258.D\data.ms

**(70) Pentachlorophenol (C)**

11.239min (-0.000) 242144.34 ng

response 195619

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 61.10  | 69.76  |
| 264.00 | 69.90  | 61.78  |
| 0.00   | 0.00   | 0.00   |

# DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 8/30/2021     | BNA_F            | <u>BF125258.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 492554           | 13.59              |
| DDD           | 4785             | 13.29              |
| DDE           | 1381             | 12.95              |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 6166          | 498720           | 1.24               |
|               |                  |                    |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP