
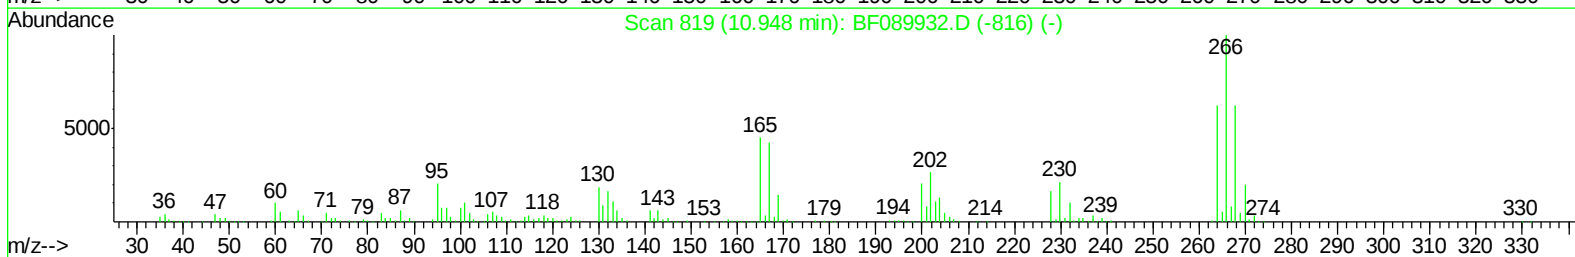
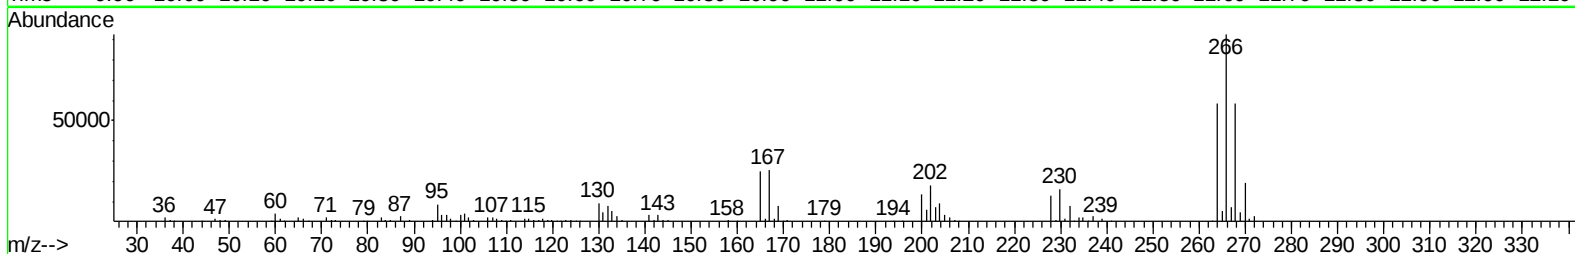


Data Path : Z:\HPCHEM1\BNA_F\Data\BF083116\
Data File : BF089937.D
Acq On : 31 Aug 2016 8:45
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 01 03:54:35 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF083116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 31 11:55:18 2016
Response via : Initial Calibration

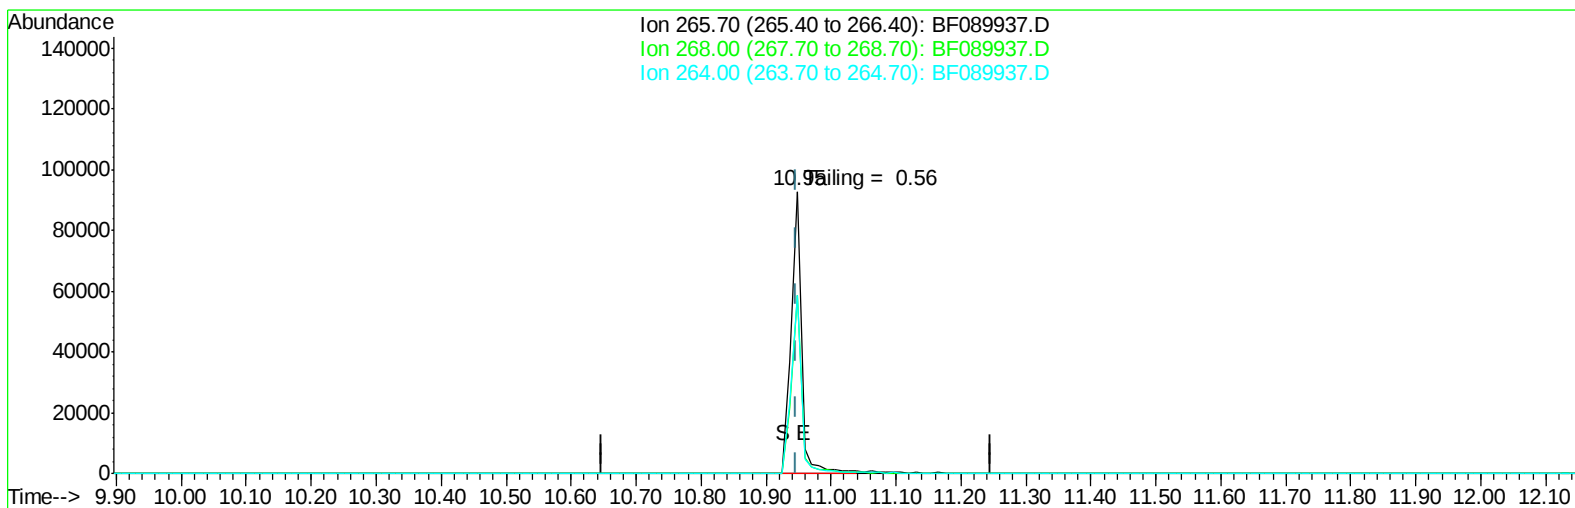

TIC: BF089937.D

(69) Pentachlorophenol (C)




10.948min (+0.001) 36240.64ng

response 103807

Ion	Exp%	Act%
265.70	100	100
268.00	63.80	63.35
264.00	63.20	63.40
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF083116\
Data File : BF089937.D
Acq On : 31 Aug 2016 8:45
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 01 03:54:35 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF083116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 31 11:55:18 2016
Response via : Initial Calibration

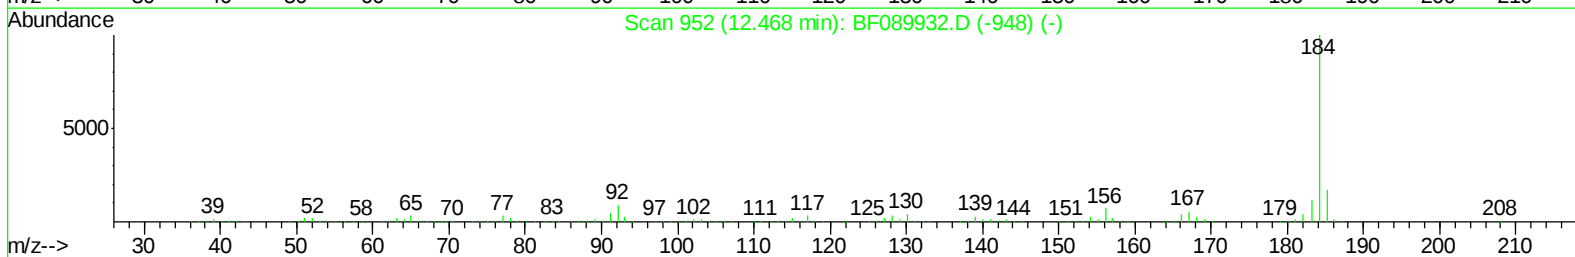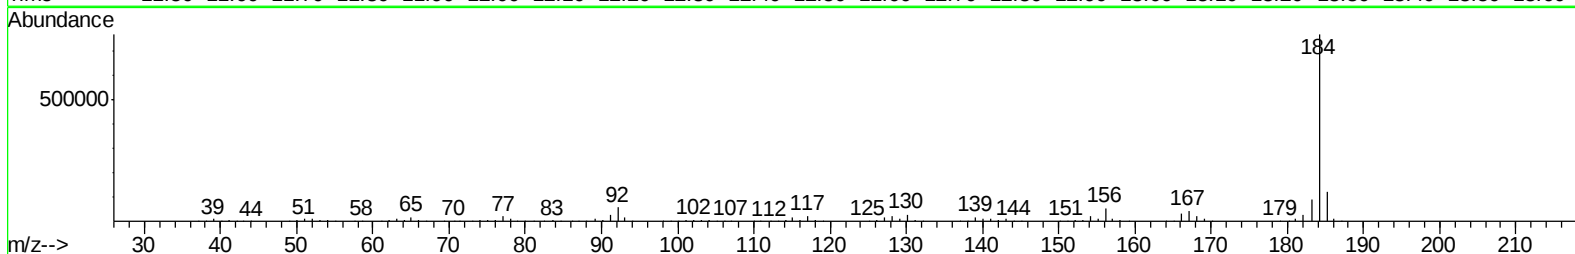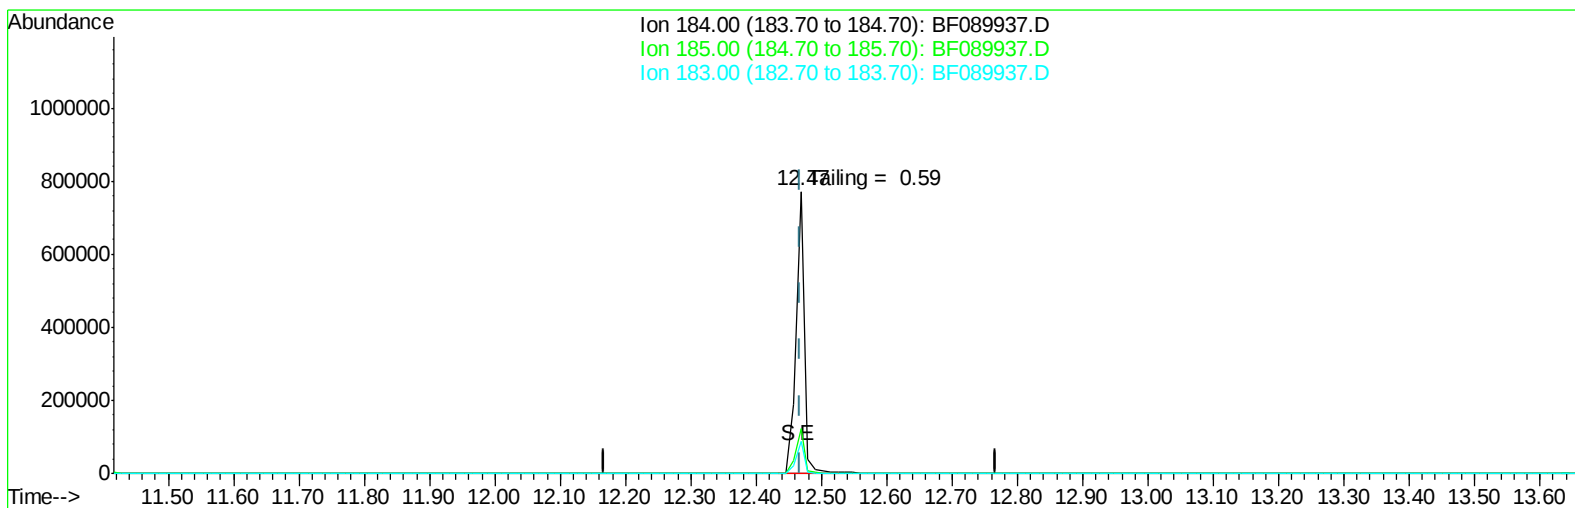

TIC: BF089937.D

(76) Benzidine

12.468min (+0.000) 52369.81ng

response 716199

Ion	Exp%	Act%
184.00	100	100
185.00	17.30	15.94
183.00	12.00	11.60
0.00	0.00	0.00