


Data Path : Z:\HPCHEM1\BNA_F\Data\BF083117\
 Data File : BF098198.D
 Acq On : 31 Aug 2017 16:22
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 01 16:30:12 2017

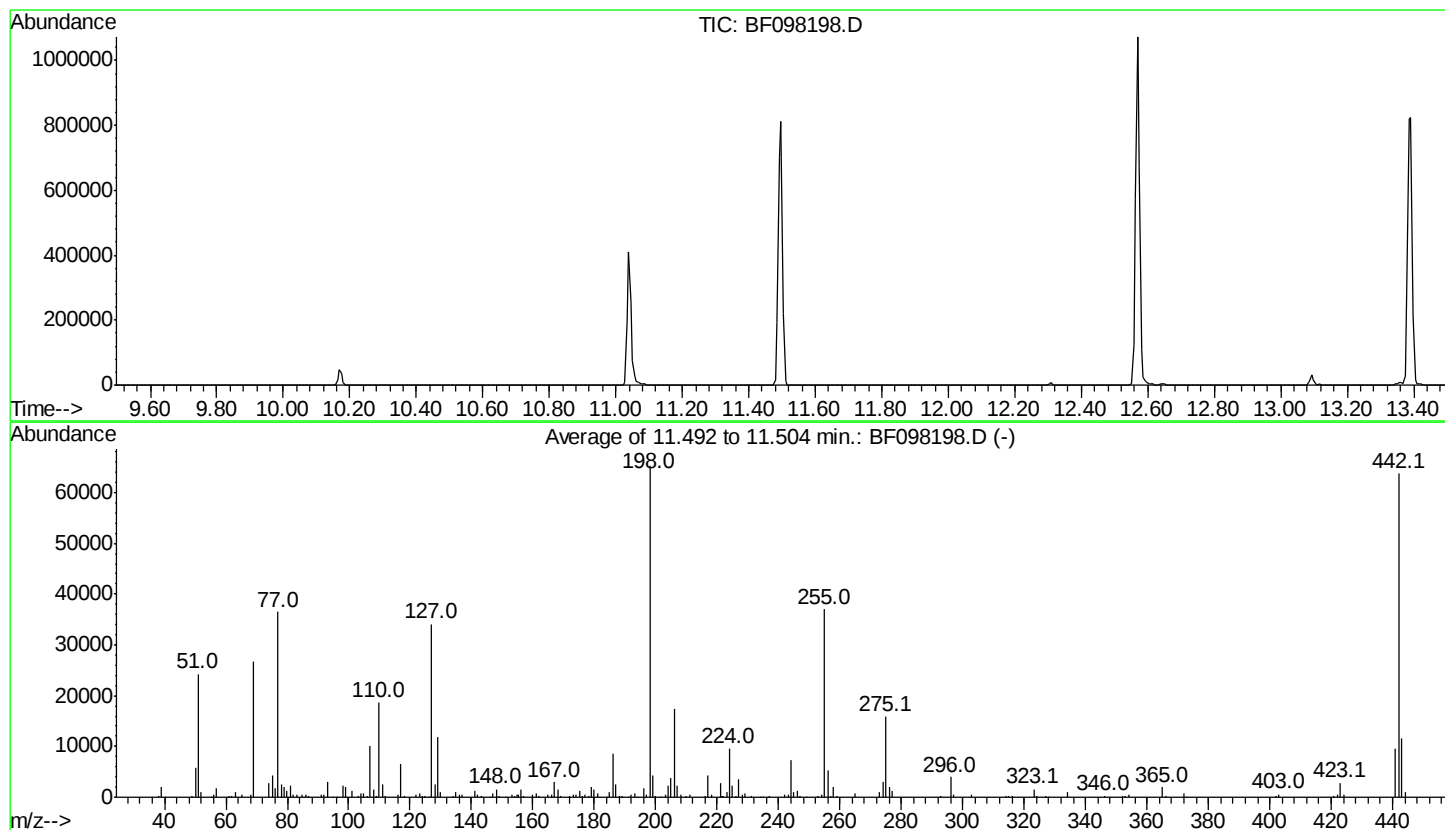

AutoFind: Scans 1599, 1600, 1601; Background Corrected with Scan 1594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.1	24249	PASS
68	69	0.00	2	1.5	410	PASS
69	198	0.00	100	41.1	26819	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.2	34077	PASS
197	198	0.00	2	0.9	592	PASS
198	198	100	100	100.0	65288	PASS
199	198	5	9	6.6	4308	PASS
275	198	10	60	24.2	15821	PASS
365	198	1	100	3.0	1947	PASS
441	442	0.01	24	15.1	9625	PASS
442	198	50	100	97.5	63666	PASS
443	442	15	24	18.4	11704	PASS