

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF083120\
 Data File : BF121483.D
 Acq On : 31 Aug 2020 18:00
 Operator : JU/CG
 Sample : L3508-25
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TR-08-082820

Quant Time: Aug 31 18:39:14 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF082720.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 28 09:25:49 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.86	152	326533	20.00	ng	0.00
21) Naphthalene-d8	8.15	136	1189794	20.00	ng	0.00
39) Acenaphthene-d10	9.90	164	590221	20.00	ng	0.00
64) Phenanthrene-d10	11.38	188	972364	20.00	ng	0.00
76) Chrysene-d12	14.02	240	678160	20.00	ng	0.00
86) Perylene-d12	15.49	264	721205	20.00	ng	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
5) 2-Fluorophenol	5.47	112	1506353	77.40	ng	0.00
7) Phenol-d6	6.48	99	1971813	72.50	ng	-0.01
23) Nitrobenzene-d5	7.42	82	1276067	73.32	ng	0.00
42) 2,4,6-Tribromophenol	10.69	330	501196	84.07	ng	0.00
45) 2-Fluorobiphenyl	9.22	172	2241429	61.28	ng	0.00
79) Terphenyl-d14	12.97	244	1801808	55.93	ng	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
9) Benzaldehyde	6.40	77	576	Below Cal		# 52
19) n-Nitroso-di-n-propylamine	7.42	70	169406	11.145	ng	# 77
25) Isophorone	7.42	82	1260215	32.194	ng	# 64
32) Benzoic acid	7.83	122	848	6.767	ng	# 79
48) 2-Nitroaniline	9.43	65	621	6.700	ng	# 5
50) Dimethylphthalate	9.61	163	179685	4.432	ng	# 99
51) 2,6-Dinitrotoluene	9.90	165	77829	15.292	ng	# 25
53) 3-Nitroaniline	9.85	138	114	5.462	ng	# 4
56) 4-Nitrophenol	9.99	139	402	7.903	ng	# 1
57) 2,4-Dinitrotoluene	9.90	165	77829	14.335	ng	# 21
62) 4-Nitroaniline	10.45	138	128	4.547	ng	# 37
65) 4,6-Dinitro-2-methylphenol	10.68	198	1093	6.069	ng	# 1
67) 4-Bromophenyl-phenylether	10.69	248	29565	2.764	ng	# 1
75) Fluoranthene	12.59	202	247504	4.602	ng	# 98
78) Pyrene	12.82	202	300144	6.197	ng	# 96
81) Benzo(a)anthracene	14.01	228	206771	4.995	ng	# 99
83) Chrysene	14.04	228	186181	4.495	ng	# 95
87) Indeno(1,2,3-cd)pyrene	16.95	276	95662	2.156	ng	# 98
88) Benzo(b)fluoranthene	15.06	252	348214	7.422	ng	# 98
89) Benzo(k)fluoranthene	15.06	252	348214	7.980	ng	# 98
90) Benzo(a)pyrene	15.43	252	179731	4.261	ng	# 96
92) Benzo(g,h,i)perylene	17.39	276	99252	2.837	ng	# 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF083120\
Data File : BF121483.D
Acq On : 31 Aug 2020 18:00
Operator : JU/CG
Sample : L3508-25
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TR-08-082820

Quant Time: Aug 31 18:39:14 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF082720.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 28 09:25:49 2020
Response via : Initial Calibration

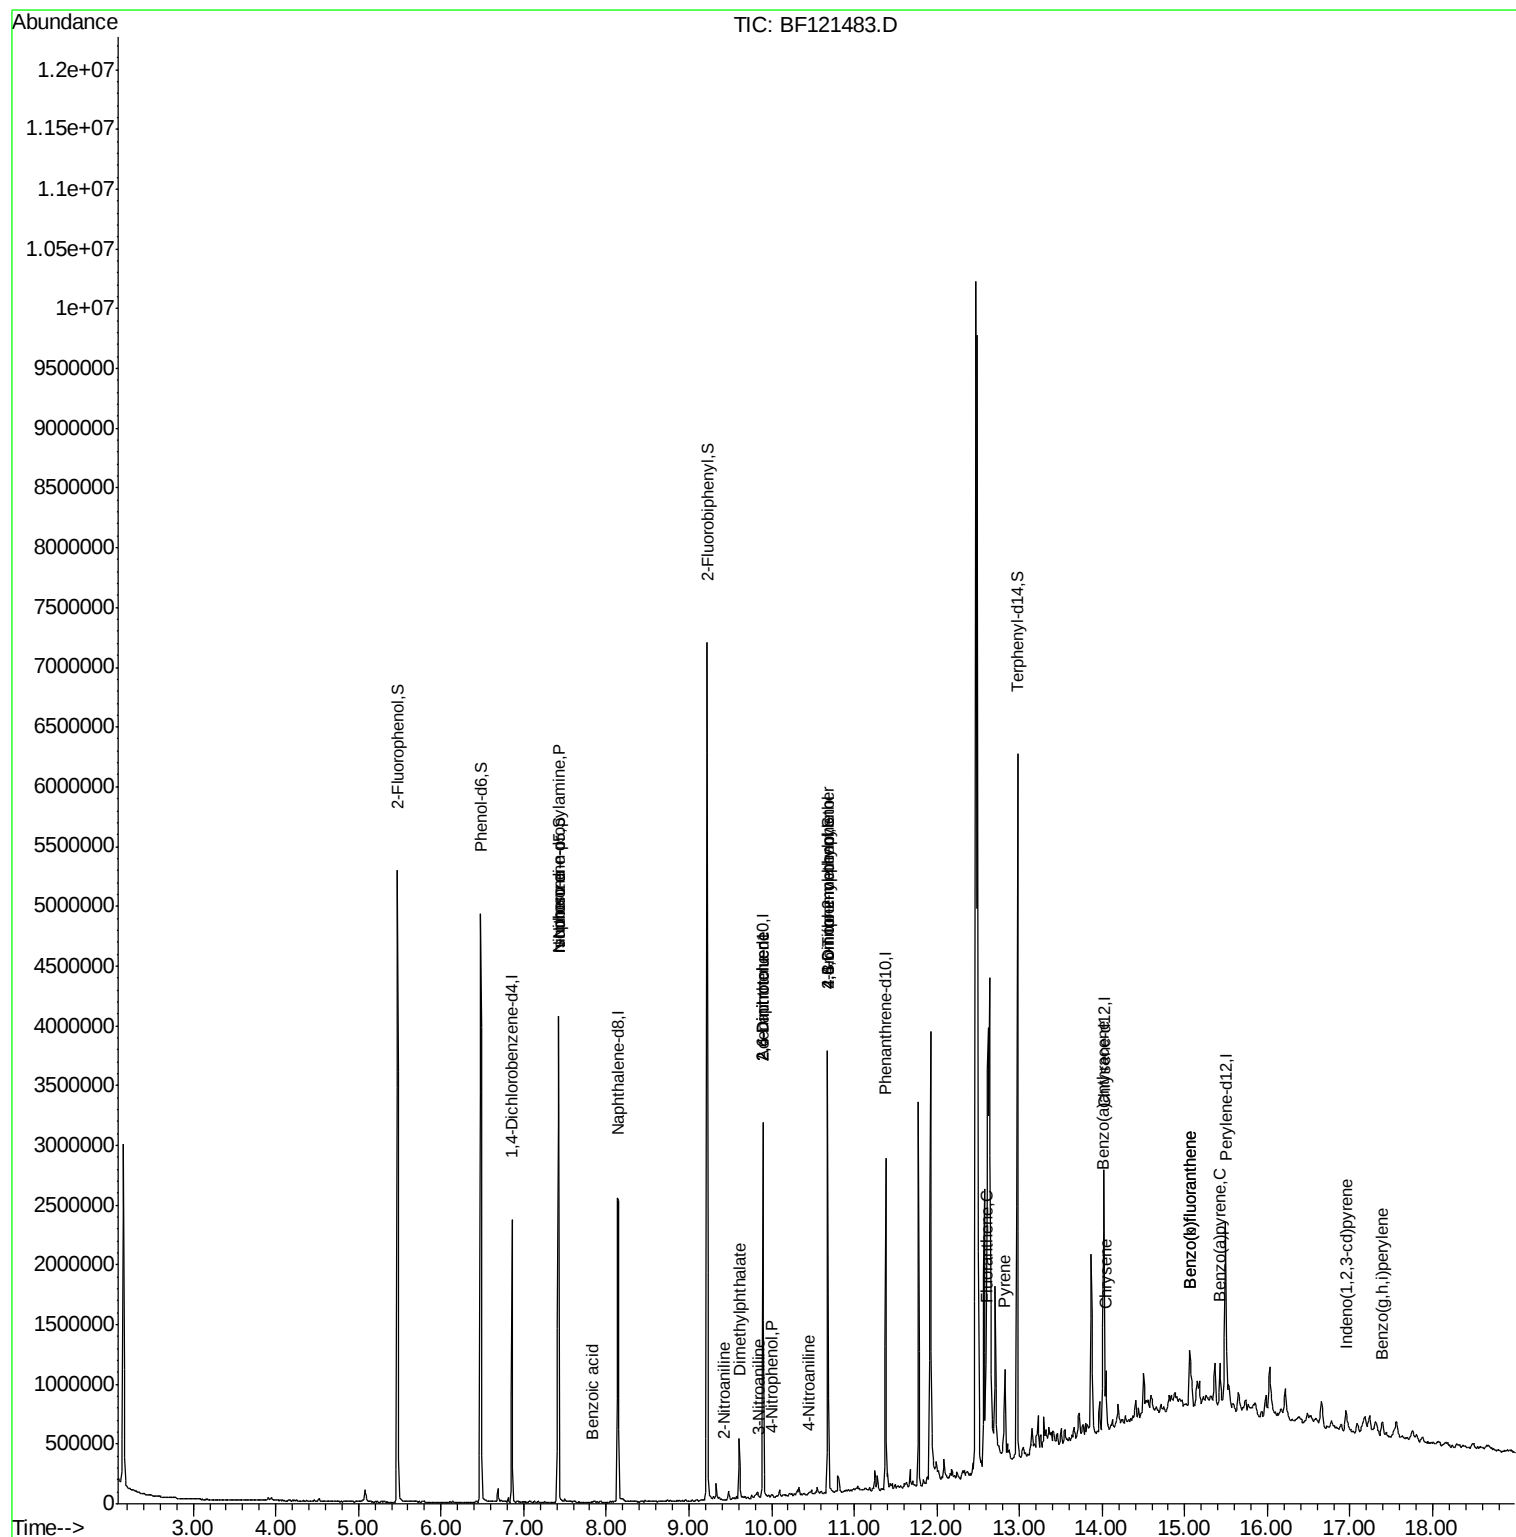




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.86 min Scan# 811
Delta R.T. -0.01 min
Lab File: BF121483.D
Acq: 31 Aug 2020 18:00

Instrument :
BNA_F
ClientSampleId :
TR-08-082820

Tot Ion:152 Resp: 326533
Ion Ratio Lower Upper
152 100
150 156.7 125.8 188.6
115 60.8 46.6 69.8




Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

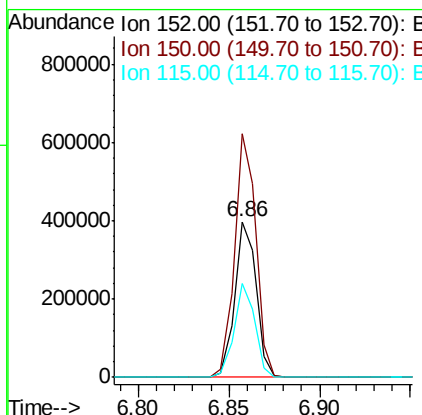



#5




2-Fluorophenol
Concen: 77.397 ng
RT: 5.47 min Scan# 576
Delta R.T. 0.00 min
Lab File: BF121483.D
Acq: 31 Aug 2020 18:00

Tgt Ion:112 Resp: 1506353
Ion Ratio Lower Upper
112 100
64 60.7 48.2 72.2
63 30.8 24.8 37.2



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

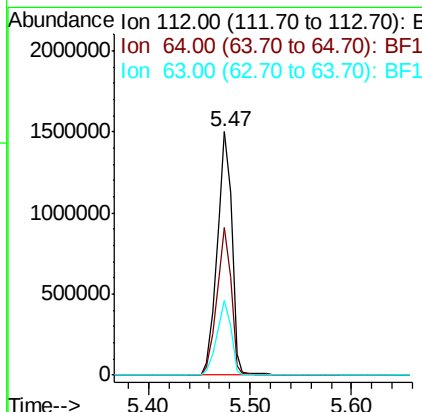



#7

Phenol-d6

Concen: 72.497 ng

RT: 6.48 min Scan# 747

Delta R.T. -0.01 min

Lab File: BF121483.D

Acq: 31 Aug 2020 18:00

Instrument :

BNA_F

ClientSampleId :

TR-08-082820





Tot Ion: 99 Resp: 1971813

Ion Ratio Lower Upper

99 100

42 17.4 13.5 20.3

71 31.4 24.6 37.0

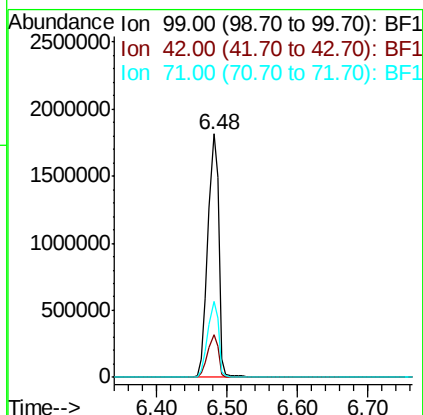

#19

n-Nitroso-di-n-propylamine

Concen: 11.145 ng

RT: 7.42 min Scan# 907

Delta R.T. 0.14 min

Lab File: BF121483.D

Acq: 31 Aug 2020 18:00

Tgt Ion: 70 Resp: 169406


Ion Ratio Lower Upper


70 100

42 45.4 45.8 68.6#

101 0.0 7.5 11.3#

130 2.2 16.5 24.7#

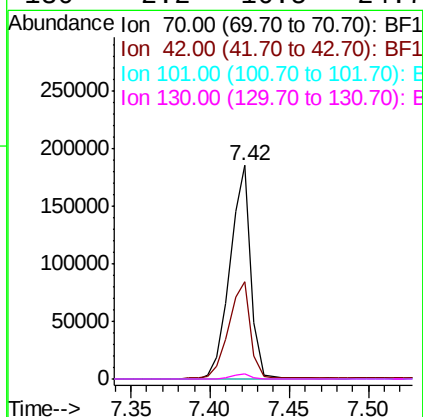







#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.15 min Scan# 1030
Delta R.T. 0.00 min
Lab File: BF121483.D
Acq: 31 Aug 2020 18:00

Instrument :
BNA_F
ClientSampleId :
TR-08-082820

Tot Ion:136	Resp: 1189794
Ion Ratio	Lower Upper
136 100	
137 10.9	9.1 13.7
54 7.4	7.0 10.4
68 5.9	5.5 8.3




Abundance Ion 136.00 (135.70 to 136.70): E
2000000
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

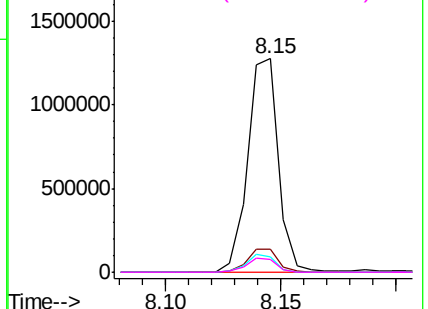




#23
Nitrobenzene-d5
Concen: 73.323 ng
RT: 7.42 min Scan# 907
Delta R.T. -0.01 min
Lab File: BF121483.D
Acq: 31 Aug 2020 18:00

Tgt Ion: 82	Resp: 1276067
Ion Ratio	Lower Upper
82 100	
128 46.4	34.1 51.1
54 49.2	41.0 61.6



Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF1

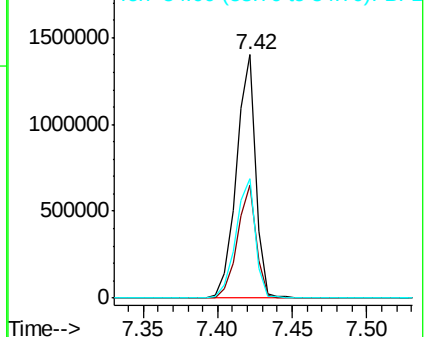



#25

Isophorone

Concen: 32.194 ng

RT: 7.42 min Scan# 907

Delta R.T. -0.26 min

Lab File: BF121483.D

Acq: 31 Aug 2020 18:00

Instrument :

BNA_F

ClientSampleId :

TR-08-082820


Tot Ion: 82 Resp: 1260215

Ion Ratio Lower Upper

82 100

95 0.0 5.6 8.4#




138 0.0 14.8 22.2#



Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 95.00 (94.70 to 95.70): BF1

Ion 138.00 (137.70 to 138.70): BF1

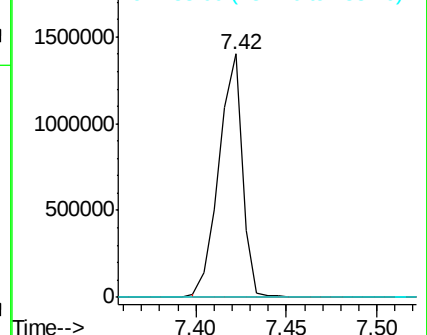

#32

Benzoic acid

Concen: 6.767 ng

RT: 7.83 min Scan# 976

Delta R.T. -0.09 min

Lab File: BF121483.D

Acq: 31 Aug 2020 18:00


Tgt Ion: 122 Resp: 848

Ion Ratio Lower Upper

122 100

105 101.9 100.8 140.8



77 116.4 71.5 111.5#




Abundance Ion 122.00 (121.70 to 122.70): BF1

Ion 105.00 (104.70 to 105.70): BF1

Ion 77.00 (76.70 to 77.70): BF1

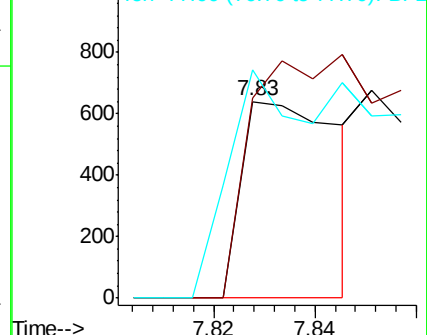







#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.90 min Scan# 1328
 Delta R.T. -0.01 min
 Lab File: BF121483.D
 Acq: 31 Aug 2020 18:00

Instrument :
 BNA_F
 ClientSampleId :
 TR-08-082820

Tot Ion:164	Resp:	590221
Ion	Ratio	Lower Upper
164	100	
162	100.3	82.4 123.6
160	45.6	37.6 56.4




Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E


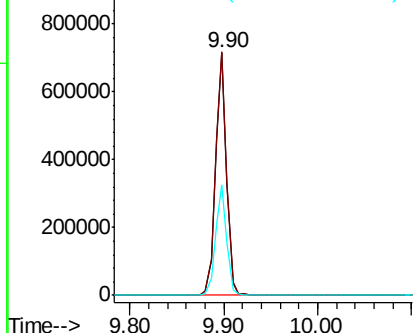



#42
 2,4,6-Tribromophenol
 Concen: 84.072 ng
 RT: 10.69 min Scan# 1462
 Delta R.T. -0.01 min
 Lab File: BF121483.D
 Acq: 31 Aug 2020 18:00

Tgt Ion:330	Resp:	501196
Ion	Ratio	Lower Upper
330	100	
332	96.7	76.2 114.2
141	29.5	24.6 36.8



Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

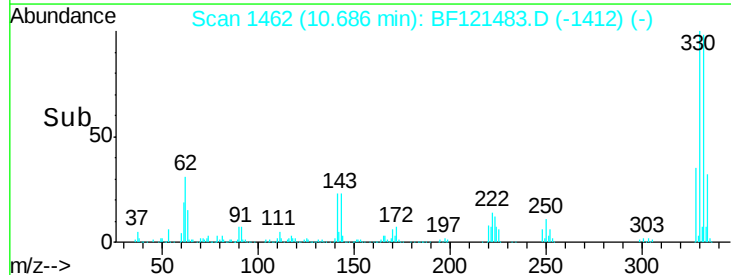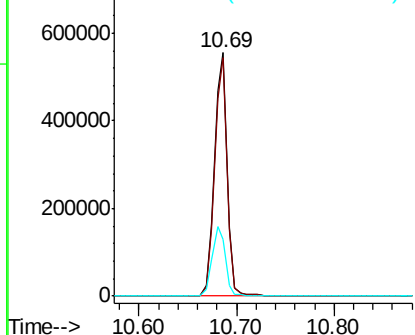







#45
 2-Fluorobiphenyl
 Concen: 61.276 ng
 RT: 9.22 min Scan# 1213
 Delta R.T. -0.01 min
 Lab File: BF121483.D
 Acq: 31 Aug 2020 18:00

Instrument :
 BNA_F
 ClientSampleId :
 TR-08-082820

Tot Ion:172 Resp: 2241429
 Ion Ratio Lower Upper
 172 100
 171 37.3 30.6 45.8
 170 25.3 20.6 31.0




Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E


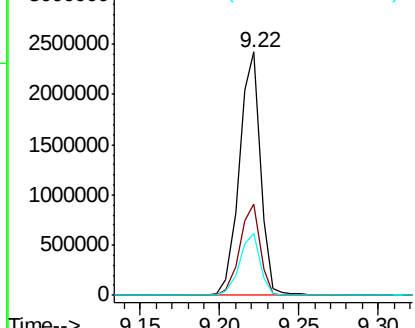



#48
 2-Nitroaniline
 Concen: 6.700 ng
 RT: 9.43 min Scan# 1248
 Delta R.T. -0.01 min
 Lab File: BF121483.D
 Acq: 31 Aug 2020 18:00

Tgt Ion: 65 Resp: 621
 Ion Ratio Lower Upper
 65 100
 92 0.0 55.6 83.4#
 138 0.0 82.9 124.3#



Abundance Ion 65.00 (64.70 to 65.70): BF1
 Ion 92.00 (91.70 to 92.70): BF1
 Ion 138.00 (137.70 to 138.70): E

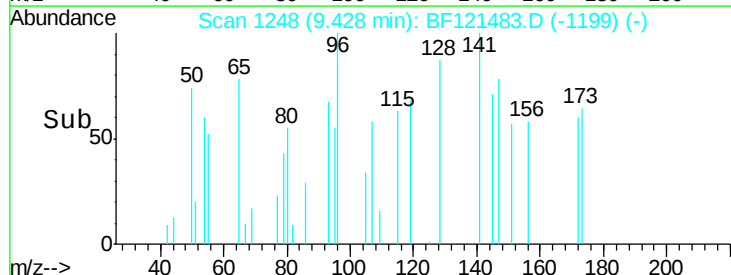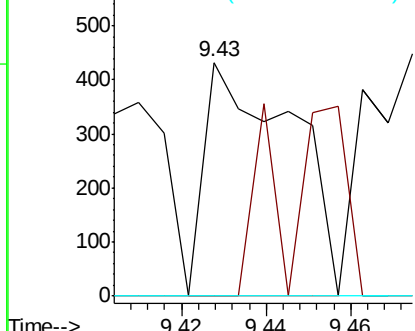


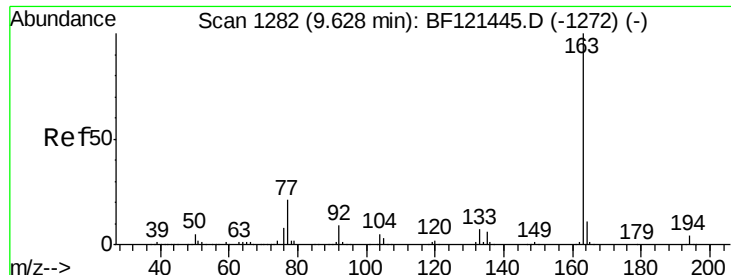

#50
Dimethylphthalate
Concen: 4.432 ng
RT: 9.61 min Scan# 1279
Delta R.T. -0.02 min
Lab File: BF121483.D
Acq: 31 Aug 2020 18:00

Instrument :
BNA_F
ClientSampleId :
TR-08-082820

Tot Ion	Ratio	Lower	Upper
163	100		
194	3.9	3.3	4.9
164	10.2	8.6	12.8






Abundance

Ion 163.00 (162.70 to 163.70): E


Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

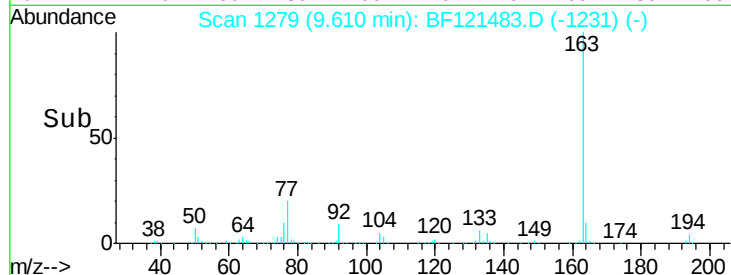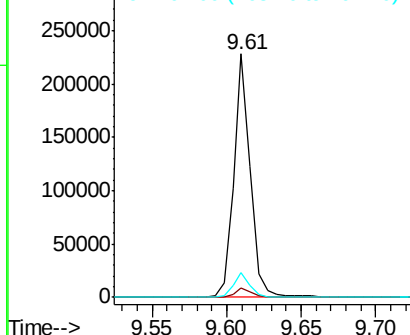

#51
2,6-Dinitrotoluene
Concen: 15.292 ng
RT: 9.90 min Scan# 1328
Delta R.T. 0.21 min
Lab File: BF121483.D
Acq: 31 Aug 2020 18:00

Tgt Ion	Ratio	Lower	Upper
165	100		
63	1.5	43.6	65.4#
89	1.5	47.4	71.2#






Abundance

Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF1

Ion 89.00 (88.70 to 89.70): BF1




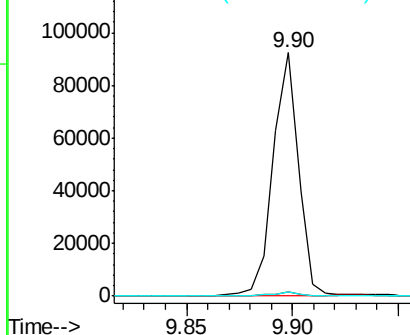




#53
 3-Nitroaniline
 Concen: 5.462 ng
 RT: 9.85 min Scan# 1320
 Delta R.T. -0.00 min
 Lab File: BF121483.D
 Acq: 31 Aug 2020 18:00




Instrument :
 BNA_F
 ClientSampleId :
 TR-08-082820


Tot Ion:138 Resp: 114
 Ion Ratio Lower Upper
 138 100
 108 0.0 11.6 17.4#
 92 0.0 88.6 132.8#

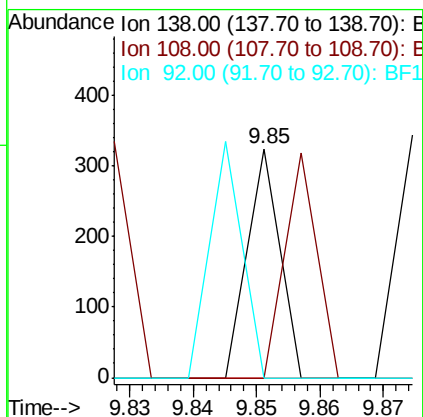

#56
 4-Nitrophenol
 Concen: 7.903 ng
 RT: 9.99 min Scan# 1344
 Delta R.T. -0.01 min
 Lab File: BF121483.D
 Acq: 31 Aug 2020 18:00

Tgt Ion:139 Resp: 402
 Ion Ratio Lower Upper
 139 100
 109 288.3 50.5 90.5#
 65 124.9 80.2 120.2#


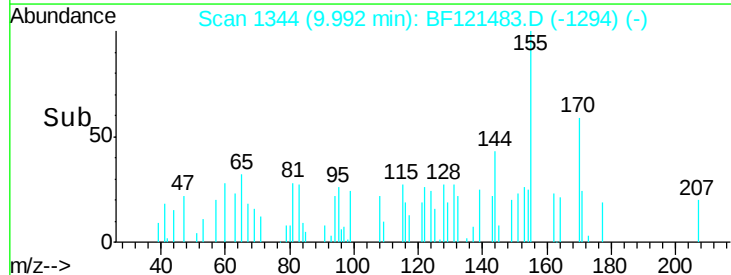
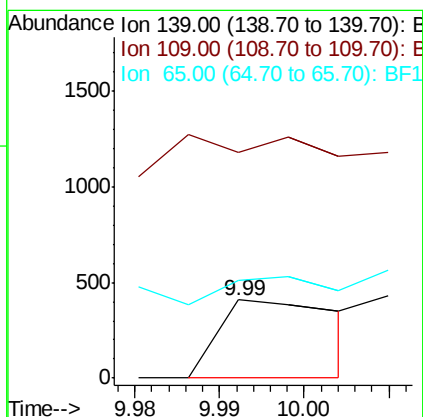





#57
 2,4-Dinitrotoluene
 Concen: 14.335 ng
 RT: 9.90 min Scan# 1328
 Delta R.T. -0.19 min
 Lab File: BF121483.D
 Acq: 31 Aug 2020 18:00




Instrument :
 BNA_F
 ClientSampleId :
 TR-08-082820


Tot Ion:	165	Resp:	77829
Ion	Ratio	Lower	Upper
165	100		
63	1.5	36.0	54.0#
89	1.5	62.6	93.8#
182	0.0	2.2	3.2#

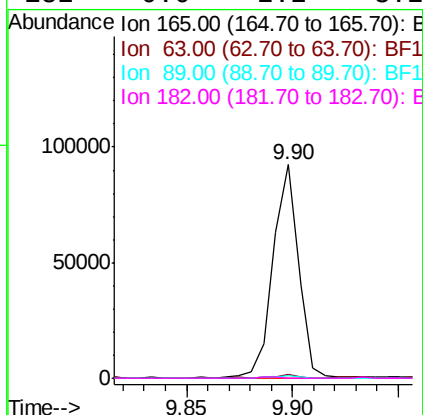

#62
 4-Nitroaniline
 Concen: 4.547 ng
 RT: 10.45 min Scan# 1422
 Delta R.T. -0.02 min
 Lab File: BF121483.D
 Acq: 31 Aug 2020 18:00

Tgt Ion:	138	Resp:	128
Ion	Ratio	Lower	Upper
138	100		
92	110.7	33.2	73.2#
108	115.4	53.6	93.6#

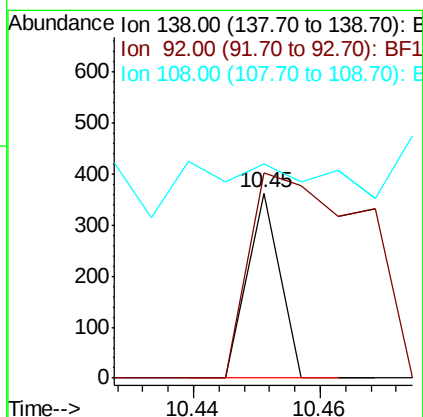



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.38 min Scan# 1580

Delta R.T. -0.01 min

Lab File: BF121483.D

Acq: 31 Aug 2020 18:00

Instrument :

BNA_F

ClientSampleId :

TR-08-082820


Tot Ion:188 Resp: 972364

Ion Ratio Lower Upper

188 100

94 11.1 8.3 12.5

80 11.6 8.6 13.0



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1



11.38

1000000

500000

0

Time-->



#65

4,6-Dinitro-2-methylphenol

Concen: 6.069 ng

RT: 10.68 min Scan# 1461

Delta R.T. 0.19 min

Lab File: BF121483.D

Acq: 31 Aug 2020 18:00


Tgt Ion:198 Resp: 1093

Ion Ratio Lower Upper

198 100

51 239.3 29.0 69.0#

105 250.0 29.1 69.1#



Abundance Ion 198.00 (197.70 to 198.70): E

Ion 51.00 (50.70 to 51.70): BF1

Ion 105.00 (104.70 to 105.70): E

10.68


3000


2000

1000

0

Time-->




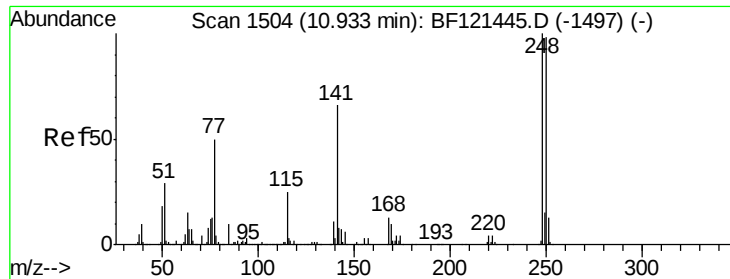




#67
4-Bromophenyl-phenylether
Concen: 2.764 ng
RT: 10.69 min Scan# 1462
Delta R.T. -0.25 min
Lab File: BF121483.D
Acq: 31 Aug 2020 18:00

Instrument :
BNA_F
ClientSampleId :
TR-08-082820

Tot Ion	Ratio	Lower	Upper
248	100		
250	190.3	78.7	118.1#
141	411.6	52.6	78.8#

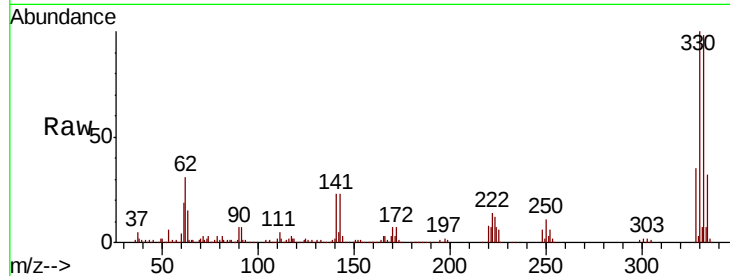


Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

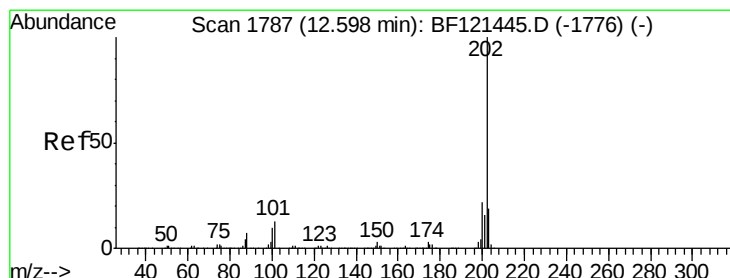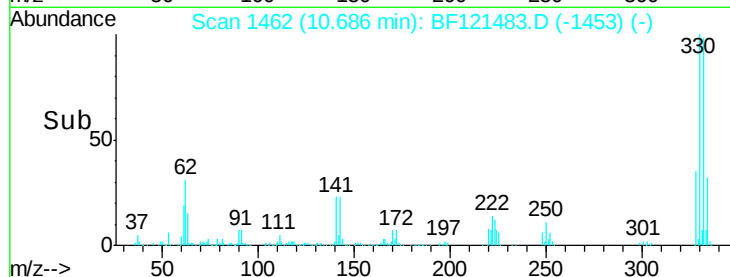
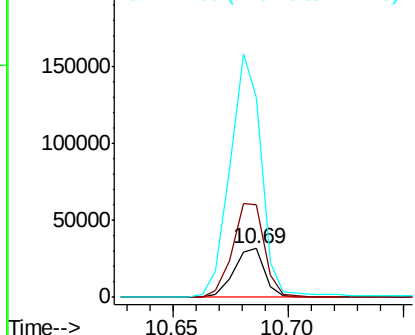



#75
Fluoranthene
Concen: 4.602 ng
RT: 12.59 min Scan# 1786
Delta R.T. -0.01 min
Lab File: BF121483.D
Acq: 31 Aug 2020 18:00

Tgt Ion	Ratio	Lower	Upper
202	100		
101	12.3	0.0	33.3
203	18.4	0.0	39.1

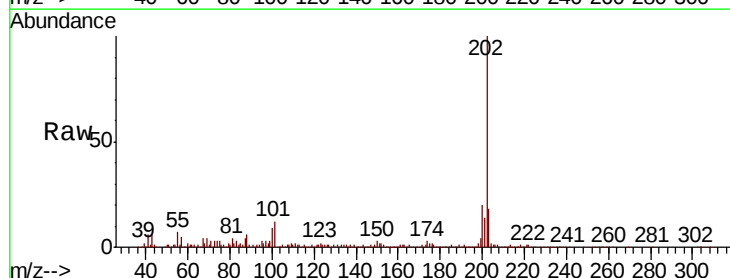

Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 203.00 (202.70 to 203.70): E



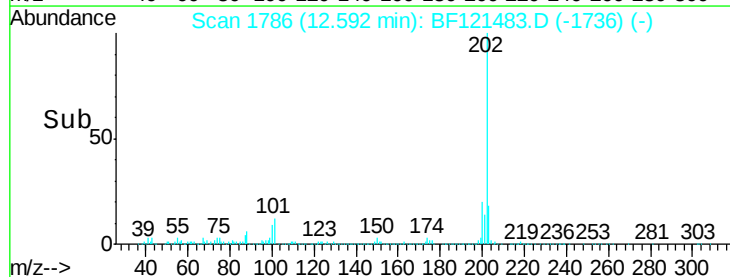
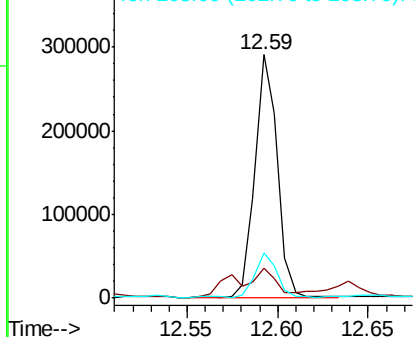




#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.02 min Scan# 2029
Delta R.T. -0.01 min
Lab File: BF121483.D
Acq: 31 Aug 2020 18:00




Instrument :
BNA_F
ClientSampleId :
TR-08-082820


Tot Ion:240 Resp: 678160
Ion Ratio Lower Upper
240 100
120 12.1 9.5 14.3
236 26.3 21.8 32.6

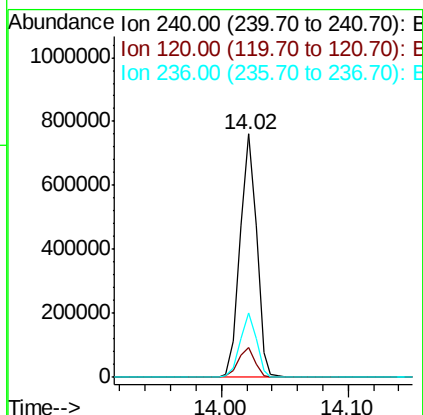

#78
Pyrene
Concen: 6.197 ng
RT: 12.82 min Scan# 1825
Delta R.T. -0.01 min
Lab File: BF121483.D
Acq: 31 Aug 2020 18:00

Tgt Ion:202 Resp: 300144
Ion Ratio Lower Upper
202 100
200 20.5 18.0 27.0
203 17.9 15.3 22.9



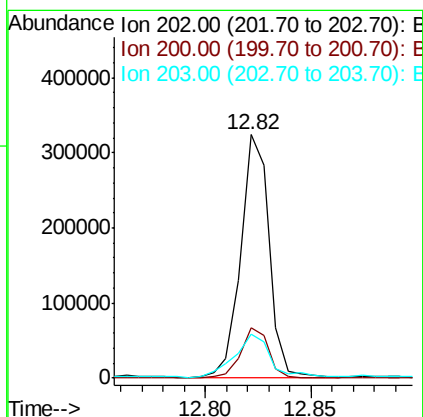





#79
 Terphenyl-d14
 Concen: 55.927 ng
 RT: 12.97 min Scan# 1851
 Delta R.T. 0.00 min
 Lab File: BF121483.D
 Acq: 31 Aug 2020 18:00




Instrument :
 BNA_F
 ClientSampleId :
 TR-08-082820


Tot Ion:244 Resp: 1801808
 Ion Ratio Lower Upper
 244 100
 212 7.4 6.3 9.5
 122 11.5 9.5 14.3

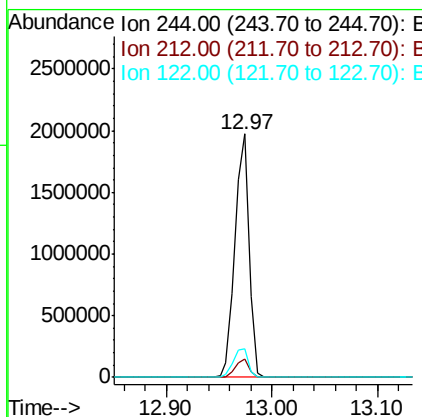

#81
 Benzo(a)anthracene
 Concen: 4.995 ng
 RT: 14.01 min Scan# 2027
 Delta R.T. -0.01 min
 Lab File: BF121483.D
 Acq: 31 Aug 2020 18:00

Tgt Ion:228 Resp: 206771
 Ion Ratio Lower Upper
 228 100
 226 29.0 23.0 34.4
 229 21.8 16.6 24.8



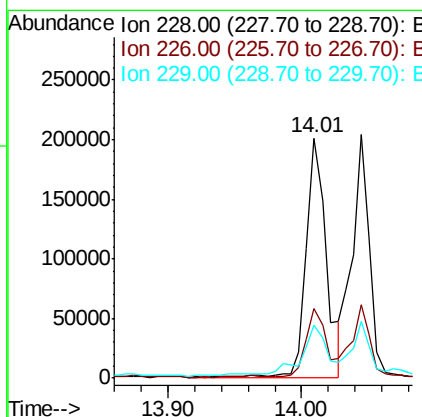





#83
Chrysene
Concen: 4.495 ng
RT: 14.04 min Scan# 2033
Delta R.T. -0.01 min
Lab File: BF121483.D
Acq: 31 Aug 2020 18:00




Instrument :
BNA_F
ClientSampled :
TR-08-082820


Tot Ion:228 Resp: 186181
Ion Ratio Lower Upper
228 100
226 30.4 26.2 39.2
229 23.5 16.6 25.0

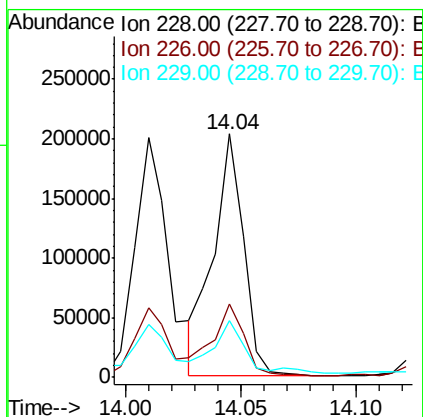

#86
Perylene-d12
Concen: 20.000 ng
RT: 15.49 min Scan# 2279
Delta R.T. 0.00 min
Lab File: BF121483.D
Acq: 31 Aug 2020 18:00

Tgt Ion:264 Resp: 721205
Ion Ratio Lower Upper
264 100
260 24.2 19.6 29.4
265 22.6 17.8 26.6


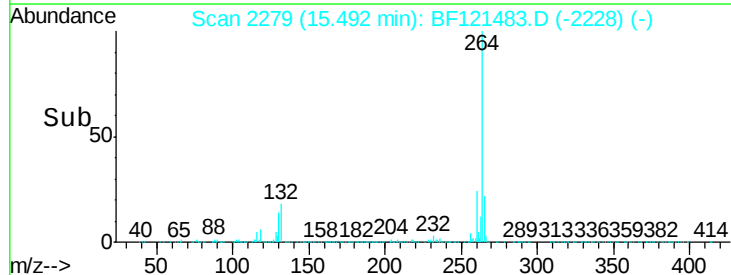
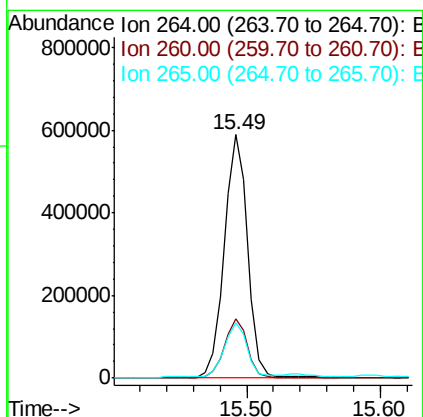



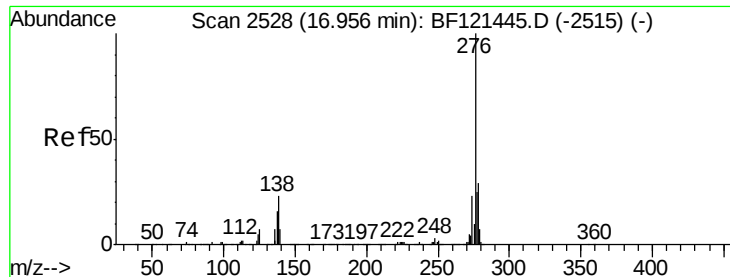

#87
 Indeno(1,2,3-cd)pyrene
 Concen: 2.156 ng
 RT: 16.95 min Scan# 2527
 Delta R.T. -0.01 min
 Lab File: BF121483.D
 Acq: 31 Aug 2020 18:00




Instrument :
 BNA_F
 ClientSampleId :
 TR-08-082820


Tot Ion:276	Resp:	95662
Ion Ratio	Lower	Upper
276	100	
138	23.7	20.6 31.0
277	25.9	20.5 30.7

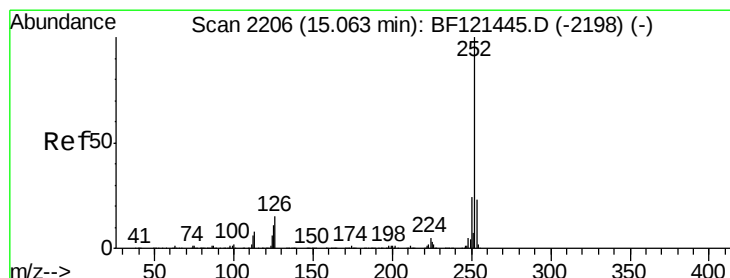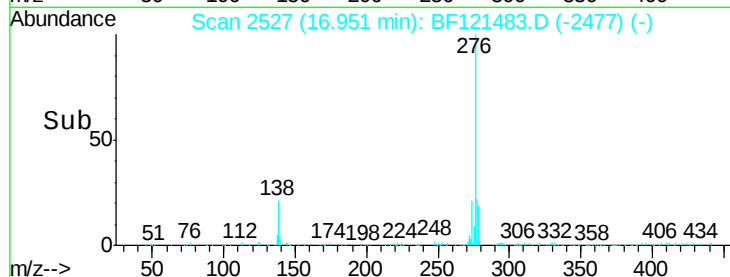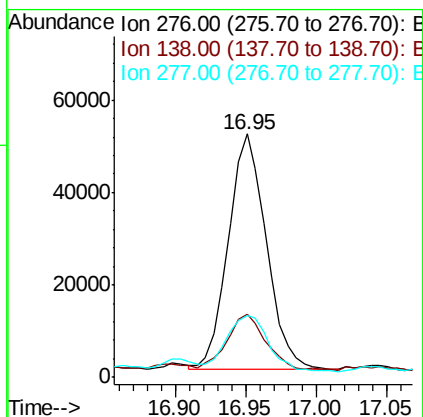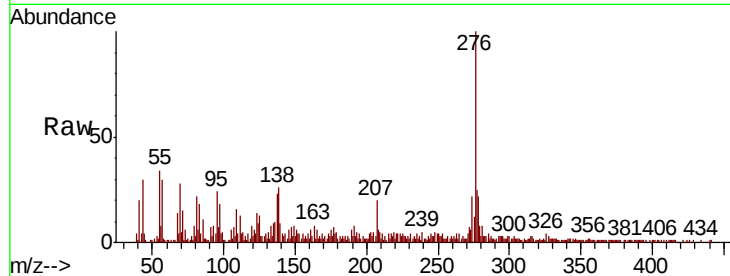

#88
 Benzo(b)fluoranthene
 Concen: 7.422 ng
 RT: 15.06 min Scan# 2206
 Delta R.T. 0.00 min
 Lab File: BF121483.D
 Acq: 31 Aug 2020 18:00

Tgt Ion:252	Resp:	348214
Ion Ratio	Lower	Upper
252	100	
253	22.8	18.3 27.5
125	13.1	9.2 13.8


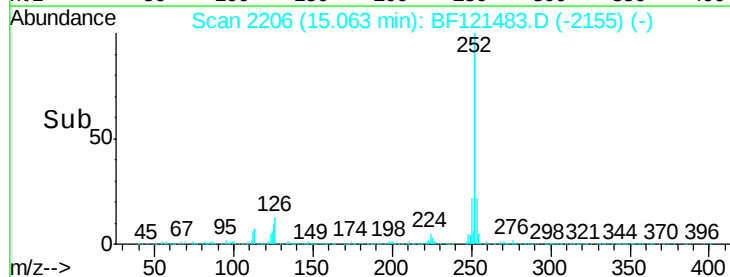
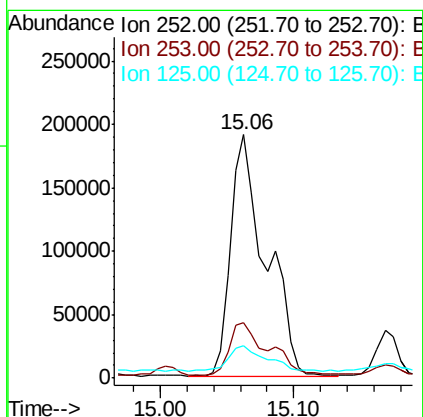
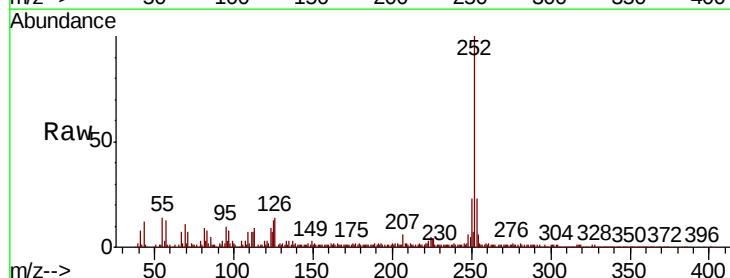




#89
Benzo(k)fluoranthene
Concen: 7.980 ng
RT: 15.06 min Scan# 2206
Delta R.T. -0.04 min
Lab File: BF121483.D
Acq: 31 Aug 2020 18:00




Instrument :
BNA_F
ClientSampleId :
TR-08-082820


Tot Ion	Ratio	Lower	Upper
252	100		
253	22.8	18.3	27.5
125	13.1	8.5	12.7#

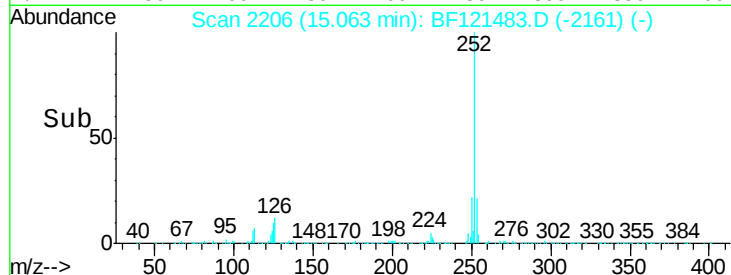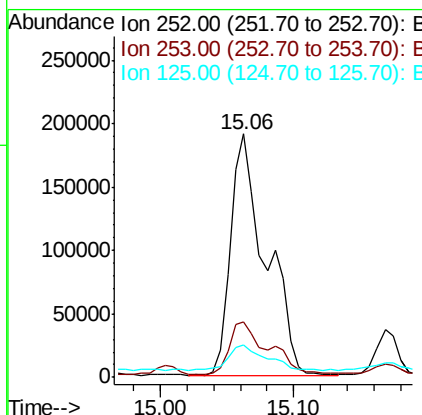

#90
Benzo(a)pyrene
Concen: 4.261 ng
RT: 15.43 min Scan# 2268
Delta R.T. -0.01 min
Lab File: BF121483.D
Acq: 31 Aug 2020 18:00

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.4	18.0	27.0
125	14.4	9.0	13.4#

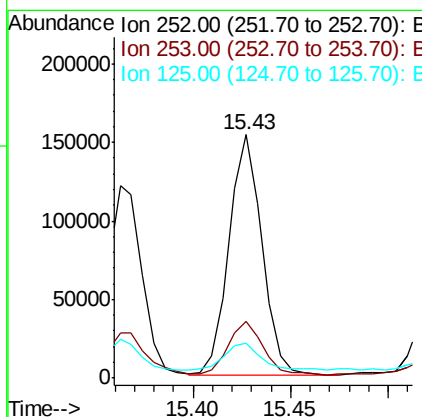




#92
 Benzo(a,h,i)perylene
 Concen: 2.837 ng
 RT: 17.39 min Scan# 2602
 Delta R.T. -0.01 min
 Lab File: BF121483.D
 Acq: 31 Aug 2020 18:00

Instrument :
 BNA_F
 ClientSampleId :
 TR-08-082820

Tot Ion	Ratio	Lower	Upper
276	100		
277	25.9	18.9	28.3
138	23.1	17.4	26.0



Abundance

Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

