
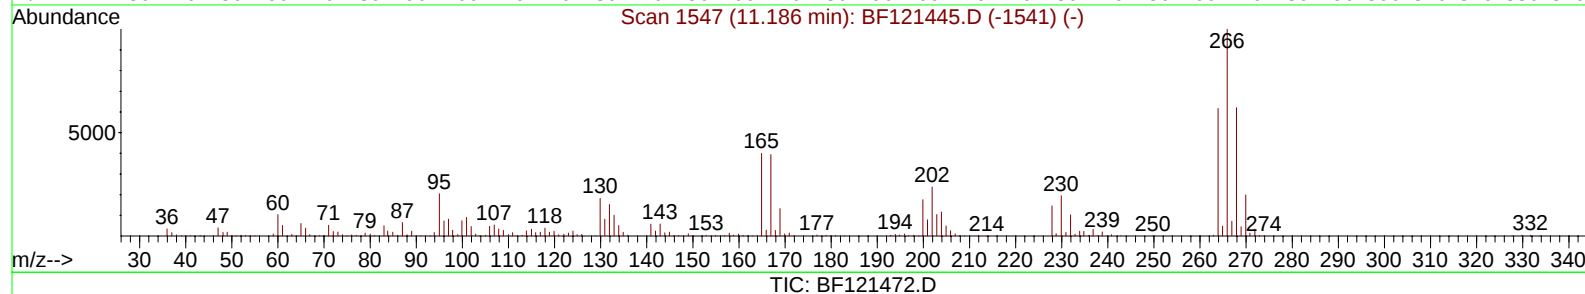
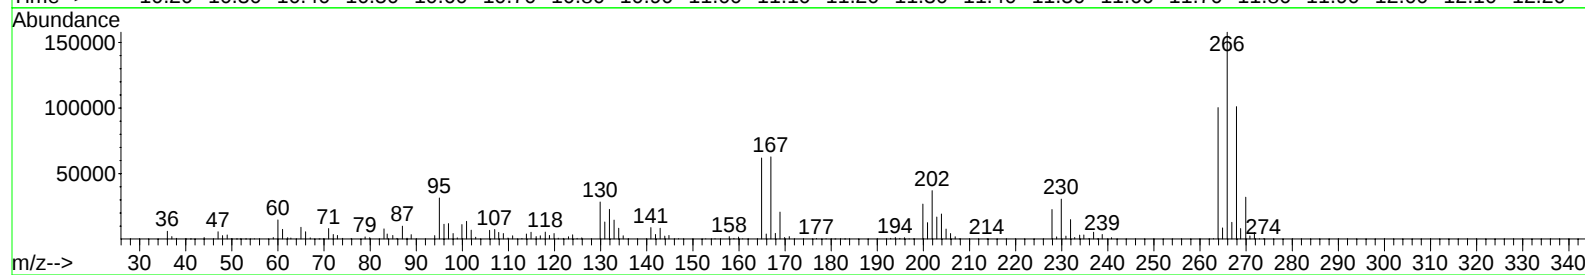


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF083120\
Data File : BF121472.D
Acq On : 31 Aug 2020 12:05
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 31 17:49:51 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF082720.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 28 09:25:49 2020
Response via : Initial Calibration

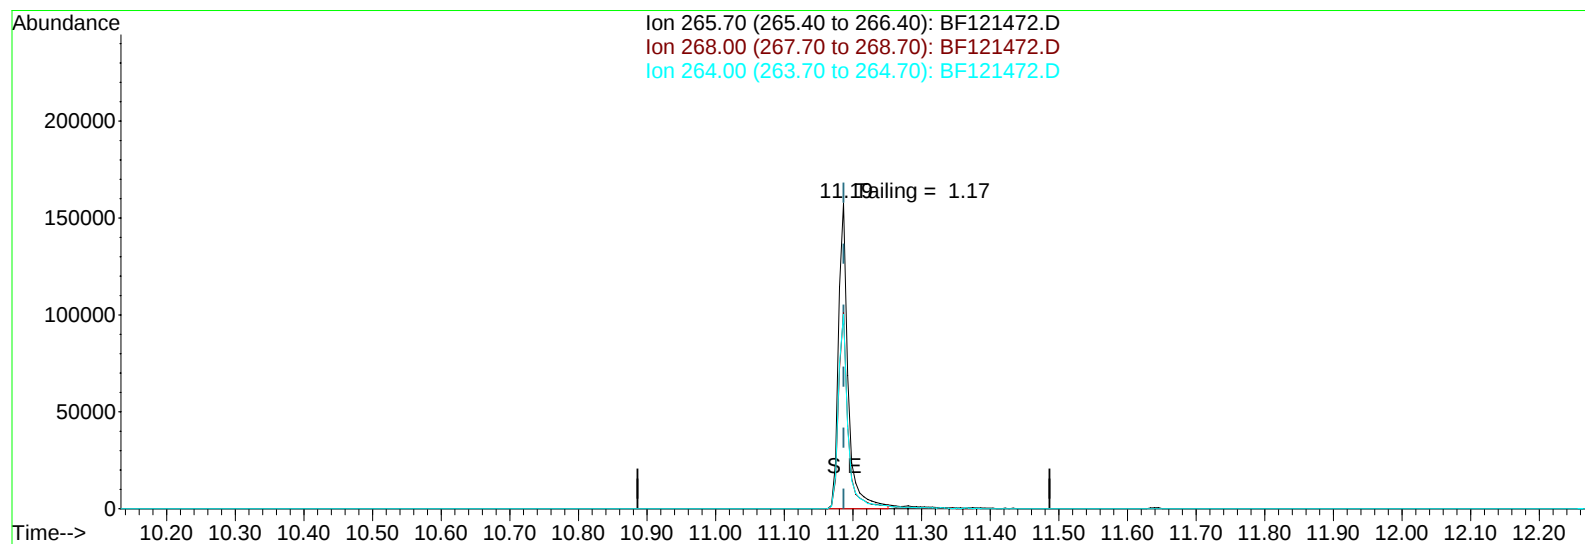

(70) Pentachlorophenol (C)




11.186min (-0.000) 35078.99ng

response 155651

Ion	Exp%	Act%
265.70	100	100
268.00	62.10	64.05
264.00	61.70	63.59
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF083120\
 Data File : BF121472.D
 Acq On : 31 Aug 2020 12:05
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 31 17:49:51 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF082720.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 28 09:25:49 2020
 Response via : Initial Calibration

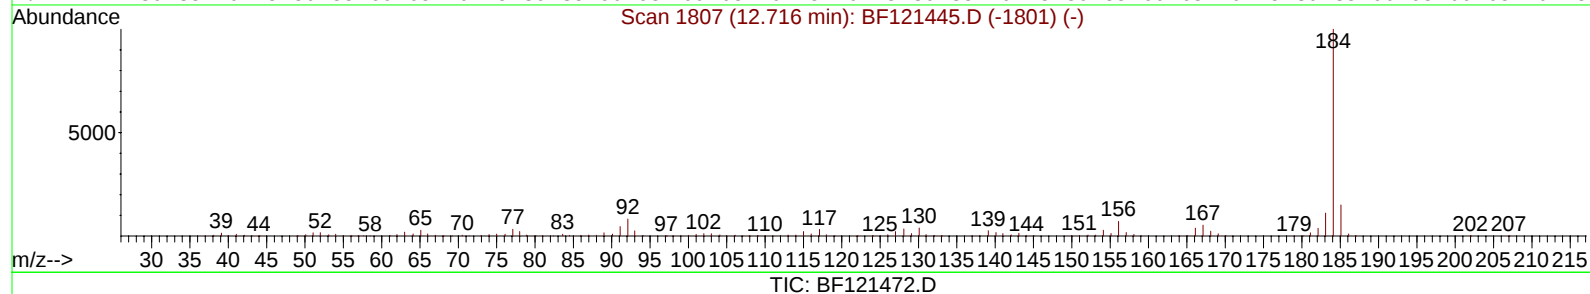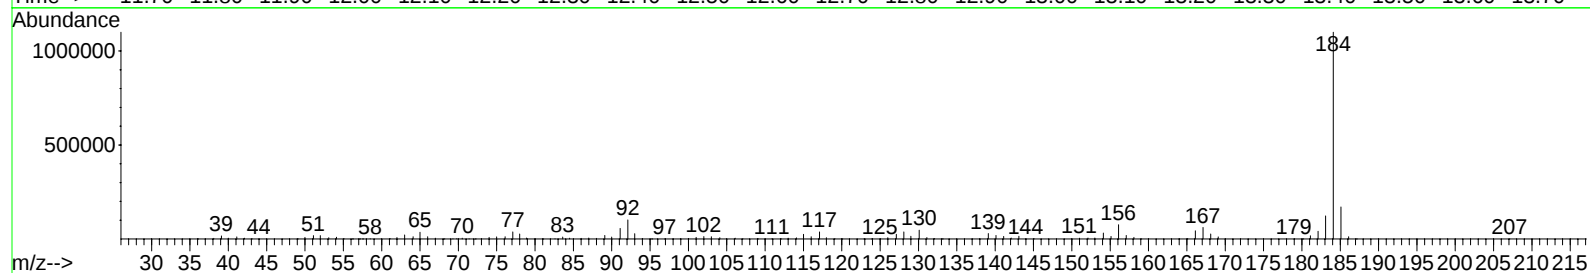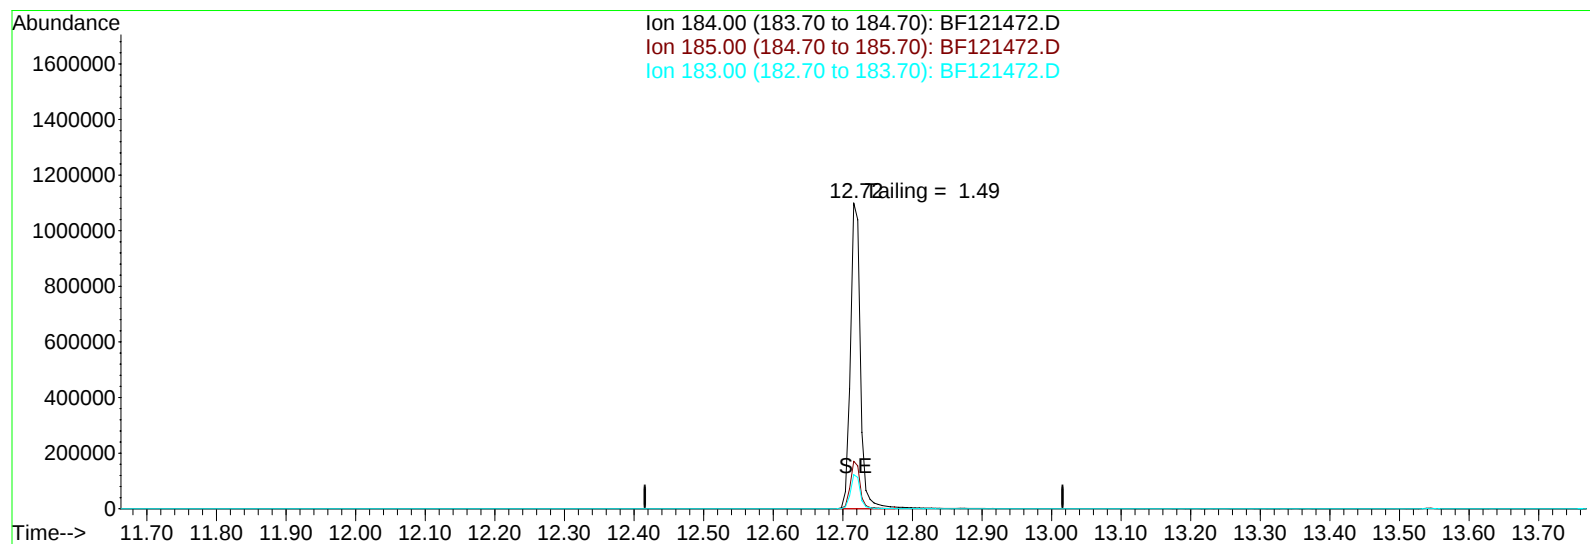

(77) Benzidine

12.716min (-12.716) 0.00ng

response 0

Ion	Exp%	Act%
184.00	100	0.00
185.00	15.10	0.00#
183.00	11.10	0.00#
0.00	0.00	0.00