

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF083120\
 Data File : BF121475.D
 Acq On : 31 Aug 2020 13:47
 Operator : JU/CG
 Sample : PB131291BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB131291BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF082720.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.228	21	24	36	rVB	147540	227134	2.24%	0.378%
2	5.104	507	513	527	rVB	100023	139805	1.38%	0.233%
3	5.487	572	578	581	rBV	6852528	6961227	68.75%	11.597%
4	6.487	742	748	751	rBV	6260947	7012853	69.26%	11.683%
5	6.857	808	811	815	rVB	2259557	1817018	17.94%	3.027%
6	7.422	901	907	910	rBV	4880112	4990684	49.29%	8.314%
7	8.139	1024	1029	1033	rBV	2460991	2406538	23.77%	4.009%
8	9.222	1206	1213	1216	rBV	8430250	8995311	88.83%	14.985%
9	9.898	1322	1328	1344	rBV	2965701	2830318	27.95%	4.715%
10	10.686	1455	1462	1465	rBV	5710892	5641227	55.71%	9.398%
11	11.380	1575	1580	1584	rBV	3279530	3015912	29.78%	5.024%
12	12.974	1844	1851	1854	rBV	9723613	10125940	100.00%	16.869%
13	14.021	2024	2029	2037	rBV	3179783	2975369	29.38%	4.957%
14	15.492	2272	2279	2284	rBV	2197313	2889323	28.53%	4.813%


Sum of corrected areas: 60028659

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF083120\
Data File : BF121475.D
Acq On : 31 Aug 2020 13:47
Operator : JU/CG
Sample : PB131291BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB131291BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF082720.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

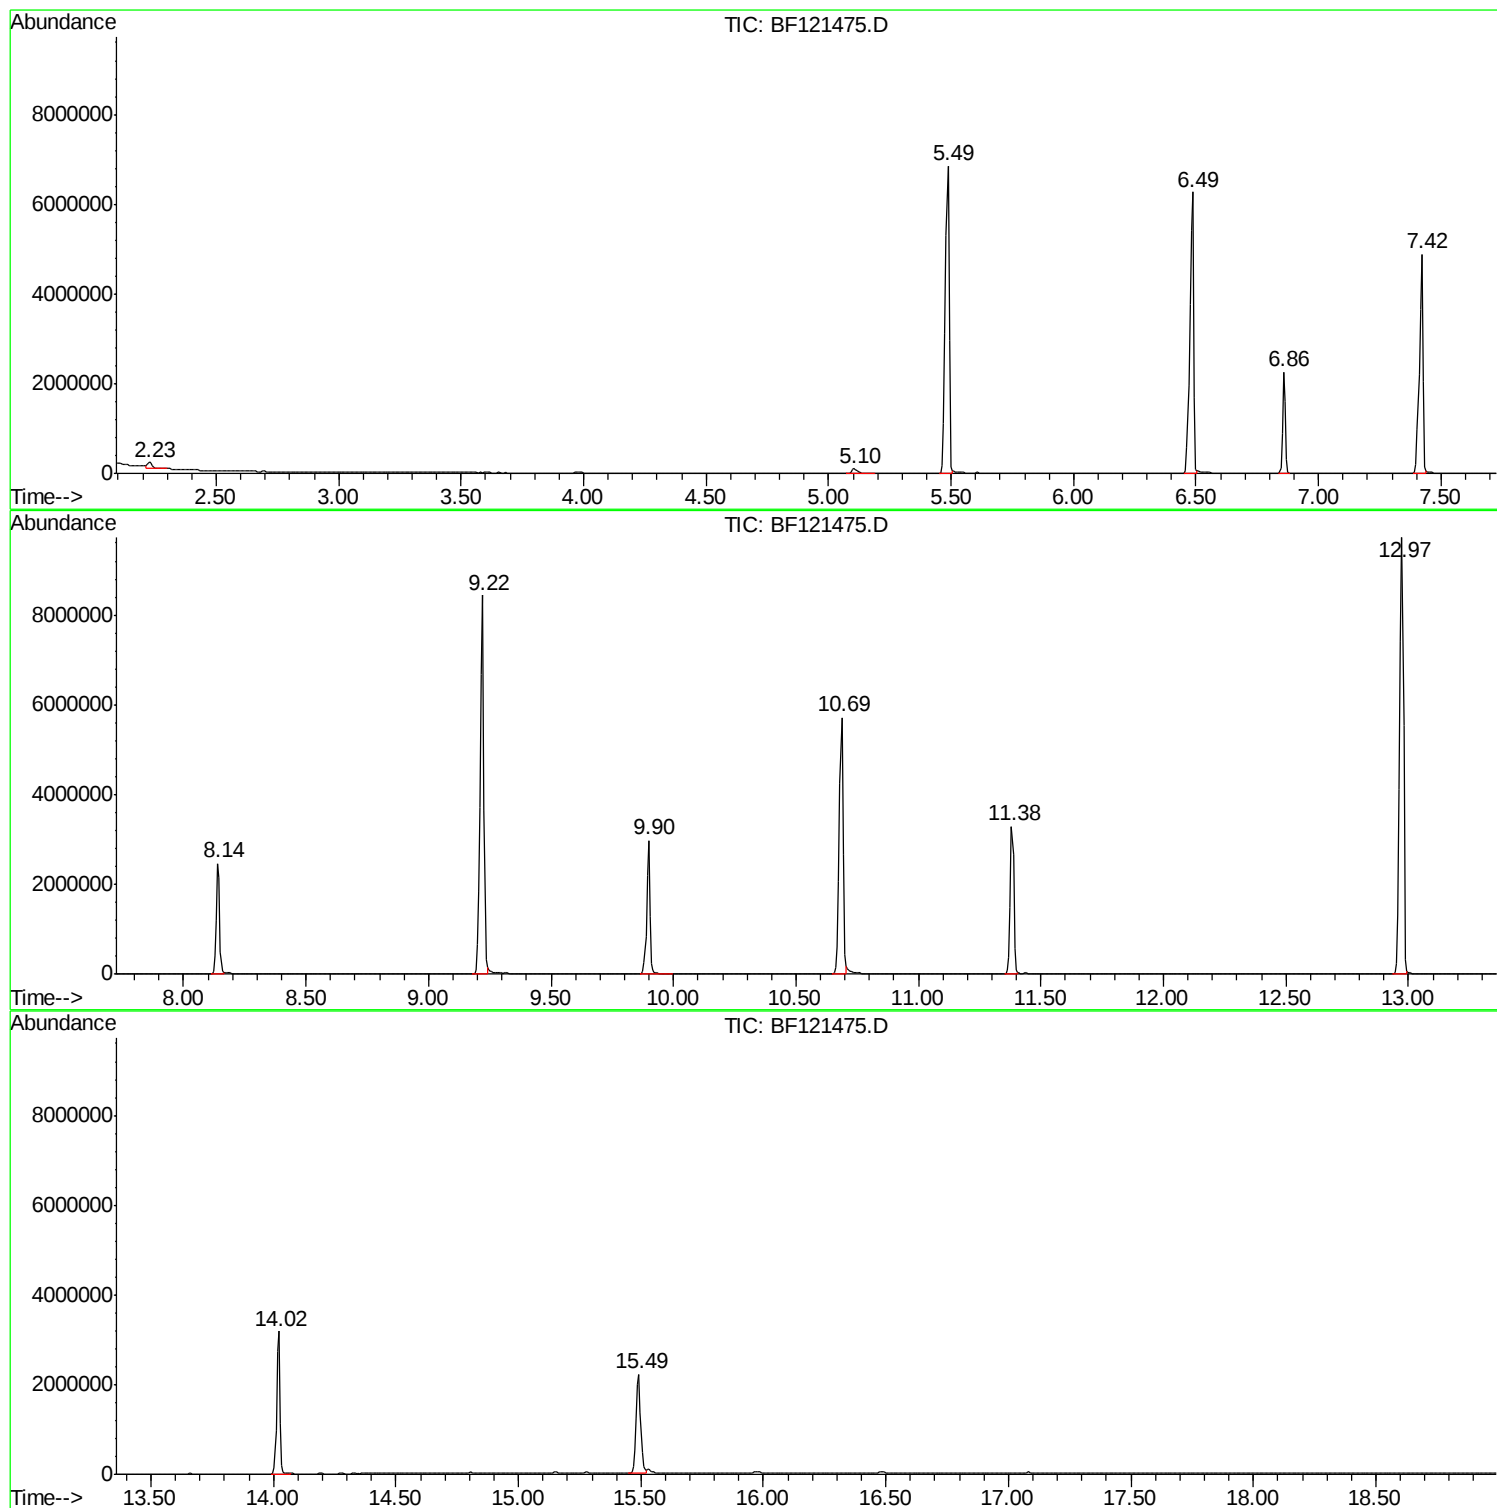

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF083120\
Data File : BF121475.D
Acq On : 31 Aug 2020 13:47
Operator : JU/CG
Sample : PB131291BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleID :
PB131291BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF082720.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.23	2.50 ng	227134	1,4-Dichlorobenzene-d4	6.86

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	25
3			N-Ethylformamide	73	C3H7NO	000627-45-2	9
4			Acetamide, N-ethyl-	87	C4H9NO	000625-50-3	9
5			3-Hexanol, 2-methyl-	116	C7H16O	000617-29-8	9

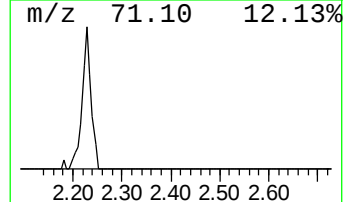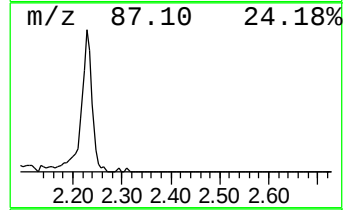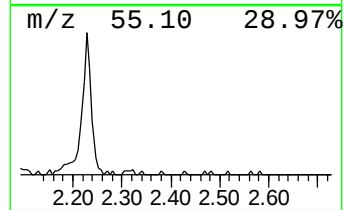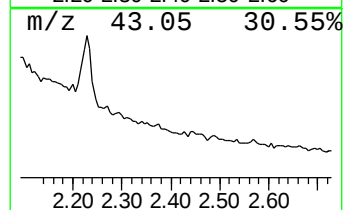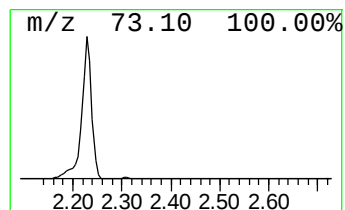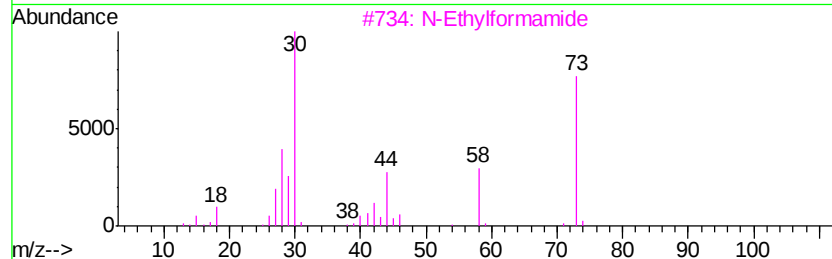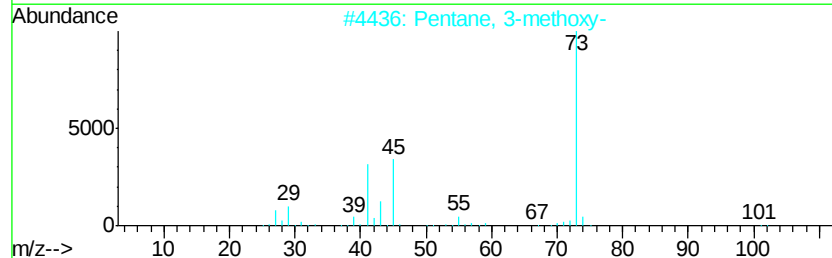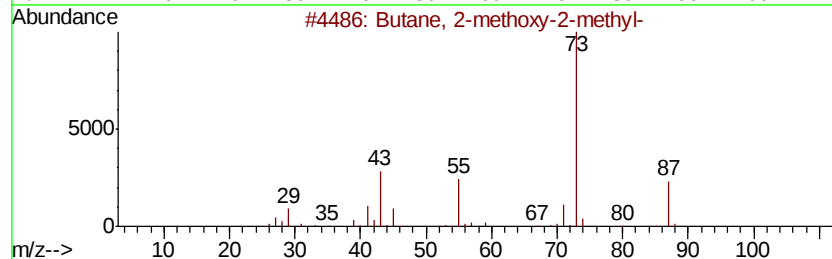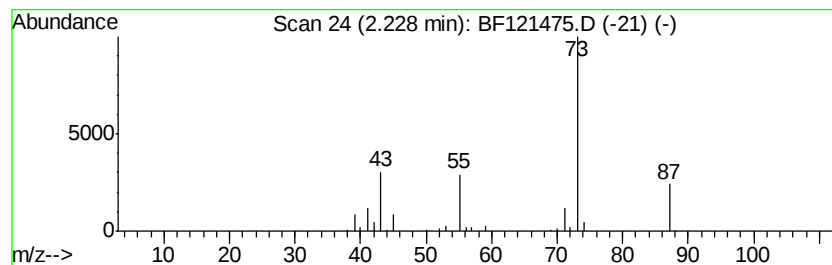

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF083120\
Data File : BF121475.D
Acq On : 31 Aug 2020 13:47
Operator : JU/CG
Sample : PB131291BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB131291BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF082720.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-methoxy...	2.23	2.5	ng	227134	1	6.86	1817020	20.0