
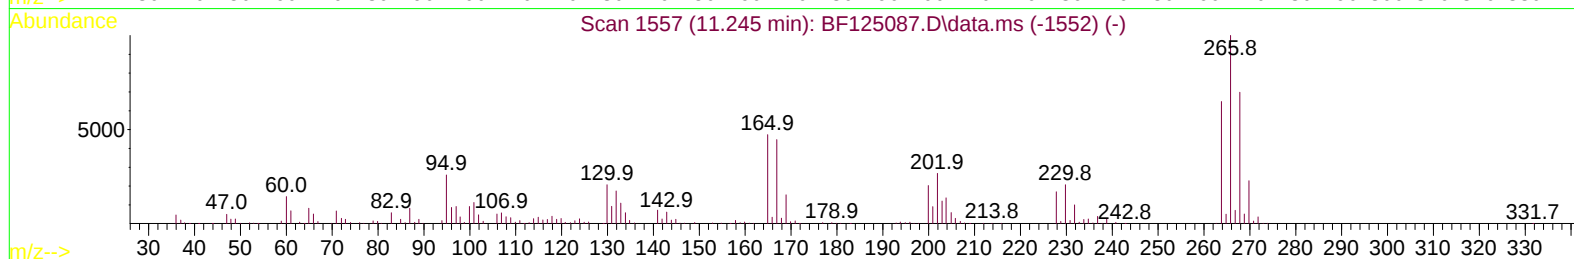
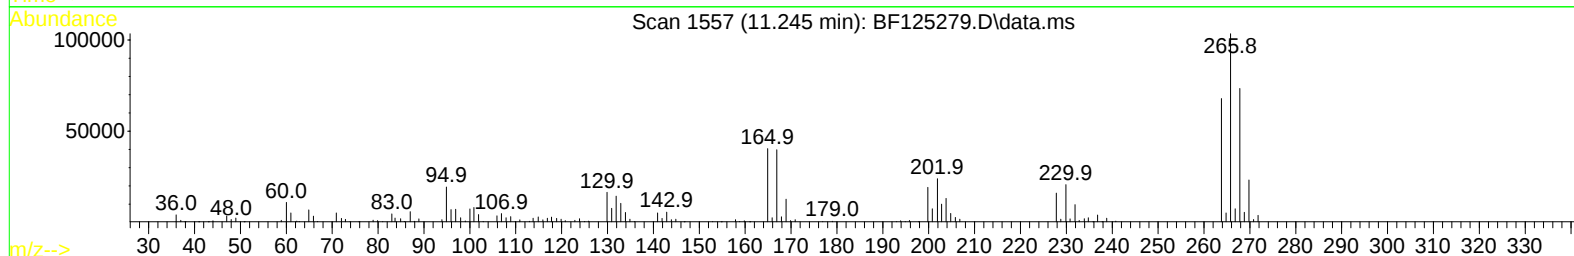


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF083121\
 Data File : BF125279.D
 Acq On : 31 Aug 2021 8:40
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 31 10:36:29 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 24 12:39:21 2021
 Response via : Initial Calibration

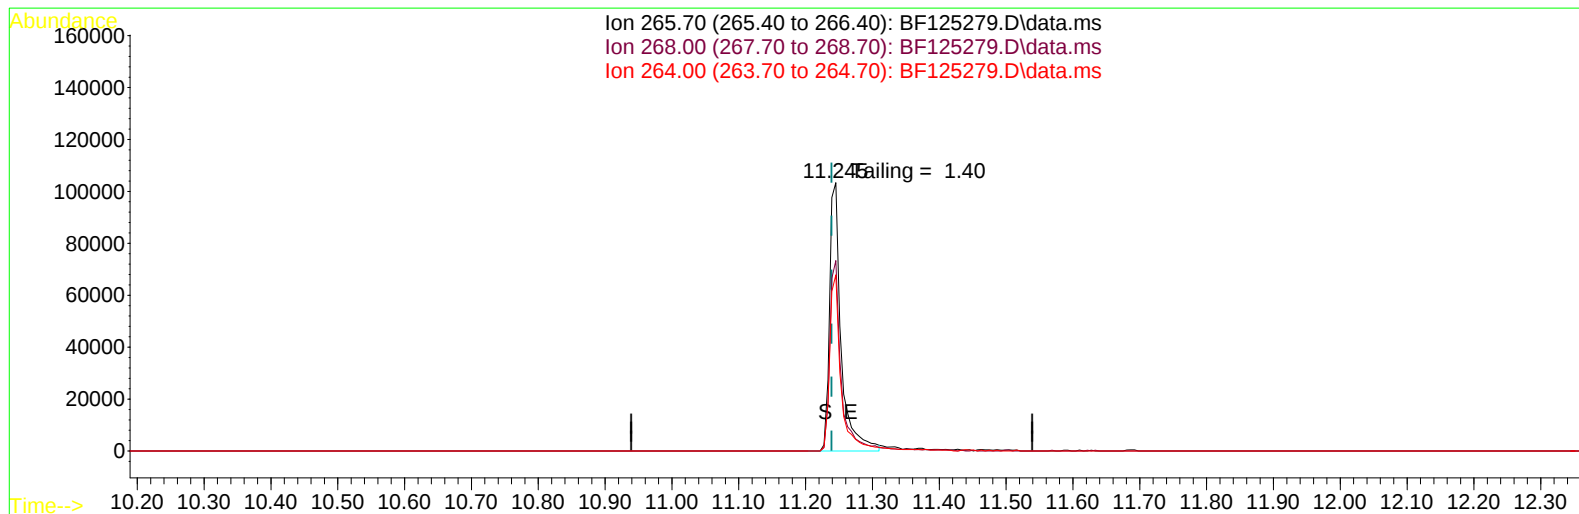

TIC: BF125279.D\data.ms

(70) Pentachlorophenol (C)




11.245min (+ 0.006) 24214.00 ng

response 128198

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	70.97
264.00	69.90	65.67
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF083121\
Data File : BF125279.D
Acq On : 31 Aug 2021 8:40
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 31 10:36:29 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 24 12:39:21 2021
Response via : Initial Calibration

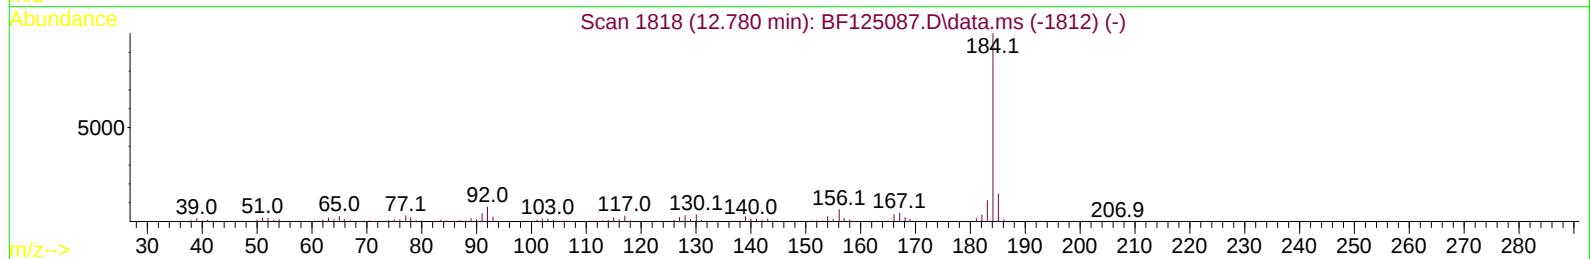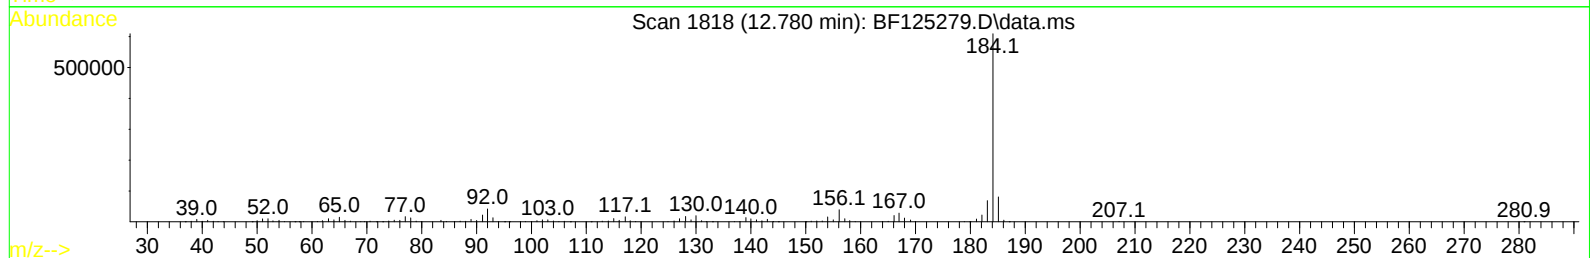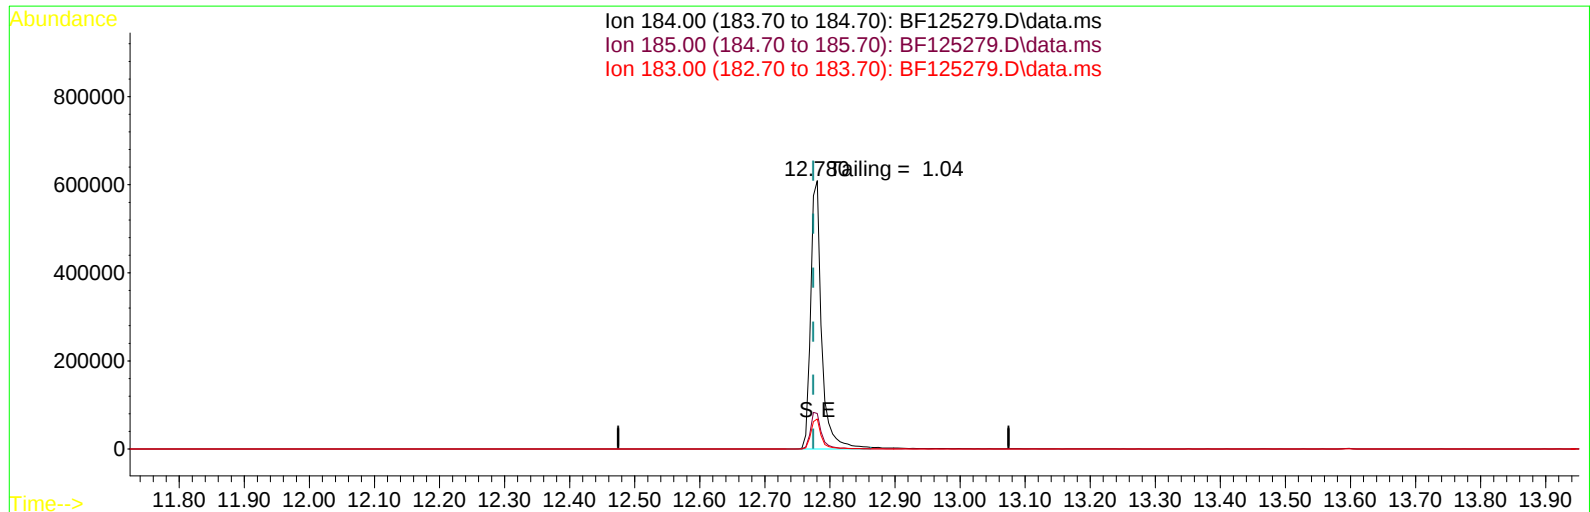

TIC: BF125279.D\data.ms

(77) Benzidine**12.780min (+ 0.006) 170918.56 ng****response 728254**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.23
183.00	10.10	11.24
0.00	0.00	0.00