

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF083121\
 Data File : BF125298.D
 Acq On : 31 Aug 2021 20:21
 Operator : JU/CG
 Sample : M3577-01 2X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 191-0827-B1-0-2

Quant Time: Sep 01 03:14:03 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 24 12:39:21 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.910	152	190337	20.000	ng	0.00
21) Naphthalene-d8	8.198	136	744660	20.000	ng	# 0.00
39) Acenaphthene-d10	9.951	164	394668	20.000	ng	0.00
64) Phenanthrene-d10	11.439	188	625966	20.000	ng	0.00
76) Chrysene-d12	14.080	240	469035	20.000	ng	# 0.00
86) Perylene-d12	15.580	264	429225	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.528	112	441615	35.118	ng	0.00
7) Phenol-d6	6.540	99	619829	38.111	ng	0.00
23) Nitrobenzene-d5	7.475	82	393896	26.630	ng	0.00
42) 2,4,6-Tribromophenol	10.739	330	123308	31.299	ng	0.00
45) 2-Fluorobiphenyl	9.269	172	788535	27.846	ng	0.00
79) Terphenyl-d14	13.021	244	695499	23.623	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF083121\
Data File : BF125298.D
Acq On : 31 Aug 2021 20:21
Operator : JU/CG
Sample : M3577-01 2X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
191-0827-B1-0-2

Quant Time: Sep 01 03:14:03 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 24 12:39:21 2021
Response via : Initial Calibration



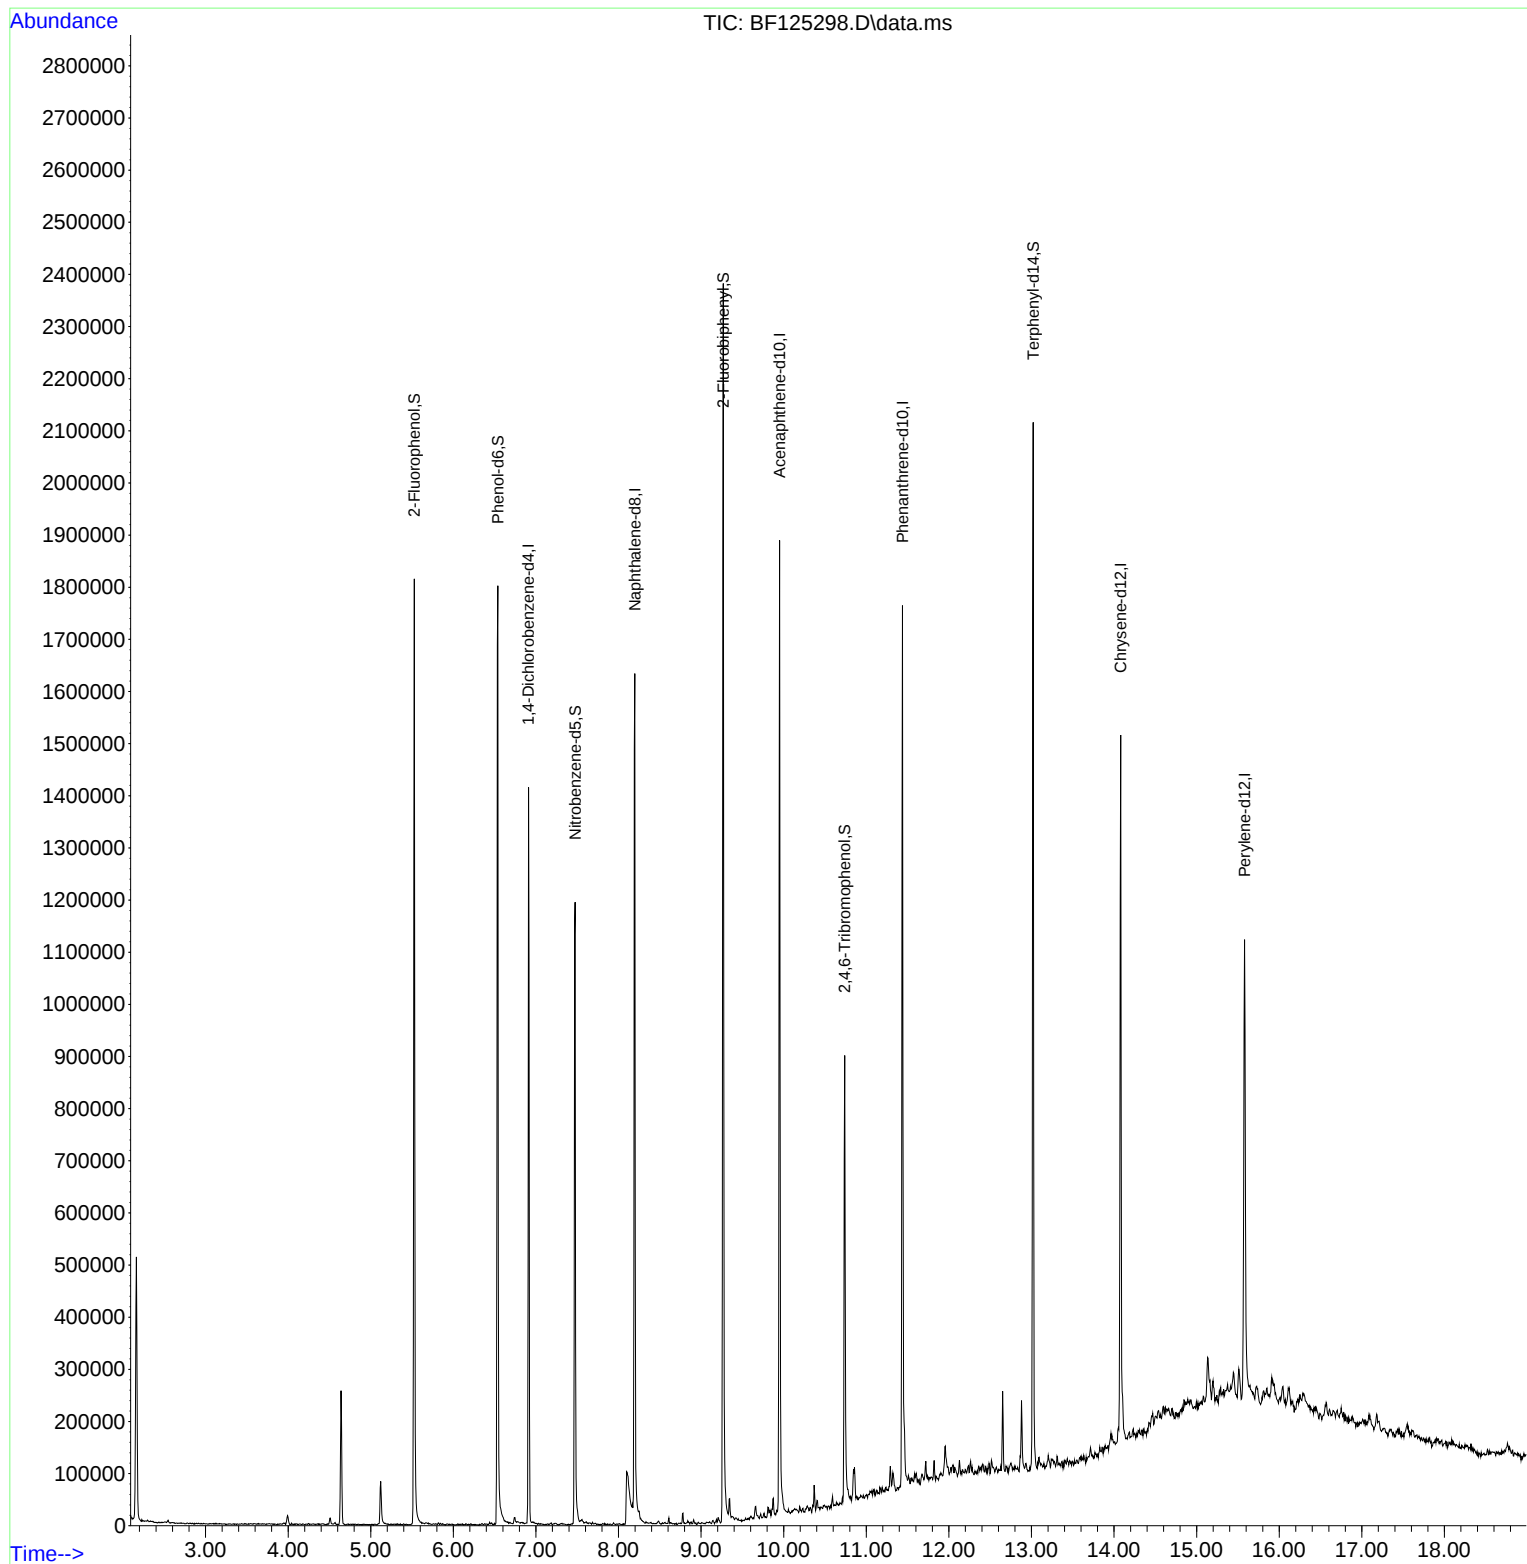




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.910 min Scan# 820
Delta R.T. -0.006 min
Lab File: BF125298.D
Acq: 31 Aug 2021 20:21




Instrument :
BNA_F
ClientSampleId :
191-0827-B1-0-2


Tgt Ion:152 Resp: 190337
Ion Ratio Lower Upper
152 100
150 159.1 117.6 176.4
115 64.0 47.1 70.7

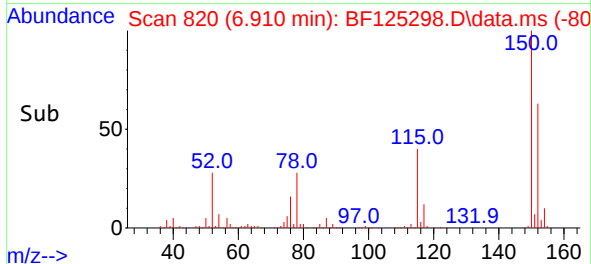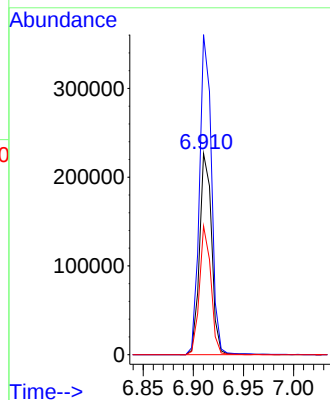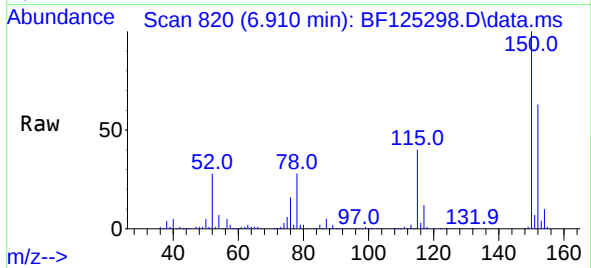

#5
2-Fluorophenol
Concen: 35.118 ng
RT: 5.528 min Scan# 585
Delta R.T. 0.000 min
Lab File: BF125298.D
Acq: 31 Aug 2021 20:21

Tgt Ion:112 Resp: 441615
Ion Ratio Lower Upper
112 100
64 70.0 44.2 66.2#
63 35.4 26.2 39.2


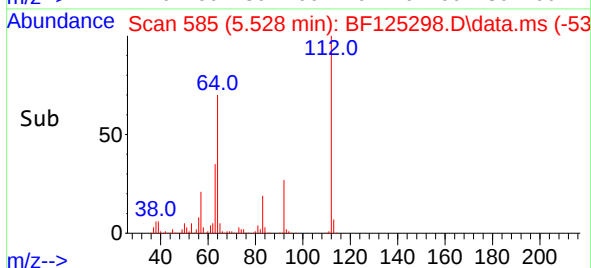
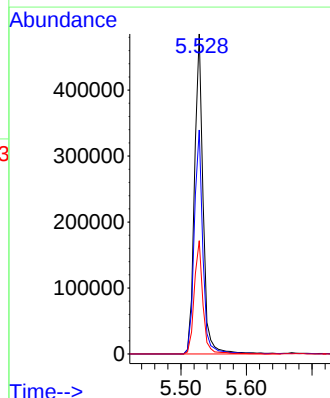
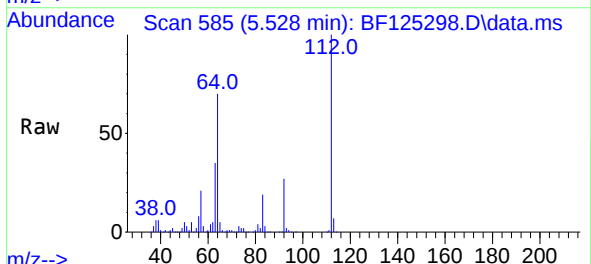


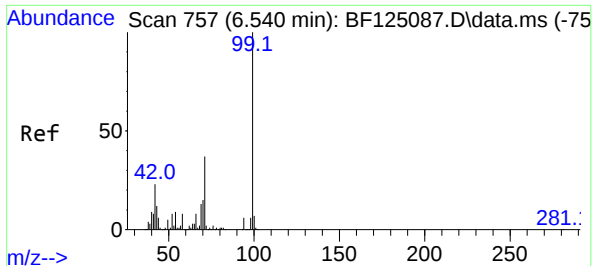

#7
Phenol-d6
Concen: 38.111 ng
RT: 6.540 min Scan# 757
Delta R.T. 0.000 min
Lab File: BF125298.D
Acq: 31 Aug 2021 20:21




Instrument :
BNA_F
ClientSampleId :
191-0827-B1-0-2


Tgt Ion: 99 Resp: 619829
Ion Ratio Lower Upper
99 100
42 19.2 23.5 35.3#
71 33.1 25.6 38.4

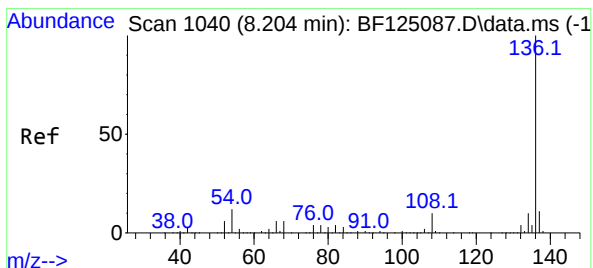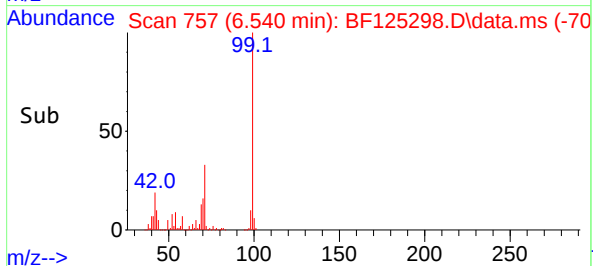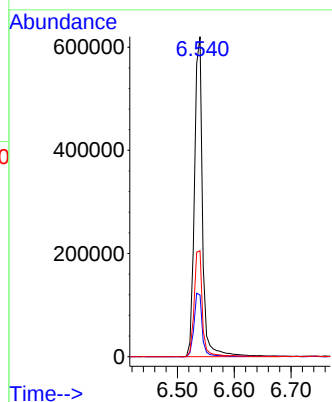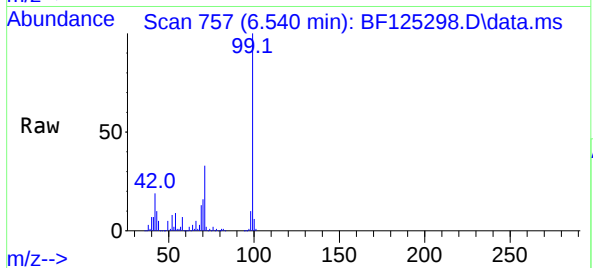

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.198 min Scan# 1039
Delta R.T. 0.000 min
Lab File: BF125298.D
Acq: 31 Aug 2021 20:21

Tgt Ion: 136 Resp: 744660
Ion Ratio Lower Upper
136 100
137 10.6 9.8 14.6
54 9.2 6.4 9.6
68 5.4 3.3 4.9#


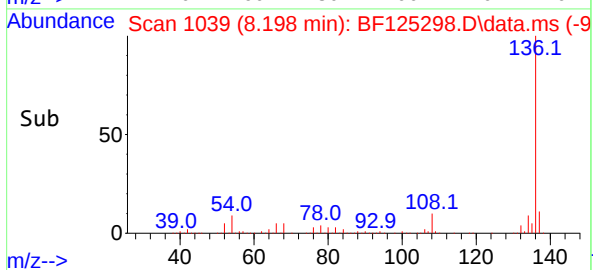
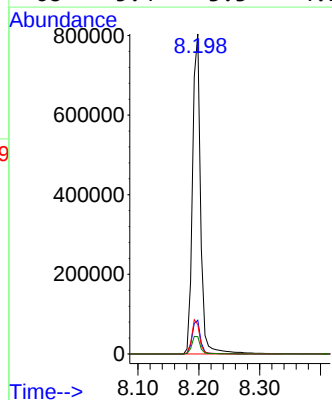
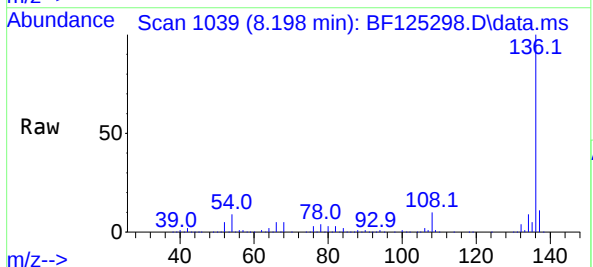


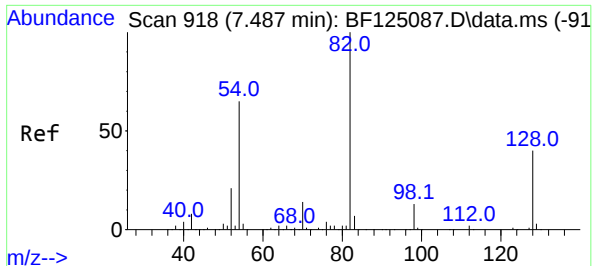

#23
Nitrobenzene-d5
Concen: 26.630 ng
RT: 7.475 min Scan# 916
Delta R.T. -0.006 min
Lab File: BF125298.D
Acq: 31 Aug 2021 20:21




Instrument :
BNA_F
ClientSampleId :
191-0827-B1-0-2


Tgt Ion: 82 Resp: 393896
Ion Ratio Lower Upper
82 100
128 41.6 40.6 60.8
54 59.8 49.6 74.4

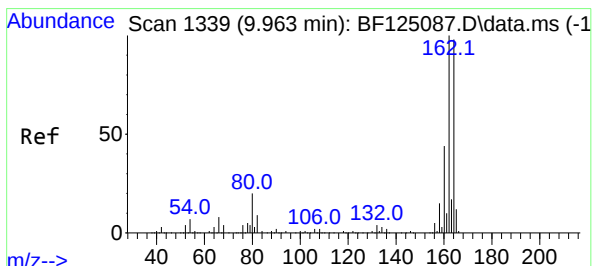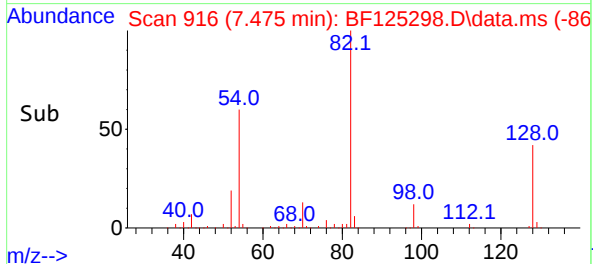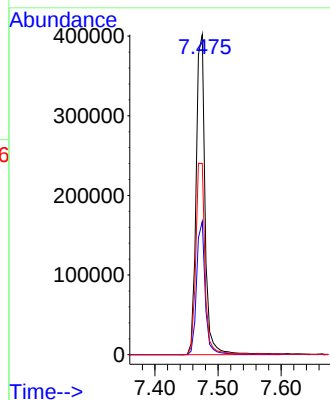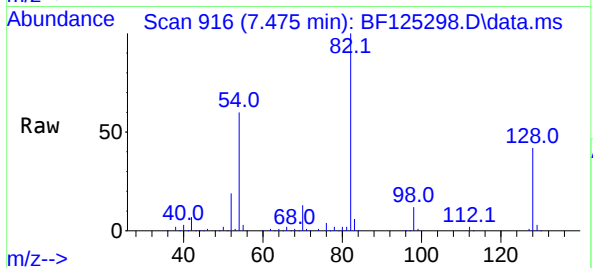

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.951 min Scan# 1337
Delta R.T. 0.000 min
Lab File: BF125298.D
Acq: 31 Aug 2021 20:21

Tgt Ion: 164 Resp: 394668
Ion Ratio Lower Upper
164 100
162 102.4 81.3 121.9
160 47.3 38.0 57.0


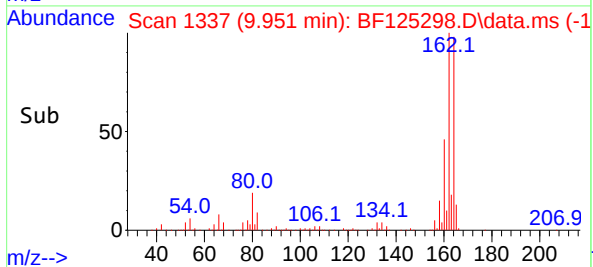
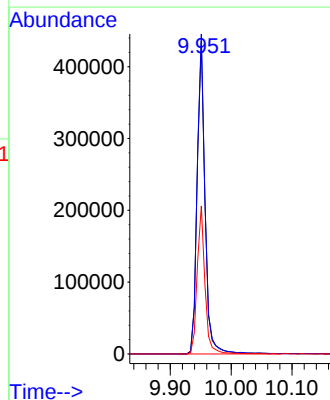
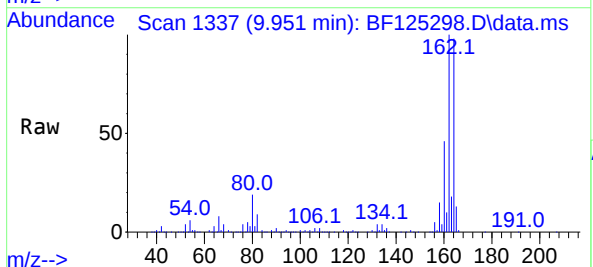


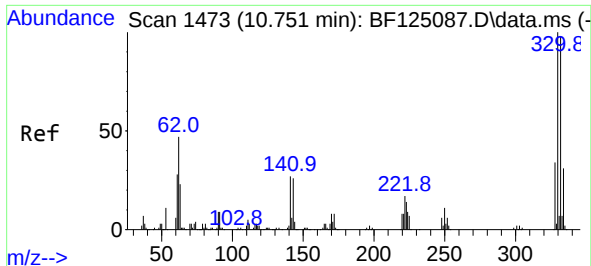

#42
2,4,6-Tribromophenol
Concen: 31.299 ng
RT: 10.739 min Scan# 1471
Delta R.T. 0.000 min
Lab File: BF125298.D
Acq: 31 Aug 2021 20:21




Instrument :
BNA_F
ClientSampleId :
191-0827-B1-0-2


Tgt Ion:330 Resp: 123308
Ion Ratio Lower Upper
330 100
332 91.4 76.2 114.4
141 29.9 44.6 66.8#

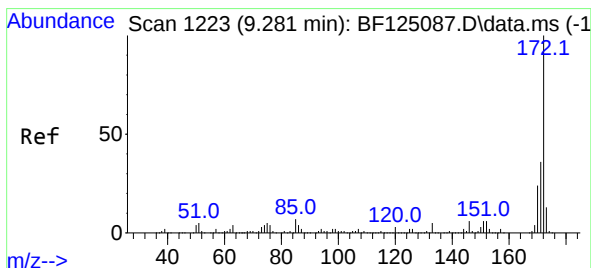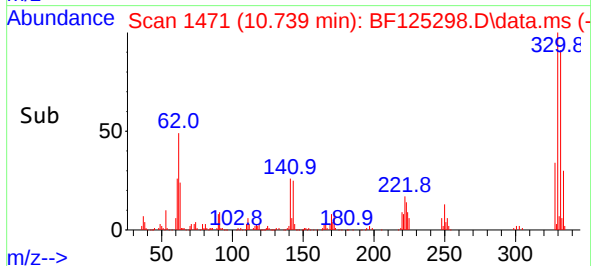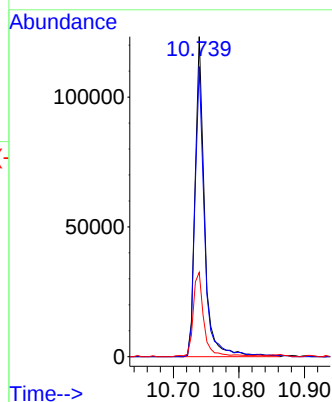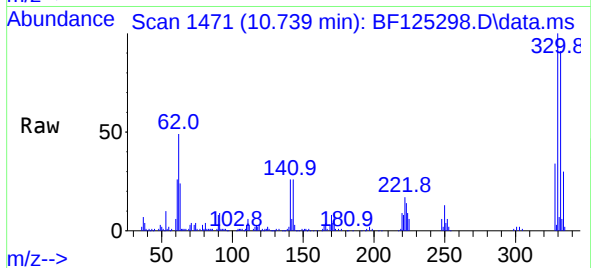

#45
2-Fluorobiphenyl
Concen: 27.846 ng
RT: 9.269 min Scan# 1221
Delta R.T. -0.006 min
Lab File: BF125298.D
Acq: 31 Aug 2021 20:21

Tgt Ion:172 Resp: 788535
Ion Ratio Lower Upper
172 100
171 34.8 26.5 39.7
170 24.1 18.8 28.2


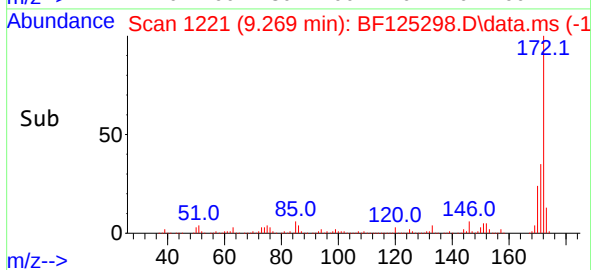
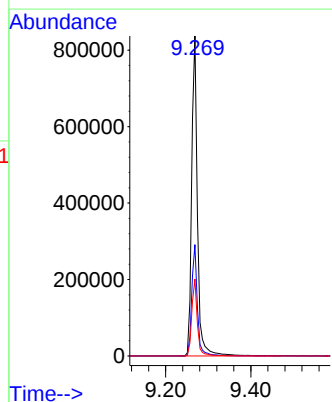
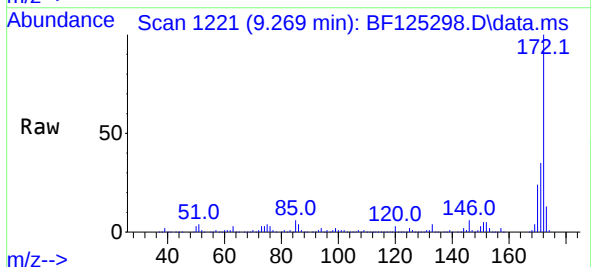


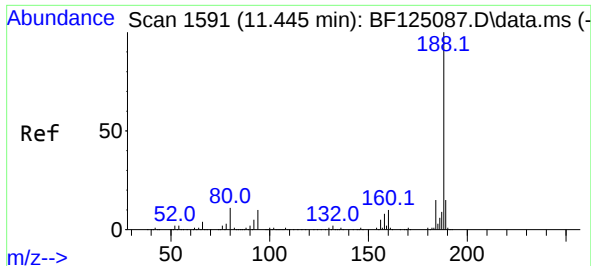

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.439 min Scan# 1590
Delta R.T. 0.000 min
Lab File: BF125298.D
Acq: 31 Aug 2021 20:21




Instrument :
BNA_F
ClientSampleId :
191-0827-B1-0-2


Tgt Ion:188 Resp: 625966
Ion Ratio Lower Upper
188 100
94 8.5 6.7 10.1
80 9.4 7.5 11.3

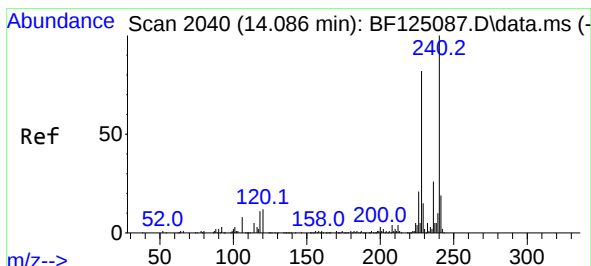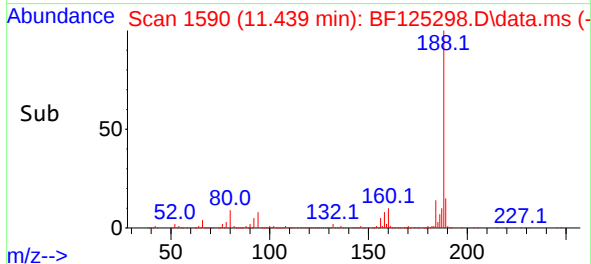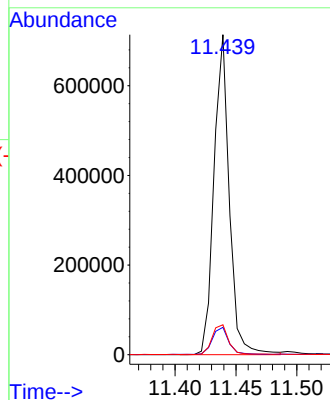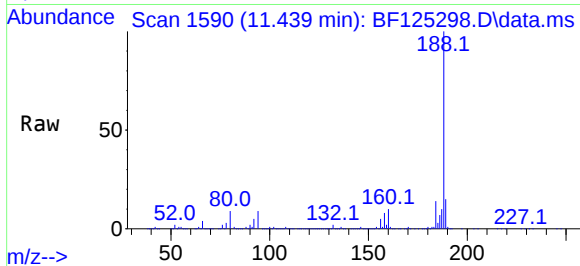

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.080 min Scan# 2039
Delta R.T. 0.000 min
Lab File: BF125298.D
Acq: 31 Aug 2021 20:21

Tgt Ion:240 Resp: 469035
Ion Ratio Lower Upper
240 100
120 9.4 10.8 16.2#
236 25.3 21.6 32.4


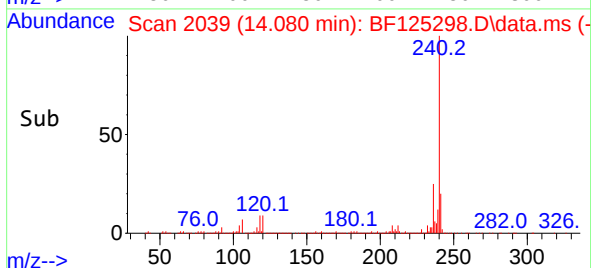
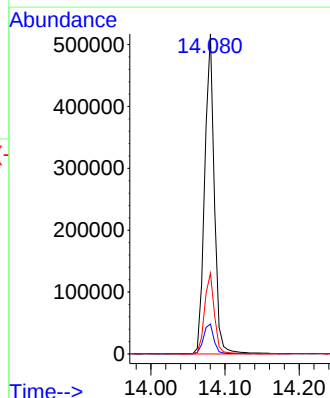
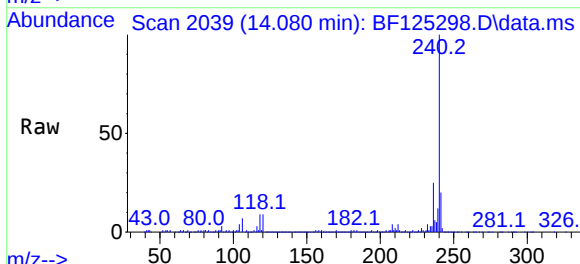


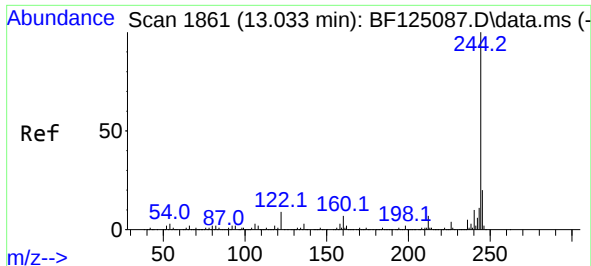

#79
Terphenyl-d14
Concen: 23.623 ng
RT: 13.021 min Scan# 1859
Delta R.T. 0.000 min
Lab File: BF125298.D
Acq: 31 Aug 2021 20:21

Instrument :
BNA_F
ClientSampleId :
191-0827-B1-0-2

Tgt Ion:244 Resp: 695499
Ion Ratio Lower Upper
244 100
212 6.5 5.9 8.9
122 8.3 9.0 13.4#

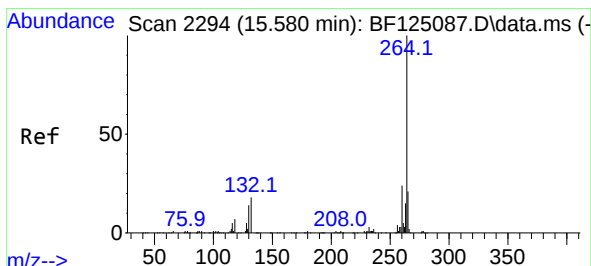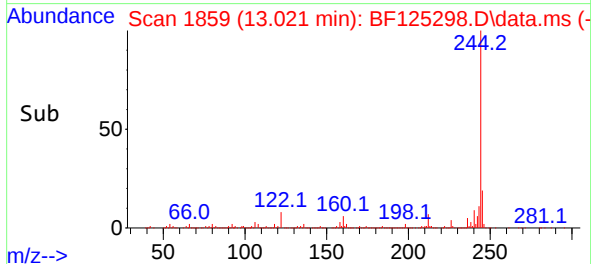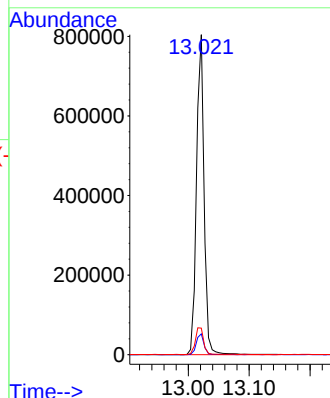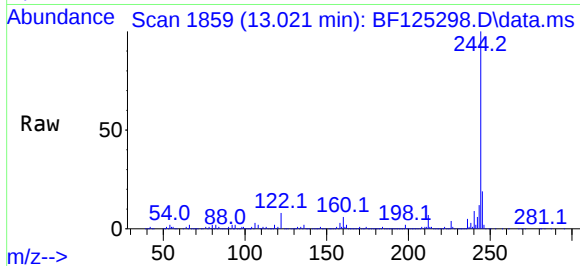

#86
Perylene-d12
Concen: 20.000 ng
RT: 15.580 min Scan# 2294
Delta R.T. 0.006 min
Lab File: BF125298.D
Acq: 31 Aug 2021 20:21

Tgt Ion:264 Resp: 429225
Ion Ratio Lower Upper
264 100
260 23.6 19.6 29.4
265 21.9 17.2 25.8

